

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121818\
 Data File : BN004091.D
 Acq On : 18 Dec 2018 23:44
 Operator : JU/SJ
 Sample : J6271-12
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9E27

Manual Integrations
 APPROVED

Sohil
 12/19/2018 4:16:45 PM

Quant Time: Dec 19 04:35:41 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 19 04:08:55 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	2005	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	9646	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	5922	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.22	188	14584m	0.40	ng/ul	0.00
16) Chrysene-d12	21.40	240	15097m	0.40	ng/ul	0.00
20) Perylene-d12	23.72	264	13546m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.21	152	4503	0.30	ng/ul	0.00
14) Fluoranthene-d10	19.24	212	13809m	0.32	ng/ul	0.00
Target Compounds						
12) Phenanthrene	17.25	178	1137m	0.024	ng/ul	Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121818\
Data File : BN004091.D
Acq On : 18 Dec 2018 23:44
Operator : JU/SJ
Sample : J6271-12
Misc :
ALS Vial : 22 Sample Multiplier: 1




Instrument :
BNA_N
ClientSampleId :
F9E27

Manual Integrations
APPROVED

Sohil
12/19/2018 4:16:45 PM

Quant Time: Dec 19 04:35:41 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 19 04:08:55 2018
Response via : Initial Calibration

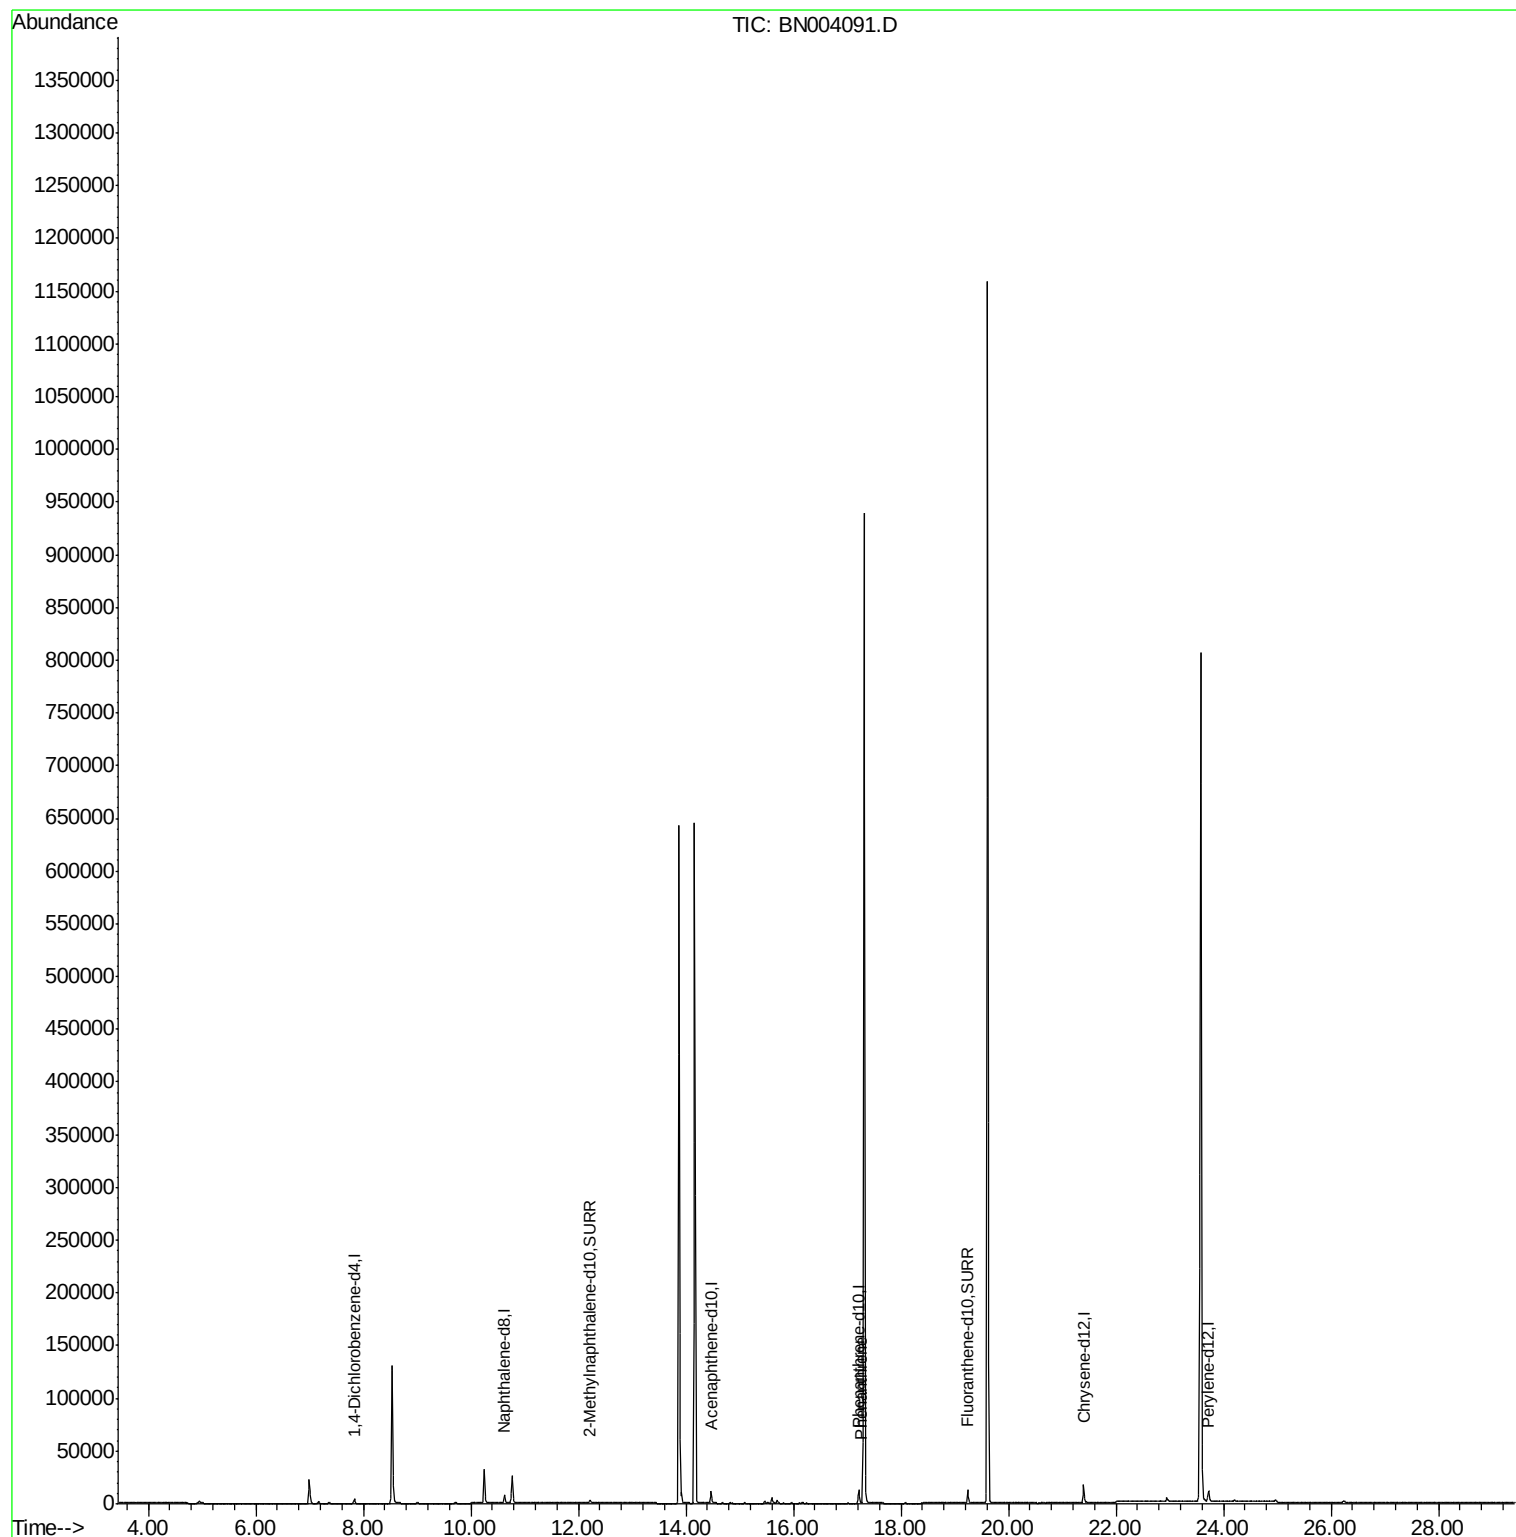

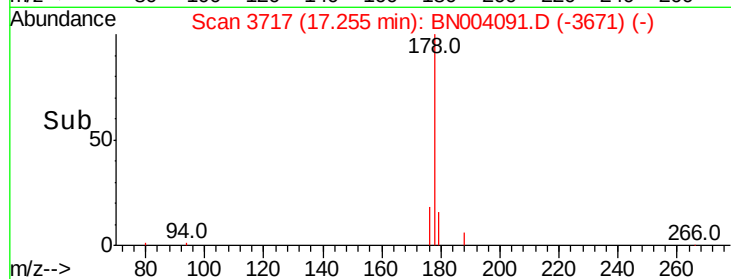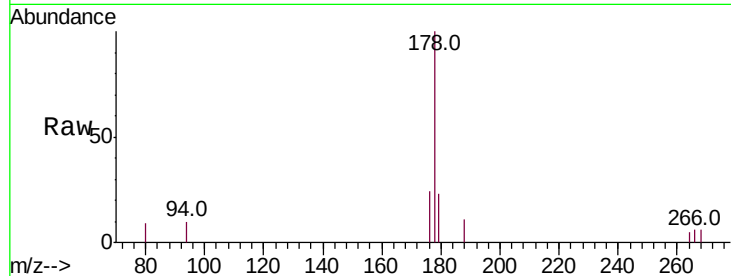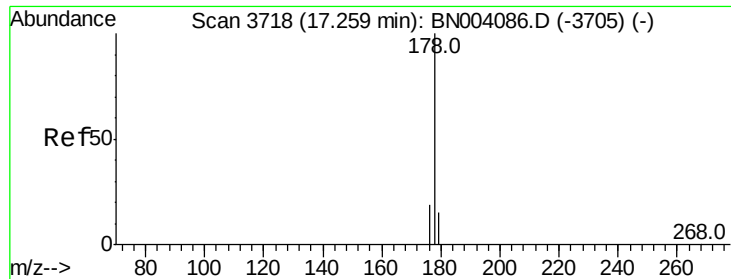

#12

Phenanthrene

Concen: 0.024 ng/ul m

RT: 17.25 min Scan# 3717

Delta R.T. -0.00 min

Lab File: BN004091.D

Acq: 18 Dec 2018 23:44

Instrument :

BNA_N

ClientSampleId :

F9E27

Tot Ion:178 Resp: 1137

Ion Ratio Lower Upper

178 100

179 22.9 12.5 18.7#

176 24.2 15.0 22.4#

Manual Integrations
APPROVED

Sohil
12/19/2018 4:16:45 PM

