




Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN121824\  
Data File : BN035697.D  
Acq On : 19 Dec 2024 09:42  
Operator : RC/JU  
Sample : PB165589BL  
Misc :  
ALS Vial : 38 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
SBLK589

Manual IntegrationsAPPROVED

Quant Time: Dec 19 11:22:48 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\SFAM-EPA-SIM-BN121624.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Dec 16 16:26:08 2024  
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/21/2024  
Supervised By :mohammad ahmed 12/24/2024

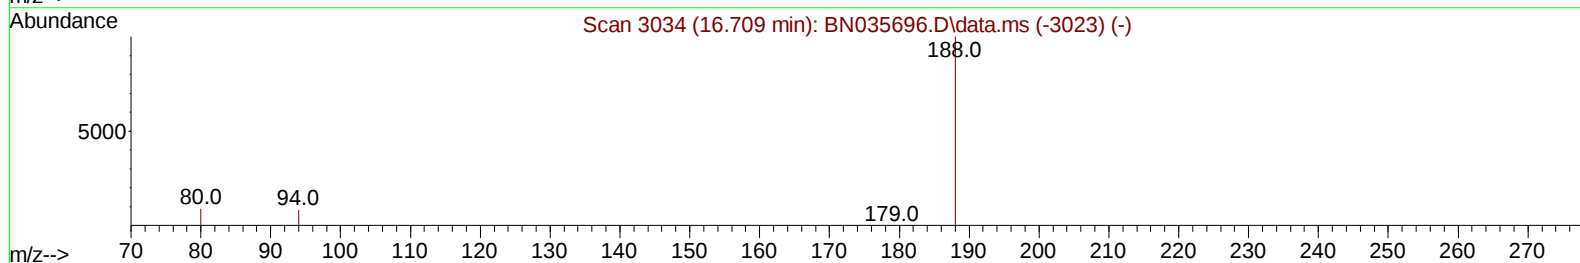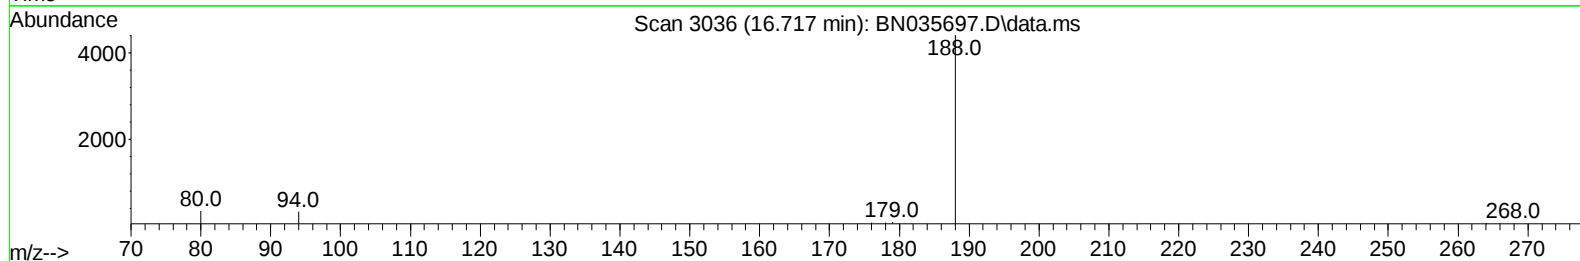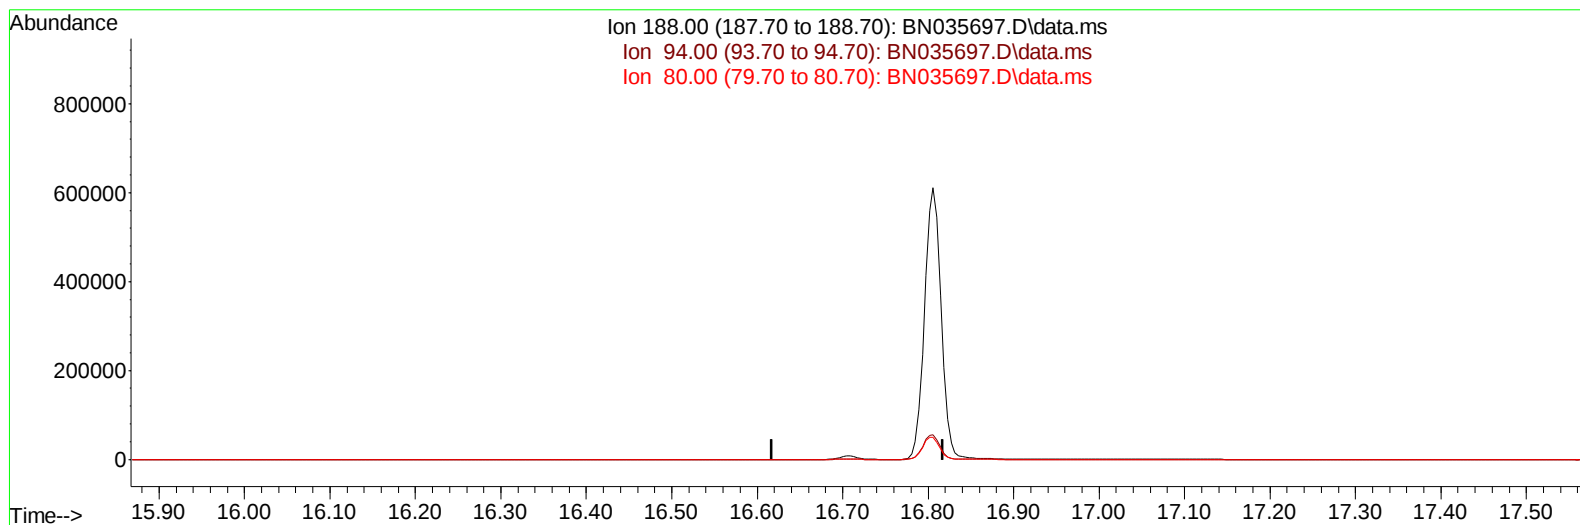

TIC: BN035697.D\data.ms

(13) Phenanthrene-d10 (I)

16.717min (-16.717) 0.00 ng/u1

response 0

| Ion    | Exp%   | Act%  |
|--------|--------|-------|
| 188.00 | 100.00 | 0.00  |
| 94.00  | 8.50   | 0.00# |
| 80.00  | 9.10   | 0.00# |
| 0.00   | 0.00   | 0.00  |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN121824\  
Data File : BN035697.D  
Acq On : 19 Dec 2024 09:42  
Operator : RC/JU  
Sample : PB165589BL  
Misc :  
ALS Vial : 38 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
SBLK589

Manual IntegrationsAPPROVED

Quant Time: Dec 19 11:22:48 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\SFAM-EPA-SIM-BN121624.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Dec 16 16:26:08 2024  
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/21/2024  
Supervised By :mohammad ahmed 12/24/2024

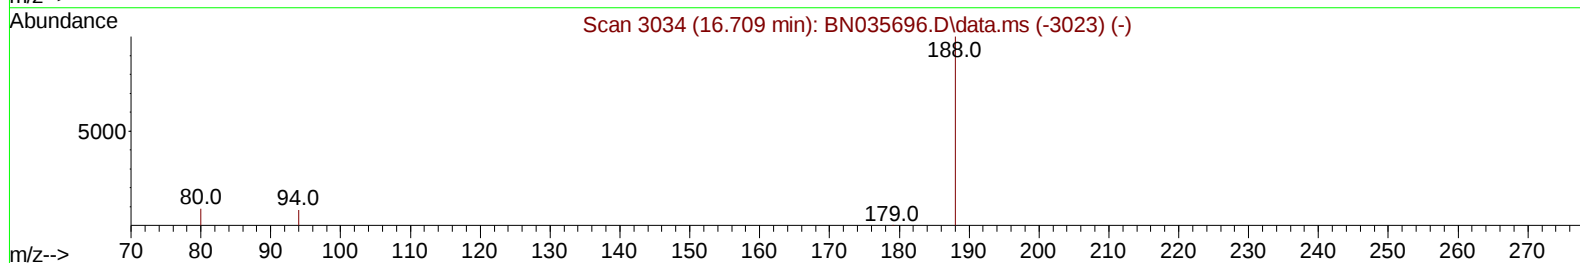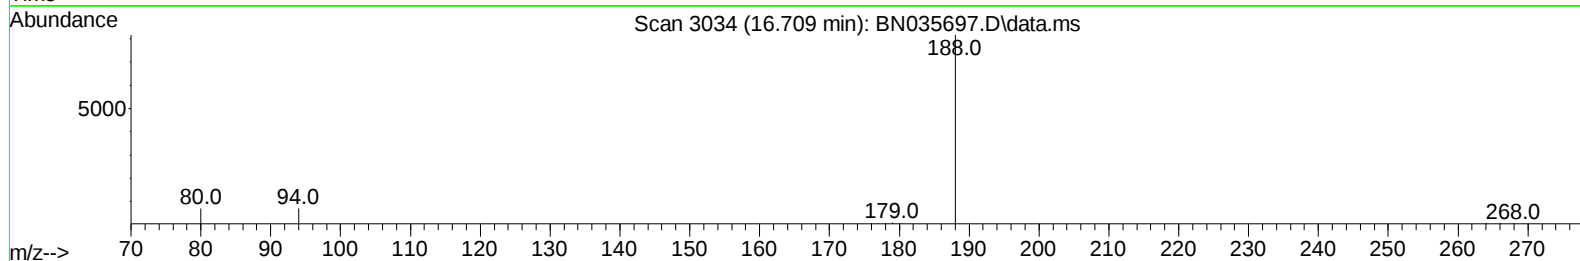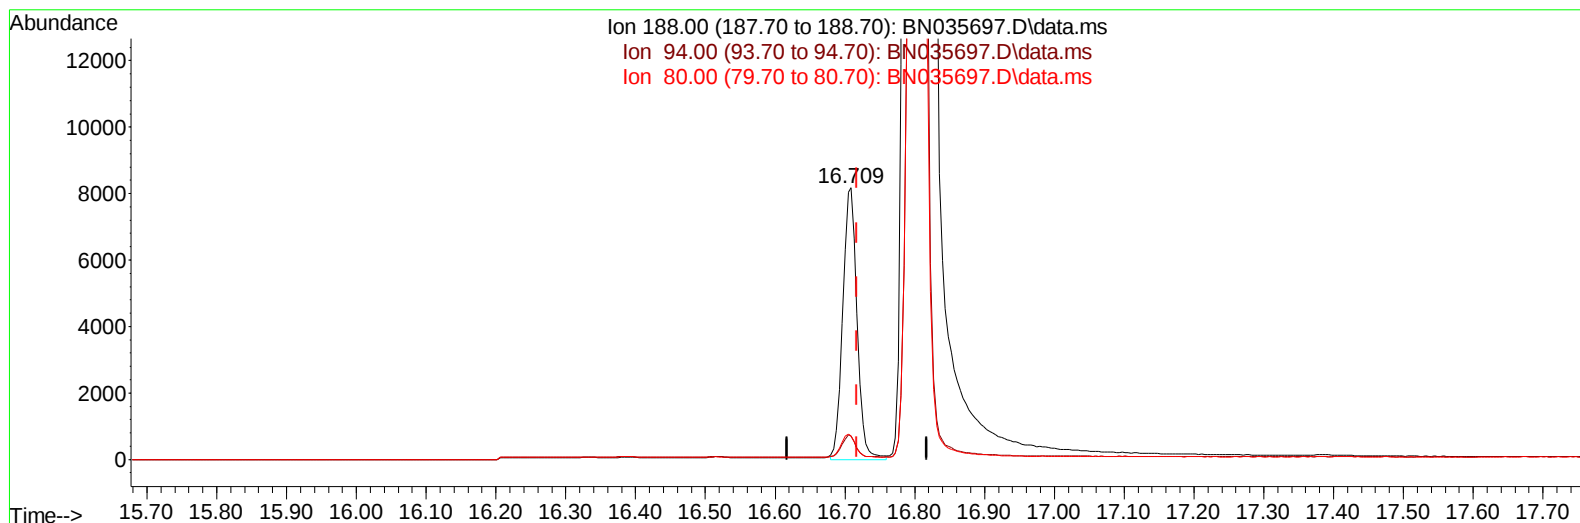

TIC: BN035697.D\data.ms

(13) Phenanthrene-d10 (I)

16.709min (-0.008) 0.40 ng/u1 m

response 11596

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 188.00 | 100.00 | 100.00 |
| 94.00  | 8.50   | 8.54   |
| 80.00  | 9.10   | 8.57   |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN121824\  
Data File : BN035697.D  
Acq On : 19 Dec 2024 09:42  
Operator : RC/JU  
Sample : PB165589BL  
Misc :  
ALS Vial : 38 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
SBLK589

## Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/21/2024  
Supervised By :mohammad ahmed 12/24/2024

Quant Time: Dec 19 11:22:48 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\SFAM-EPA-SIM-BN121624.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Dec 16 16:26:08 2024  
Response via : Initial Calibration

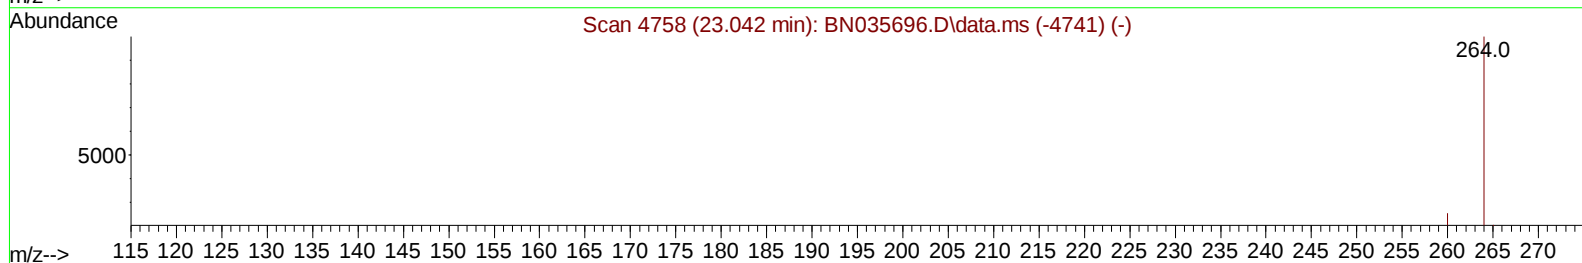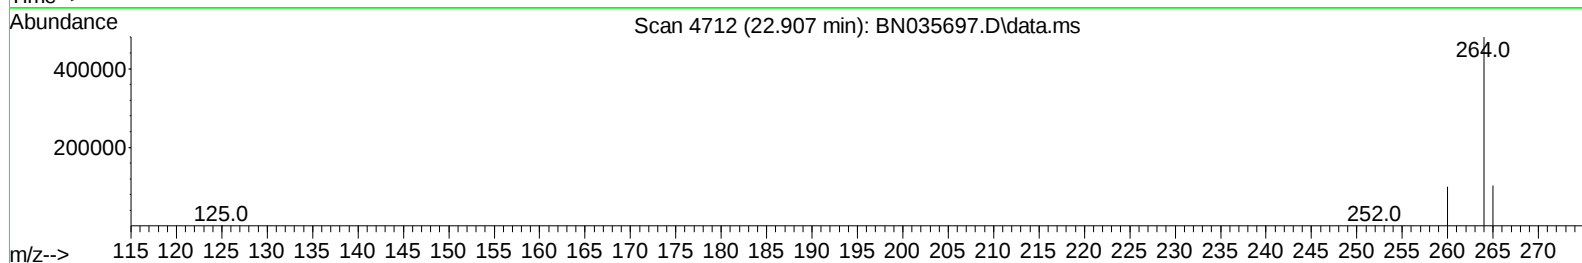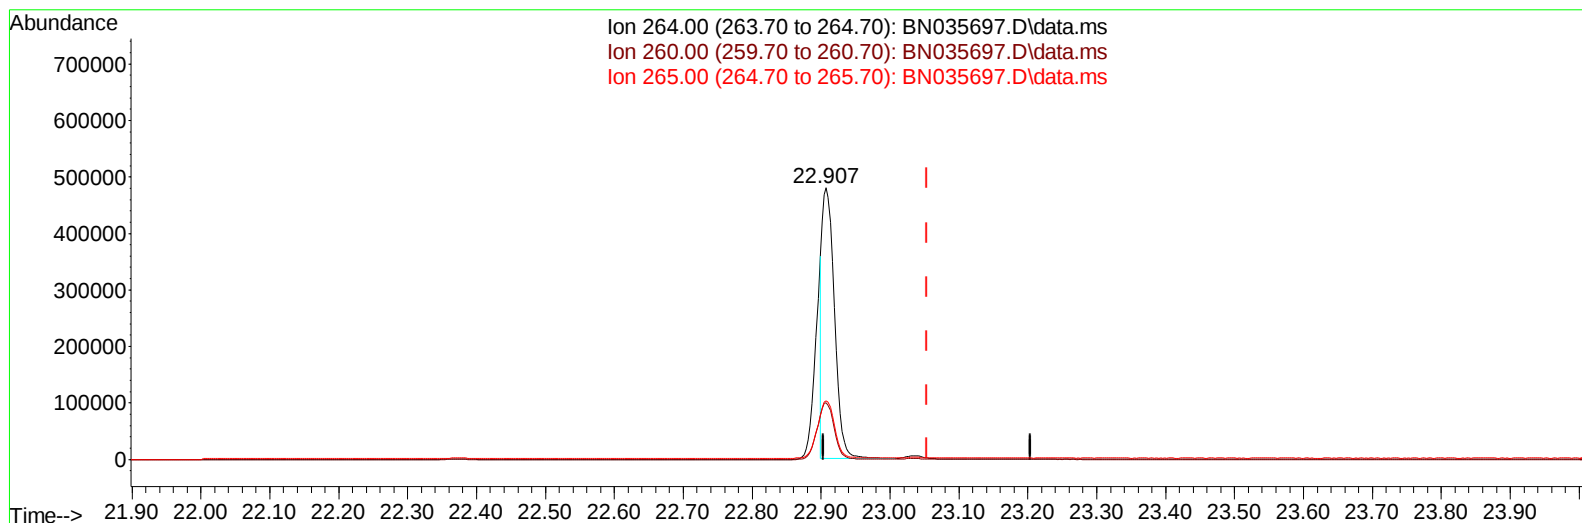

TIC: BN035697.D\data.ms

## (23) Perylene-d12 (I)

22.907min (-0.146) 0.40 ng/u1

response 596873

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 264.00 | 100.00 | 100.00 |
| 260.00 | 27.40  | 20.97# |
| 265.00 | 62.10  | 21.62# |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN121824\  
Data File : BN035697.D  
Acq On : 19 Dec 2024 09:42  
Operator : RC/JU  
Sample : PB165589BL  
Misc :  
ALS Vial : 38 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
SBLK589

## Manual IntegrationsAPPROVED

Quant Time: Dec 19 11:22:48 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\SFAM-EPA-SIM-BN121624.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Dec 16 16:26:08 2024  
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/21/2024  
Supervised By :mohammad ahmed 12/24/2024

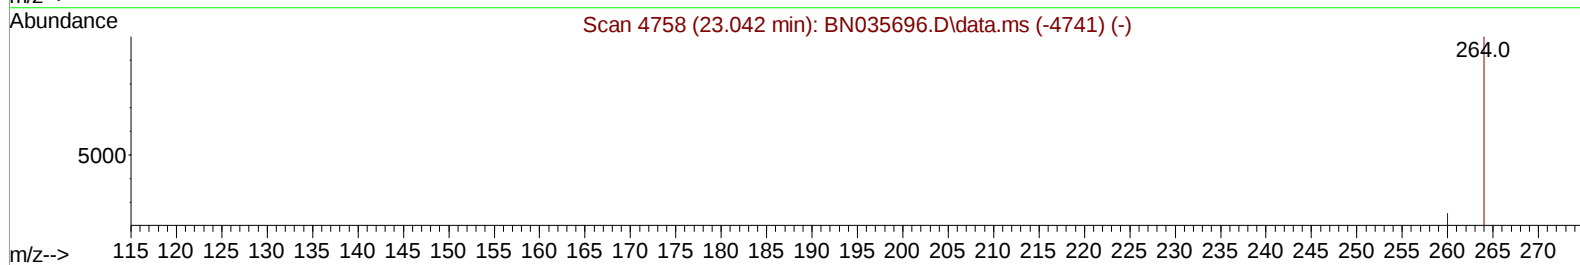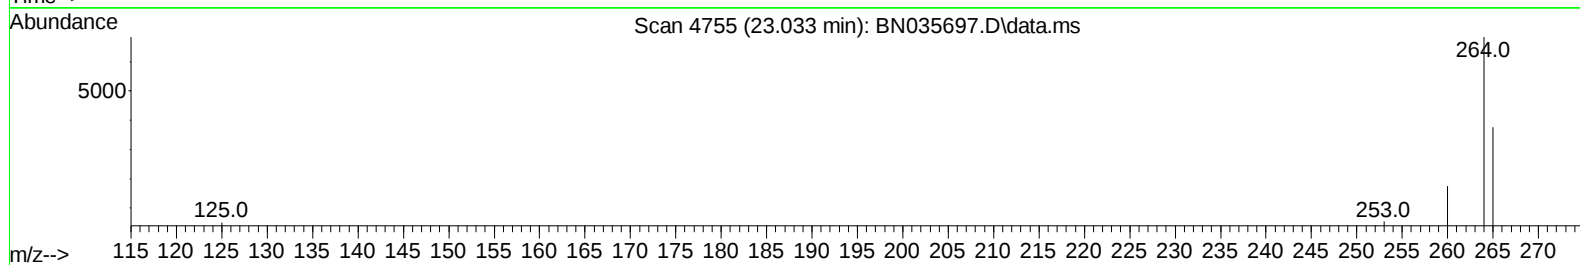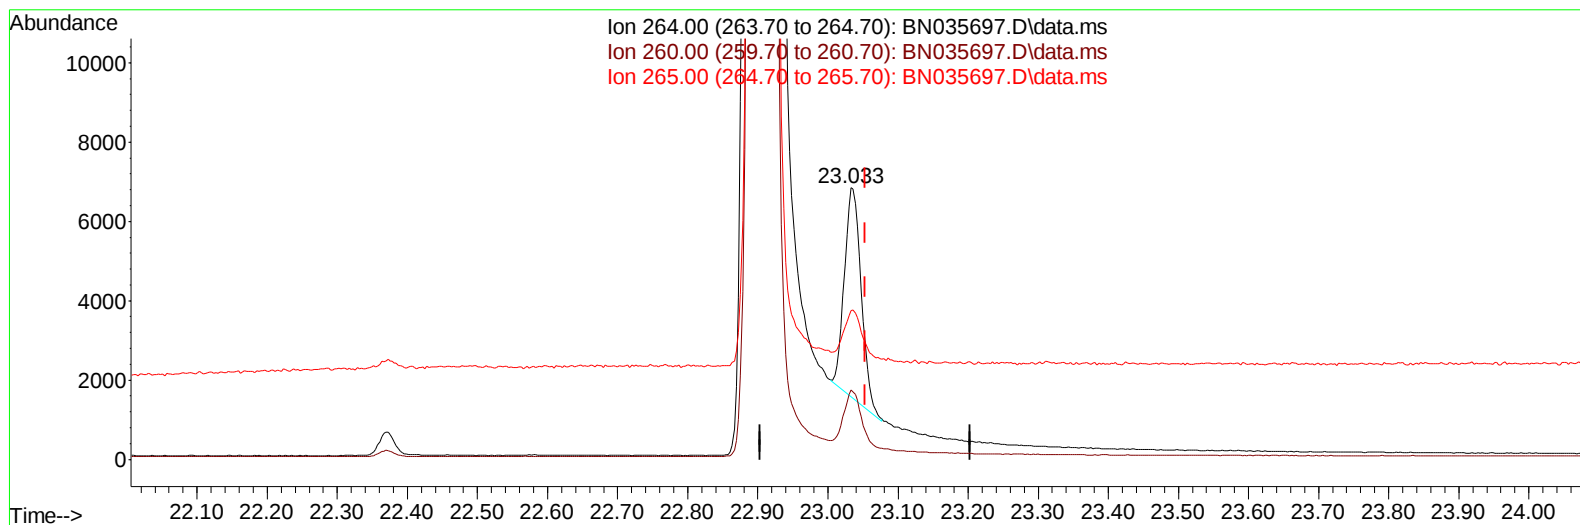

TIC: BN035697.D\data.ms

## (23) Perylene-d12 (I)

23.033min (-0.020) 0.40 ng/ul m

response 8756

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 264.00 | 100.00 | 100.00 |
| 260.00 | 27.40  | 25.68  |
| 265.00 | 62.10  | 54.92  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN121824\  
 Data File : BN035697.D  
 Acq On : 19 Dec 2024 09:42  
 Operator : RC/JU  
 Sample : PB165589BL  
 Misc :  
 ALS Vial : 38 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 SBLK589

## Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/21/2024  
 Supervised By :mohammad ahmed 12/24/2024

Quant Time: Dec 19 11:22:48 2024  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\SFAM-EPA-SIM-BN121624.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Mon Dec 16 16:26:08 2024  
 Response via : Initial Calibration

| Compound                    | R.T.   | QIon | Response | Conc  | Units | Dev(Min) |
|-----------------------------|--------|------|----------|-------|-------|----------|
| -----                       |        |      |          |       |       |          |
| Internal Standards          |        |      |          |       |       |          |
| 1) 1,4-Dichlorobenzene-d4   | 7.276  | 152  | 2960     | 0.400 | ng/ul | 0.00     |
| 4) Naphthalene-d8           | 10.020 | 136  | 7763     | 0.400 | ng/ul | -0.01    |
| 9) Acenaphthene-d10         | 13.939 | 164  | 5582     | 0.400 | ng/ul | 0.00     |
| 13) Phenanthrene-d10        | 16.709 | 188  | 11596m   | 0.400 | ng/ul | 0.00     |
| 17) Chrysene-d12            | 20.955 | 240  | 9327     | 0.400 | ng/ul | 0.00     |
| 23) Perylene-d12            | 23.033 | 264  | 8756m    | 0.400 | ng/ul | -0.02    |
|                             |        |      |          |       |       |          |
| System Monitoring Compounds |        |      |          |       |       |          |
| 3) 1,4-Dioxane-d8           | 2.951  | 96   | 17318    | 6.599 | ng/ul | 0.00     |
| 6) 2-Methylnaphthalene-d10  | 11.626 | 152  | 4272     | 0.386 | ng/ul | -0.01    |
| 18) Fluoranthene-d10        | 18.763 | 212  | 9678     | 0.355 | ng/ul | 0.00     |

|                  |        |
|------------------|--------|
| Target Compounds | Qvalue |
| -----            |        |

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN121824\  
Data File : BN035697.D  
Acq On : 19 Dec 2024 09:42  
Operator : RC/JU  
Sample : PB165589BL  
Misc :  
ALS Vial : 38 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
SBLK589

## Manual IntegrationsAPPROVED

Quant Time: Dec 19 11:22:48 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\SFAM-EPA-SIM-BN121624.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Dec 16 16:26:08 2024  
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/21/2024  
Supervised By :mohammad ahmed 12/24/2024

