




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121824\
Data File : BN035699.D
Acq On : 19 Dec 2024 10:54
Operator : RC/JU
Sample : P5258-04
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E28X0

Manual IntegrationsAPPROVED

Quant Time: Dec 19 11:41:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 16 16:26:08 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/21/2024
Supervised By :mohammad ahmed 12/24/2024

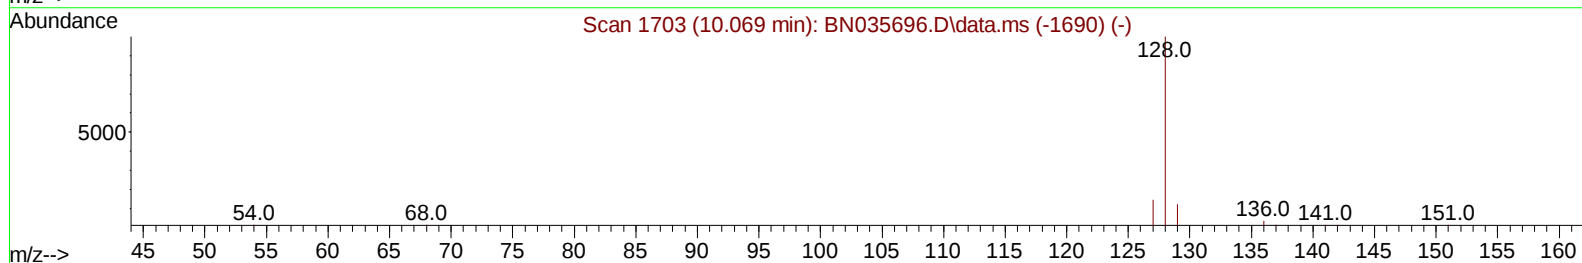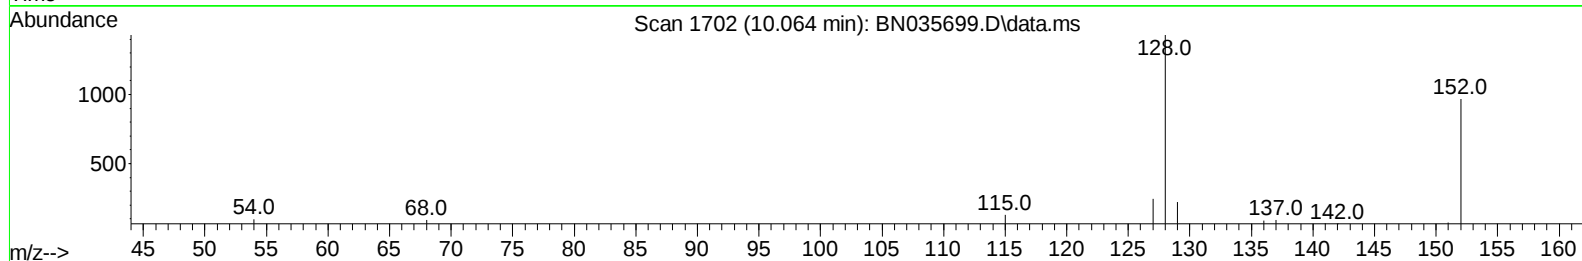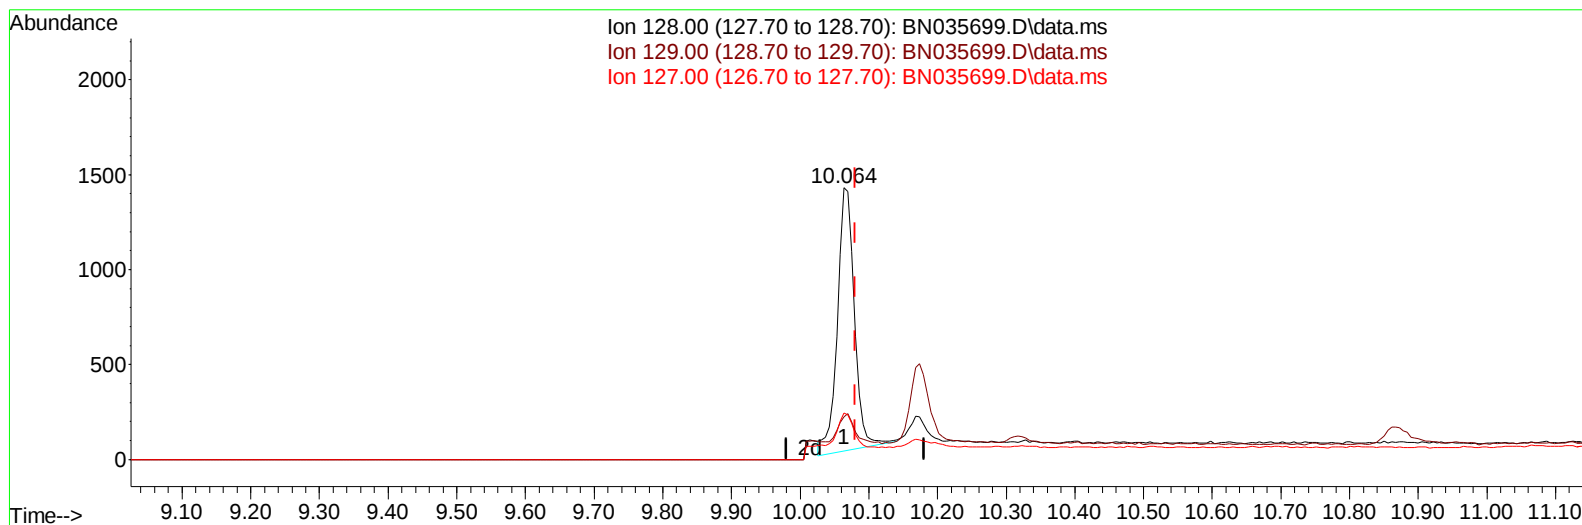

TIC: BN035699.D\data.ms

(5) Naphthalene

10.064min (-0.016) 0.11 ng/u1

response 2386

Ion	Exp%	Act%
128.00	100.00	100.00
129.00	13.50	15.59
127.00	15.00	17.13
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121824\
Data File : BN035699.D
Acq On : 19 Dec 2024 10:54
Operator : RC/JU
Sample : P5258-04
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E28X0

Manual IntegrationsAPPROVED

Quant Time: Dec 19 11:41:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 16 16:26:08 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/21/2024
Supervised By :mohammad ahmed 12/24/2024

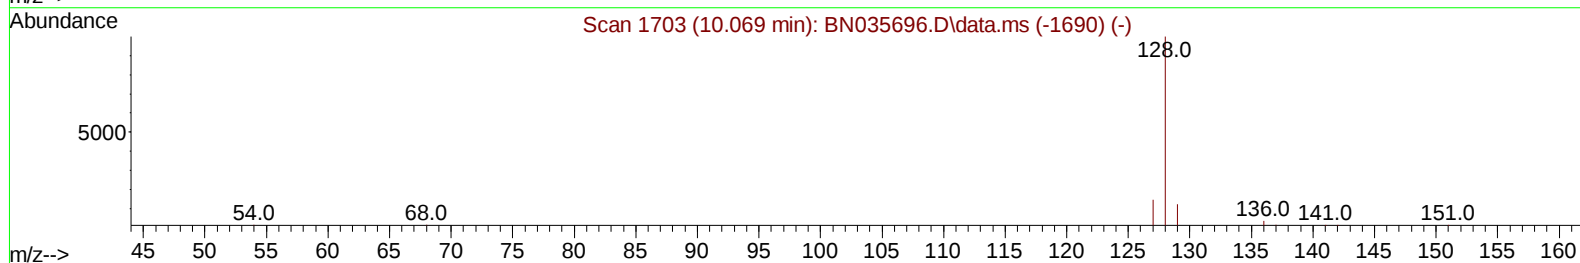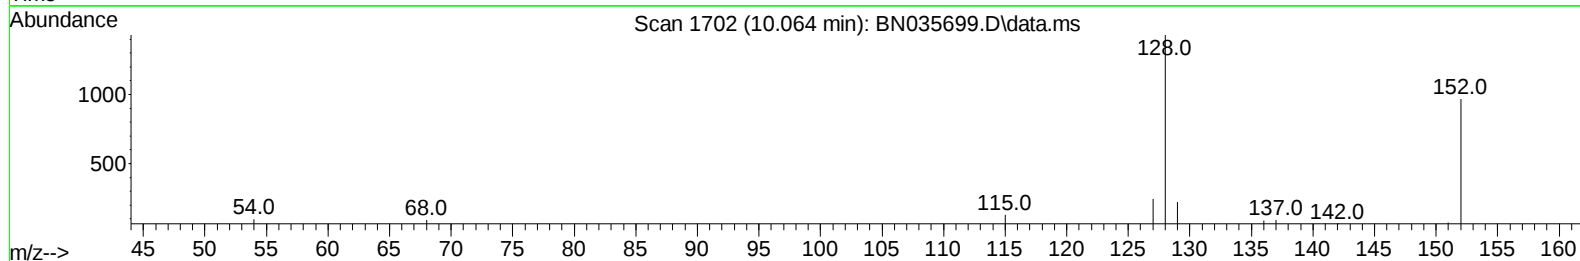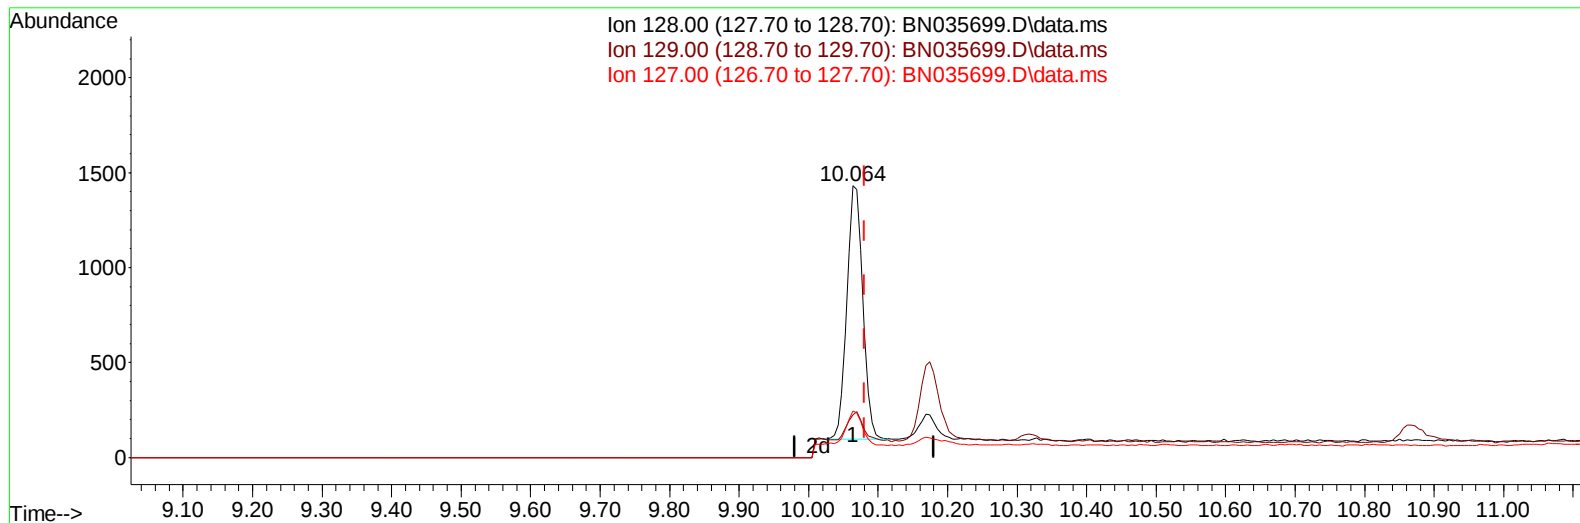

TIC: BN035699.D\data.ms

(5) Naphthalene

10.064min (-0.016) 0.10 ng/ul m

response 2127

Ion	Exp%	Act%
128.00	100.00	100.00
129.00	13.50	15.59
127.00	15.00	17.13
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121824\
Data File : BN035699.D
Acq On : 19 Dec 2024 10:54
Operator : RC/JU
Sample : P5258-04
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E28X0

Manual IntegrationsAPPROVED

Quant Time: Dec 19 11:41:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 16 16:26:08 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/21/2024
Supervised By :mohammad ahmed 12/24/2024

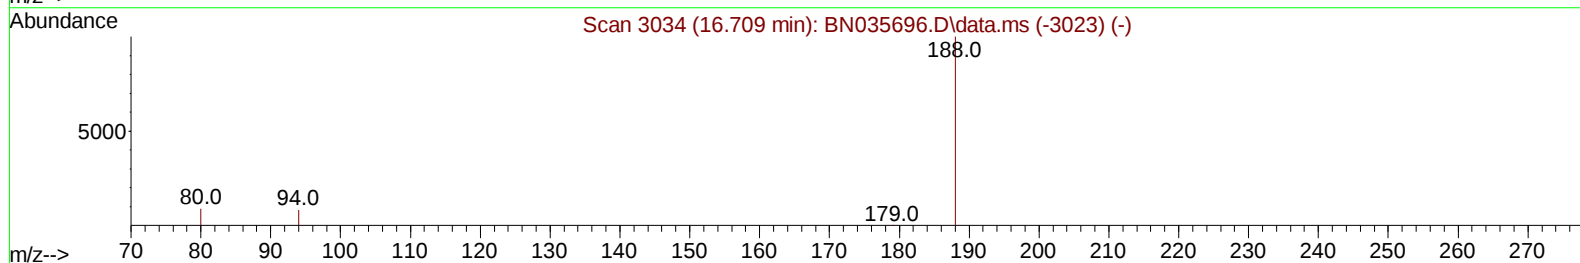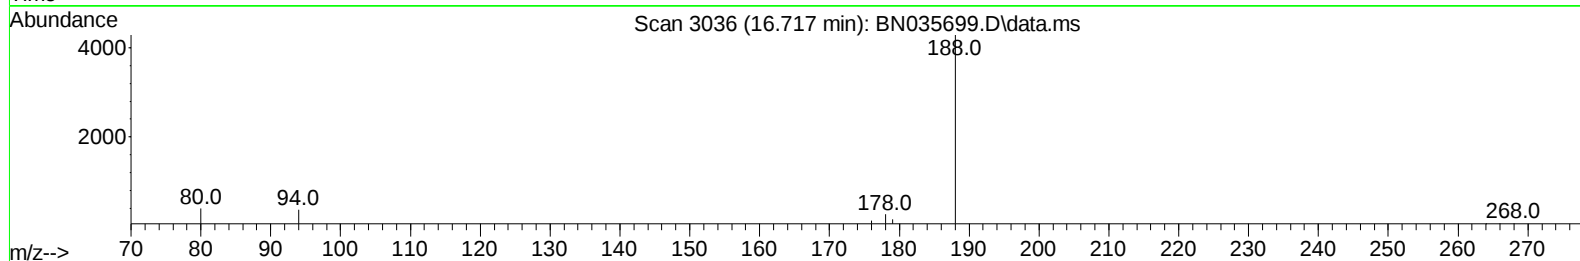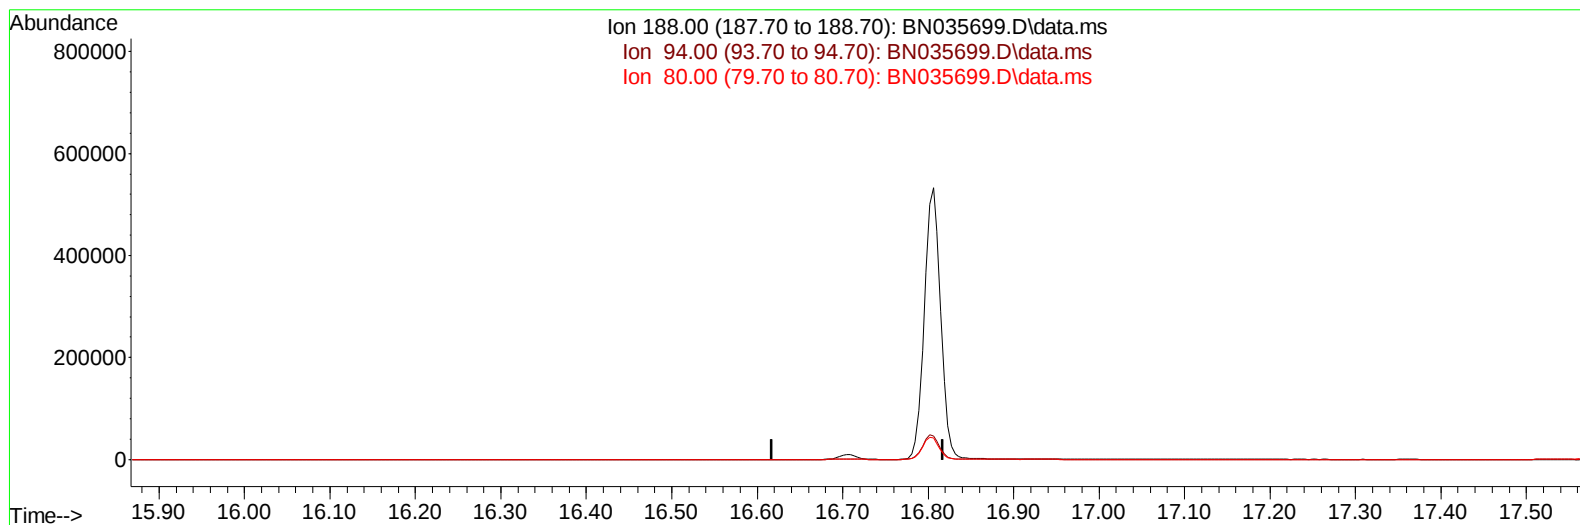

TIC: BN035699.D\data.ms

(13) Phenanthrene-d10 (I)

16.717min (-16.717) 0.00 ng/u1

response 0

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	8.50	0.00#
80.00	9.10	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121824\
Data File : BN035699.D
Acq On : 19 Dec 2024 10:54
Operator : RC/JU
Sample : P5258-04
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E28X0

Manual IntegrationsAPPROVED

Quant Time: Dec 19 11:41:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 16 16:26:08 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/21/2024
Supervised By :mohammad ahmed 12/24/2024

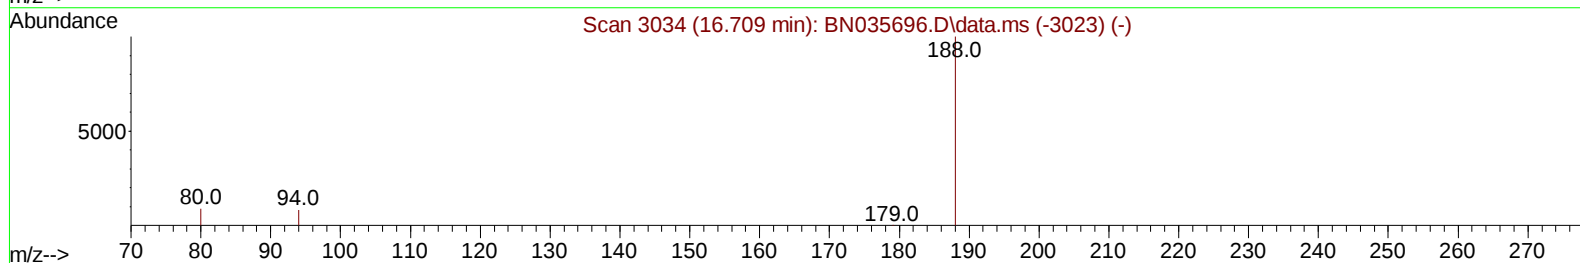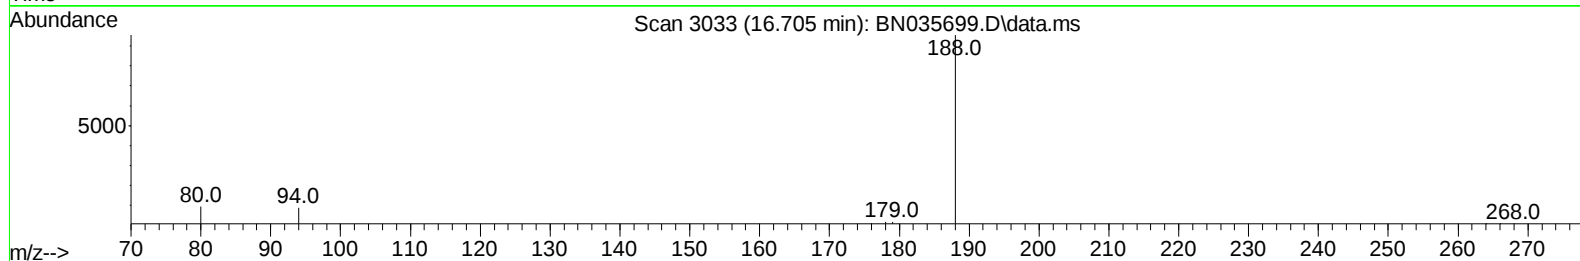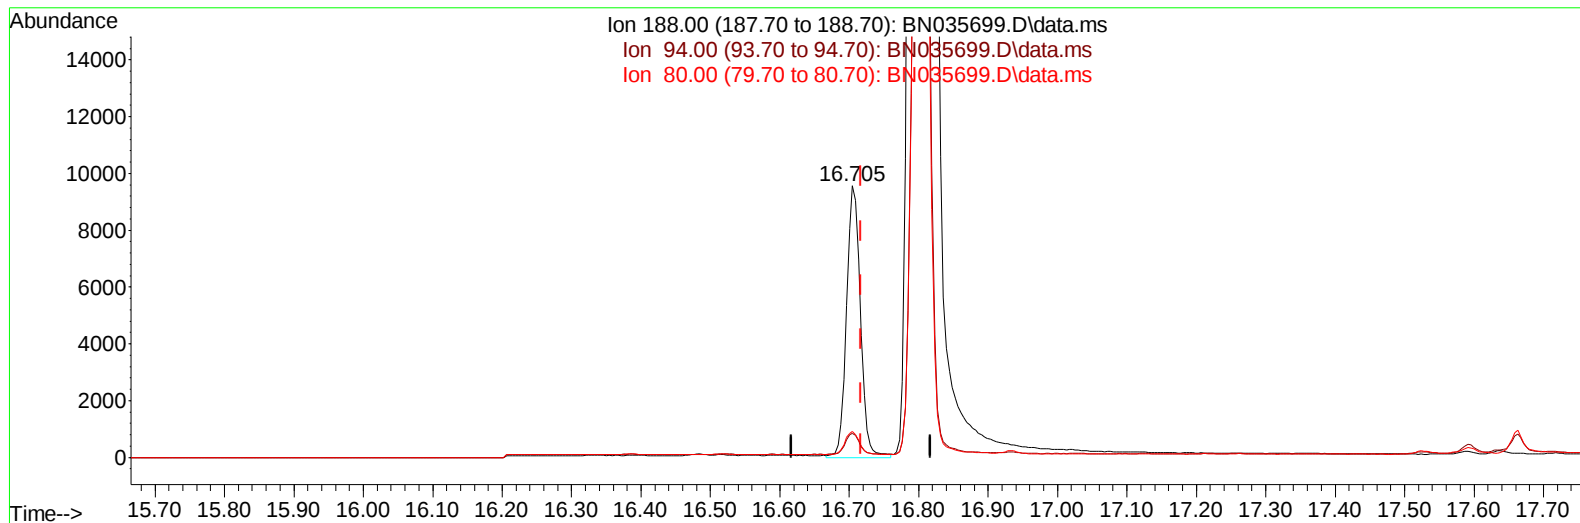

TIC: BN035699.D\data.ms

(13) Phenanthrene-d10 (I)

16.705min (-0.012) 0.40 ng/ul m

response 13319

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	8.50	8.90
80.00	9.10	9.57
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121824\
Data File : BN035699.D
Acq On : 19 Dec 2024 10:54
Operator : RC/JU
Sample : P5258-04
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E28X0

Manual IntegrationsAPPROVED

Quant Time: Dec 19 11:41:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 16 16:26:08 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/21/2024
Supervised By :mohammad ahmed 12/24/2024

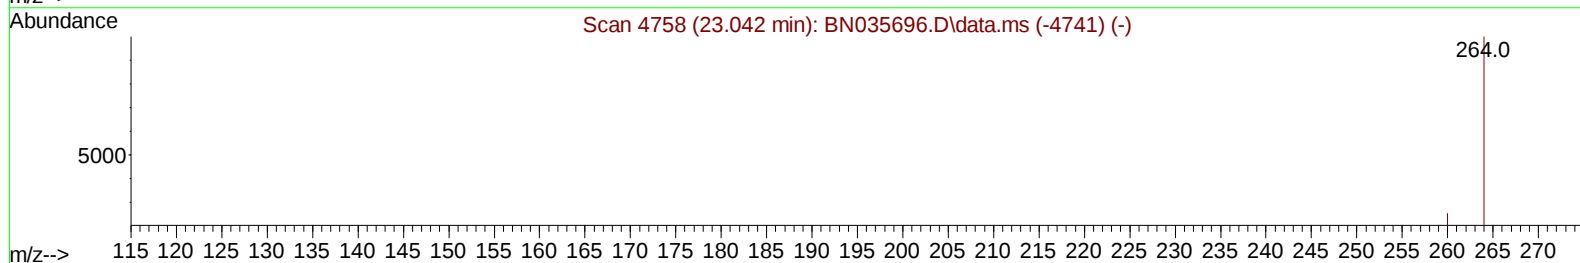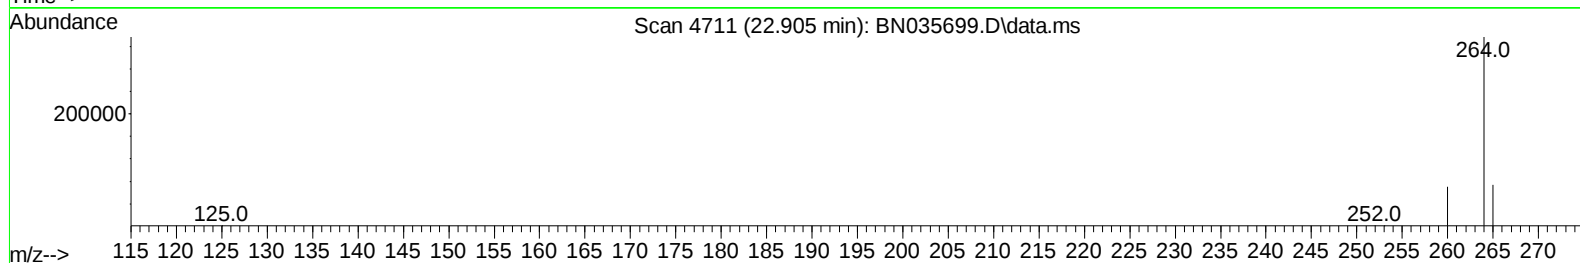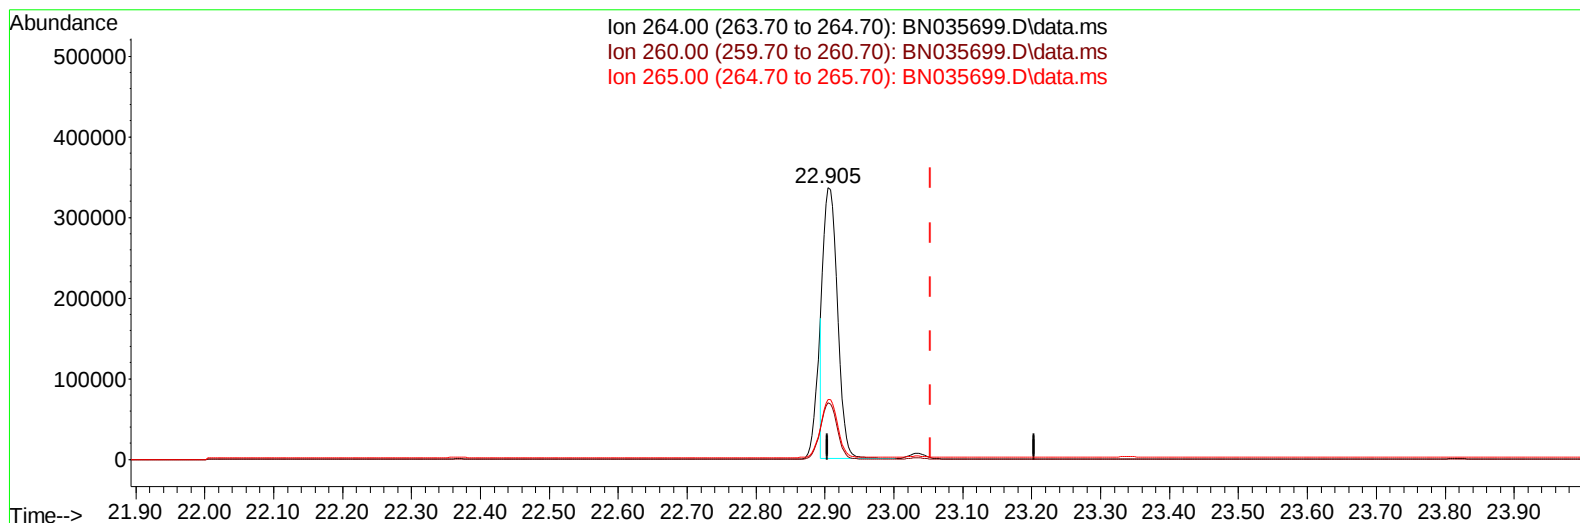

TIC: BN035699.D\data.ms

(23) Perylene-d12 (I)

22.905min (-0.149) 0.40 ng/u1

response 488008

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.40	20.90#
265.00	62.10	22.06#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121824\
Data File : BN035699.D
Acq On : 19 Dec 2024 10:54
Operator : RC/JU
Sample : P5258-04
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E28X0

Manual IntegrationsAPPROVED

Quant Time: Dec 19 11:41:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 16 16:26:08 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/21/2024
Supervised By :mohammad ahmed 12/24/2024

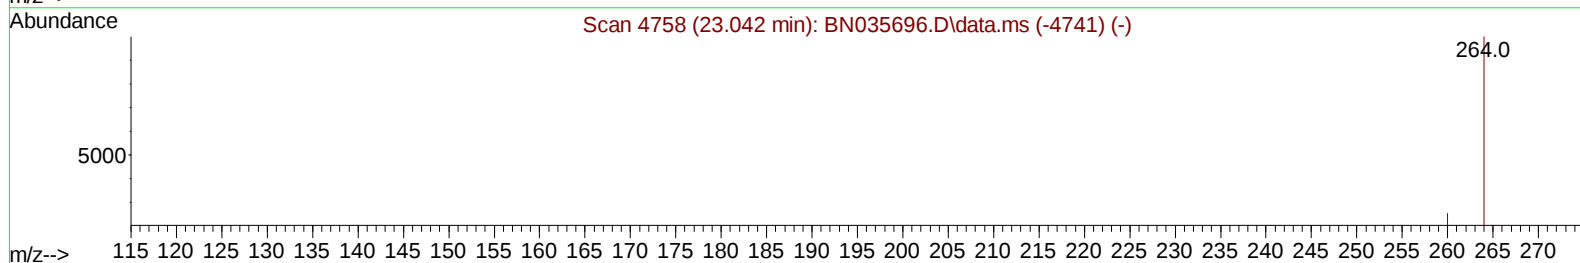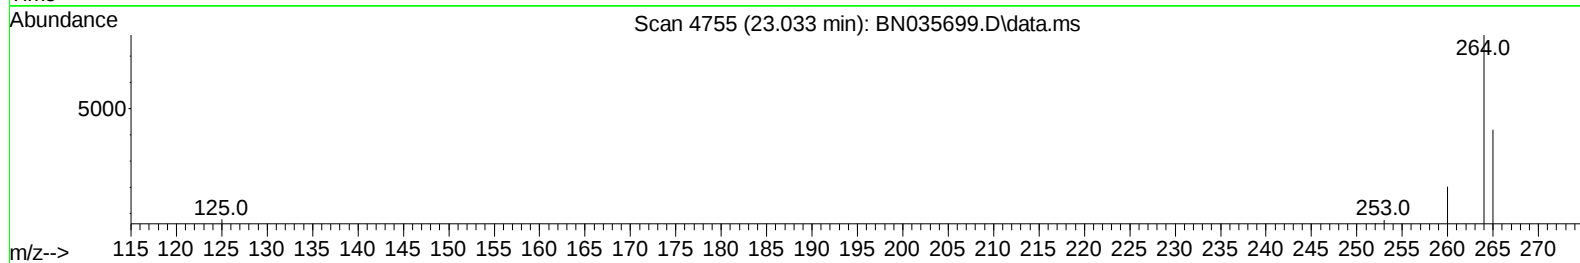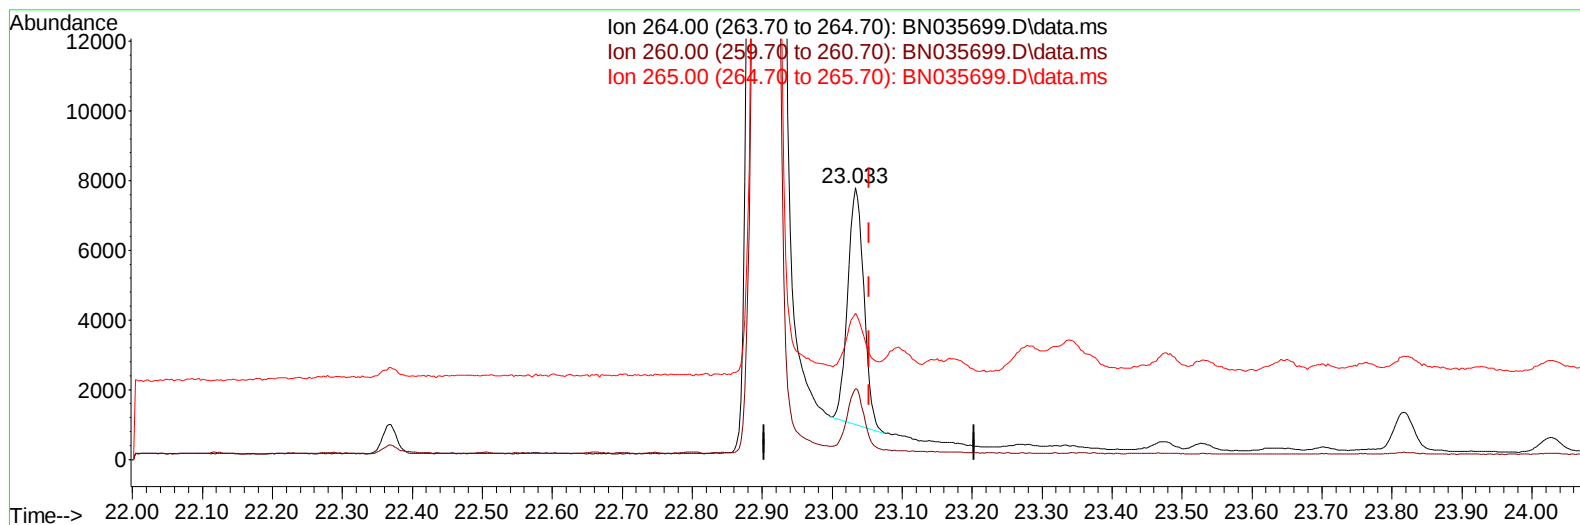

TIC: BN035699.D\data.ms

(23) Perylene-d12 (I)

23.033min (-0.020) 0.40 ng/ul m

response 10892

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.40	26.06
265.00	62.10	53.93
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121824\
Data File : BN035699.D
Acq On : 19 Dec 2024 10:54
Operator : RC/JU
Sample : P5258-04
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E28X0

Manual IntegrationsAPPROVED

Quant Time: Dec 19 11:41:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 16 16:26:08 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/21/2024
Supervised By :mohammad ahmed 12/24/2024

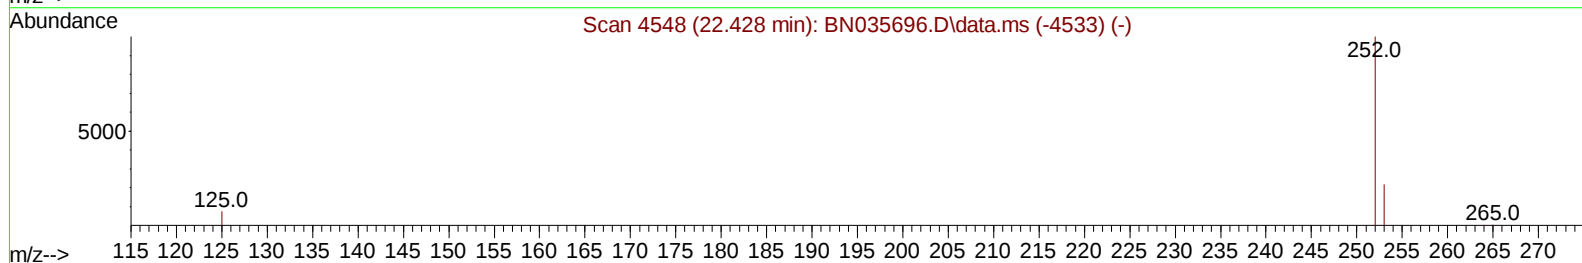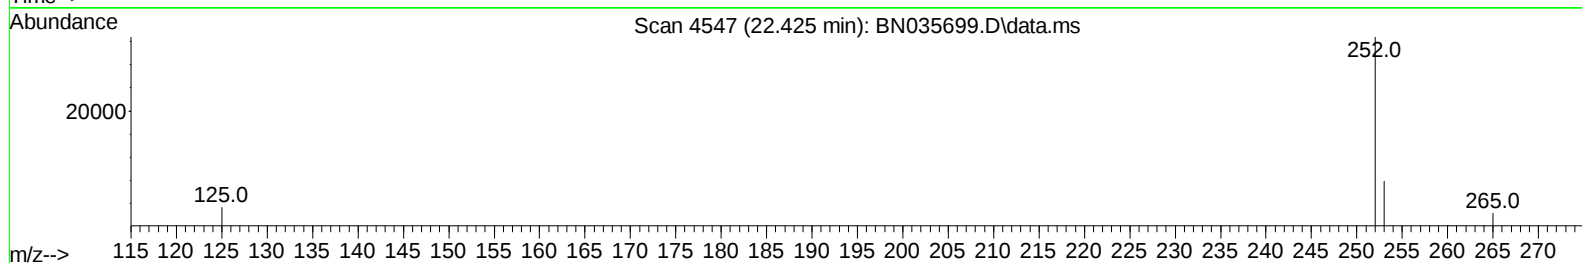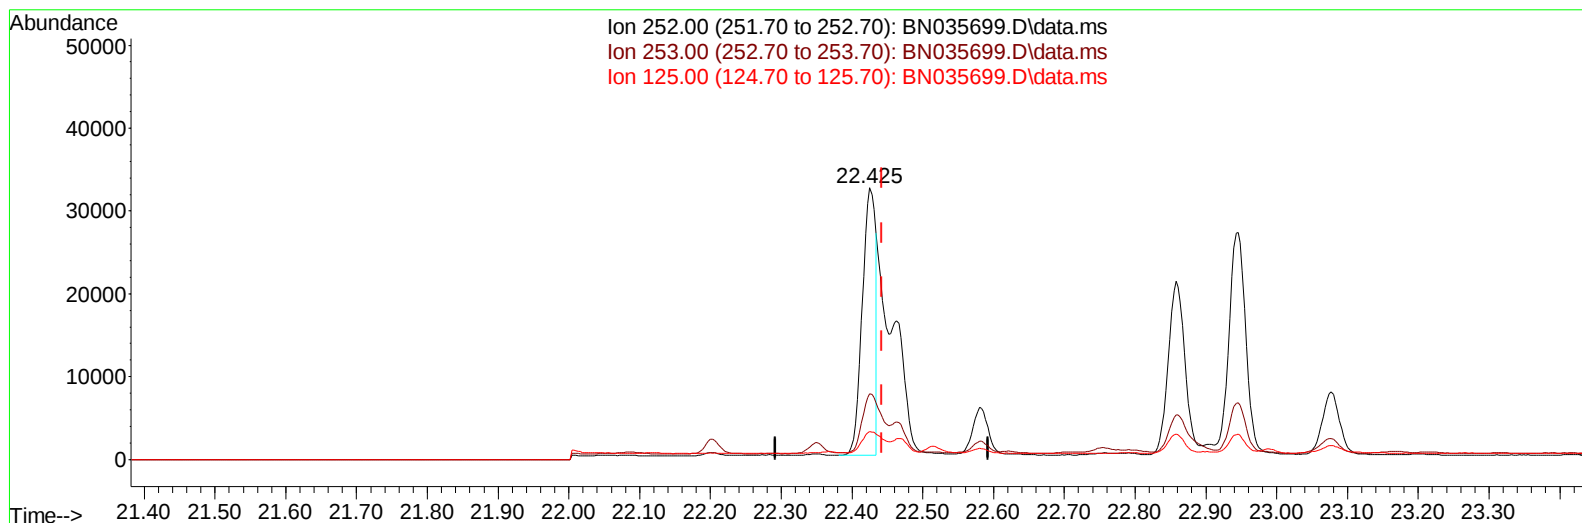

TIC: BN035699.D\data.ms

(24) Benzo(b)fluoranthene

22.425min (-0.017) 1.32 ng/u1

response 42220

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	28.20	24.26
125.00	18.80	10.35
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121824\
Data File : BN035699.D
Acq On : 19 Dec 2024 10:54
Operator : RC/JU
Sample : P5258-04
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E28X0

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/21/2024
Supervised By :mohammad ahmed 12/24/2024

Quant Time: Dec 19 11:41:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 16 16:26:08 2024
Response via : Initial Calibration

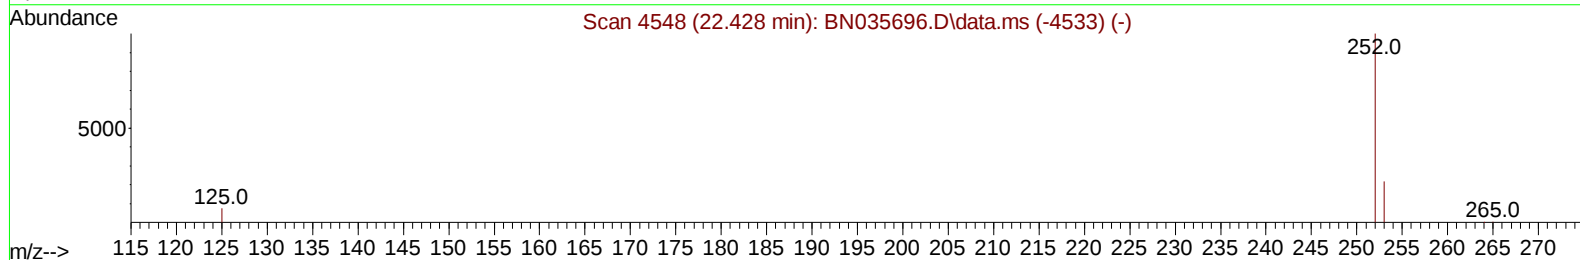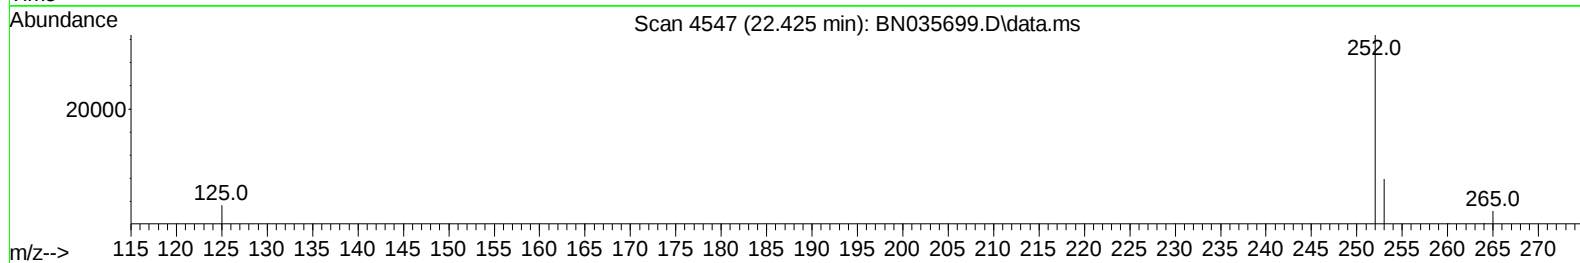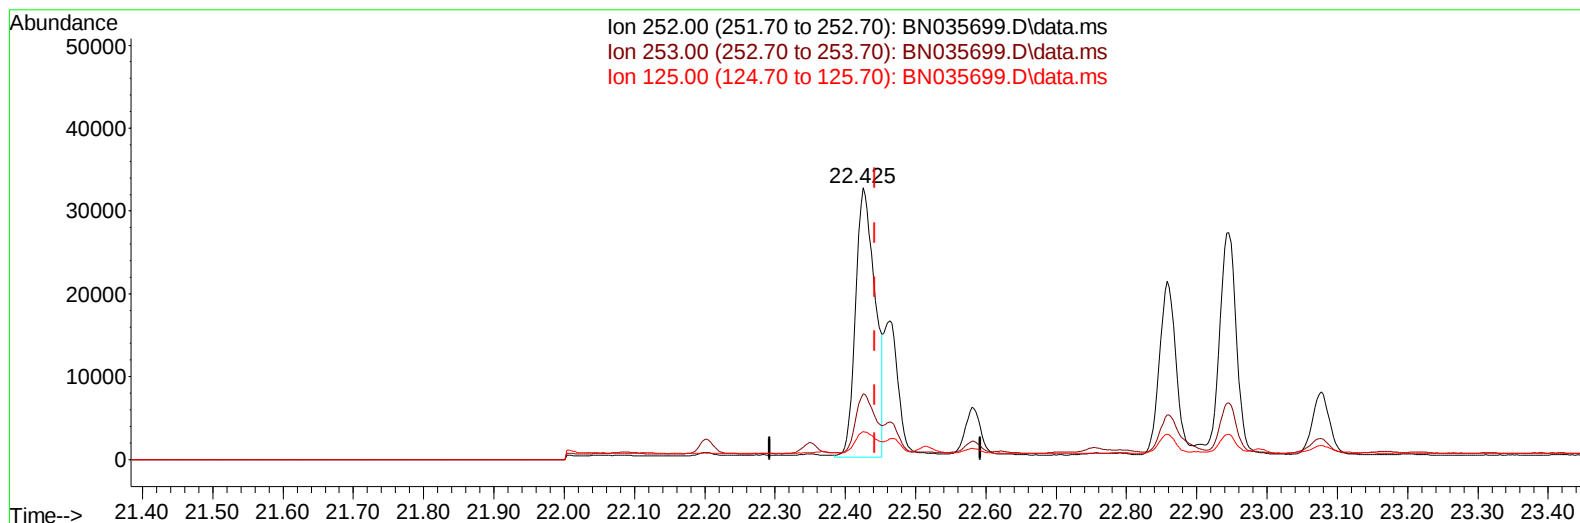

TIC: BN035699.D\data.ms

(24) Benzo(b)fluoranthene

22.425min (-0.017) 1.95 ng/u1 m

response 62667

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	28.20	24.26
125.00	18.80	10.35
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121824\
Data File : BN035699.D
Acq On : 19 Dec 2024 10:54
Operator : RC/JU
Sample : P5258-04
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E28X0

Manual IntegrationsAPPROVED

Quant Time: Dec 19 11:41:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 16 16:26:08 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/21/2024
Supervised By :mohammad ahmed 12/24/2024

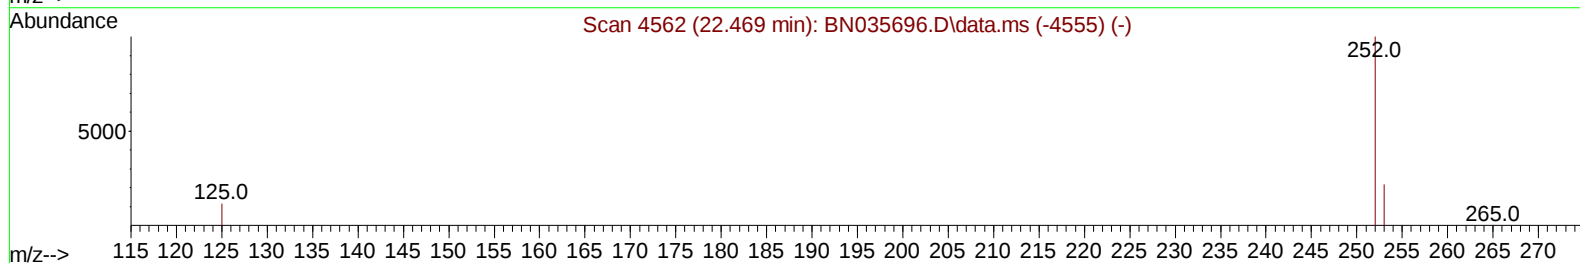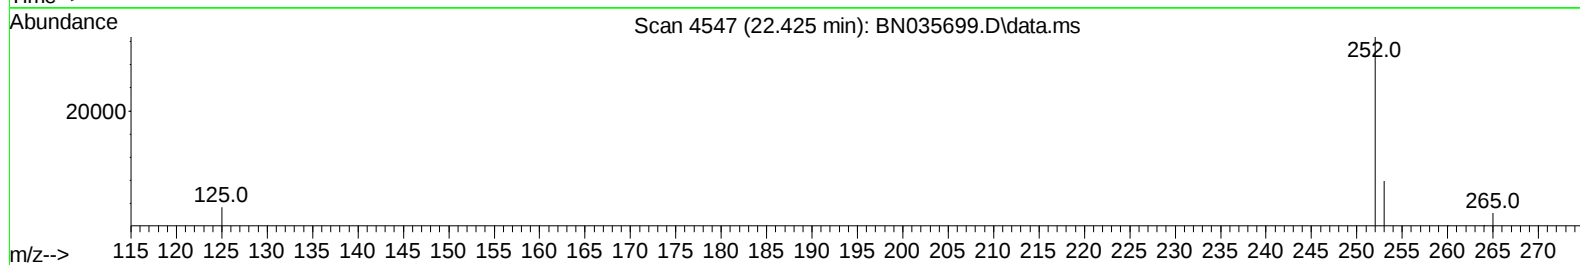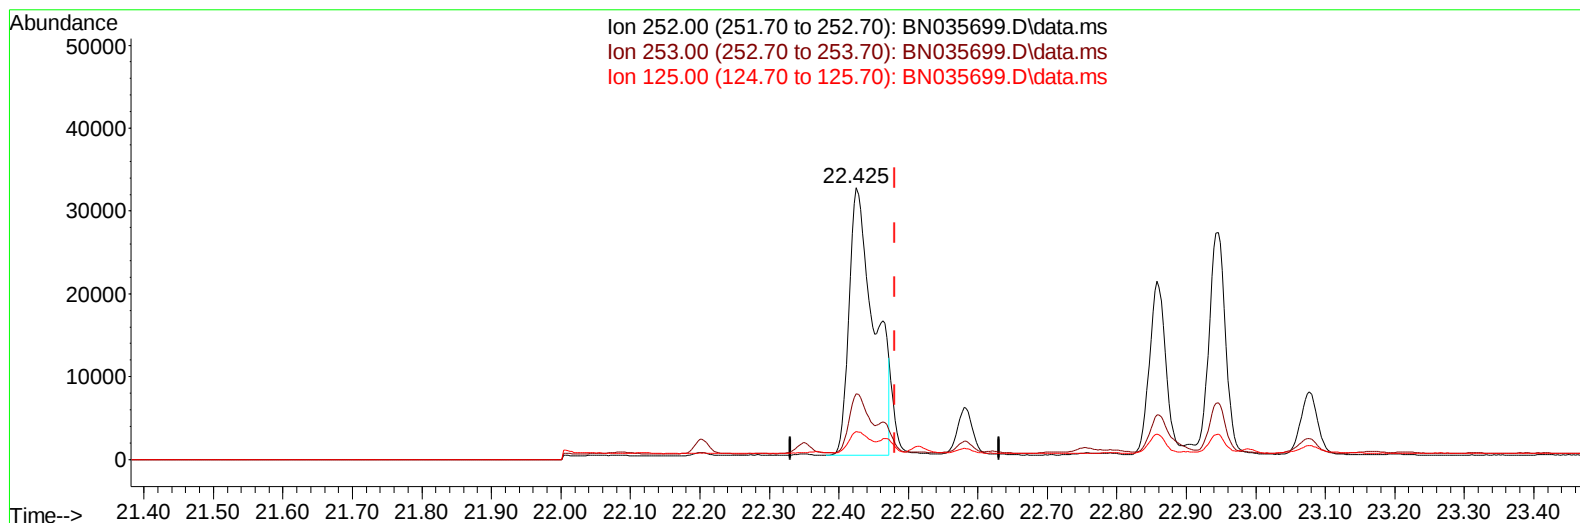

TIC: BN035699.D\data.ms

(25) Benzo(k)fluoranthene

22.425min (-0.055) 2.26 ng/u1

response 80212

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	27.60	24.26
125.00	19.10	10.35#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121824\
Data File : BN035699.D
Acq On : 19 Dec 2024 10:54
Operator : RC/JU
Sample : P5258-04
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E28X0

Manual IntegrationsAPPROVED

Quant Time: Dec 19 11:41:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 16 16:26:08 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/21/2024
Supervised By :mohammad ahmed 12/24/2024

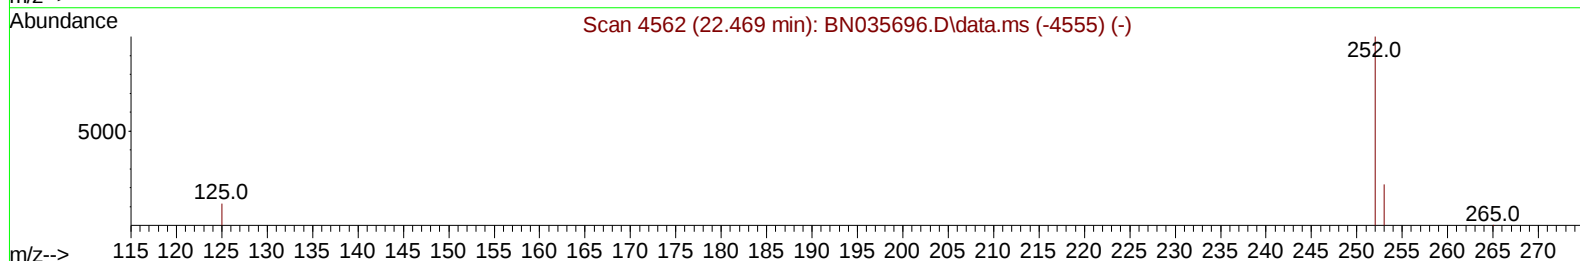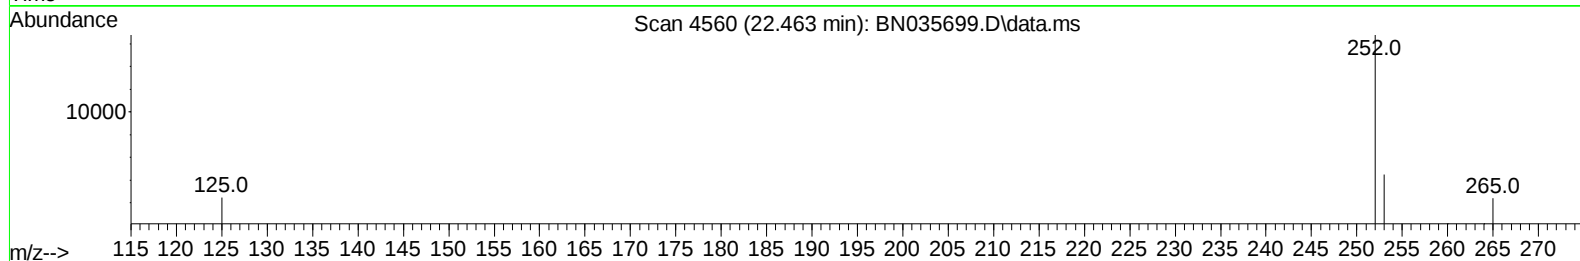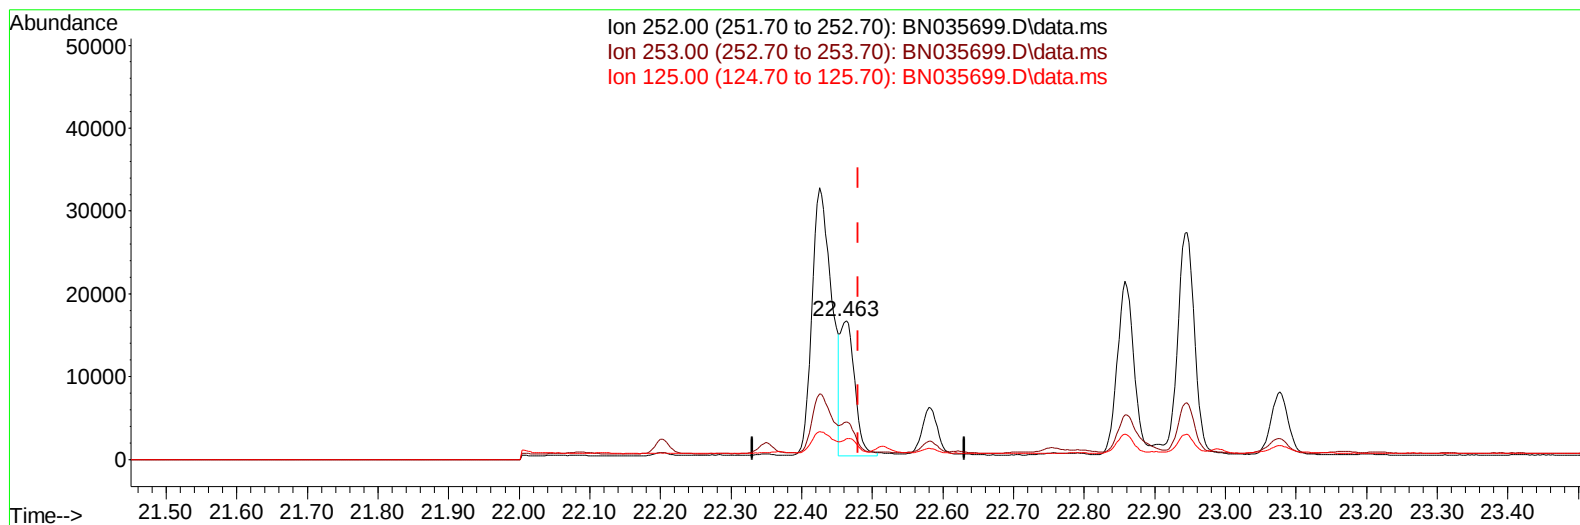

TIC: BN035699.D\data.ms

(25) Benzo(k)fluoranthene

22.463min (-0.017) 0.66 ng/u1 m

response 23447

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	27.60	26.93
125.00	19.10	14.89#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121824\
Data File : BN035699.D
Acq On : 19 Dec 2024 10:54
Operator : RC/JU
Sample : P5258-04
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E28X0

Manual IntegrationsAPPROVED

Quant Time: Dec 19 11:41:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 16 16:26:08 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/21/2024
Supervised By :mohammad ahmed 12/24/2024

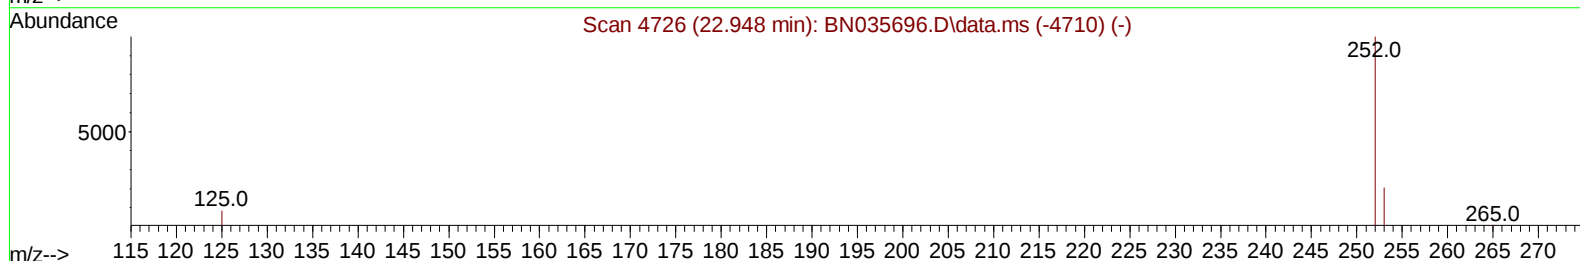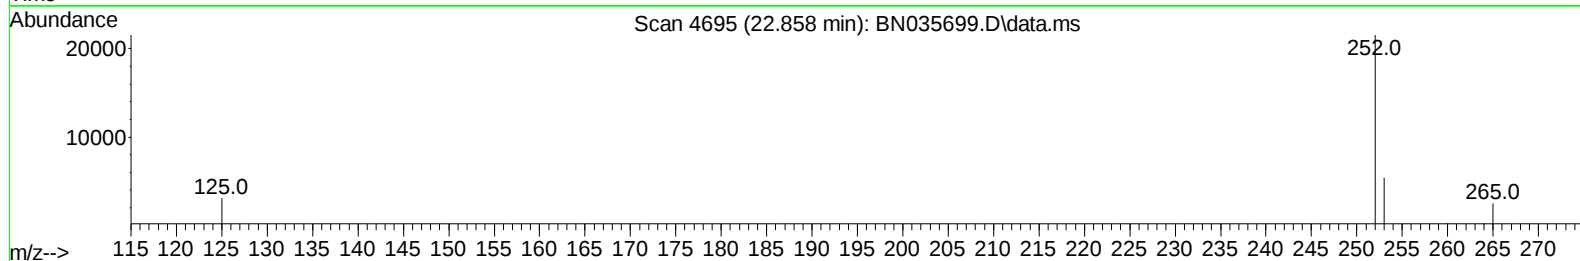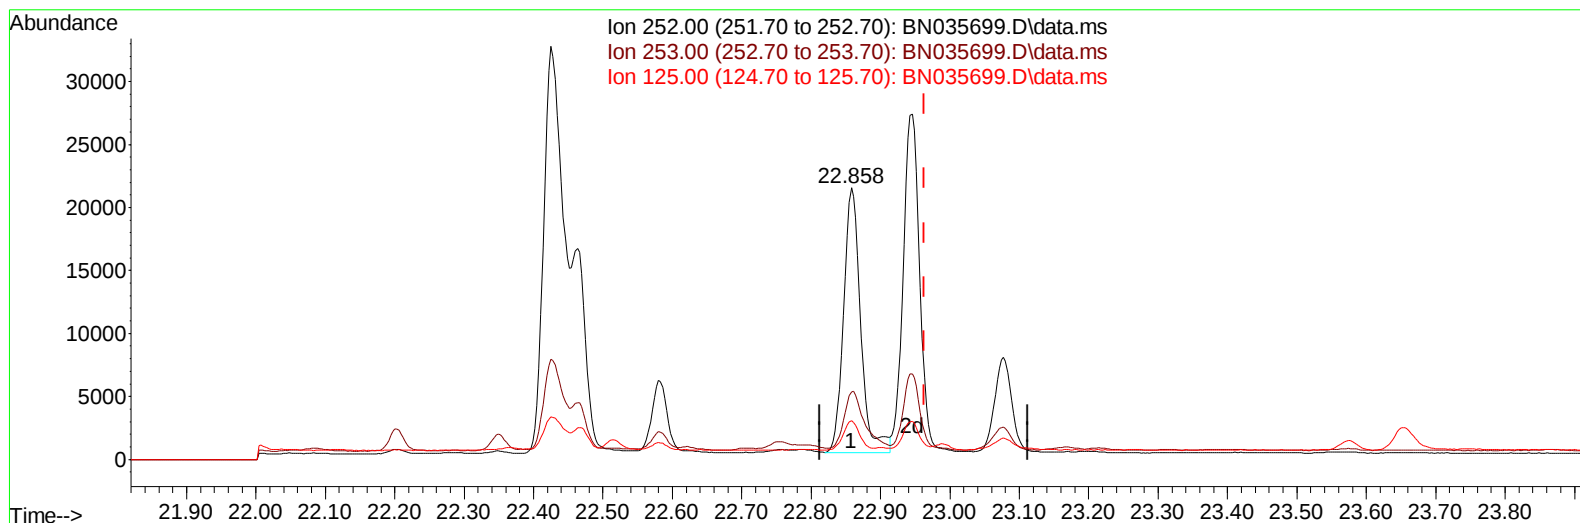

TIC: BN035699.D\data.ms

(26) Benzo(a)pyrene (C)

22.858min (-0.105) 1.16 ng/u1

response 35932

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	30.10	25.01
125.00	23.90	14.22#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121824\
Data File : BN035699.D
Acq On : 19 Dec 2024 10:54
Operator : RC/JU
Sample : P5258-04
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E28X0

Manual IntegrationsAPPROVED

Quant Time: Dec 19 11:41:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 16 16:26:08 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/21/2024
Supervised By :mohammad ahmed 12/24/2024

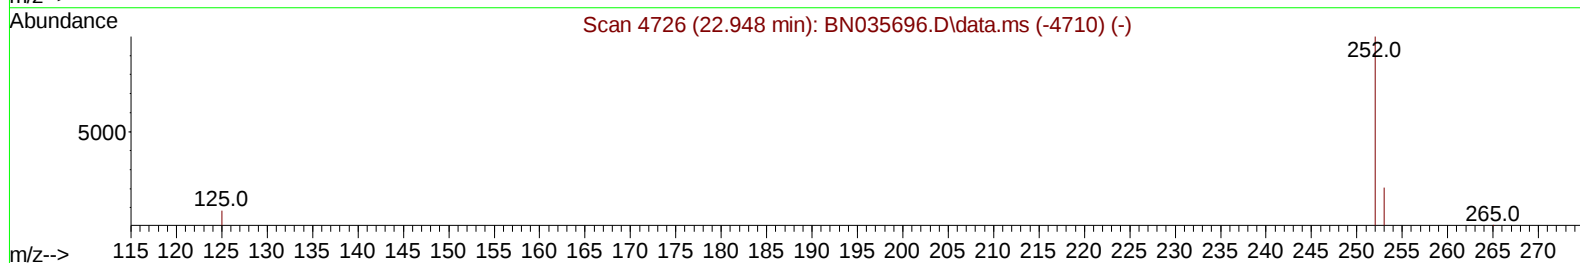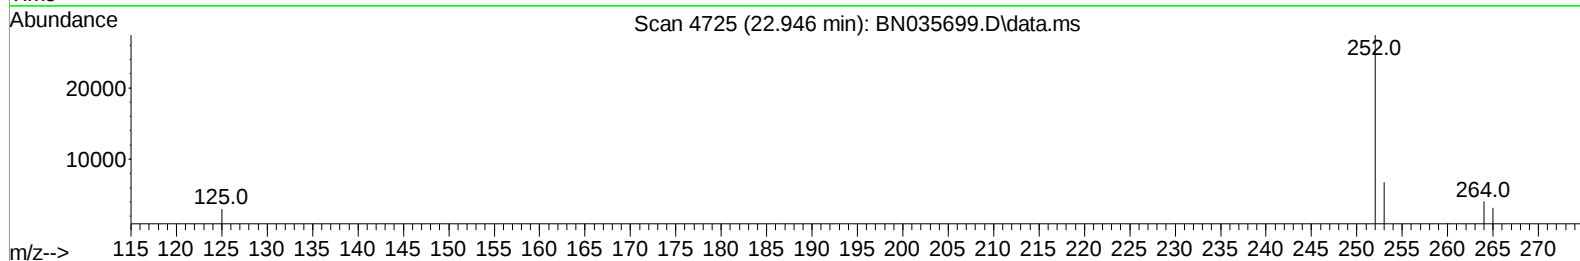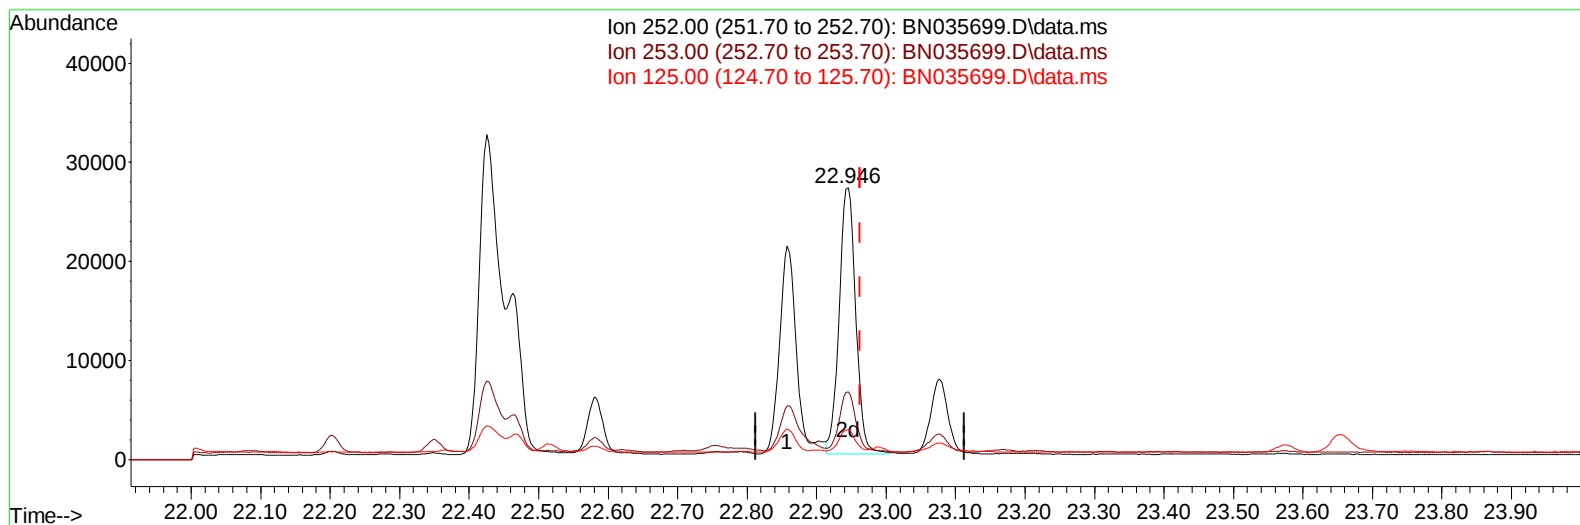

TIC: BN035699.D\data.ms

(26) Benzo(a)pyrene (C)

22.946min (-0.017) 1.42 ng/u1 m

response 44291

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	30.10	24.84
125.00	23.90	11.06#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121824\
Data File : BN035699.D
Acq On : 19 Dec 2024 10:54
Operator : RC/JU
Sample : P5258-04
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E28X0

Manual IntegrationsAPPROVED

Quant Time: Dec 19 11:41:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 16 16:26:08 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/21/2024
Supervised By :mohammad ahmed 12/24/2024

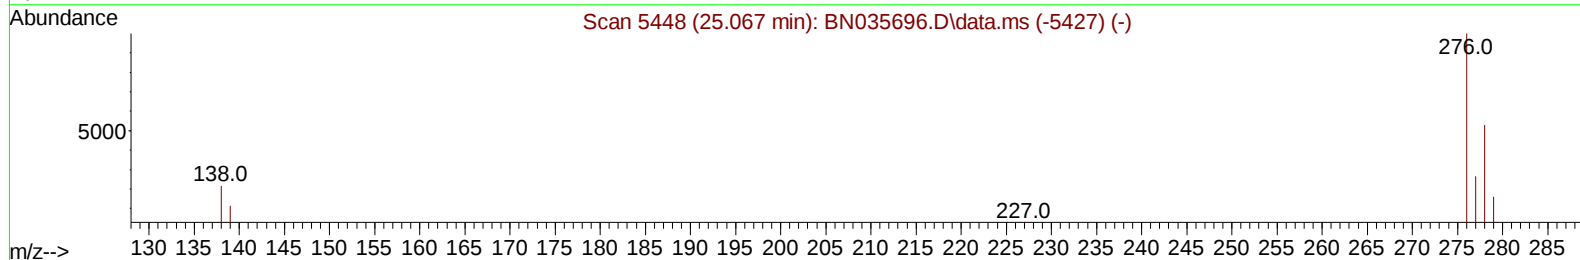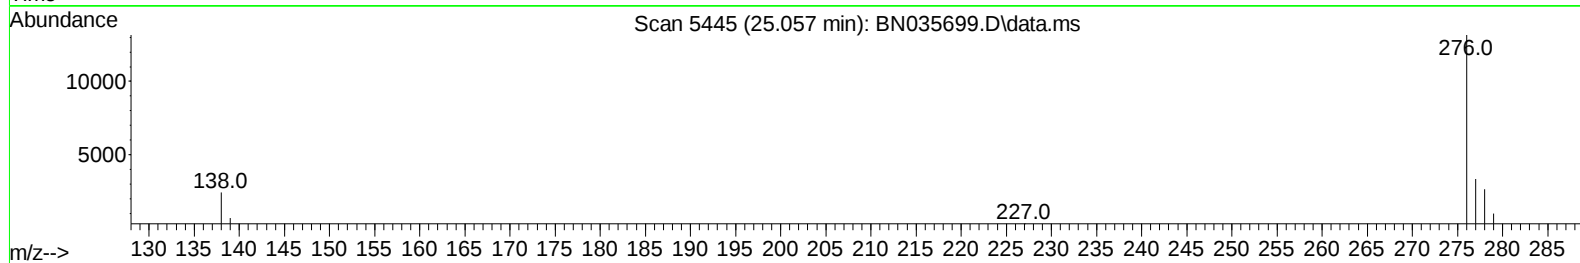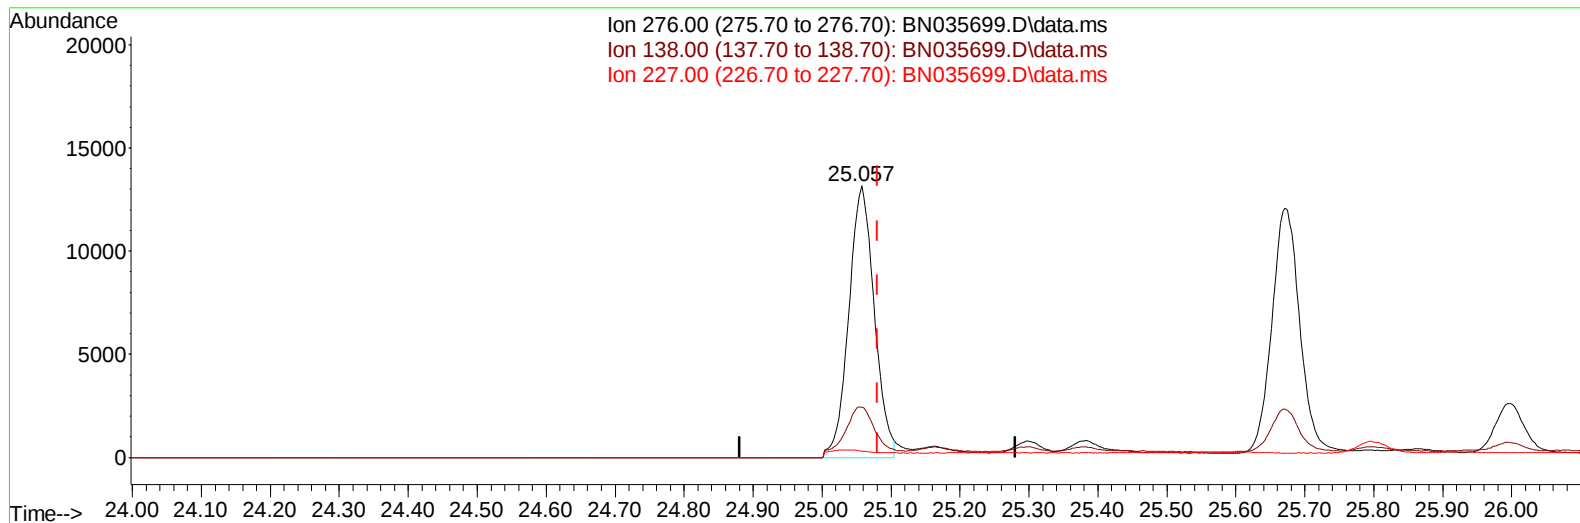

TIC: BN035699.D\data.ms

(27) Indeno(1,2,3-cd)pyrene

25.057min (-0.023) 0.89 ng/u1

response 33495

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	18.40	22.46#
227.00	27.00	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121824\
Data File : BN035699.D
Acq On : 19 Dec 2024 10:54
Operator : RC/JU
Sample : P5258-04
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E28X0

Manual IntegrationsAPPROVED

Quant Time: Dec 19 11:41:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 16 16:26:08 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/21/2024
Supervised By :mohammad ahmed 12/24/2024

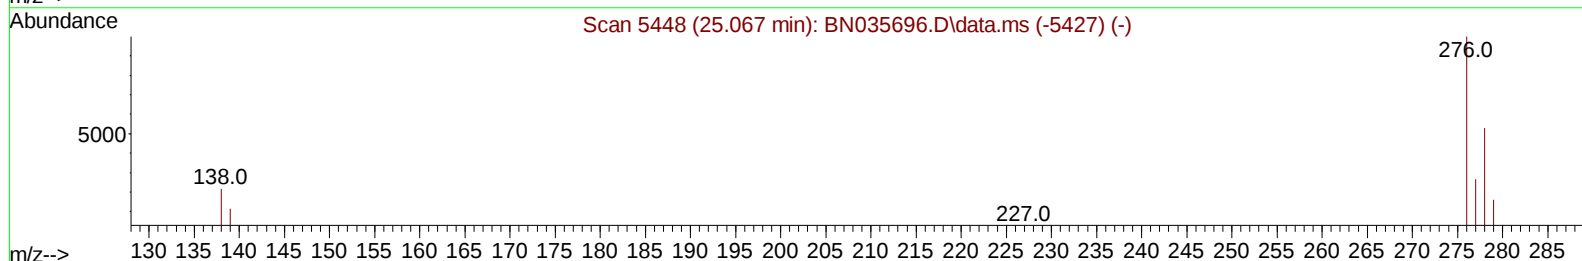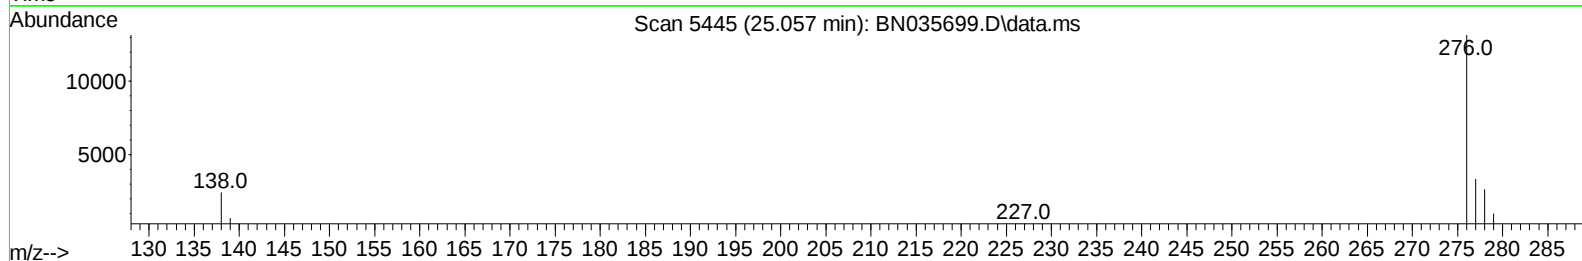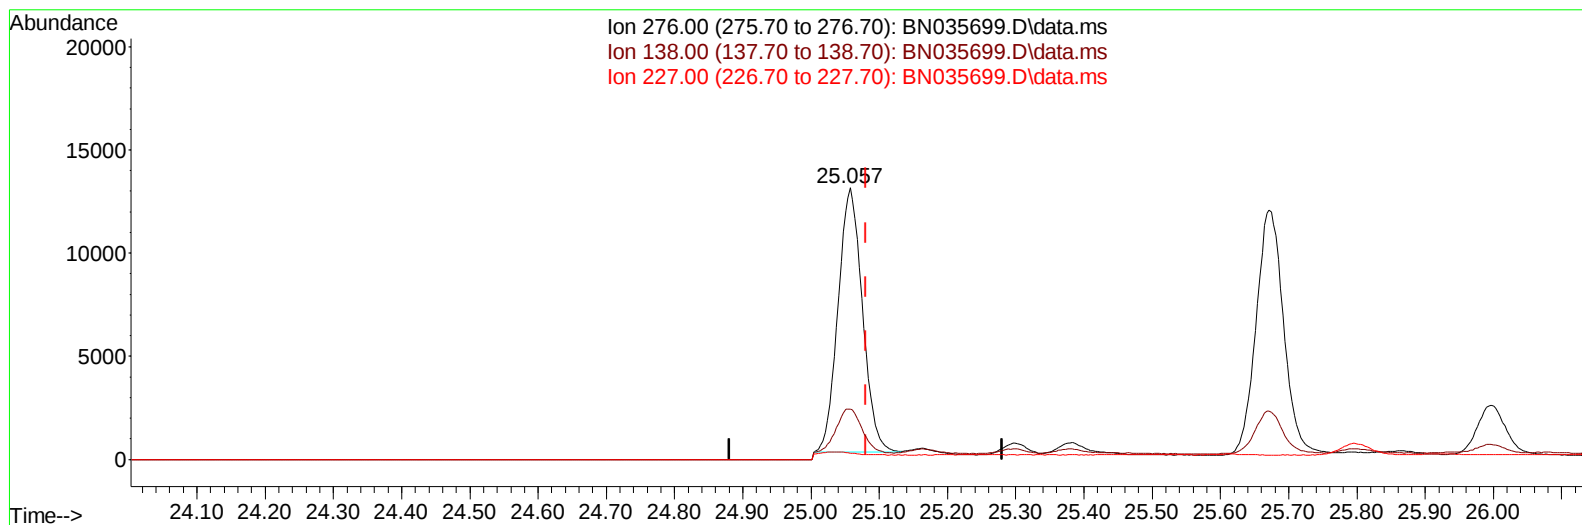

TIC: BN035699.D\data.ms

(27) Indeno(1,2,3-cd)pyrene

25.057min (-0.023) 0.84 ng/u1 m

response 31795

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	18.40	23.66#
227.00	27.00	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121824\
Data File : BN035699.D
Acq On : 19 Dec 2024 10:54
Operator : RC/JU
Sample : P5258-04
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E28X0

Manual IntegrationsAPPROVED

Quant Time: Dec 19 11:41:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 16 16:26:08 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/21/2024
Supervised By :mohammad ahmed 12/24/2024

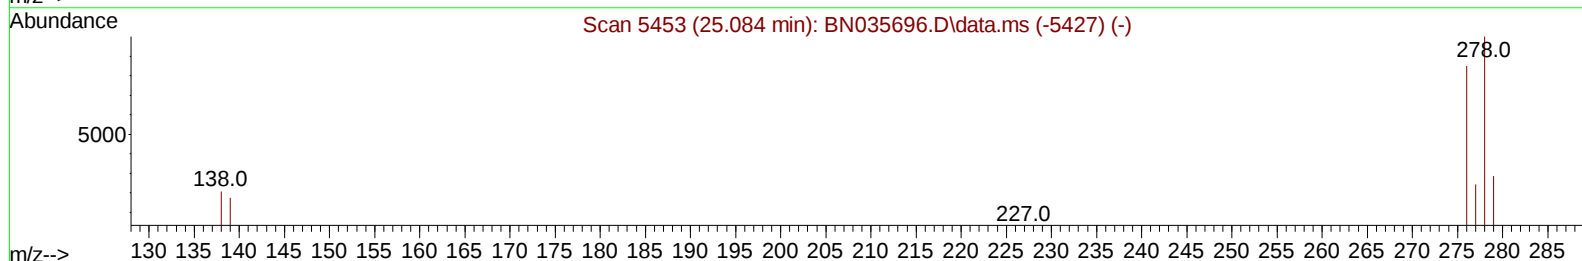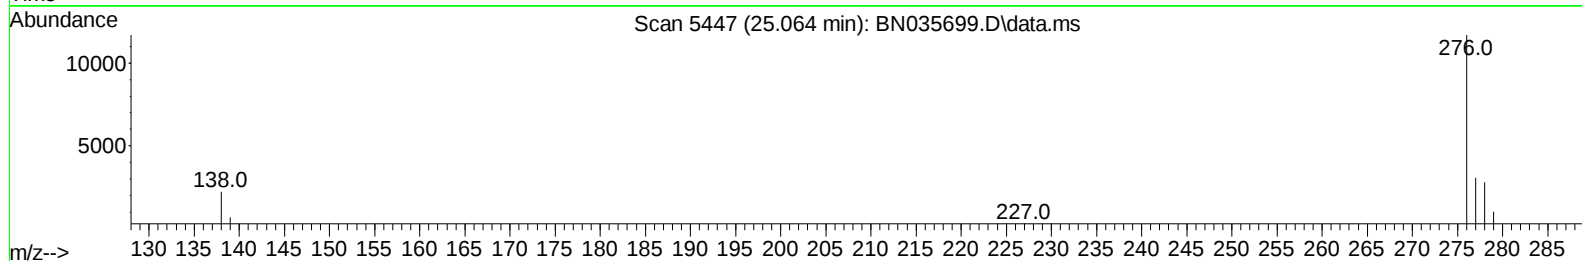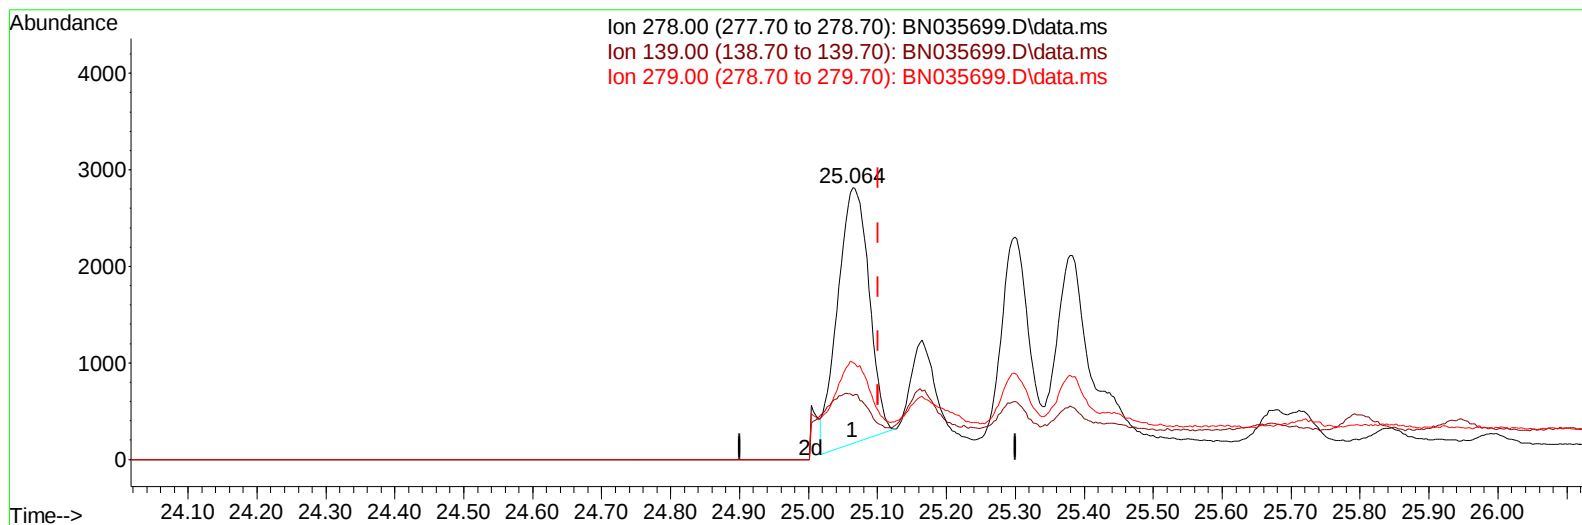

TIC: BN035699.D\data.ms

(28) Dibenzo(a,h)anthracene

25.064min (-0.037) 0.29 ng/u1

response 8396

Ion	Exp%	Act%
278.00	100.00	100.00
139.00	24.80	23.39
279.00	30.00	35.66
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121824\
Data File : BN035699.D
Acq On : 19 Dec 2024 10:54
Operator : RC/JU
Sample : P5258-04
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E28X0

Manual IntegrationsAPPROVED

Quant Time: Dec 19 11:41:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 16 16:26:08 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/21/2024
Supervised By :mohammad ahmed 12/24/2024

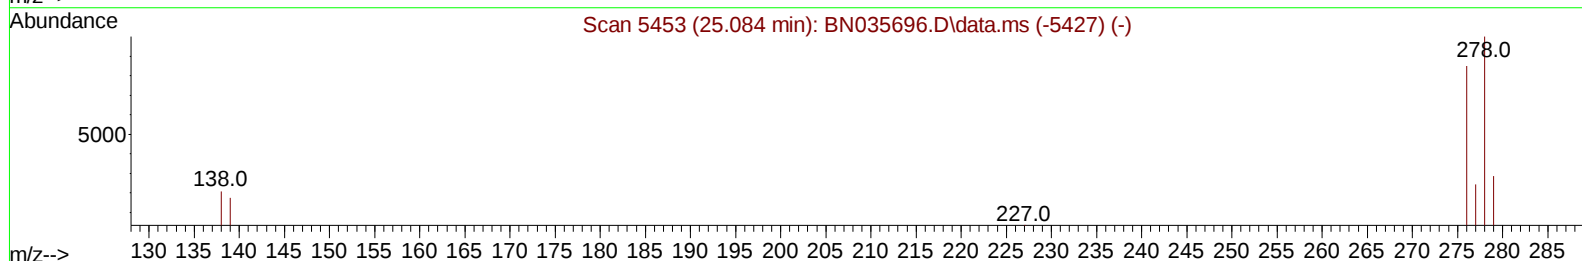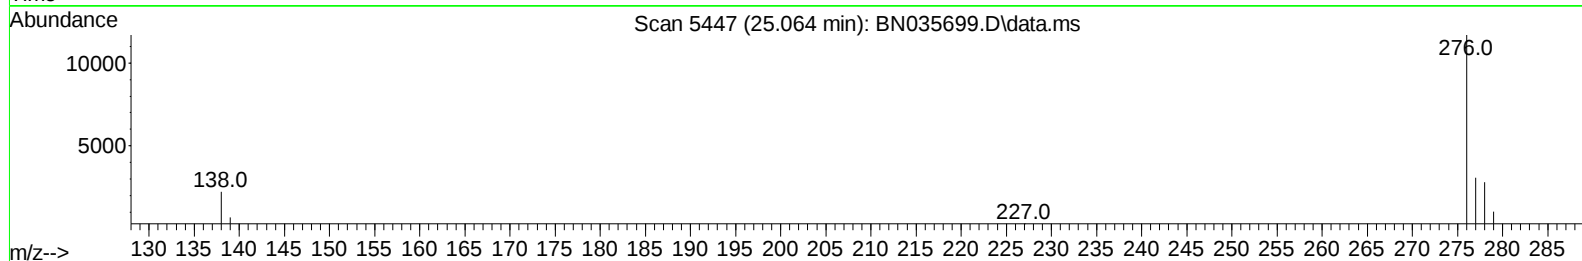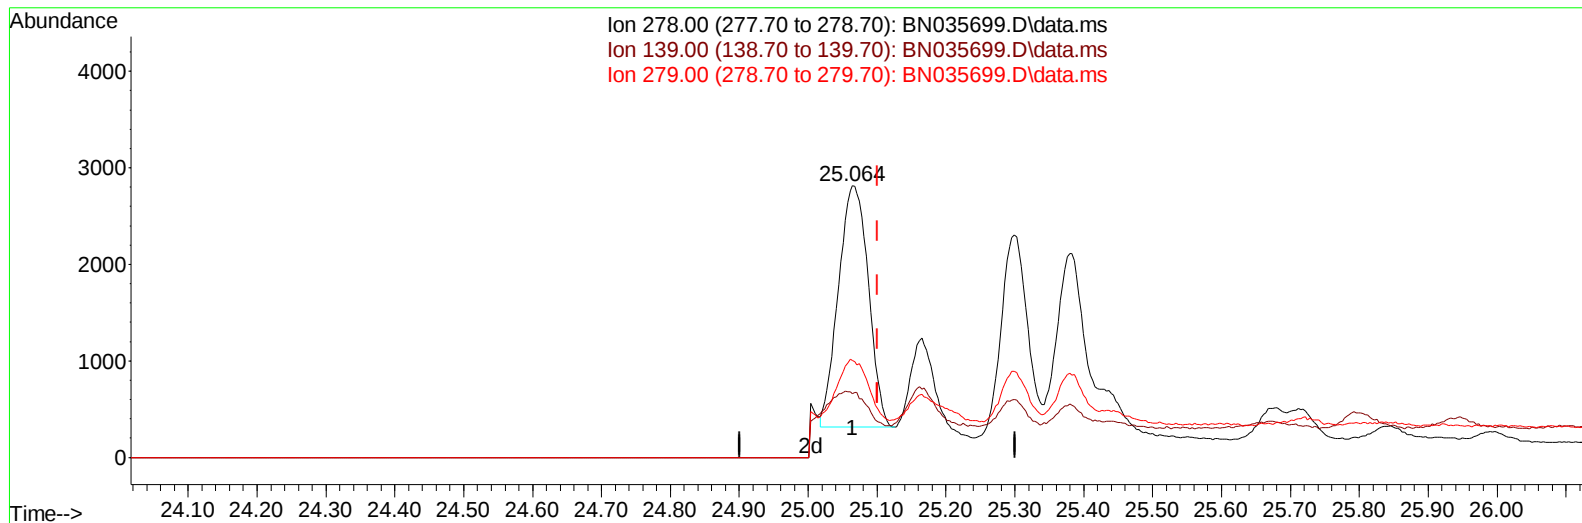

TIC: BN035699.D\data.ms

(28) Dibenzo(a,h)anthracene

25.064min (-0.037) 0.26 ng/ul m

response 7553

Ion	Exp%	Act%
278.00	100.00	100.00
139.00	24.80	23.39
279.00	30.00	35.66
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121824\
Data File : BN035699.D
Acq On : 19 Dec 2024 10:54
Operator : RC/JU
Sample : P5258-04
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E28X0

Manual IntegrationsAPPROVED

Quant Time: Dec 19 11:41:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 16 16:26:08 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/21/2024
Supervised By :mohammad ahmed 12/24/2024

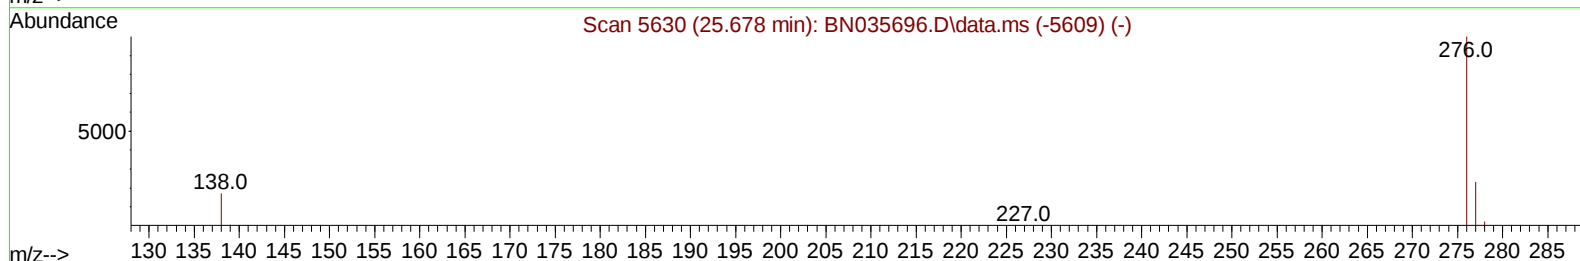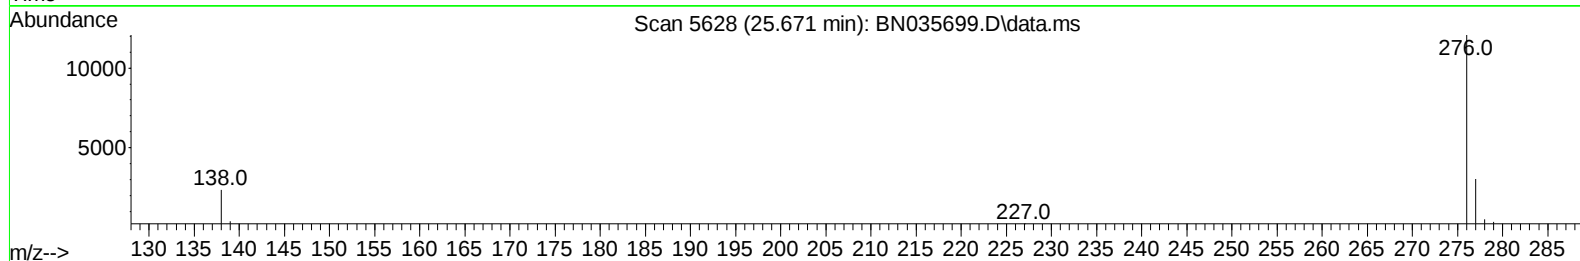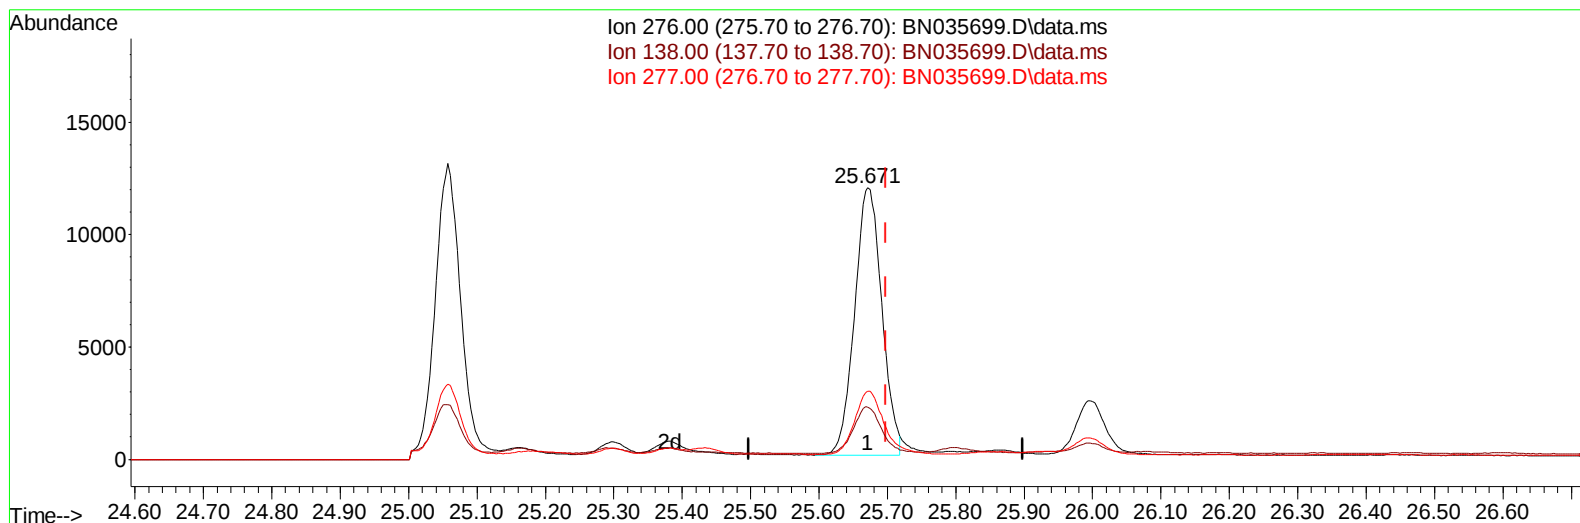

TIC: BN035699.D\data.ms

(29) Benzo(g,h,i)perylene

25.671min (-0.027) 1.08 ng/u1

response 32818

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	24.50	19.32#
277.00	27.00	25.14
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121824\
Data File : BN035699.D
Acq On : 19 Dec 2024 10:54
Operator : RC/JU
Sample : P5258-04
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E28X0

Manual IntegrationsAPPROVED

Quant Time: Dec 19 11:41:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 16 16:26:08 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/21/2024
Supervised By :mohammad ahmed 12/24/2024

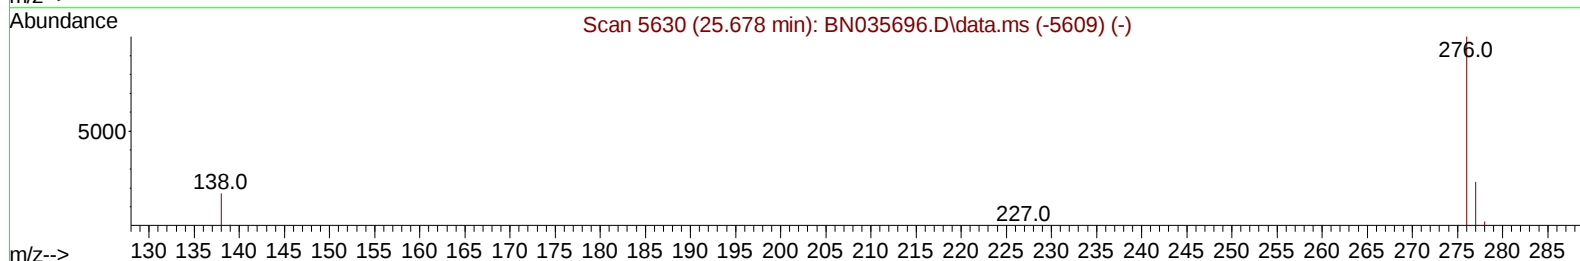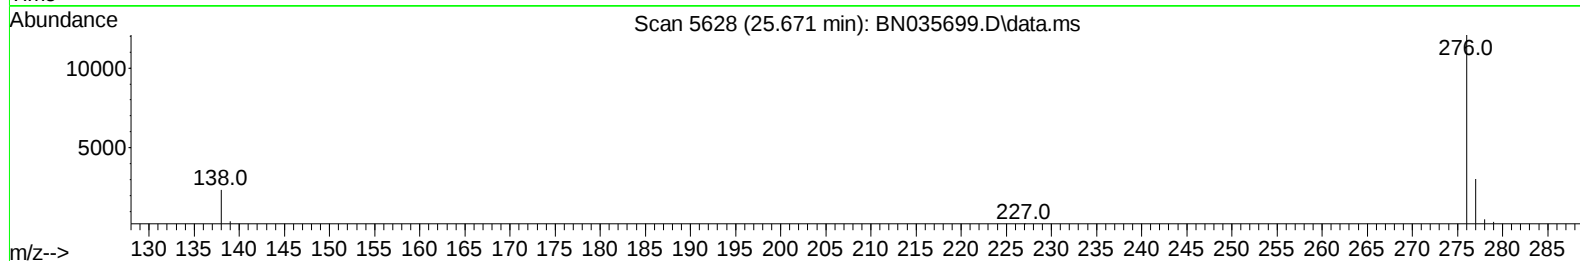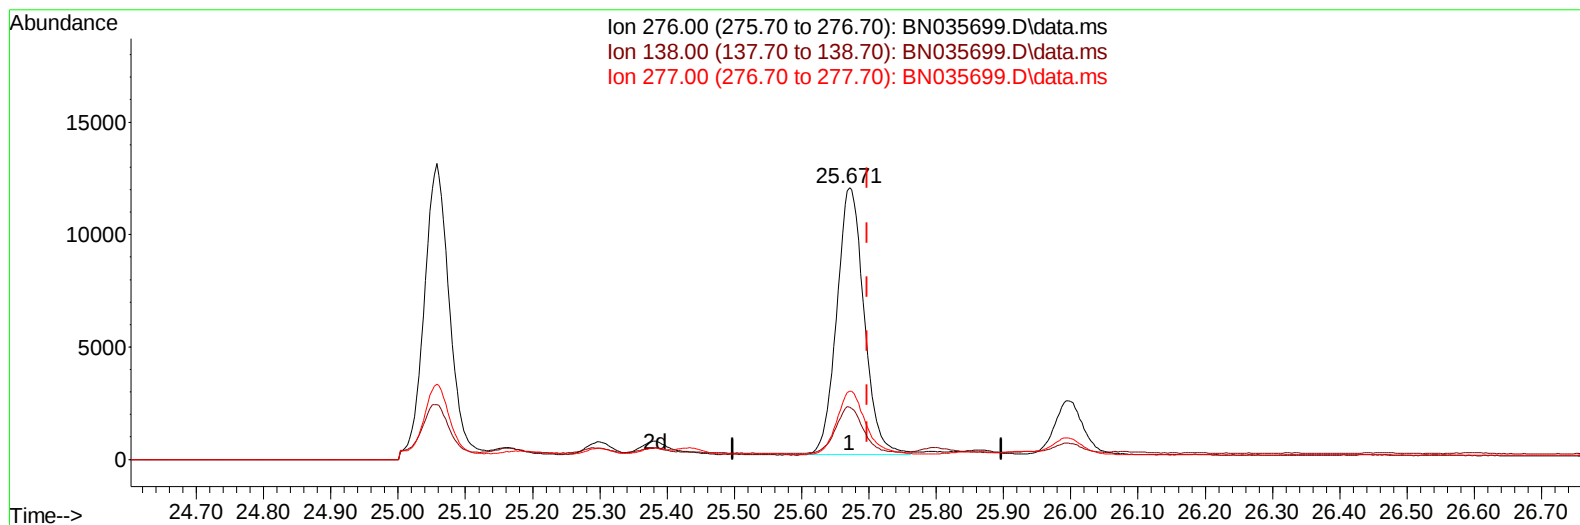

TIC: BN035699.D\data.ms

(29) Benzo(g,h,i)perylene

25.671min (-0.027) 1.10 ng/ul m

response 33537

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	24.50	19.32#
277.00	27.00	25.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121824\
 Data File : BN035699.D
 Acq On : 19 Dec 2024 10:54
 Operator : RC/JU
 Sample : P5258-04
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E28X0

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/21/2024
 Supervised By :mohammad ahmed 12/24/2024

Quant Time: Dec 19 11:41:58 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN121624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 16 16:26:08 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.276	152	3323	0.400	ng/ul	0.00
4) Naphthalene-d8	10.020	136	8540	0.400	ng/ul	-0.01
9) Acenaphthene-d10	13.935	164	6318	0.400	ng/ul	-0.01
13) Phenanthrene-d10	16.705	188	13319m	0.400	ng/ul	-0.01
17) Chrysene-d12	20.950	240	11413	0.400	ng/ul	-0.01
23) Perylene-d12	23.033	264	10892m	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.951	96	15104	5.127	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.620	152	3914	0.322	ng/ul	-0.02
18) Fluoranthene-d10	18.758	212	7953	0.238	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.064	128	2127m	0.102	ng/ul	
7) 2-Methylnaphthalene	11.697	142	1278	0.091	ng/ul	100
8) 1-Methylnaphthalene	11.923	142	1121	0.077	ng/ul	100
10) Acenaphthylene	13.648	152	2553	0.104	ng/ul#	92
11) Acenaphthene	14.000	153	2413	0.130	ng/ul	99
12) Fluorene	15.004	166	2582	0.120	ng/ul#	97
15) Phenanthrene	16.747	178	48616	1.458	ng/ul	98
16) Anthracene	16.840	178	11721	0.376	ng/ul	99
19) Fluoranthene	18.791	202	96680	2.369	ng/ul	98
20) Pyrene	19.158	202	85119	1.893	ng/ul	99
21) Benzo(a)anthracene	20.935	228	44531	1.176	ng/ul	99
22) Chrysene	20.988	228	47699	1.214	ng/ul	97
24) Benzo(b)fluoranthene	22.425	252	62667m	1.952	ng/ul	
25) Benzo(k)fluoranthene	22.463	252	23447m	0.660	ng/ul	
26) Benzo(a)pyrene	22.946	252	44291m	1.425	ng/ul	
27) Indeno(1,2,3-cd)pyrene	25.057	276	31795m	0.840	ng/ul	
28) Dibenzo(a,h)anthracene	25.064	278	7553m	0.261	ng/ul	
29) Benzo(g,h,i)perylene	25.671	276	33537m	1.104	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121824\
Data File : BN035699.D
Acq On : 19 Dec 2024 10:54
Operator : RC/JU
Sample : P5258-04
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E28X0

Manual IntegrationsAPPROVED

Quant Time: Dec 19 11:41:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 16 16:26:08 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/21/2024
Supervised By :mohammad ahmed 12/24/2024

