




Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN121824\  
Data File : BN035708.D  
Acq On : 19 Dec 2024 16:17  
Operator : RC/JU  
Sample : P5258-03DL 5X  
Misc :  
ALS Vial : 49 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
E28W9DL

Manual IntegrationsAPPROVED

Quant Time: Dec 19 16:53:27 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\SFAM-EPA-SIM-BN121624.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Dec 16 16:26:08 2024  
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/21/2024  
Supervised By :mohammad ahmed 12/24/2024

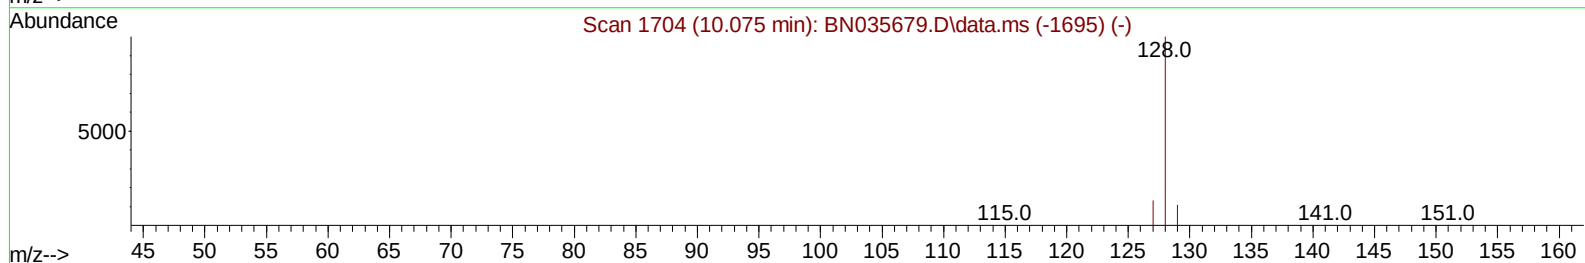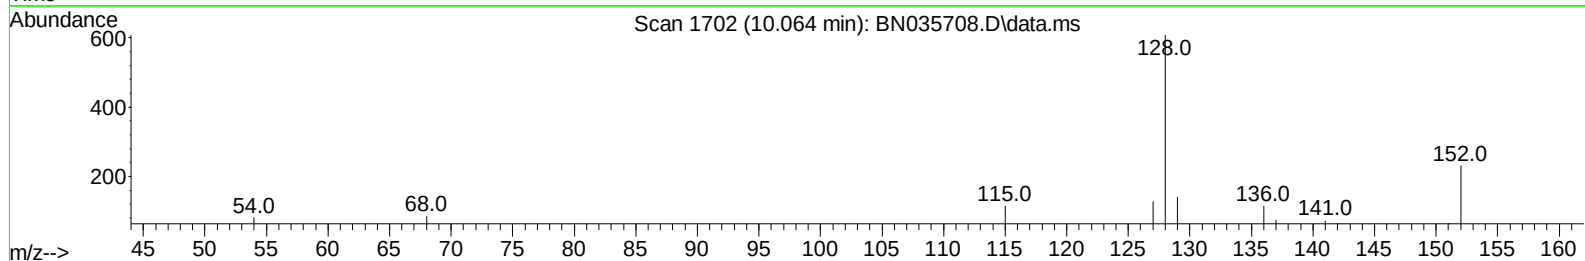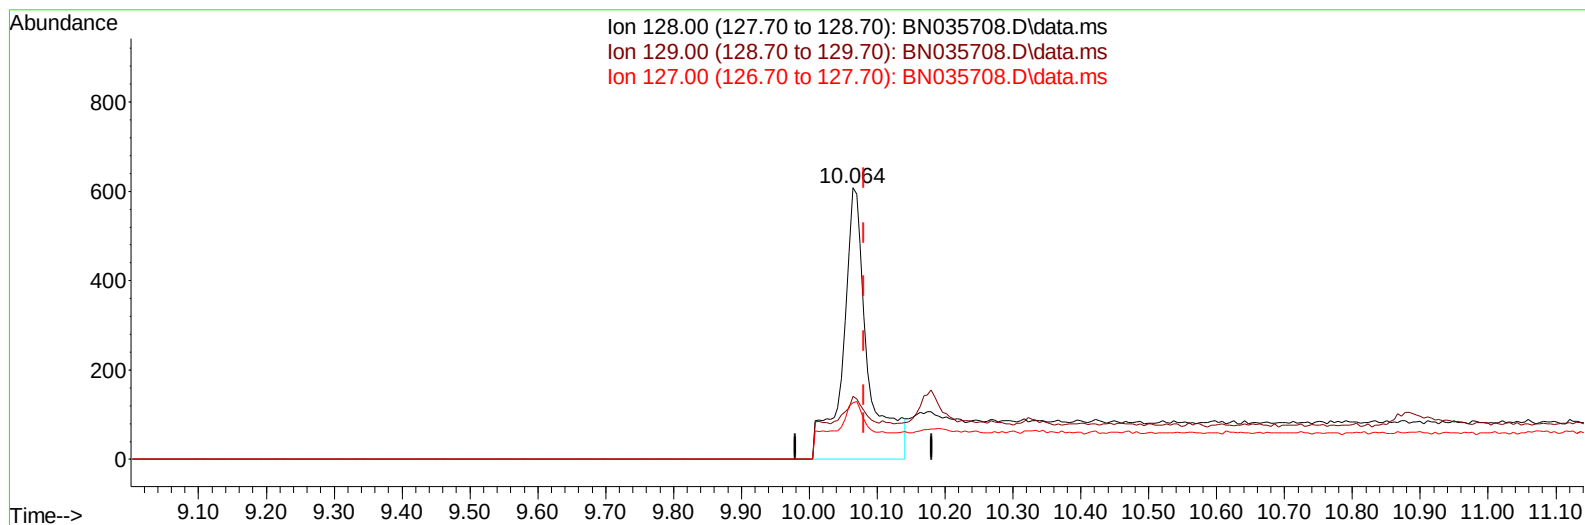

TIC: BN035708.D\data.ms

(5) Naphthalene

10.064min (-0.016) 0.07 ng/u1

response 1552

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 128.00 | 100.00 | 100.00 |
| 129.00 | 13.50  | 23.19# |
| 127.00 | 15.00  | 20.89# |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN121824\  
Data File : BN035708.D  
Acq On : 19 Dec 2024 16:17  
Operator : RC/JU  
Sample : P5258-03DL 5X  
Misc :  
ALS Vial : 49 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
E28W9DL

Manual IntegrationsAPPROVED

Quant Time: Dec 19 16:53:27 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\SFAM-EPA-SIM-BN121624.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Dec 16 16:26:08 2024  
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/21/2024  
Supervised By :mohammad ahmed 12/24/2024

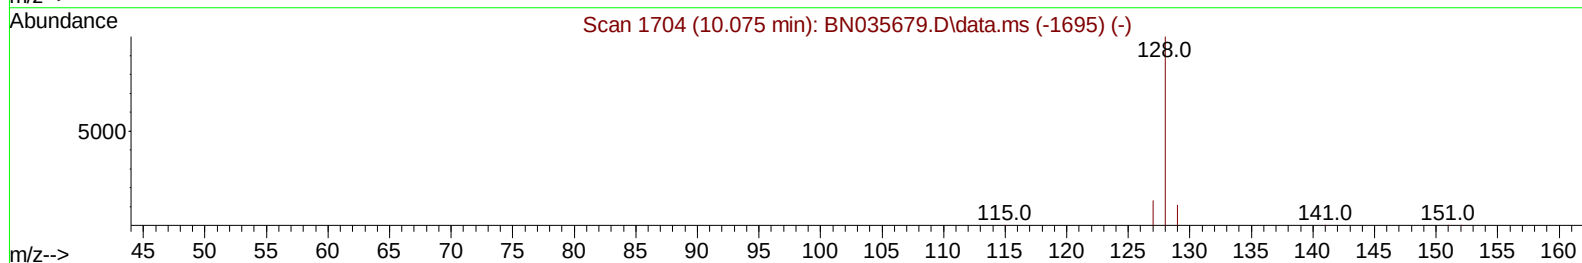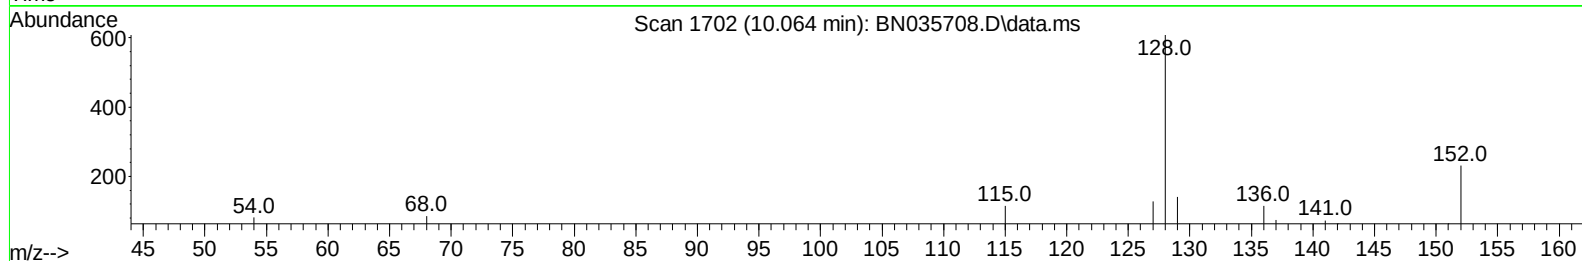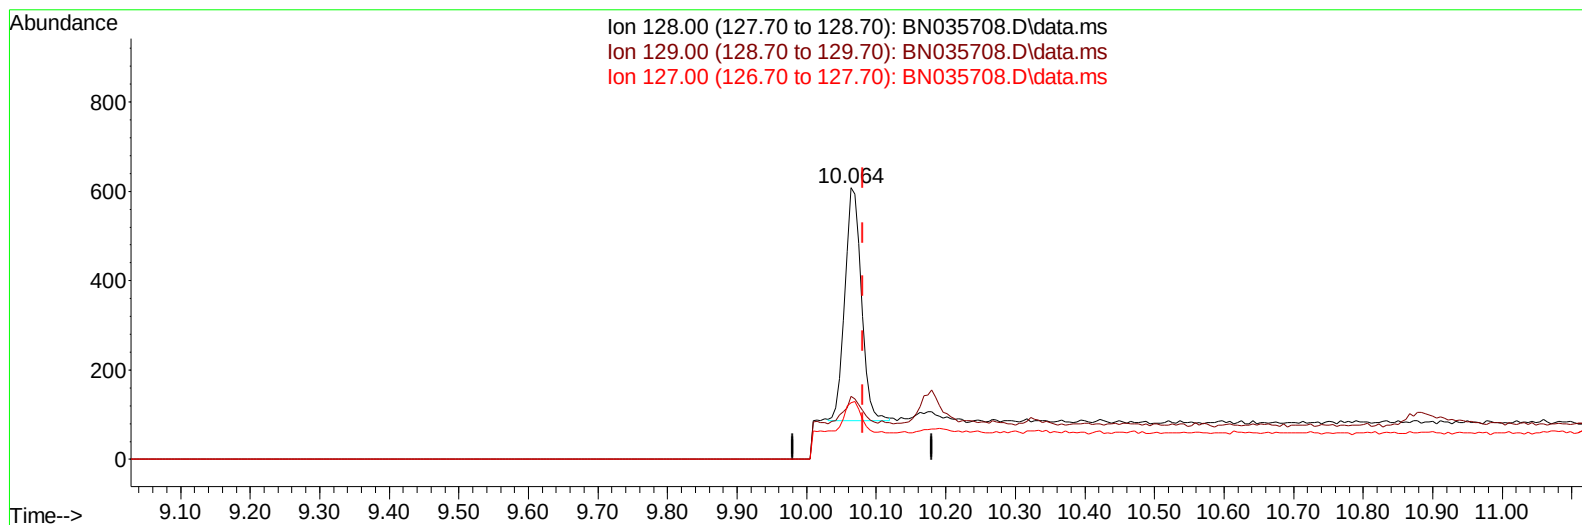

TIC: BN035708.D\data.ms

(5) Naphthalene

10.064min (-0.016) 0.04 ng/ul m

response 861

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 128.00 | 100.00 | 100.00 |
| 129.00 | 13.50  | 23.19# |
| 127.00 | 15.00  | 20.89# |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN121824\  
Data File : BN035708.D  
Acq On : 19 Dec 2024 16:17  
Operator : RC/JU  
Sample : P5258-03DL 5X  
Misc :  
ALS Vial : 49 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
E28W9DL

Manual IntegrationsAPPROVED

Quant Time: Dec 19 16:53:27 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\SFAM-EPA-SIM-BN121624.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Dec 16 16:26:08 2024  
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/21/2024  
Supervised By :mohammad ahmed 12/24/2024

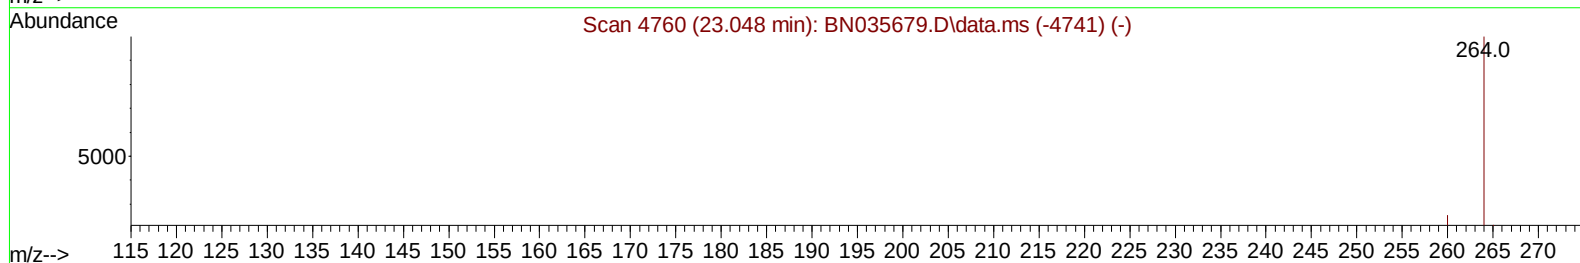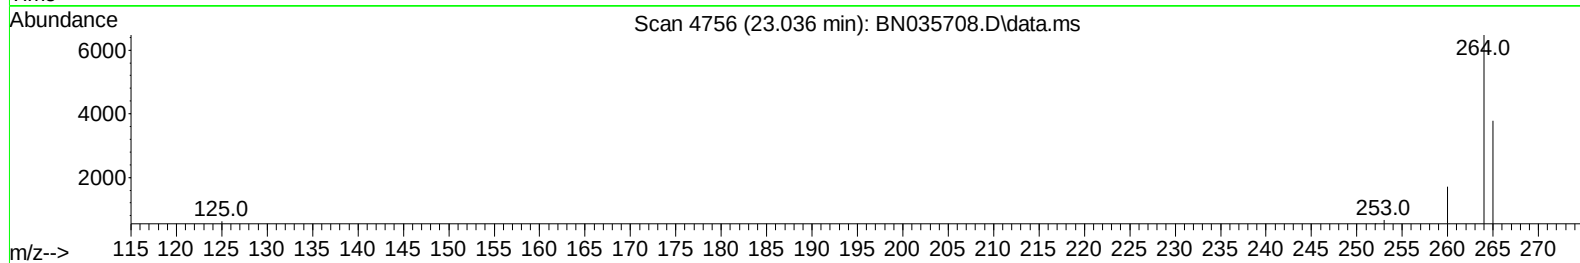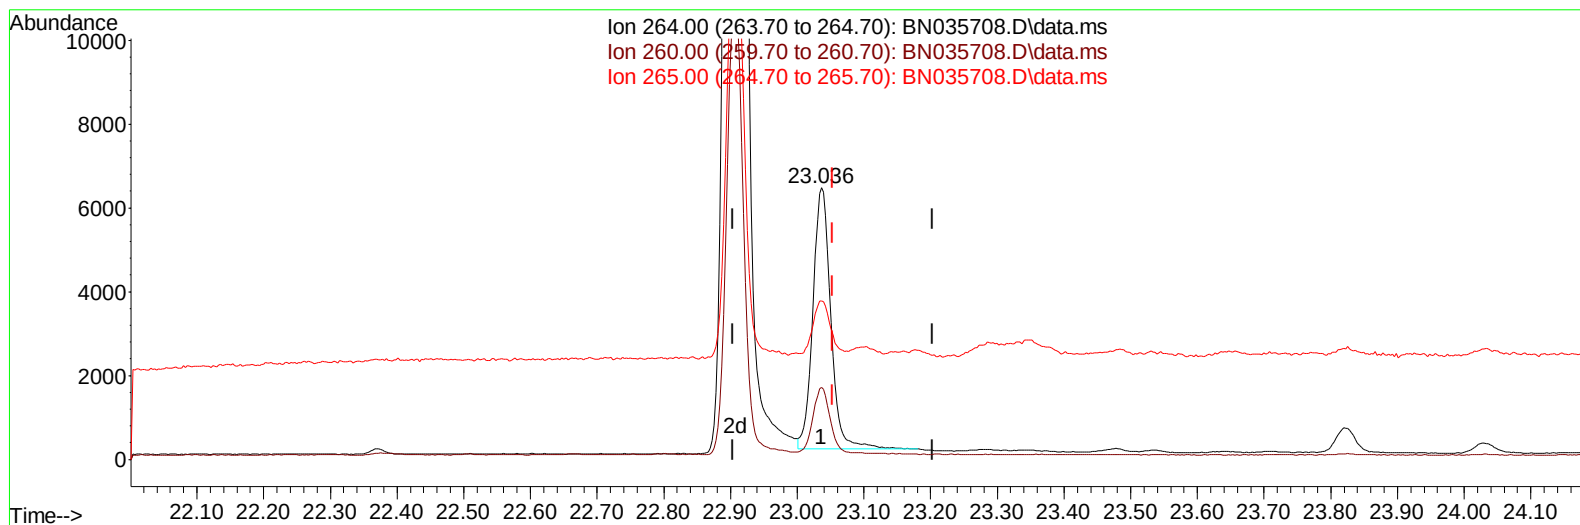

TIC: BN035708.D\data.ms

(23) Perylene-d12 (I)

23.036min (-0.017) 0.40 ng/u1

response 11575

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 264.00 | 100.00 | 100.00 |
| 260.00 | 27.40  | 26.47  |
| 265.00 | 62.10  | 58.48  |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN121824\  
Data File : BN035708.D  
Acq On : 19 Dec 2024 16:17  
Operator : RC/JU  
Sample : P5258-03DL 5X  
Misc :  
ALS Vial : 49 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
E28W9DL

Manual IntegrationsAPPROVED

Quant Time: Dec 19 16:53:27 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\SFAM-EPA-SIM-BN121624.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Dec 16 16:26:08 2024  
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/21/2024  
Supervised By :mohammad ahmed 12/24/2024

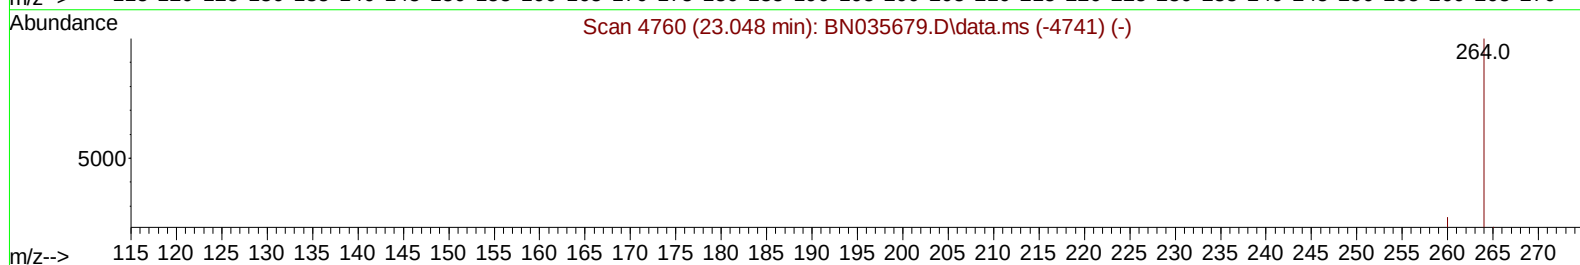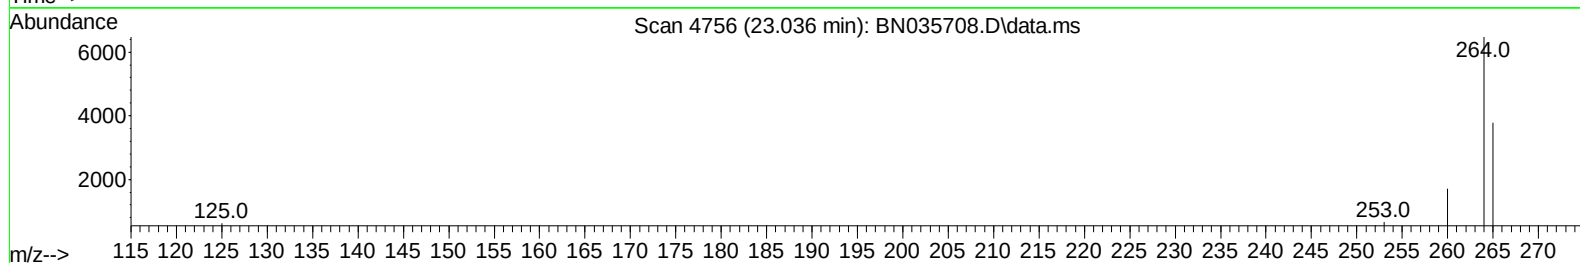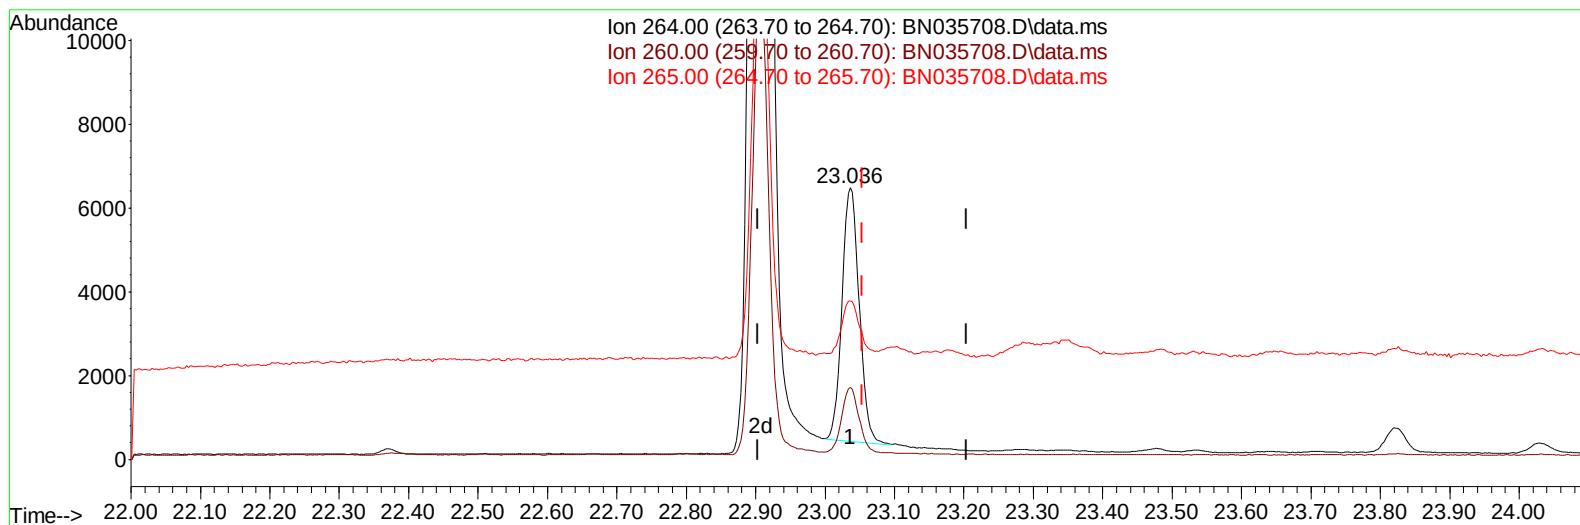

TIC: BN035708.D\data.ms

(23) Perylene-d12 (I)

23.036min (-0.017) 0.40 ng/ul m

response 10407

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 264.00 | 100.00 | 100.00 |
| 260.00 | 27.40  | 26.47  |
| 265.00 | 62.10  | 58.48  |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN121824\  
Data File : BN035708.D  
Acq On : 19 Dec 2024 16:17  
Operator : RC/JU  
Sample : P5258-03DL 5X  
Misc :  
ALS Vial : 49 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
E28W9DL

Manual IntegrationsAPPROVED

Quant Time: Dec 19 16:53:27 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\SFAM-EPA-SIM-BN121624.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Dec 16 16:26:08 2024  
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/21/2024  
Supervised By :mohammad ahmed 12/24/2024

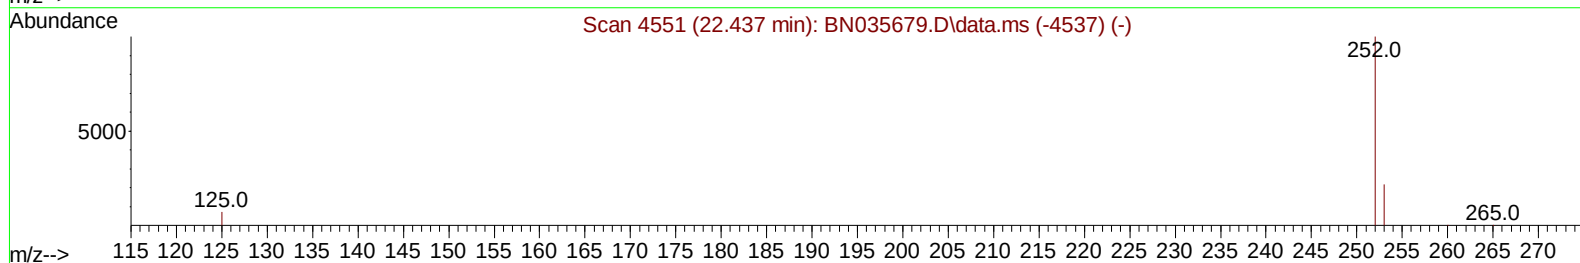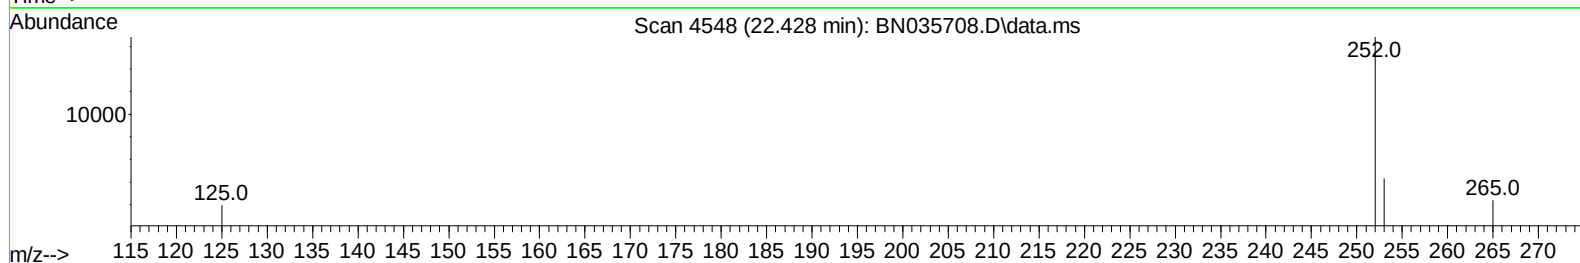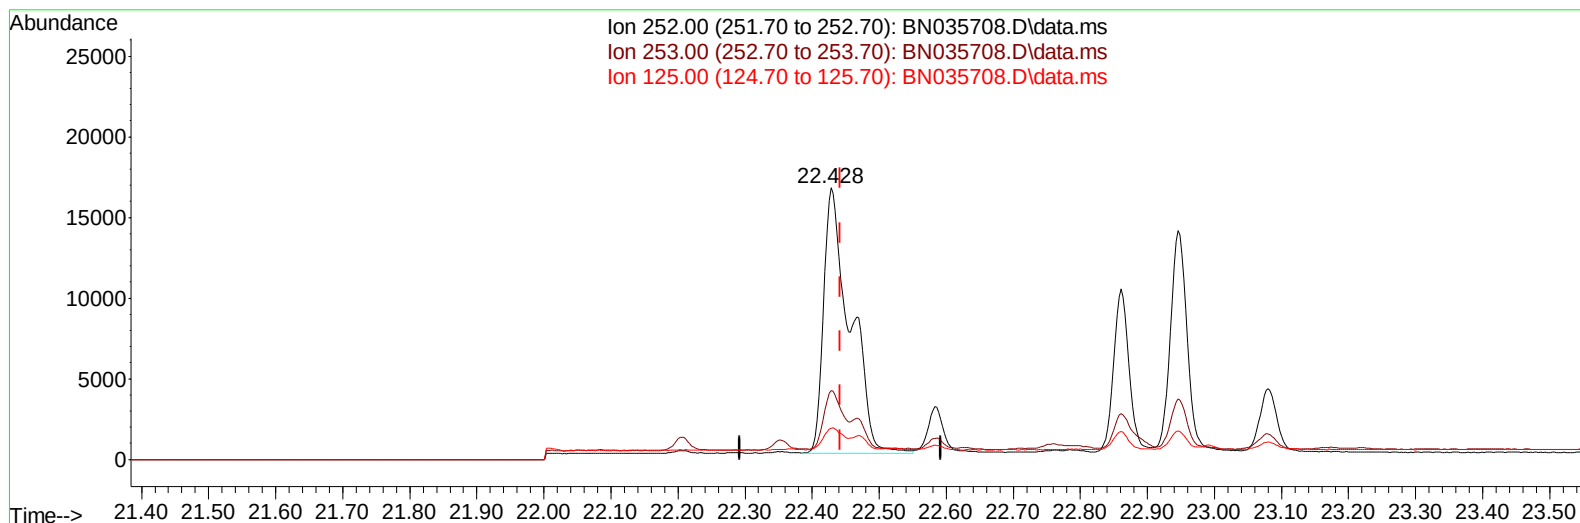

TIC: BN035708.D\data.ms

(24) Benzo(b)fluoranthene

22.428min (-0.014) 1.46 ng/uI

response 44764

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 252.00 | 100.00 | 100.00 |
| 253.00 | 28.20  | 25.46  |
| 125.00 | 18.80  | 11.56  |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN121824\  
Data File : BN035708.D  
Acq On : 19 Dec 2024 16:17  
Operator : RC/JU  
Sample : P5258-03DL 5X  
Misc :  
ALS Vial : 49 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
E28W9DL

Manual IntegrationsAPPROVED

Quant Time: Dec 19 16:53:27 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\SFAM-EPA-SIM-BN121624.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Dec 16 16:26:08 2024  
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/21/2024  
Supervised By :mohammad ahmed 12/24/2024

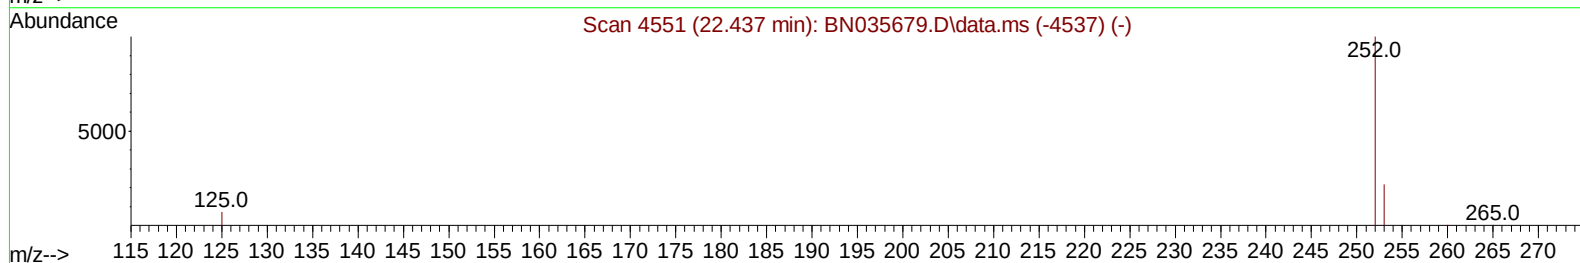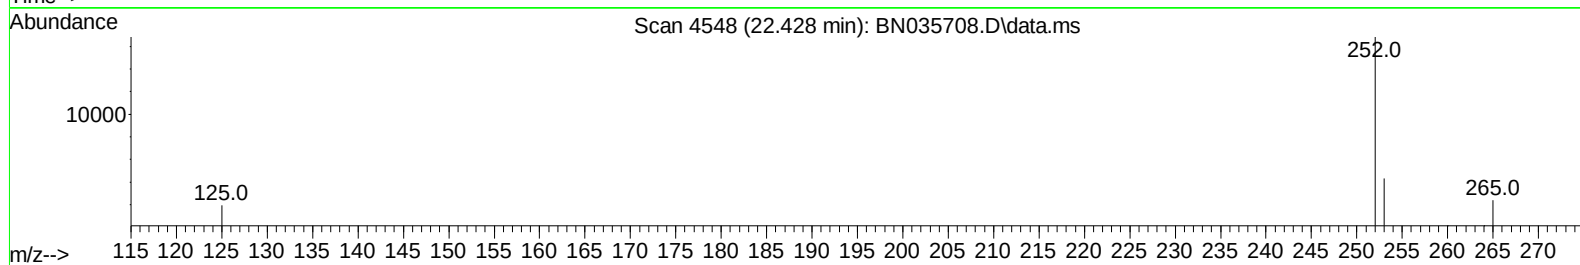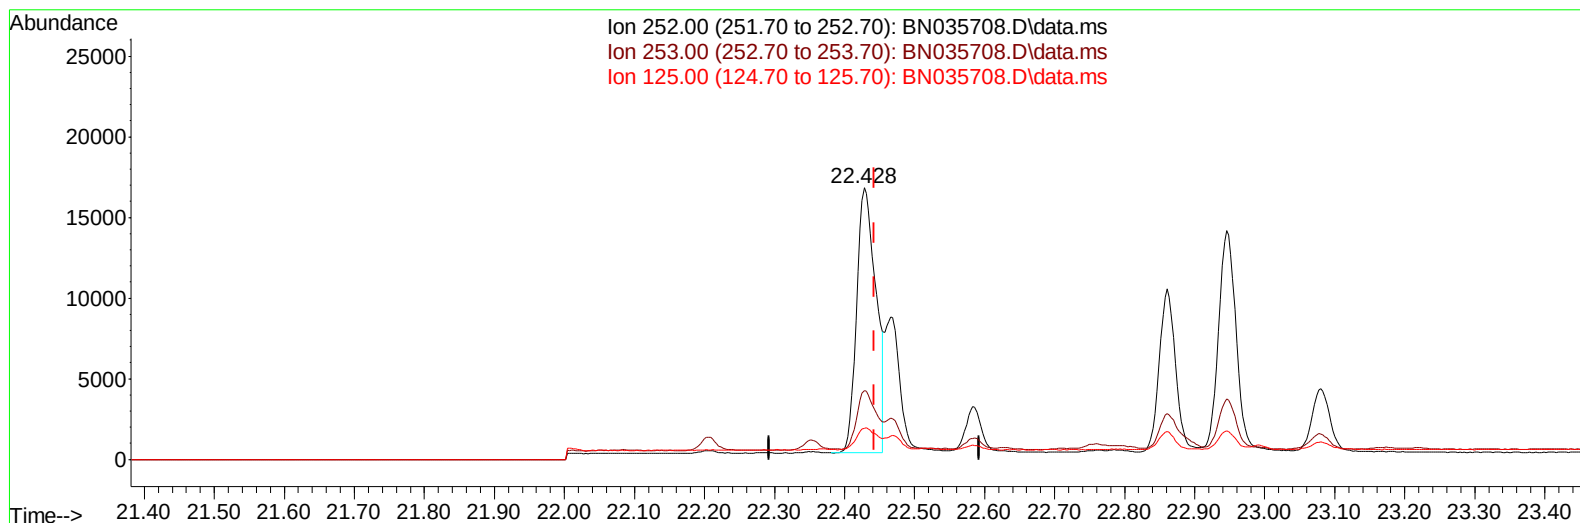

TIC: BN035708.D\data.ms

(24) Benzo(b)fluoranthene

22.428min (-0.014) 1.03 ng/ul m

response 31584

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 252.00 | 100.00 | 100.00 |
| 253.00 | 28.20  | 25.46  |
| 125.00 | 18.80  | 11.56  |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN121824\  
Data File : BN035708.D  
Acq On : 19 Dec 2024 16:17  
Operator : RC/JU  
Sample : P5258-03DL 5X  
Misc :  
ALS Vial : 49 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
E28W9DL

Manual IntegrationsAPPROVED

Quant Time: Dec 19 16:53:27 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\SFAM-EPA-SIM-BN121624.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Dec 16 16:26:08 2024  
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/21/2024  
Supervised By :mohammad ahmed 12/24/2024

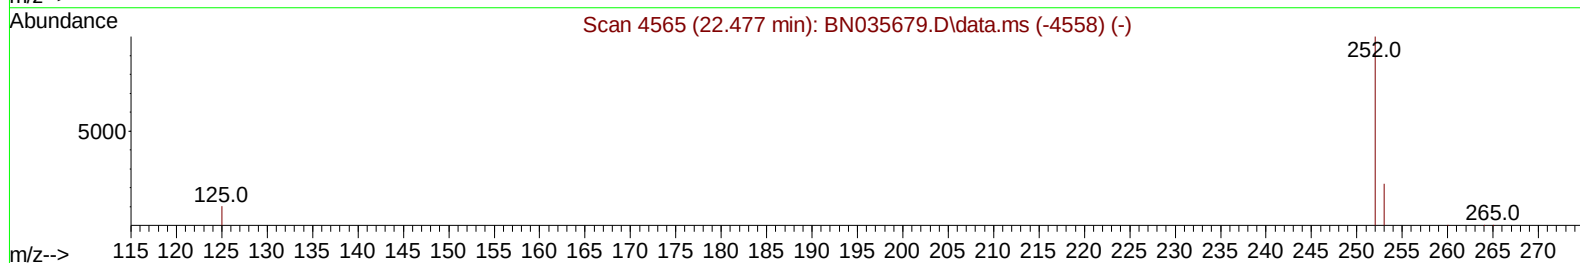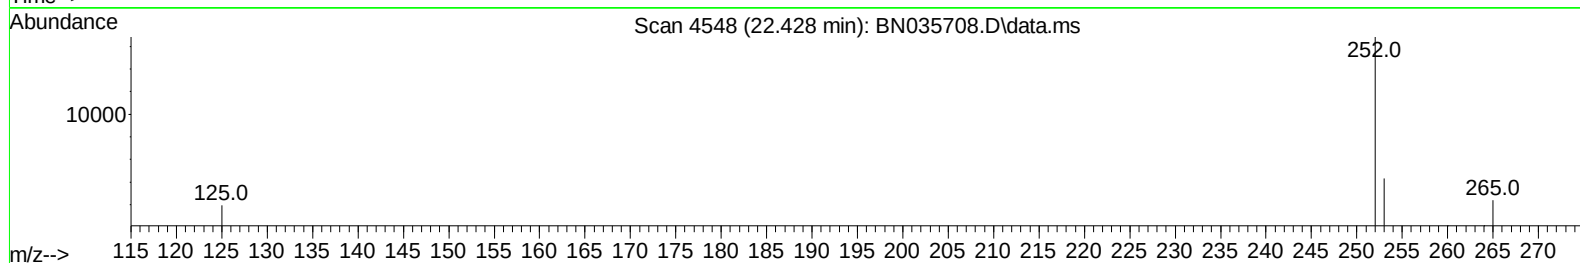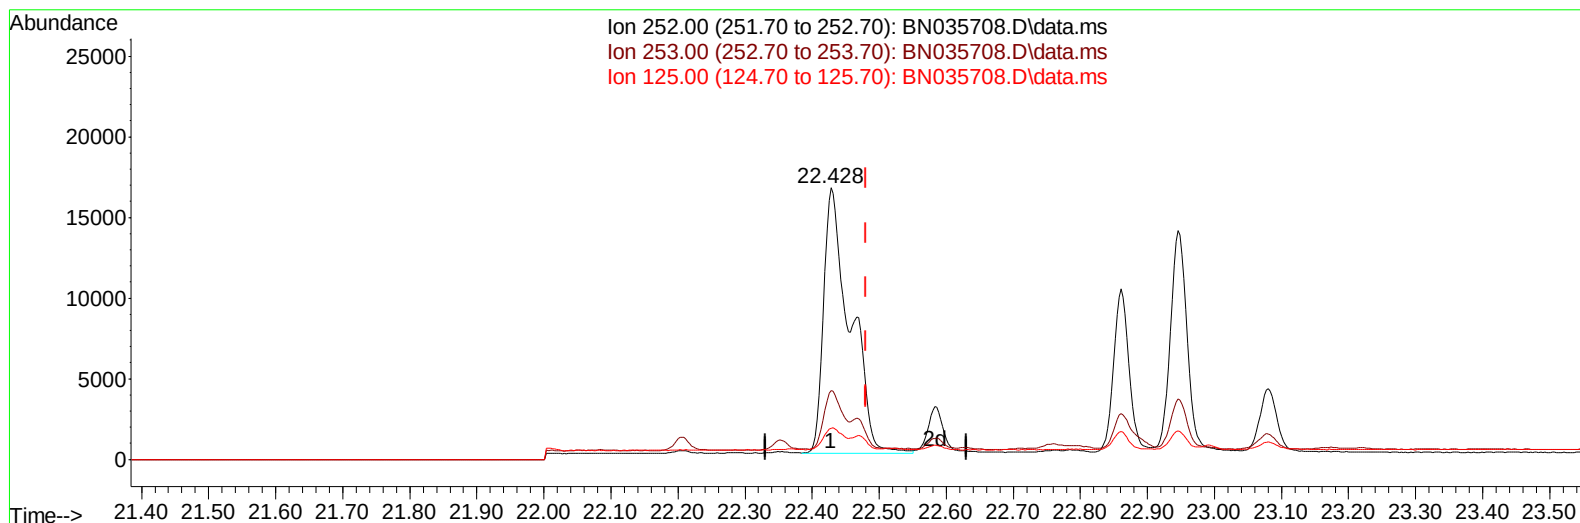

TIC: BN035708.D\data.ms

(25) Benzo(k)fluoranthene

22.428min (-0.052) 1.32 ng/u1

response 44764

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 252.00 | 100.00 | 100.00 |
| 253.00 | 27.60  | 25.46  |
| 125.00 | 19.10  | 11.56# |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN121824\  
Data File : BN035708.D  
Acq On : 19 Dec 2024 16:17  
Operator : RC/JU  
Sample : P5258-03DL 5X  
Misc :  
ALS Vial : 49 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
E28W9DL

Manual IntegrationsAPPROVED

Quant Time: Dec 19 16:53:27 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\SFAM-EPA-SIM-BN121624.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Dec 16 16:26:08 2024  
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/21/2024  
Supervised By :mohammad ahmed 12/24/2024

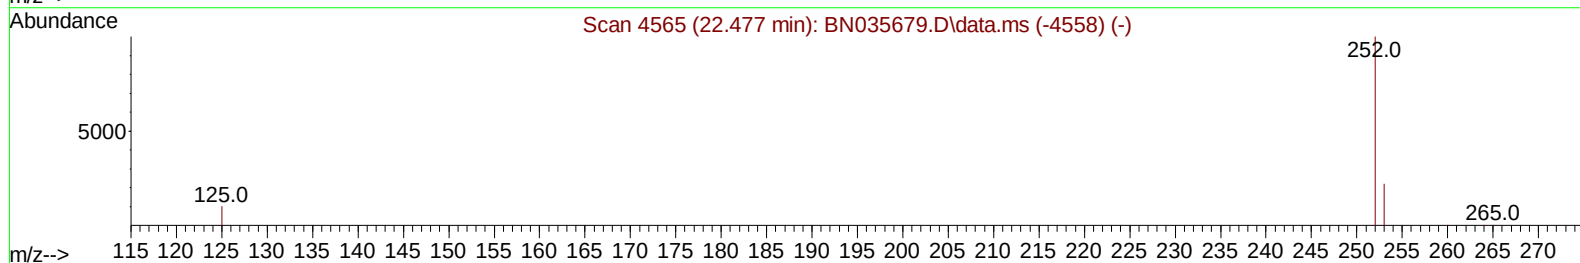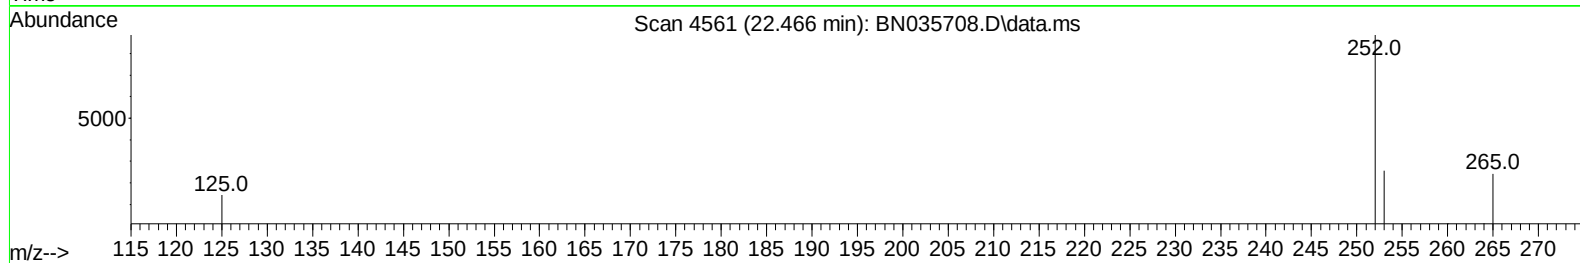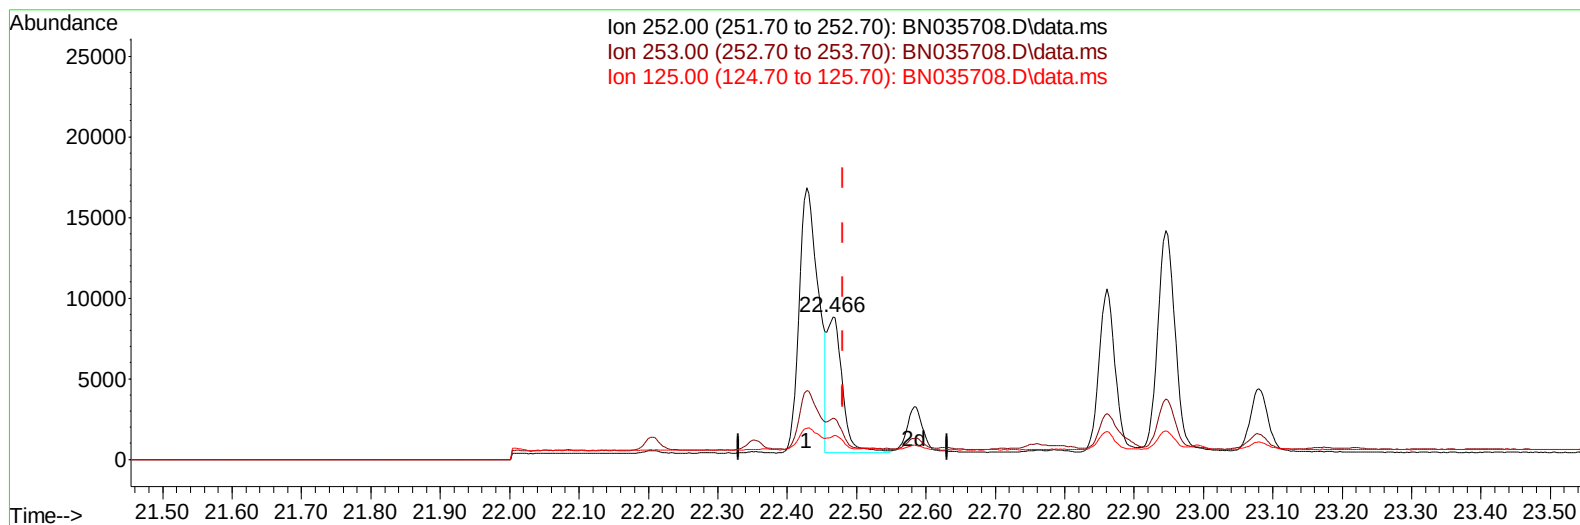

TIC: BN035708.D\data.ms

(25) Benzo(k)fluoranthene

22.466min (-0.014) 0.38 ng/ul m

response 12873

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 252.00 | 100.00 | 100.00 |
| 253.00 | 27.60  | 28.98  |
| 125.00 | 19.10  | 16.28  |
| 0.00   | 0.00   | 0.00   |






Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN121824\  
Data File : BN035708.D  
Acq On : 19 Dec 2024 16:17  
Operator : RC/JU  
Sample : P5258-03DL 5X  
Misc :  
ALS Vial : 49 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
E28W9DL

Manual IntegrationsAPPROVED

Quant Time: Dec 19 16:53:27 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\SFAM-EPA-SIM-BN121624.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Dec 16 16:26:08 2024  
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/21/2024  
Supervised By :mohammad ahmed 12/24/2024

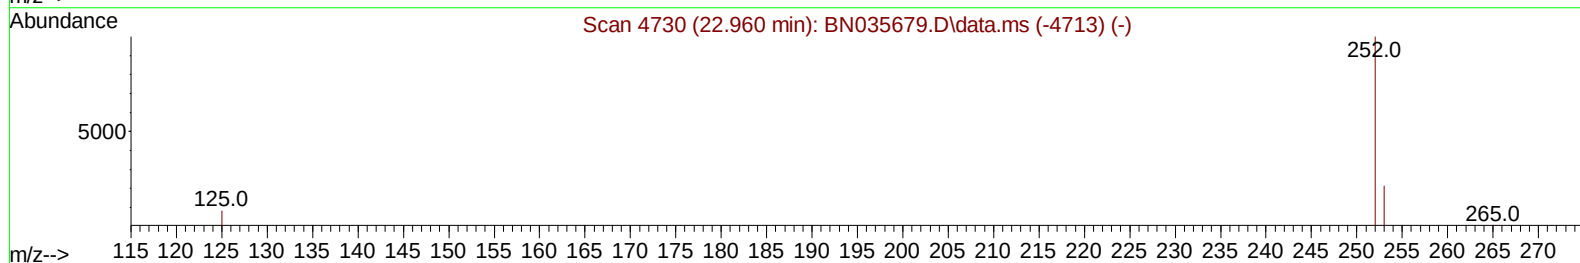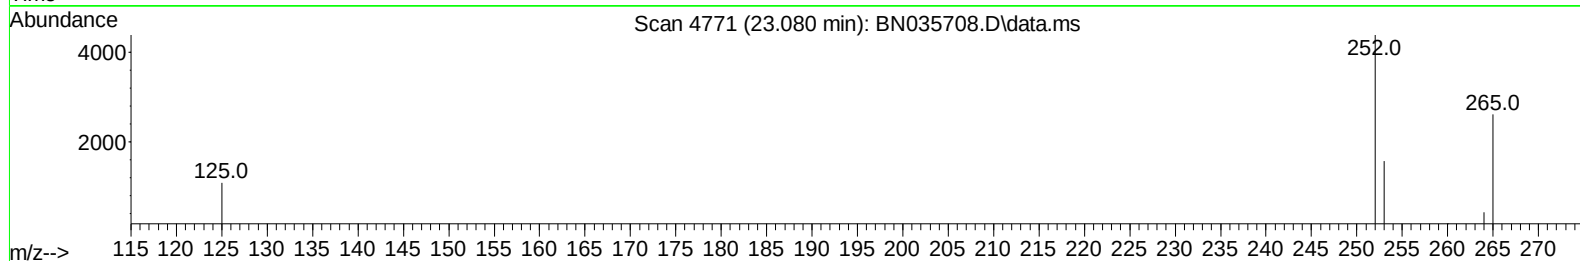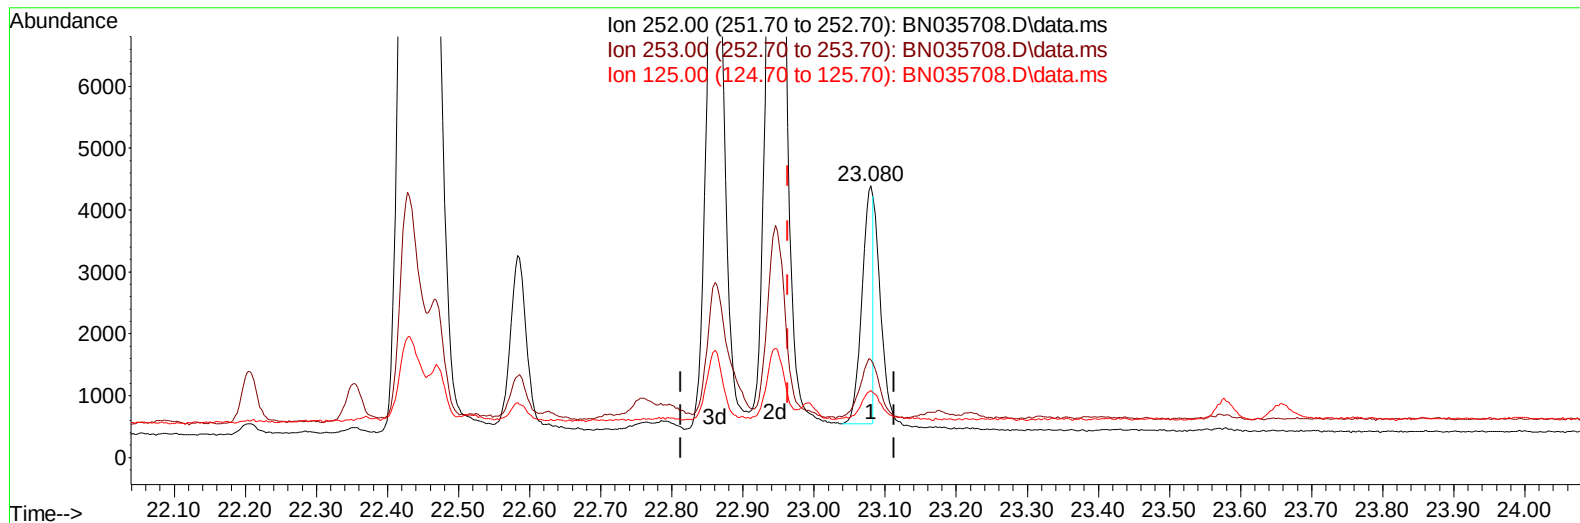

TIC: BN035708.D\data.ms

(26) Benzo(a)pyrene (C)

23.080min (+ 0.117) 0.14 ng/u1

response 4256

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 252.00 | 100.00 | 100.00 |
| 253.00 | 30.10  | 35.86  |
| 125.00 | 23.90  | 24.54  |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN121824\  
Data File : BN035708.D  
Acq On : 19 Dec 2024 16:17  
Operator : RC/JU  
Sample : P5258-03DL 5X  
Misc :  
ALS Vial : 49 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
E28W9DL

Manual IntegrationsAPPROVED

Quant Time: Dec 19 16:53:27 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\SFAM-EPA-SIM-BN121624.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Dec 16 16:26:08 2024  
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/21/2024  
Supervised By :mohammad ahmed 12/24/2024

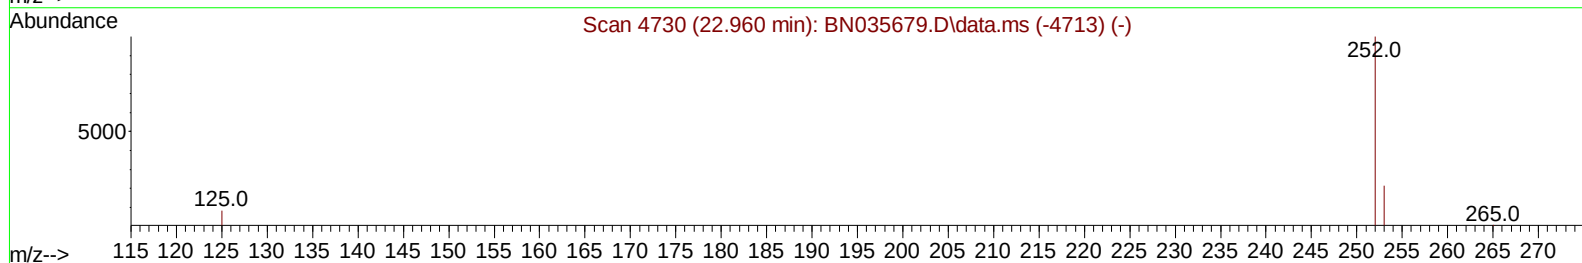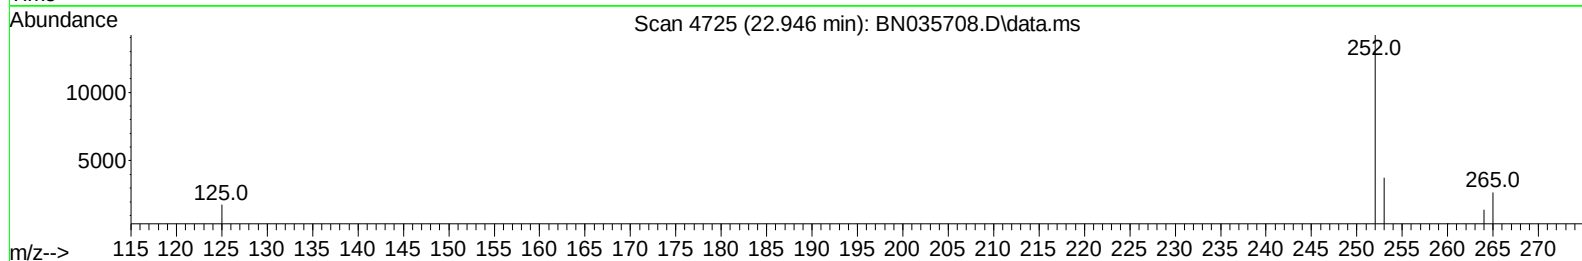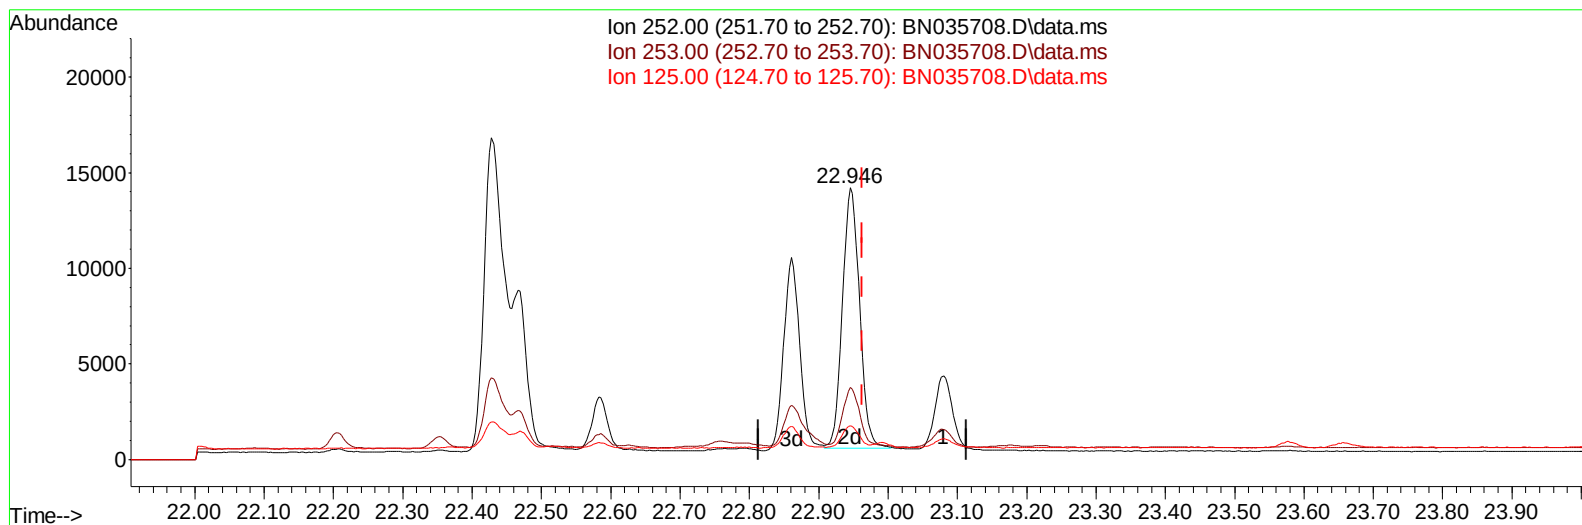

TIC: BN035708.D\data.ms

(26) Benzo(a)pyrene (C)

22.946min (-0.017) 0.79 ng/ul m

response 23340

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 252.00 | 100.00 | 100.00 |
| 253.00 | 30.10  | 26.44  |
| 125.00 | 23.90  | 12.46# |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN121824\  
Data File : BN035708.D  
Acq On : 19 Dec 2024 16:17  
Operator : RC/JU  
Sample : P5258-03DL 5X  
Misc :  
ALS Vial : 49 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
E28W9DL

Manual IntegrationsAPPROVED

Quant Time: Dec 19 16:53:27 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\SFAM-EPA-SIM-BN121624.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Dec 16 16:26:08 2024  
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/21/2024  
Supervised By :mohammad ahmed 12/24/2024

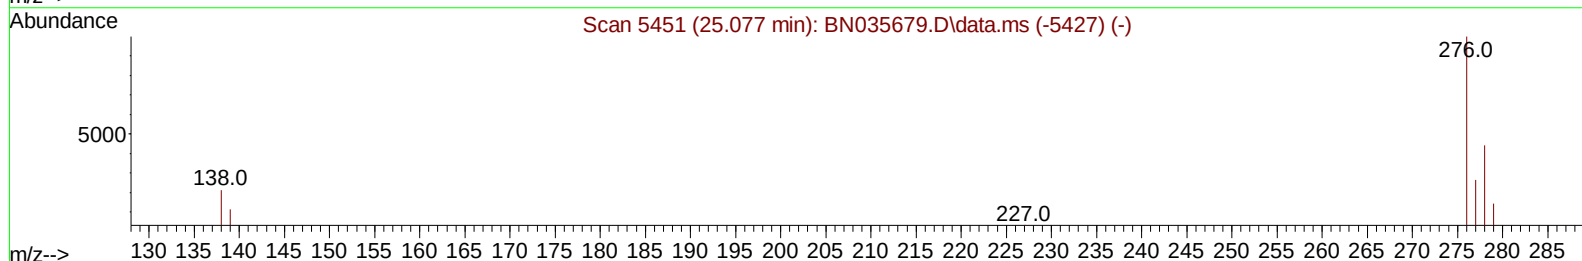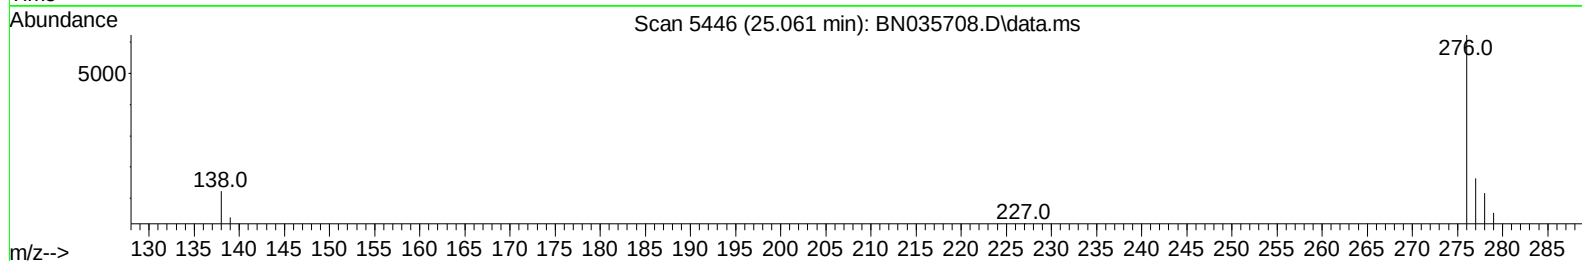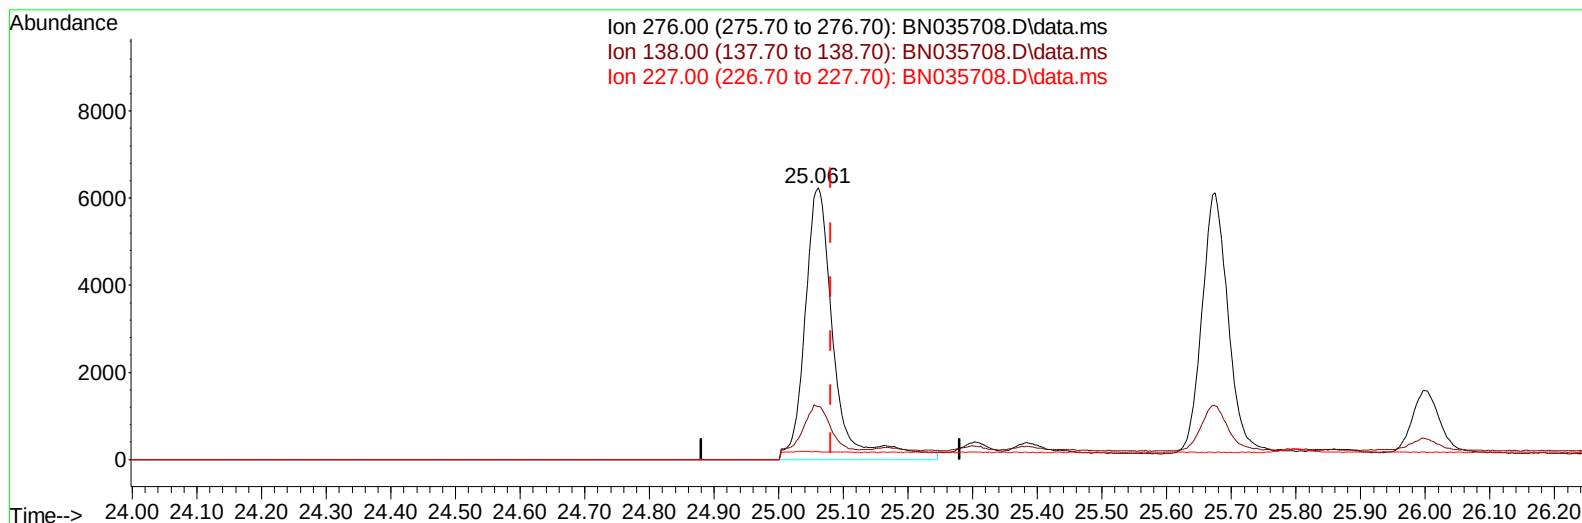

TIC: BN035708.D\data.ms

(27) Indeno(1,2,3-cd)pyrene

25.061min (-0.020) 0.53 ng/u1

response 19194

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 276.00 | 100.00 | 100.00 |
| 138.00 | 18.40  | 31.92# |
| 227.00 | 27.00  | 0.00#  |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN121824\  
Data File : BN035708.D  
Acq On : 19 Dec 2024 16:17  
Operator : RC/JU  
Sample : P5258-03DL 5X  
Misc :  
ALS Vial : 49 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
E28W9DL

Manual IntegrationsAPPROVED

Quant Time: Dec 19 16:53:27 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\SFAM-EPA-SIM-BN121624.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Dec 16 16:26:08 2024  
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/21/2024  
Supervised By :mohammad ahmed 12/24/2024

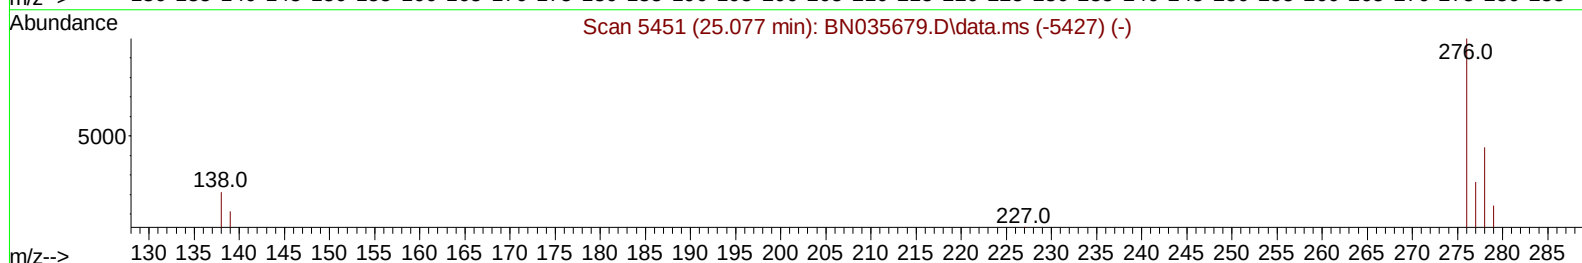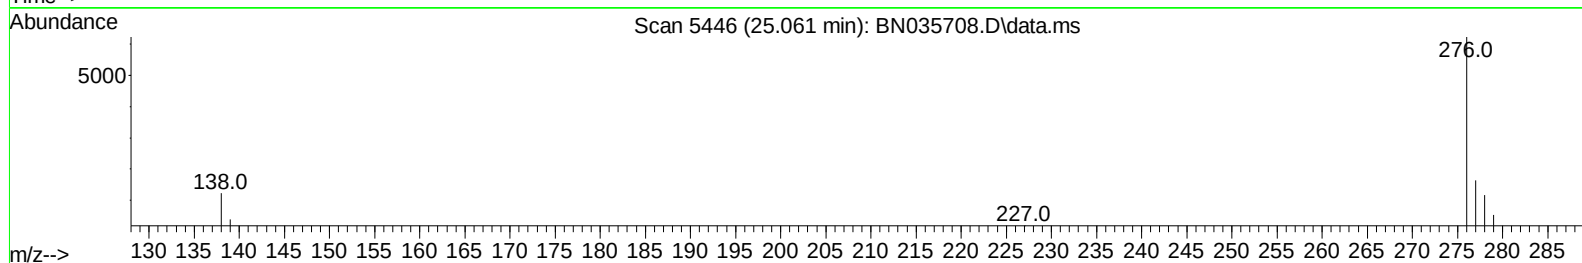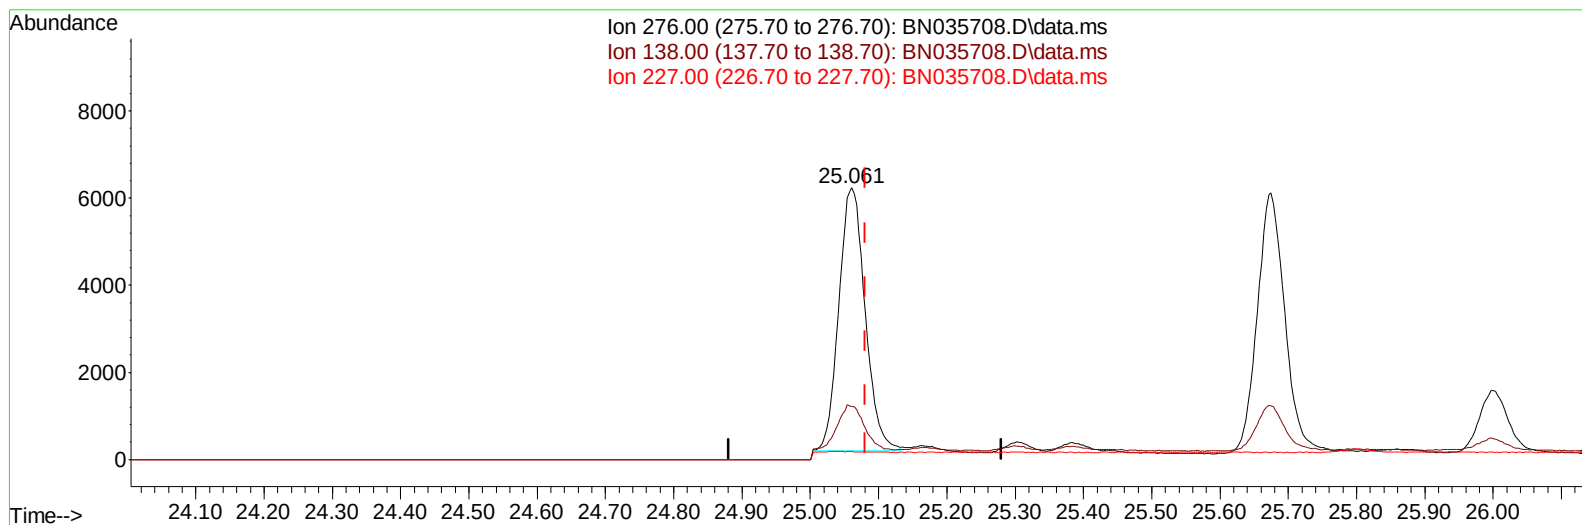

TIC: BN035708.D\data.ms

(27) Indeno(1,2,3-cd)pyrene

25.061min (-0.020) 0.44 ng/ul m

response 16039

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 276.00 | 100.00 | 100.00 |
| 138.00 | 18.40  | 38.19# |
| 227.00 | 27.00  | 0.00#  |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN121824\  
Data File : BN035708.D  
Acq On : 19 Dec 2024 16:17  
Operator : RC/JU  
Sample : P5258-03DL 5X  
Misc :  
ALS Vial : 49 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
E28W9DL

Manual IntegrationsAPPROVED

Quant Time: Dec 19 16:53:27 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\SFAM-EPA-SIM-BN121624.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Dec 16 16:26:08 2024  
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/21/2024  
Supervised By :mohammad ahmed 12/24/2024

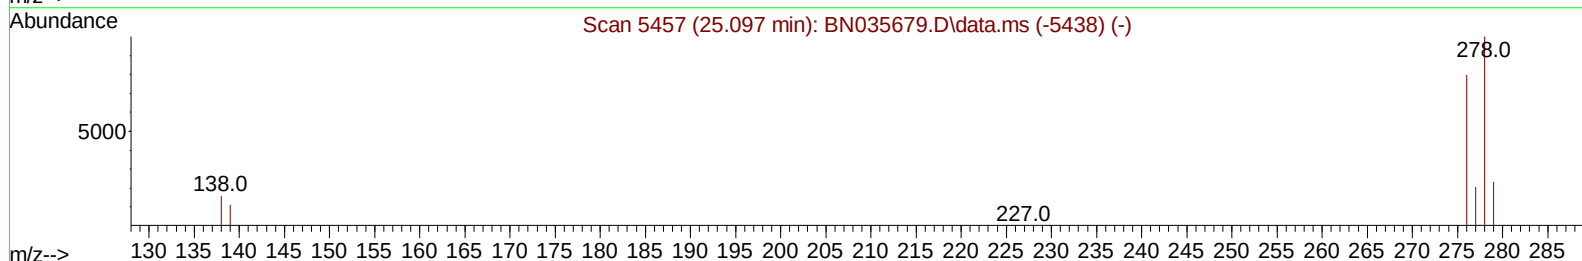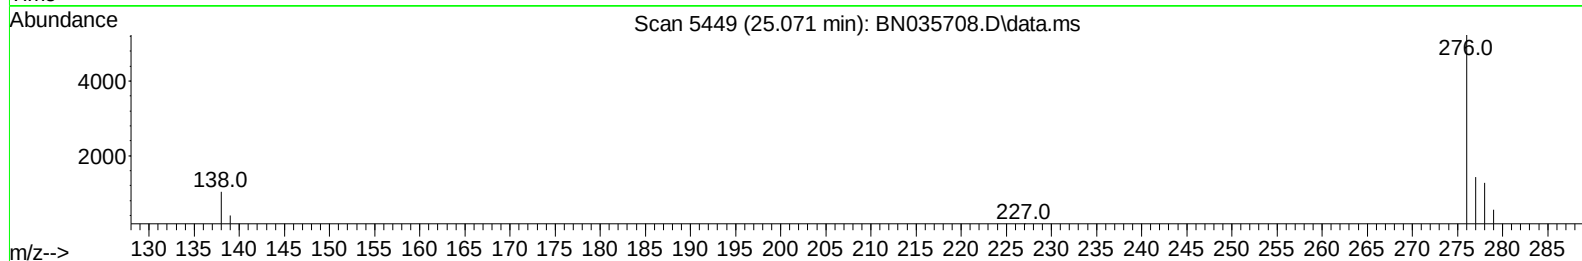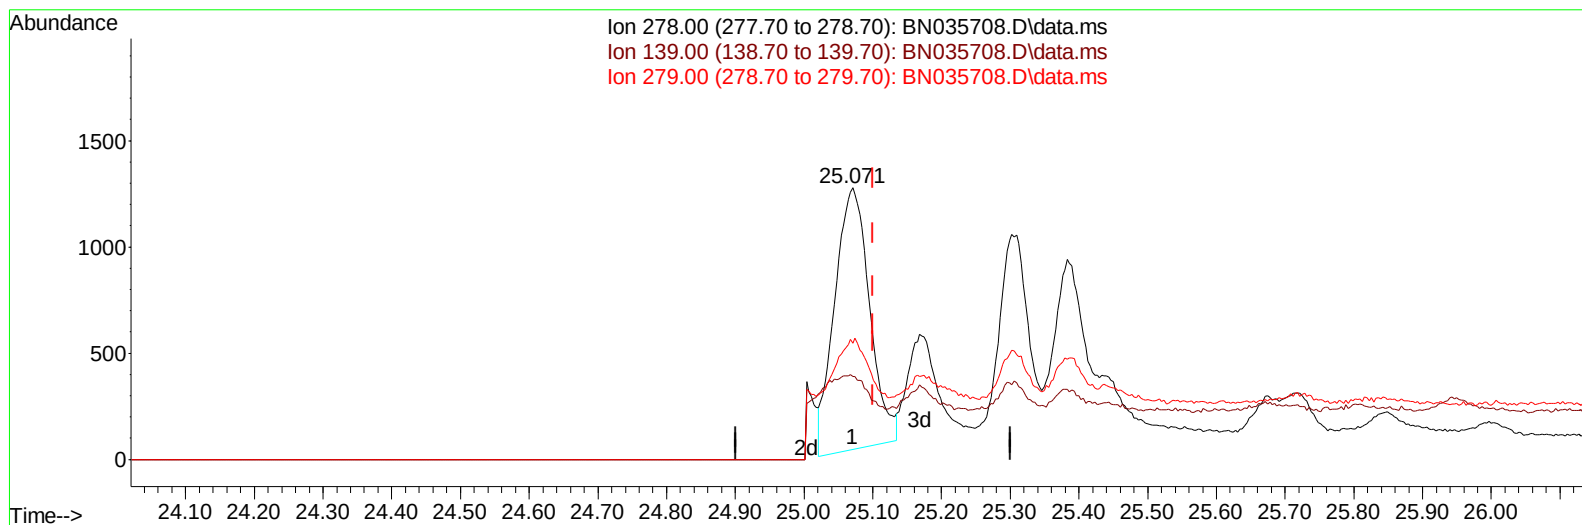

TIC: BN035708.D\data.ms

(28) Dibenzo(a,h)anthracene

25.071min (-0.030) 0.16 ng/u1

response 4356

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 278.00 | 100.00 | 100.00 |
| 139.00 | 24.80  | 30.59# |
| 279.00 | 30.00  | 42.88# |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN121824\  
Data File : BN035708.D  
Acq On : 19 Dec 2024 16:17  
Operator : RC/JU  
Sample : P5258-03DL 5X  
Misc :  
ALS Vial : 49 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
E28W9DL

Manual IntegrationsAPPROVED

Quant Time: Dec 19 16:53:27 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\SFAM-EPA-SIM-BN121624.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Dec 16 16:26:08 2024  
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/21/2024  
Supervised By :mohammad ahmed 12/24/2024

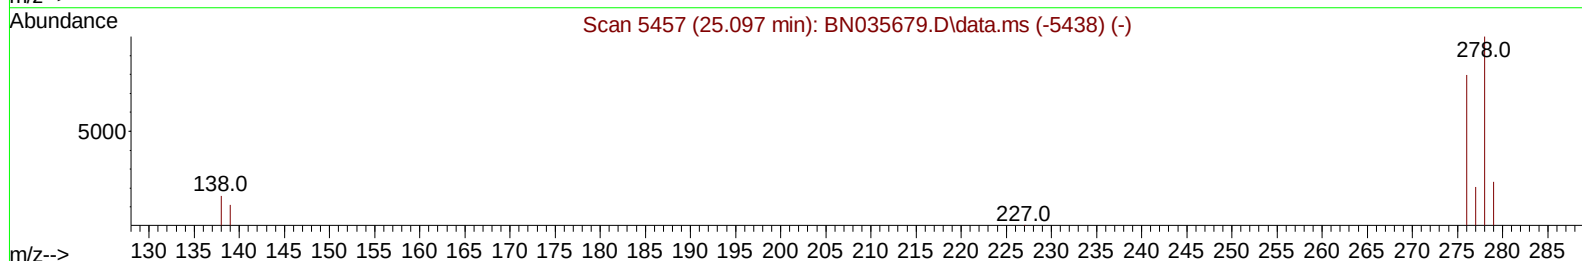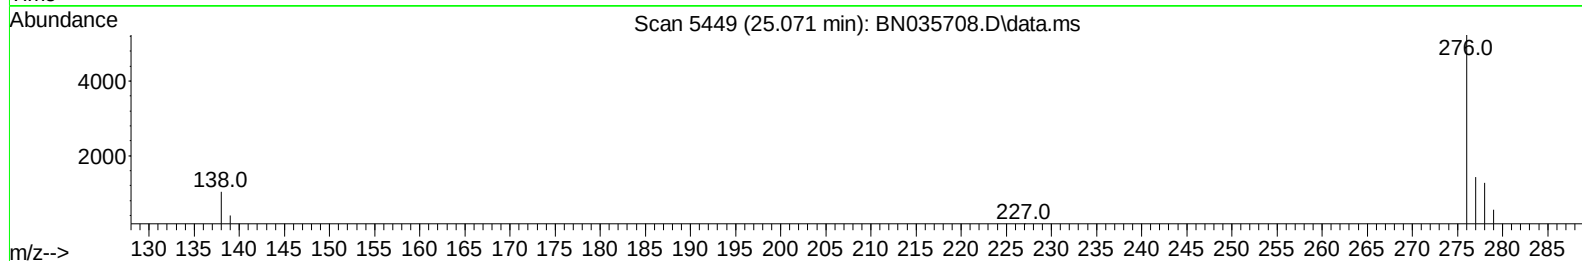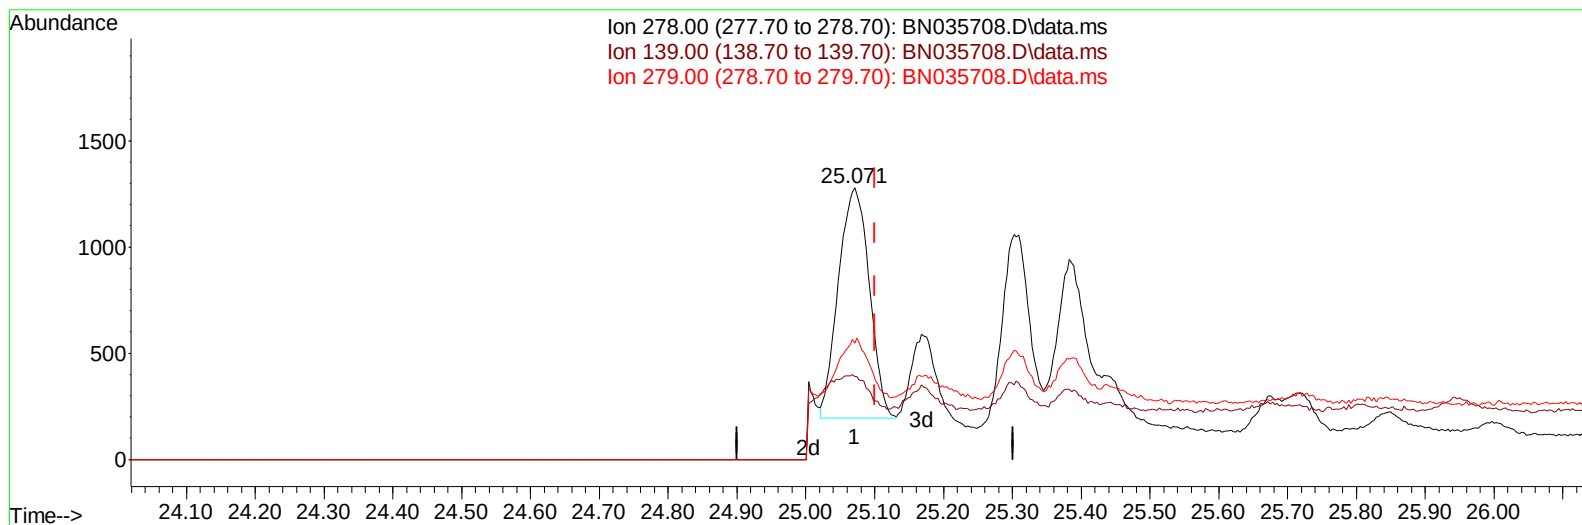

TIC: BN035708.D\data.ms

(28) Dibenzo(a,h)anthracene

25.071min (-0.030) 0.12 ng/ul m

response 3372

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 278.00 | 100.00 | 100.00 |
| 139.00 | 24.80  | 30.59# |
| 279.00 | 30.00  | 42.88# |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN121824\  
 Data File : BN035708.D  
 Acq On : 19 Dec 2024 16:17  
 Operator : RC/JU  
 Sample : P5258-03DL 5X  
 Misc :  
 ALS Vial : 49 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 E28W9DL

## Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/21/2024  
 Supervised By :mohammad ahmed 12/24/2024

Quant Time: Dec 19 16:53:27 2024  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\SFAM-EPA-SIM-BN121624.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Mon Dec 16 16:26:08 2024  
 Response via : Initial Calibration

| Compound                    | R.T.   | QIon | Response | Conc  | Units  | Dev(Min) |
|-----------------------------|--------|------|----------|-------|--------|----------|
| -----                       |        |      |          |       |        |          |
| Internal Standards          |        |      |          |       |        |          |
| 1) 1,4-Dichlorobenzene-d4   | 7.276  | 152  | 3436     | 0.400 | ng/ul  | 0.00     |
| 4) Naphthalene-d8           | 10.020 | 136  | 8747     | 0.400 | ng/ul  | -0.01    |
| 9) Acenaphthene-d10         | 13.935 | 164  | 6037     | 0.400 | ng/ul  | -0.01    |
| 13) Phenanthrene-d10        | 16.705 | 188  | 11728    | 0.400 | ng/ul  | -0.01    |
| 17) Chrysene-d12            | 20.953 | 240  | 9748     | 0.400 | ng/ul  | -0.01    |
| 23) Perylene-d12            | 23.036 | 264  | 10407m   | 0.400 | ng/ul  | -0.02    |
| System Monitoring Compounds |        |      |          |       |        |          |
| 3) 1,4-Dioxane-d8           | 2.951  | 96   | 3287     | 1.079 | ng/ul  | 0.00     |
| 6) 2-Methylnaphthalene-d10  | 11.626 | 152  | 749      | 0.060 | ng/ul  | -0.01    |
| 18) Fluoranthene-d10        | 18.758 | 212  | 1222     | 0.043 | ng/ul  | 0.00     |
| Target Compounds            |        |      |          |       |        |          |
|                             |        |      |          |       |        | Qvalue   |
| 5) Naphthalene              | 10.064 | 128  | 861m     | 0.040 | ng/ul  |          |
| 7) 2-Methylnaphthalene      | 11.703 | 142  | 441      | 0.031 | ng/ul  | 95       |
| 8) 1-Methylnaphthalene      | 11.928 | 142  | 406      | 0.027 | ng/ul  | 98       |
| 11) Acenaphthene            | 14.000 | 153  | 2115     | 0.120 | ng/ul  | 98       |
| 12) Fluorene                | 15.004 | 166  | 1846     | 0.090 | ng/ul# | 98       |
| 15) Phenanthrene            | 16.747 | 178  | 34409    | 1.172 | ng/ul  | 98       |
| 16) Anthracene              | 16.840 | 178  | 7273     | 0.265 | ng/ul  | 99       |
| 19) Fluoranthene            | 18.791 | 202  | 60618    | 1.739 | ng/ul  | 99       |
| 20) Pyrene                  | 19.158 | 202  | 53023    | 1.381 | ng/ul  | 99       |
| 21) Benzo(a)anthracene      | 20.938 | 228  | 24060    | 0.744 | ng/ul  | 100      |
| 22) Chrysene                | 20.988 | 228  | 24457    | 0.729 | ng/ul  | 98       |
| 24) Benzo(b)fluoranthene    | 22.428 | 252  | 31584m   | 1.030 | ng/ul  |          |
| 25) Benzo(k)fluoranthene    | 22.466 | 252  | 12873m   | 0.379 | ng/ul  |          |
| 26) Benzo(a)pyrene          | 22.946 | 252  | 23340m   | 0.786 | ng/ul  |          |
| 27) Indeno(1,2,3-cd)pyrene  | 25.061 | 276  | 16039m   | 0.444 | ng/ul  |          |
| 28) Dibenzo(a,h)anthracene  | 25.071 | 278  | 3372m    | 0.122 | ng/ul  |          |
| 29) Benzo(g,h,i)perylene    | 25.675 | 276  | 17092    | 0.589 | ng/ul  | 94       |
| -----                       |        |      |          |       |        |          |

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN121824\  
Data File : BN035708.D  
Acq On : 19 Dec 2024 16:17  
Operator : RC/JU  
Sample : P5258-03DL 5X  
Misc :  
ALS Vial : 49 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
E28W9DL

## Manual IntegrationsAPPROVED

Quant Time: Dec 19 16:53:27 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\SFAM-EPA-SIM-BN121624.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Dec 16 16:26:08 2024  
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/21/2024  
Supervised By :mohammad ahmed 12/24/2024

