
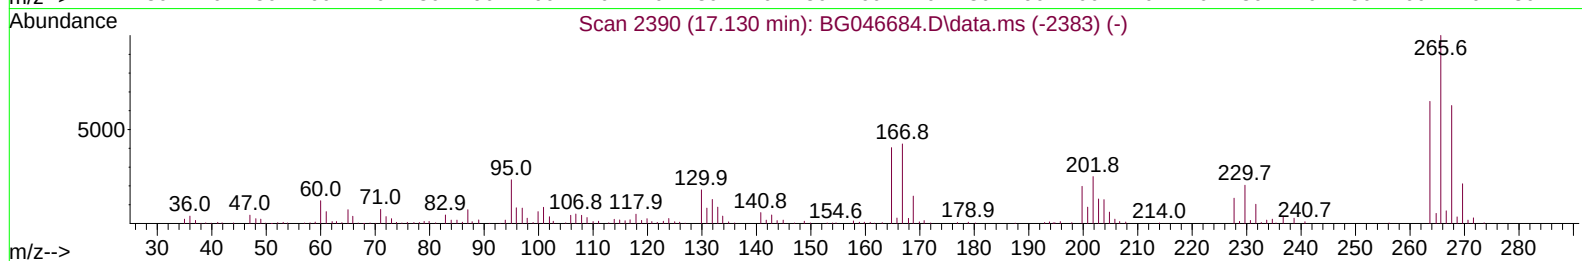
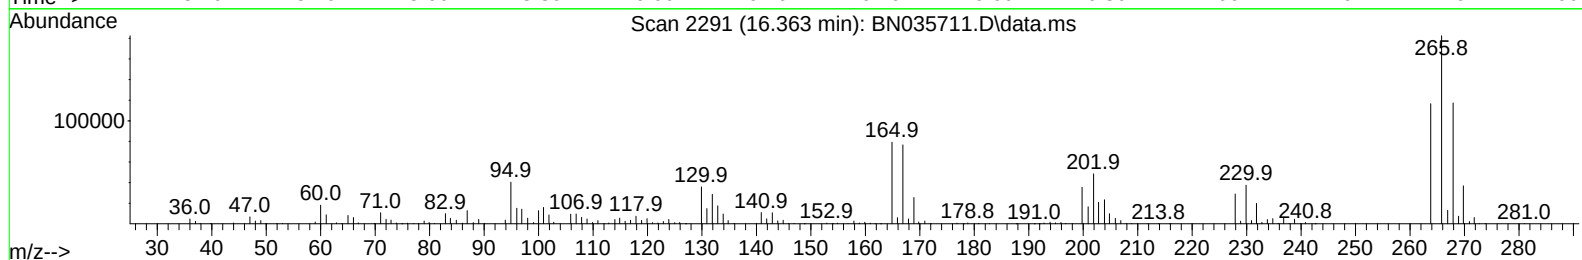


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN121924\  
Data File : BN035711.D  
Acq On : 19 Dec 2024 18:44  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 20 01:29:26 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Dec 20 01:29:08 2024  
Response via : Initial Calibration

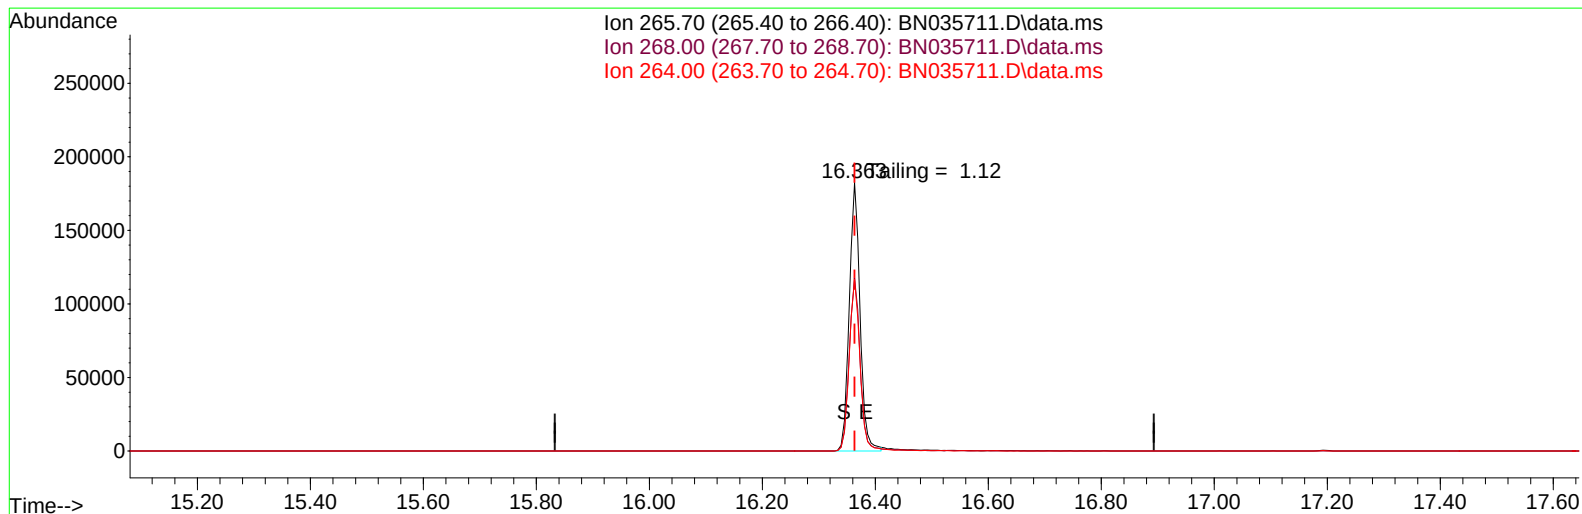

TIC: BN035711.D\data.ms

**(70) Pentachlorophenol (C)**




16.363min ( 0.000) 25694.23 ng

response 246608

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 64.25  |
| 264.00 | 61.60  | 63.89  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN121924\  
Data File : BN035711.D  
Acq On : 19 Dec 2024 18:44  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 20 01:29:26 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Dec 20 01:29:08 2024  
Response via : Initial Calibration

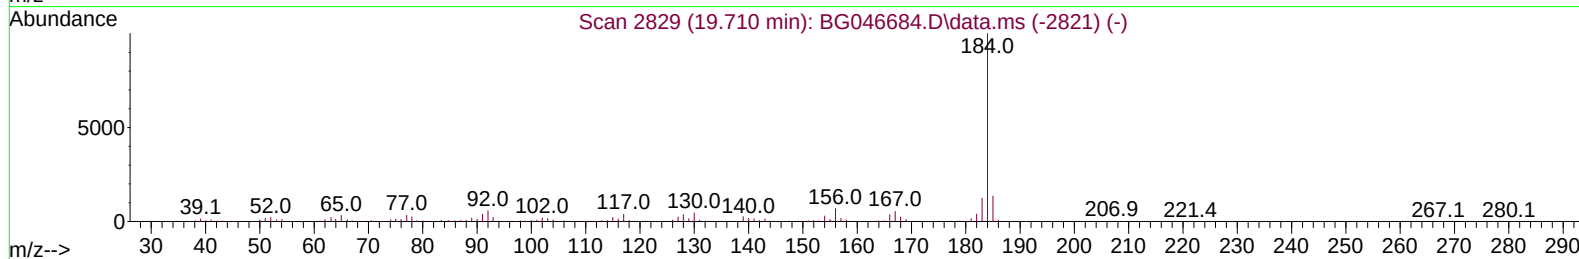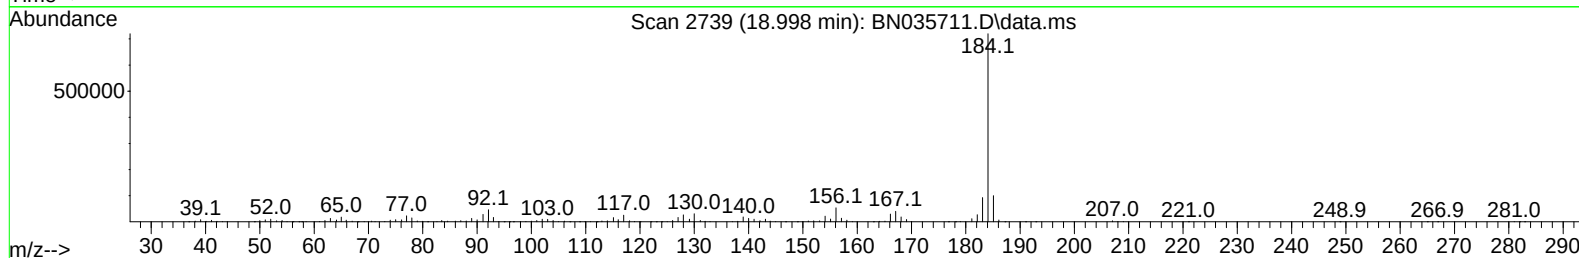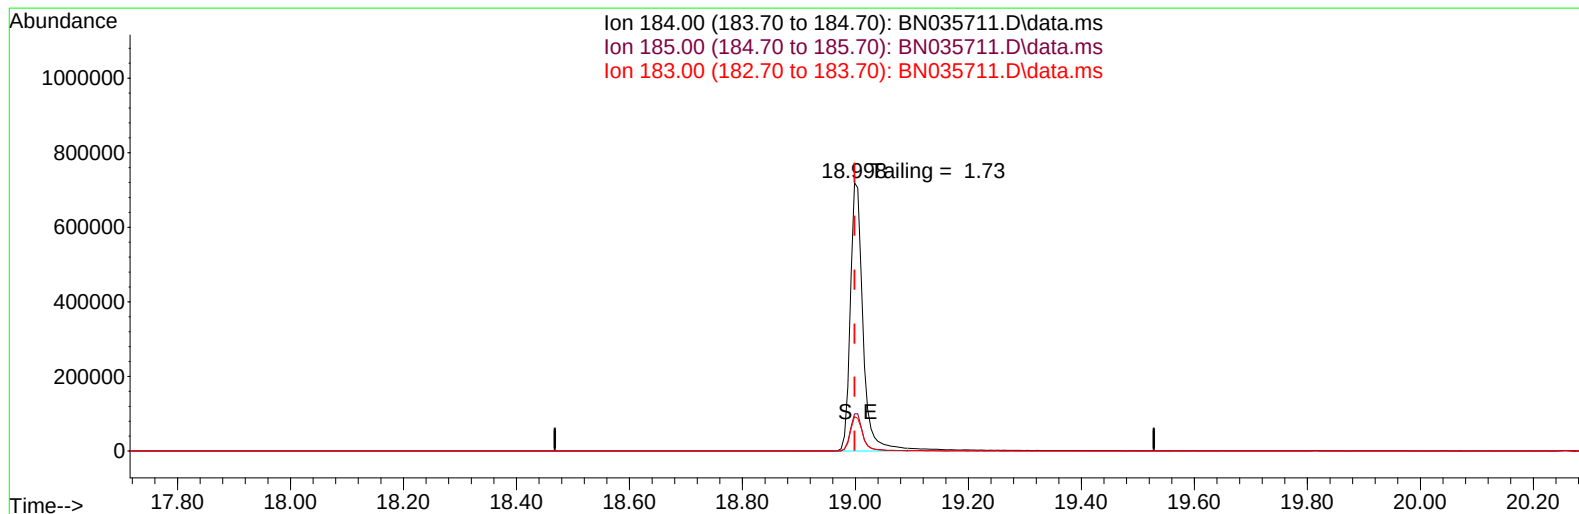

TIC: BN035711.D\data.ms

**(77) Benzidine**

18.998min ( 0.000) 0.00 ng

response 1146216

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 13.87  |
| 183.00 | 13.20  | 12.84  |
| 0.00   | 0.00   | 0.00   |