
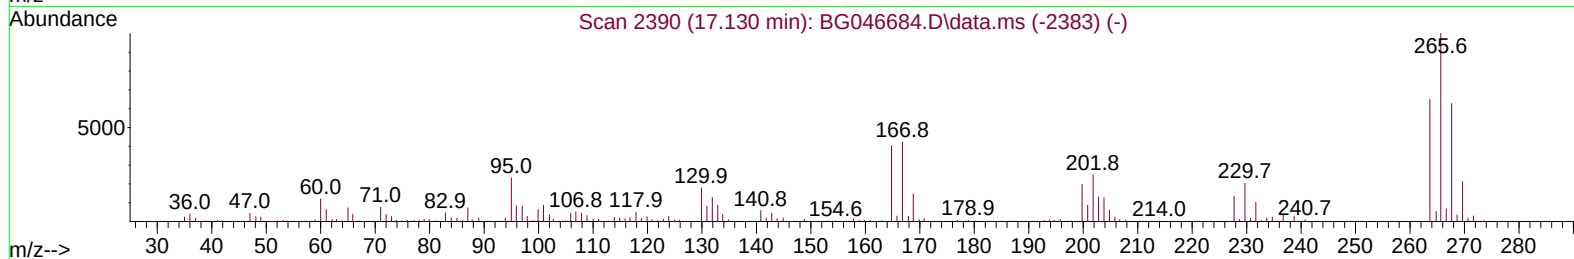
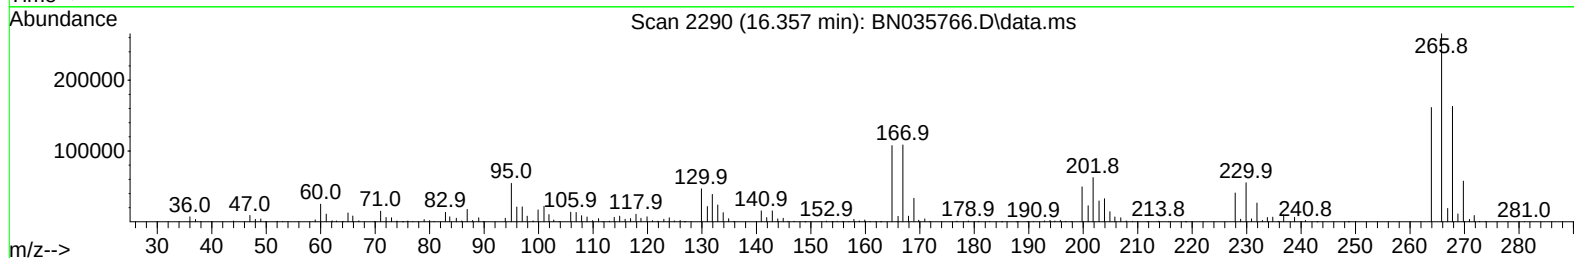


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121924\
Data File : BN035766.D
Acq On : 21 Dec 2024 05:46
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 57 Sample Multiplier: 1

Quant Time: Dec 21 06:30:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 21 06:29:35 2024
Response via : Initial Calibration

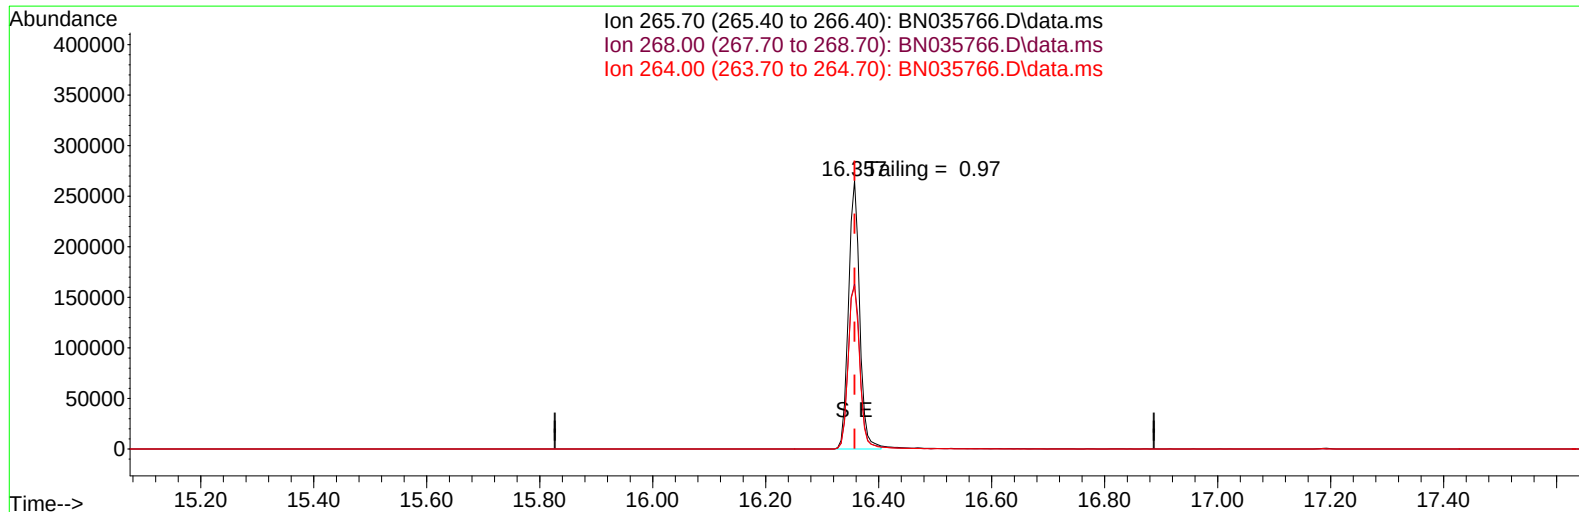

TIC: BN035766.D\data.ms

(70) Pentachlorophenol (C)




16.357min (0.000) 26639.20 ng

response 369196

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.38
264.00	61.60	60.75
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121924\
Data File : BN035766.D
Acq On : 21 Dec 2024 05:46
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 57 Sample Multiplier: 1

Quant Time: Dec 21 06:30:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 21 06:29:35 2024
Response via : Initial Calibration

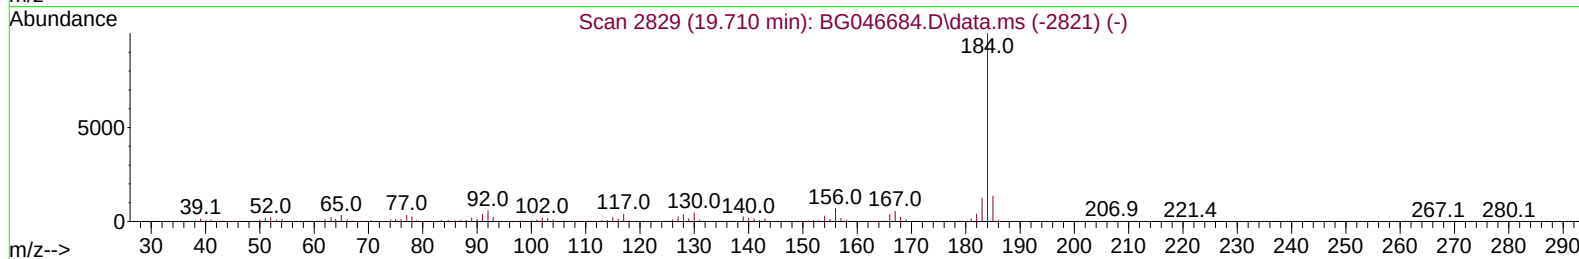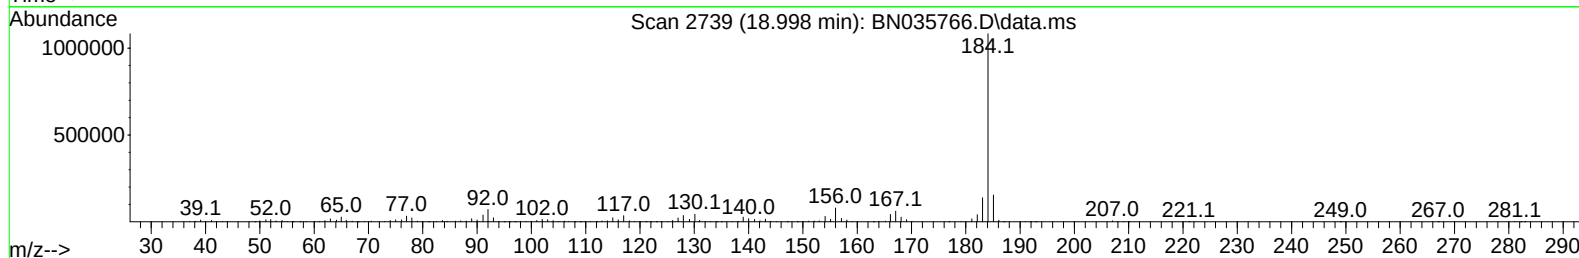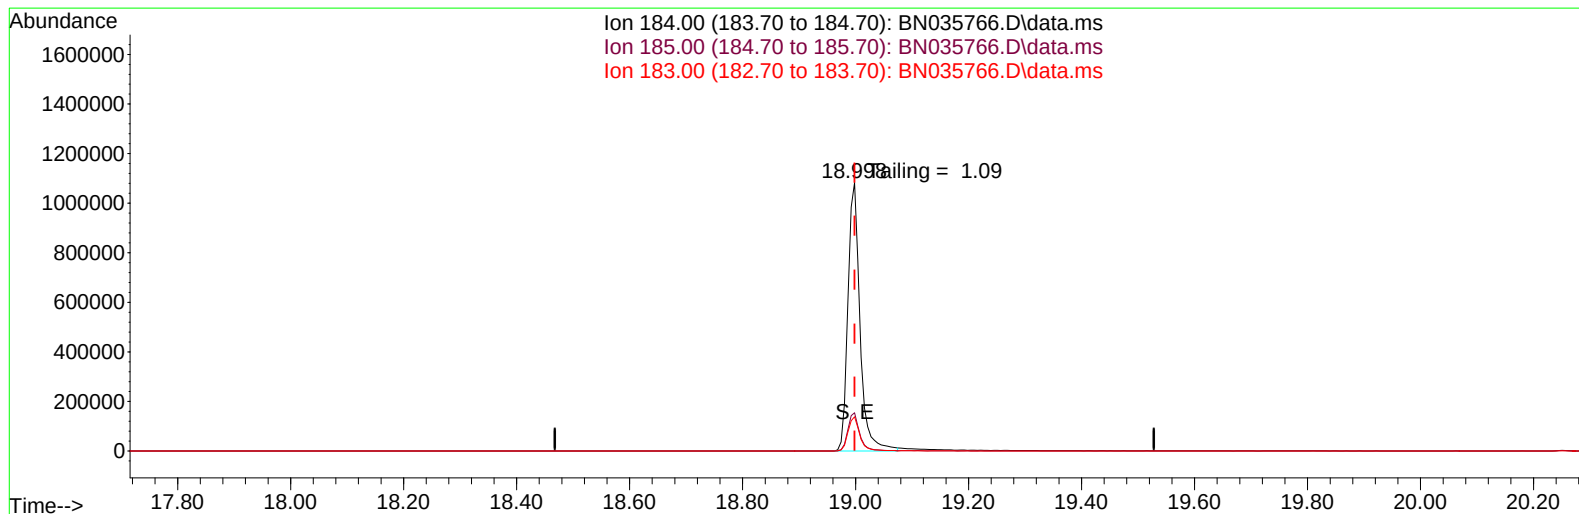

TIC: BN035766.D\data.ms

(77) Benzidine

18.998min (0.000) 0.00 ng

response 1653686

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.25
183.00	13.20	12.75
0.00	0.00	0.00