
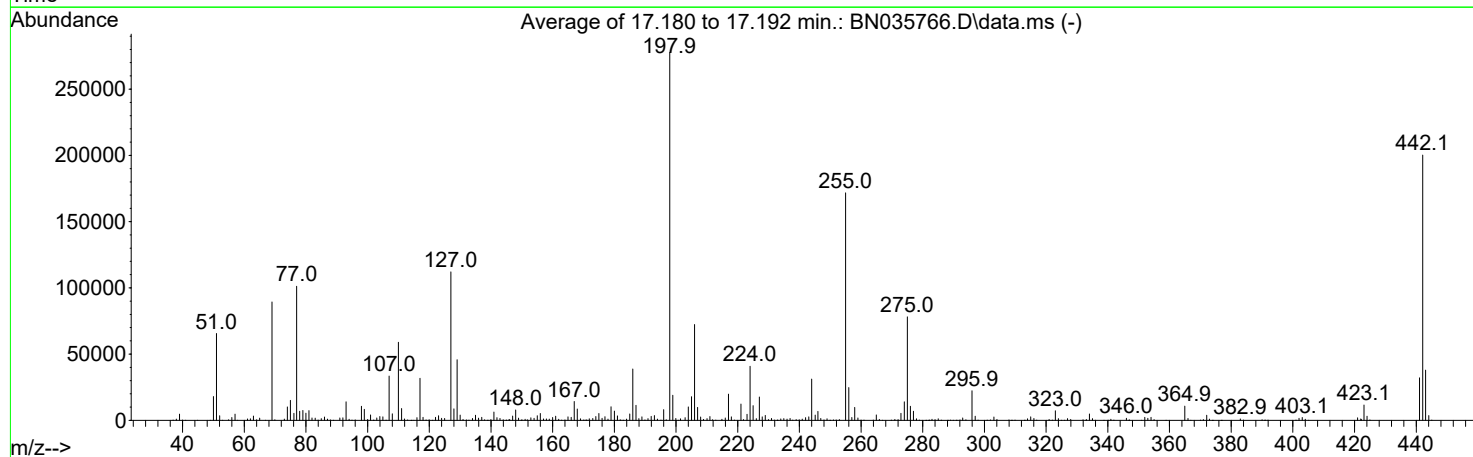


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121924\
Data File : BN035766.D
Acq On : 21 Dec 2024 05:46
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN112724.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Dec 19 23:06:19 2024

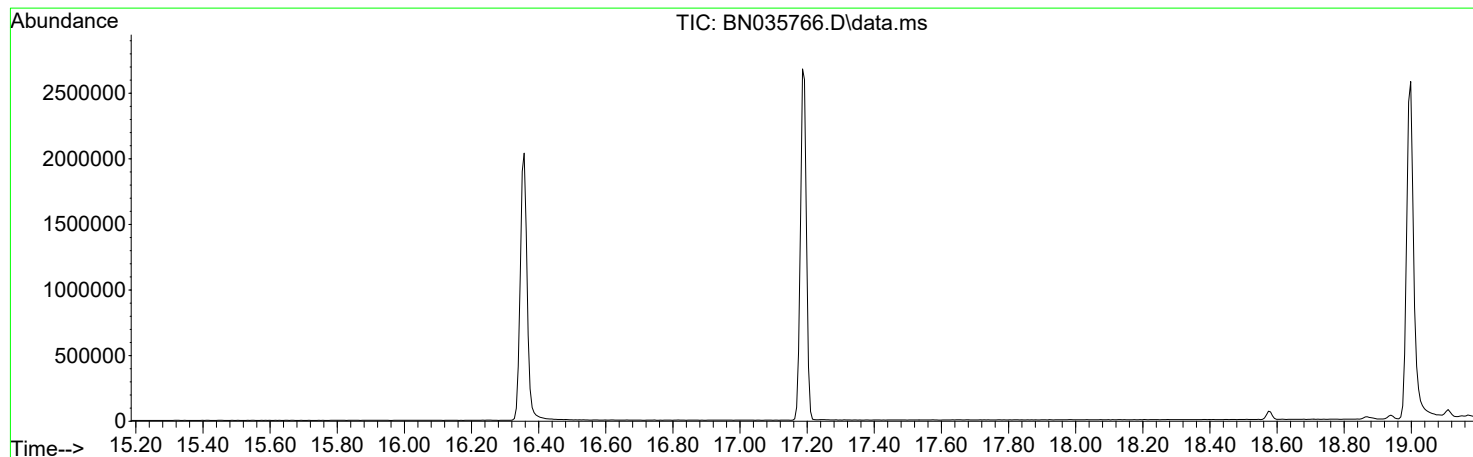

AutoFind: Scans 2430, 2431, 2432; Background Corrected with Scan 2424

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.6	65568	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	32.2	89411	PASS
70	69	0.00	2	0.5	449	PASS
127	198	10	80	40.4	112067	PASS
197	198	0.00	2	0.2	502	PASS
198	198	100	100	100.0	277653	PASS
199	198	5	9	6.8	18975	PASS
275	198	10	60	28.1	78101	PASS
365	198	1	100	3.9	10706	PASS
441	198	0.01	100	11.6	32087	PASS
442	442	50	100	100.0	200197	PASS
443	442	15	24	19.0	37976	PASS

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/19/2024	BNA_N	<u>BN035766.D</u>
Compound Name	Response	Retention Time
DDT	636526	20.251
DDD	227650	19.81
DDE	3673	19.292
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
231323	867849	26.65

Instrument :
BNA_N
ClientSampleId :
DFTPP