
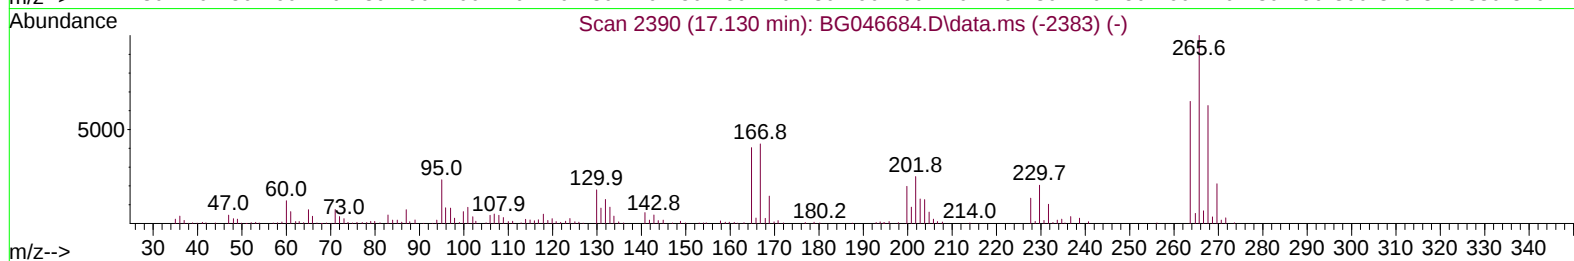
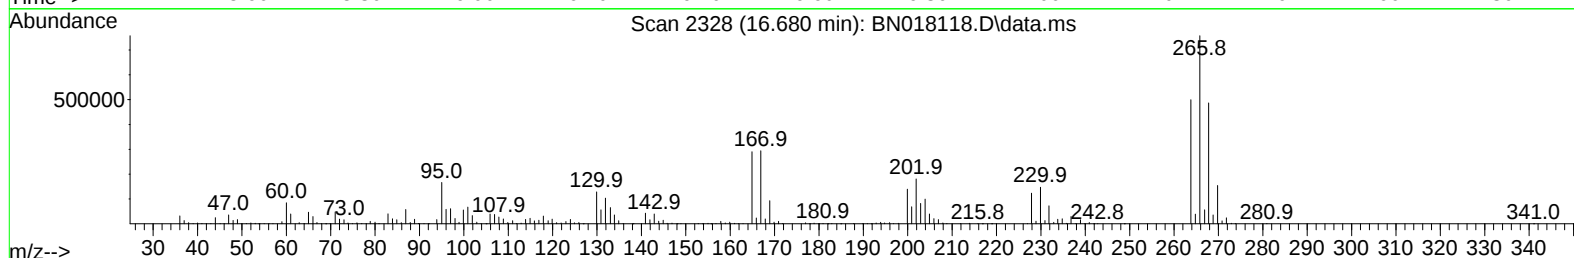


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122021\
Data File : BN018118.D
Acq On : 20 Dec 2021 12:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 20 15:03:46 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 20 15:03:29 2021
Response via : Initial Calibration

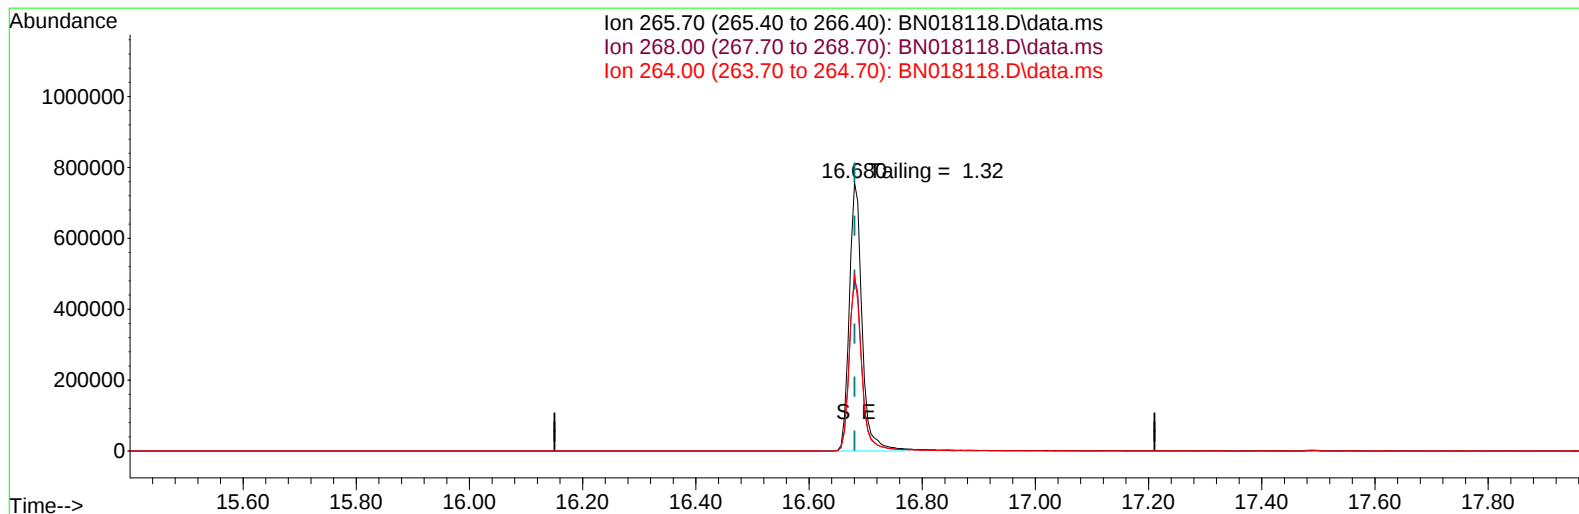

TIC: BN018118.D\data.ms

(70) Pentachlorophenol (C)




16.680min (0.000) 31204.74 ng

response 1197497

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.30
264.00	61.60	65.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122021\
Data File : BN018118.D
Acq On : 20 Dec 2021 12:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 20 15:03:46 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 20 15:03:29 2021
Response via : Initial Calibration

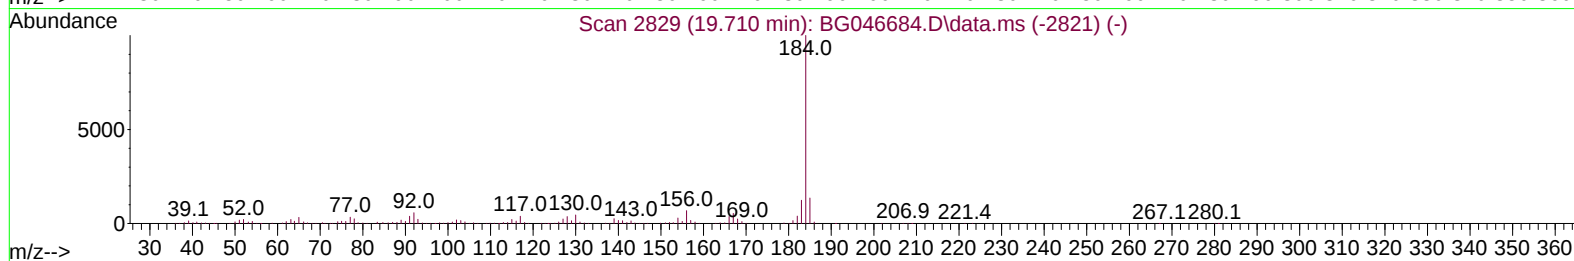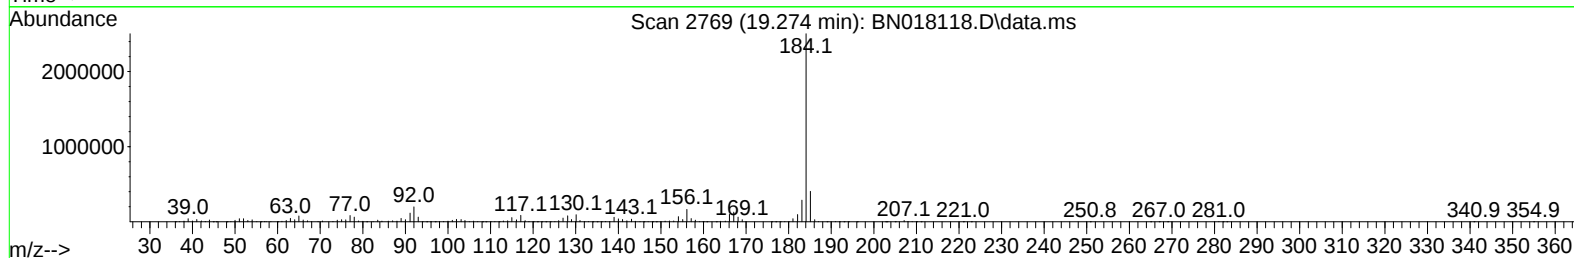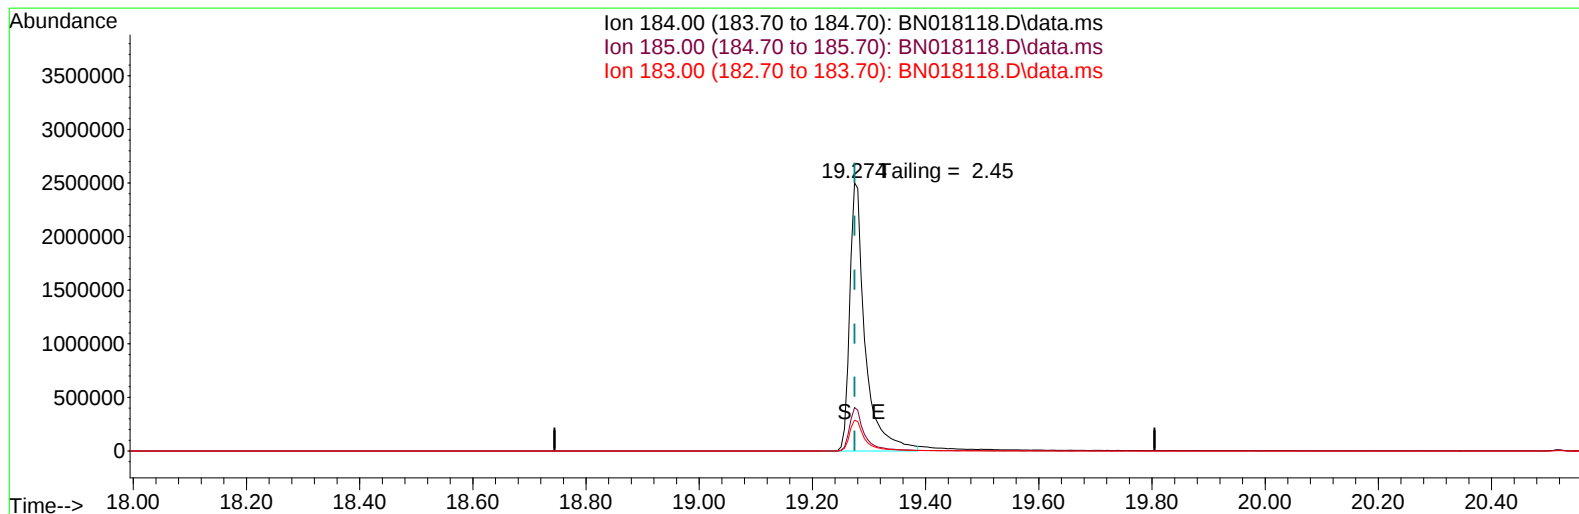

TIC: BN018118.D\data.ms

(77) Benzidine**19.274min (0.000) 1430075.91 ng****response 4893171**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	16.22
183.00	13.20	11.50
0.00	0.00	0.00