
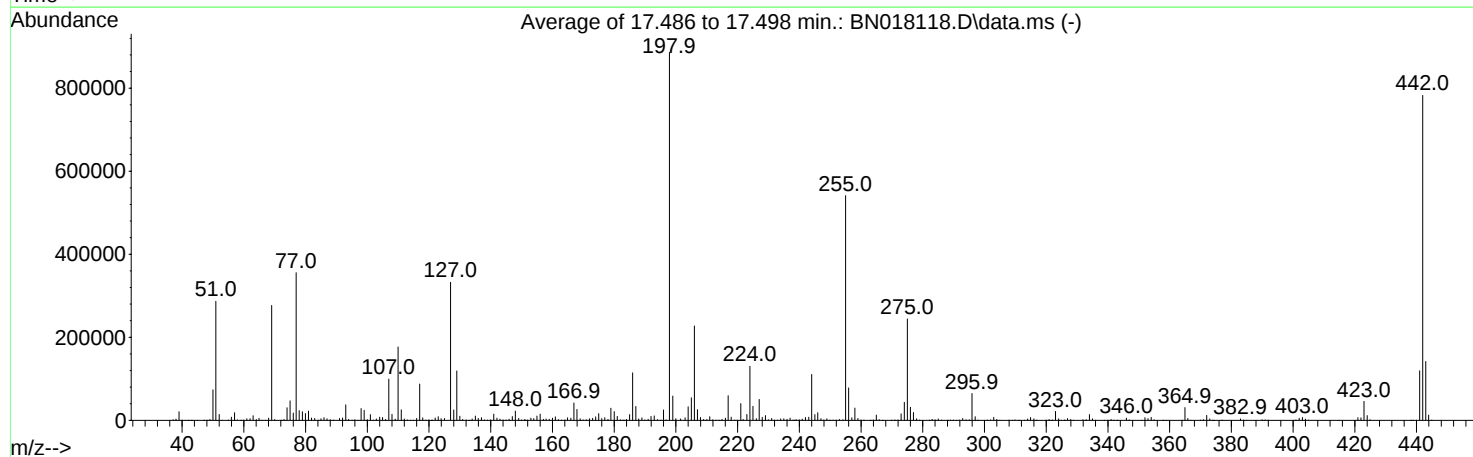


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122021\
 Data File : BN018118.D
 Acq On : 20 Dec 2021 12:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN121421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Dec 20 14:16:44 2021

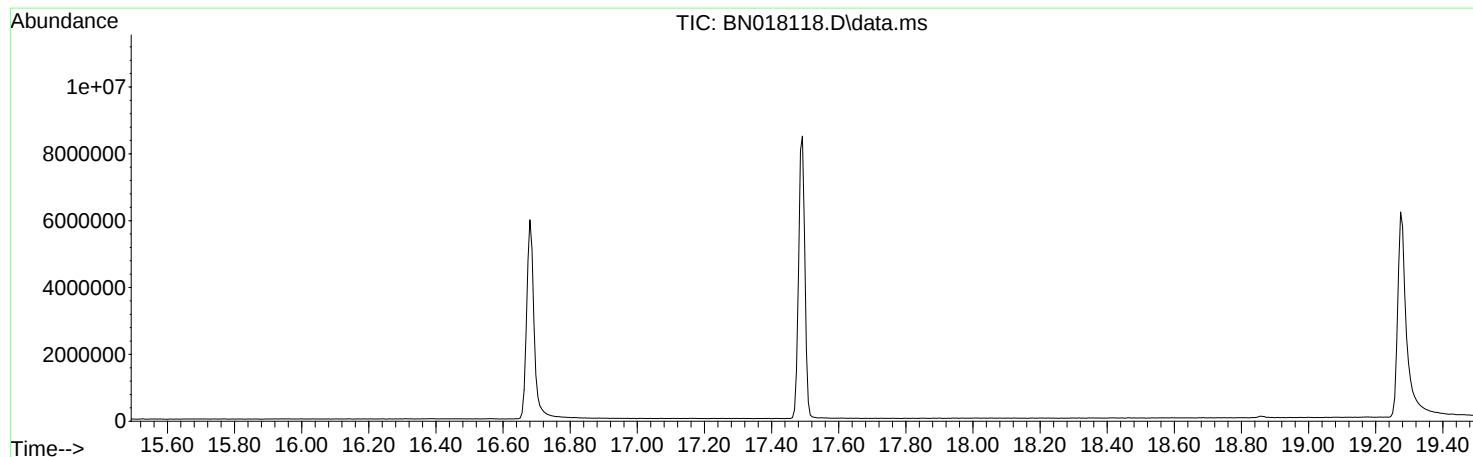

AutoFind: Scans 2465, 2466, 2467; Background Corrected with Scan 2458

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.4	286886	PASS
68	69	0.00	2	1.9	5254	PASS
69	198	0.00	100	31.2	276827	PASS
70	69	0.00	2	0.7	1881	PASS
127	198	10	80	37.5	332608	PASS
197	198	0.00	2	0.1	1082	PASS
198	198	100	100	100.0	885952	PASS
199	198	5	9	6.6	58461	PASS
275	198	10	60	27.6	244352	PASS
365	198	1	100	3.5	30864	PASS
441	198	0.01	100	13.5	119603	PASS
442	442	50	100	100.0	782763	PASS
443	442	15	24	18.1	141923	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
12/20/2021	BNA_N	<u>BN018118.D</u>
Compound Name	Response	Retention Time
DDT	2882158	20.51
DDD	54020	20.08
DDE	4145	19.57
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
58165	2940323	1.98

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122021\
 Data File : BN018118.D
 Acq On : 20 Dec 2021 12:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Dec 20 15:03:46 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 20 15:03:29 2021
 Response via : Initial Calibration

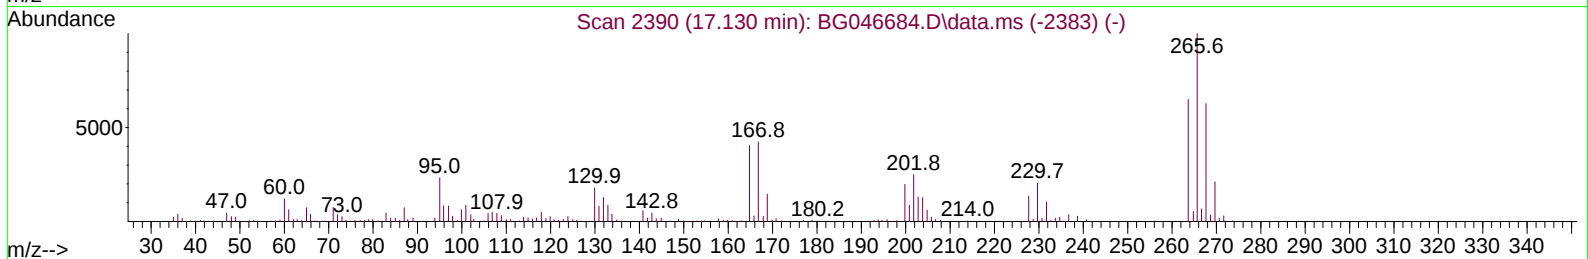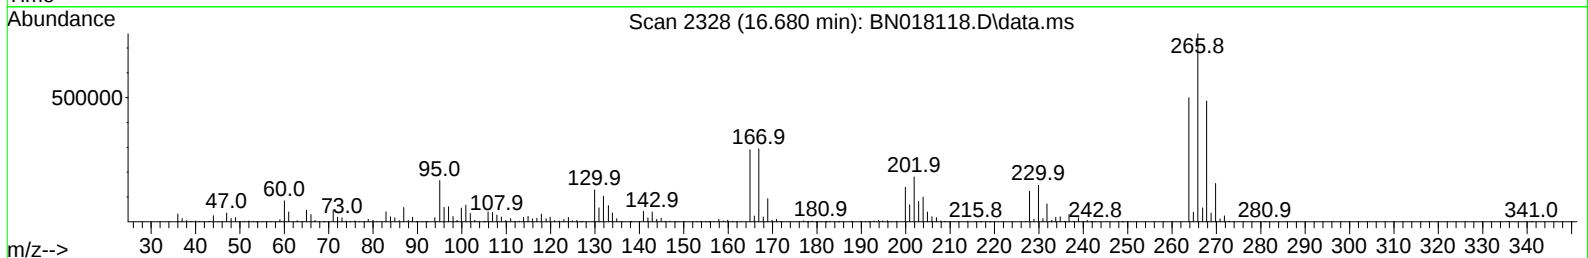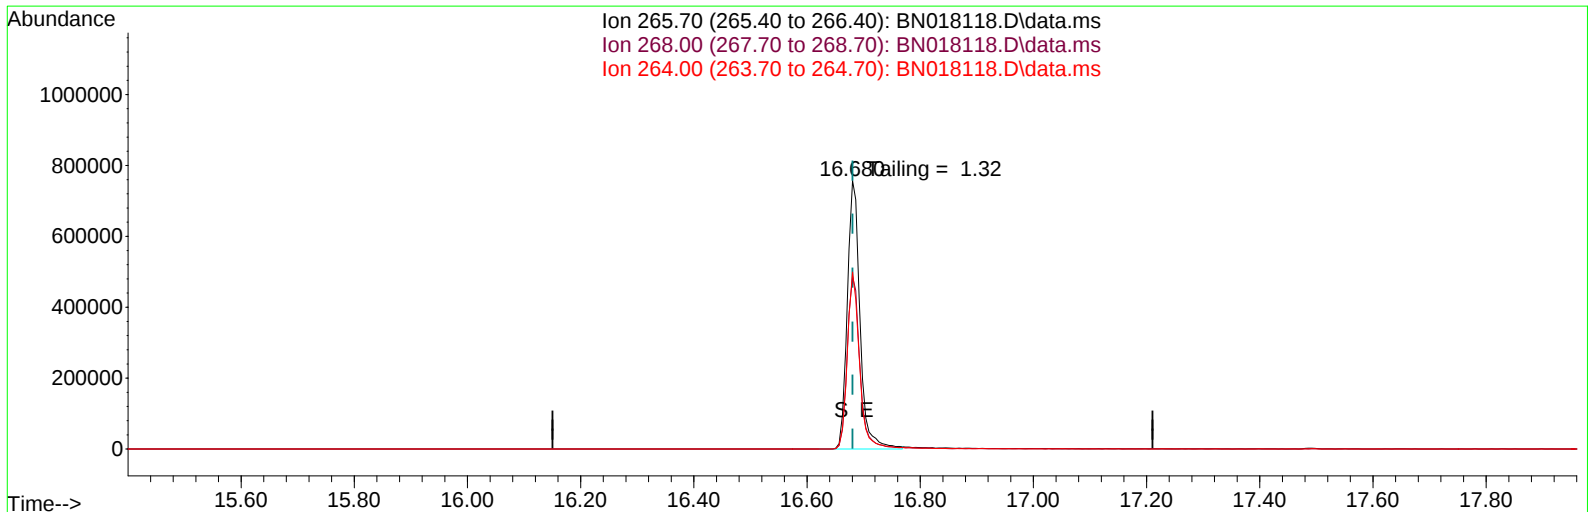

TIC: BN018118.D\data.ms

(70) Pentachlorophenol (C)

16.680min (0.000) 31204.74 ng




response 1197497

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.30
264.00	61.60	65.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122021\
Data File : BN018118.D
Acq On : 20 Dec 2021 12:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 20 15:03:46 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 20 15:03:29 2021
Response via : Initial Calibration

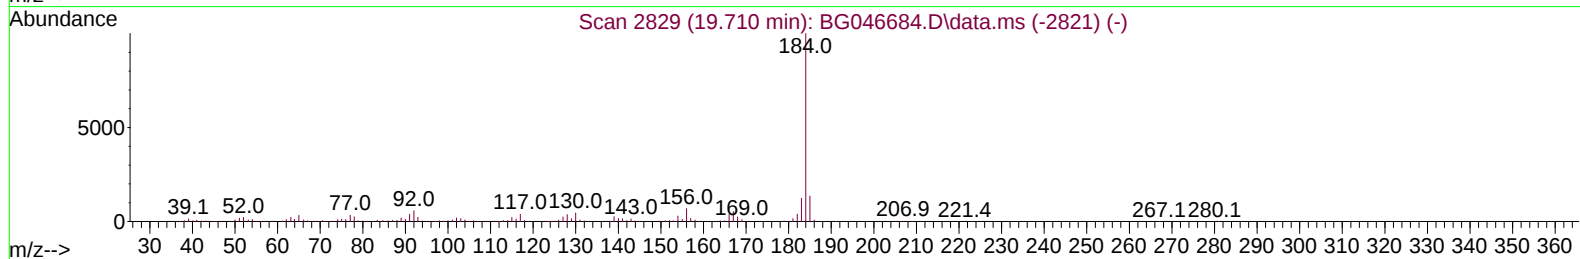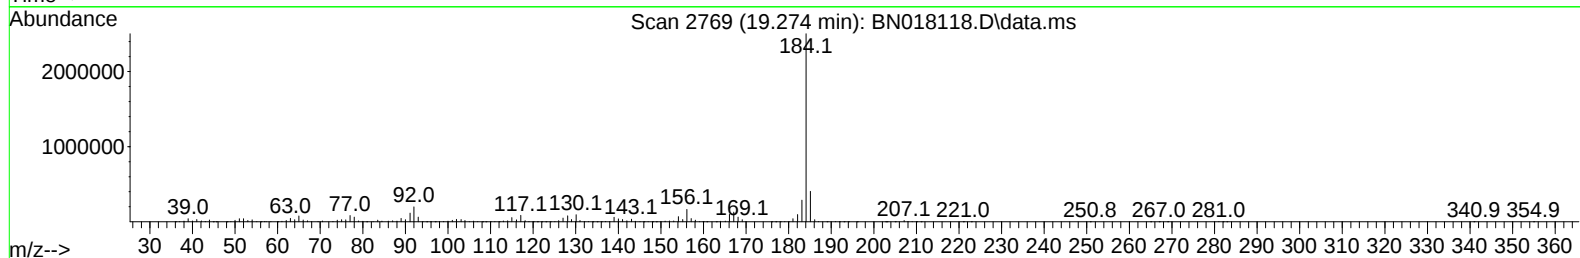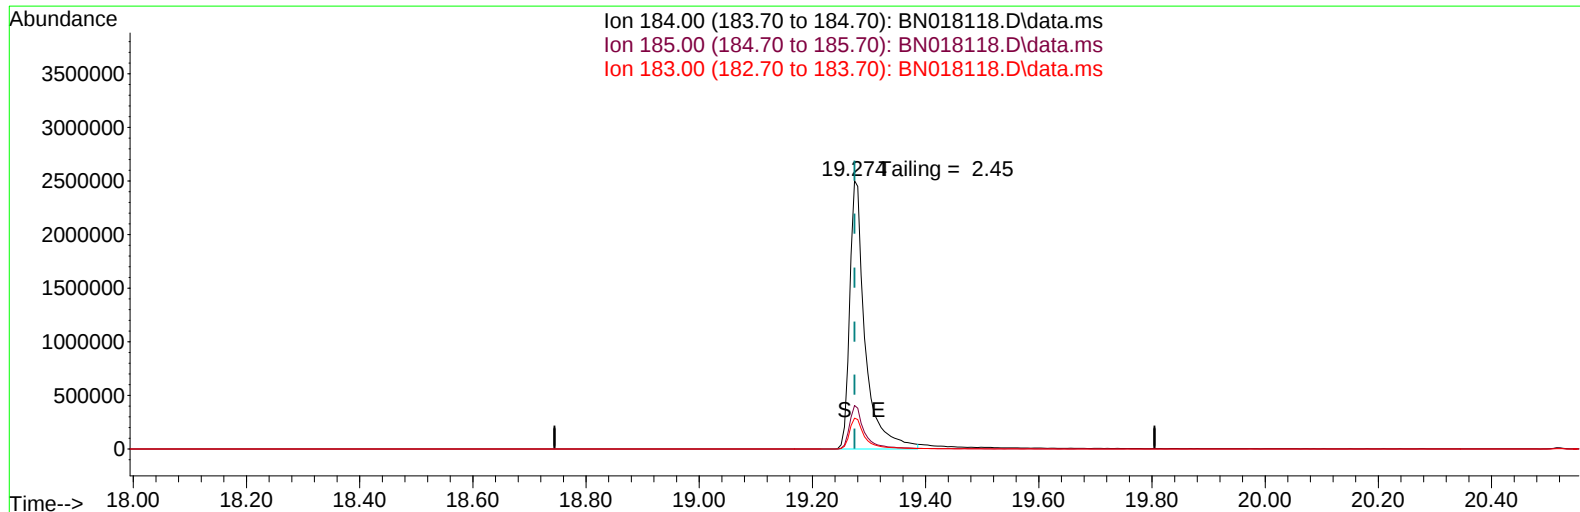

TIC: BN018118.D\data.ms

(77) Benzidine

19.274min (0.000) 1430075.91 ng

response 4893171

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	16.22
183.00	13.20	11.50
0.00	0.00	0.00