

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122022\
 Data File : BN023291.D
 Acq On : 20 Dec 2022 10:08
 Operator : CG/JU
 Sample : PB149667BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK667

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN121522.M
 Title : SVOA CALIBRATION

Signal : TIC: BN023291.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.340	39	43	52	rVB	62828	94826	1.21%	0.121%
2	3.769	113	116	142	rBV	897603	1425248	18.13%	1.814%
3	4.111	170	174	182	rVB	18643	30035	0.38%	0.038%
4	7.152	684	691	710	rVB	1218275	1880296	23.92%	2.394%
5	7.322	713	720	731	rVB	992384	1465462	18.64%	1.866%
6	7.522	747	754	767	rBV	1240173	1895245	24.11%	2.413%
7	7.999	826	835	845	rVB	1038546	1631150	20.75%	2.077%
8	8.710	949	956	972	rBV	1550842	2414134	30.71%	3.073%
9	9.169	1025	1034	1042	rBV	1138961	1880330	23.92%	2.394%
10	9.893	1149	1157	1173	rBV	1008732	1582997	20.13%	2.015%
11	10.434	1240	1249	1258	rBV	1583770	2568865	32.67%	3.270%
12	10.816	1306	1314	1324	rVB	1564562	2598136	33.05%	3.308%
13	10.951	1330	1337	1352	rBV	1609548	2712310	34.50%	3.453%
14	12.404	1578	1584	1593	rVB2	28129	48905	0.62%	0.062%
15	14.057	1858	1865	1875	rBV	2834299	3771093	47.97%	4.801%
16	14.339	1906	1913	1923	rBV	3279270	4703115	59.82%	5.987%
17	14.645	1958	1965	1974	rBV	2546080	3694774	47.00%	4.704%
18	14.839	1991	1998	2017	rBV	1390473	1994087	25.36%	2.539%
19	15.057	2030	2035	2038	rVB7	6511	10689	0.14%	0.014%
20	15.639	2127	2134	2147	rBV	4126552	5875067	74.73%	7.479%
21	15.751	2147	2153	2166	rVV	1227906	1618177	20.58%	2.060%
22	15.875	2170	2174	2180	rVB2	20659	30483	0.39%	0.039%
23	16.416	2262	2266	2275	rVB9	5003	7872	0.10%	0.010%
24	17.392	2425	2432	2439	rBV	3350315	4584351	58.31%	5.836%
25	17.492	2442	2449	2474	rVB	4835295	6640814	84.47%	8.454%
26	17.775	2493	2497	2500	rBV3	4829	8863	0.11%	0.011%
27	19.345	2760	2764	2770	rBV	58356	84897	1.08%	0.108%
28	19.416	2772	2776	2782	rVV	55769	75070	0.95%	0.096%
29	19.786	2833	2839	2849	rBV	6046637	7862054	100.00%	10.009%
30	21.574	3138	3143	3150	rBV	3501815	4714236	59.96%	6.002%
31	23.868	3526	3533	3551	rVB2	3262442	6538588	83.17%	8.324%
32	24.027	3553	3560	3573	rVB2	2041994	4108529	52.26%	5.230%




Sum of corrected areas: 78550698

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122022\
Data File : BN023291.D
Acq On : 20 Dec 2022 10:08
Operator : CG/JU
Sample : PB149667BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK667

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN121522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

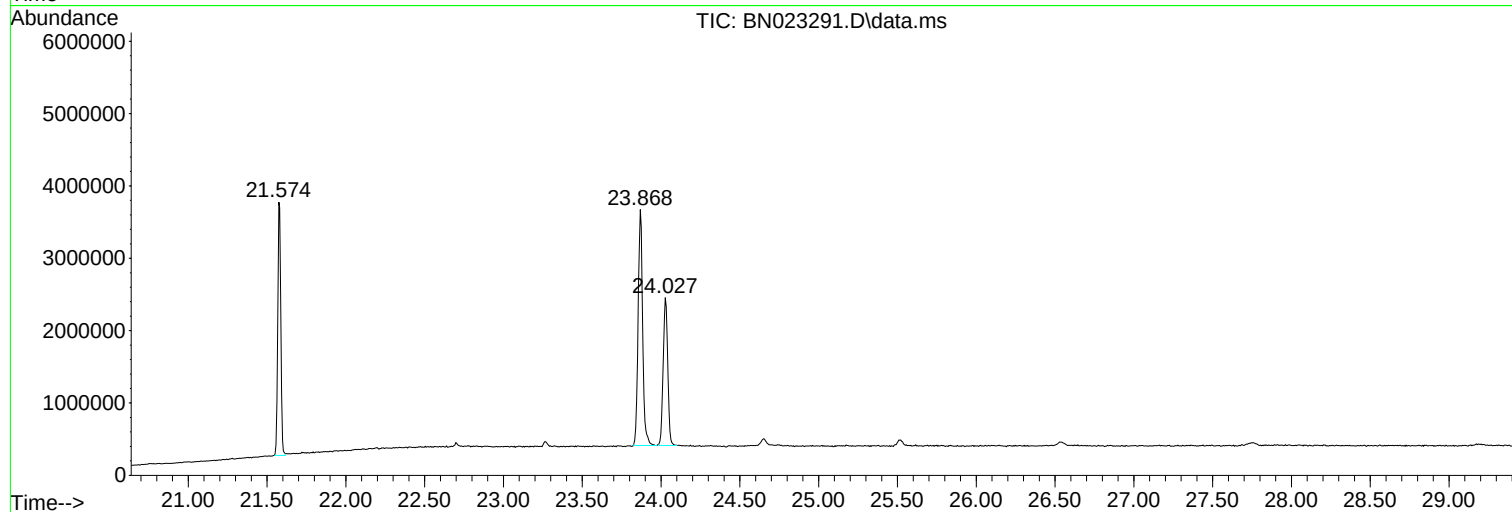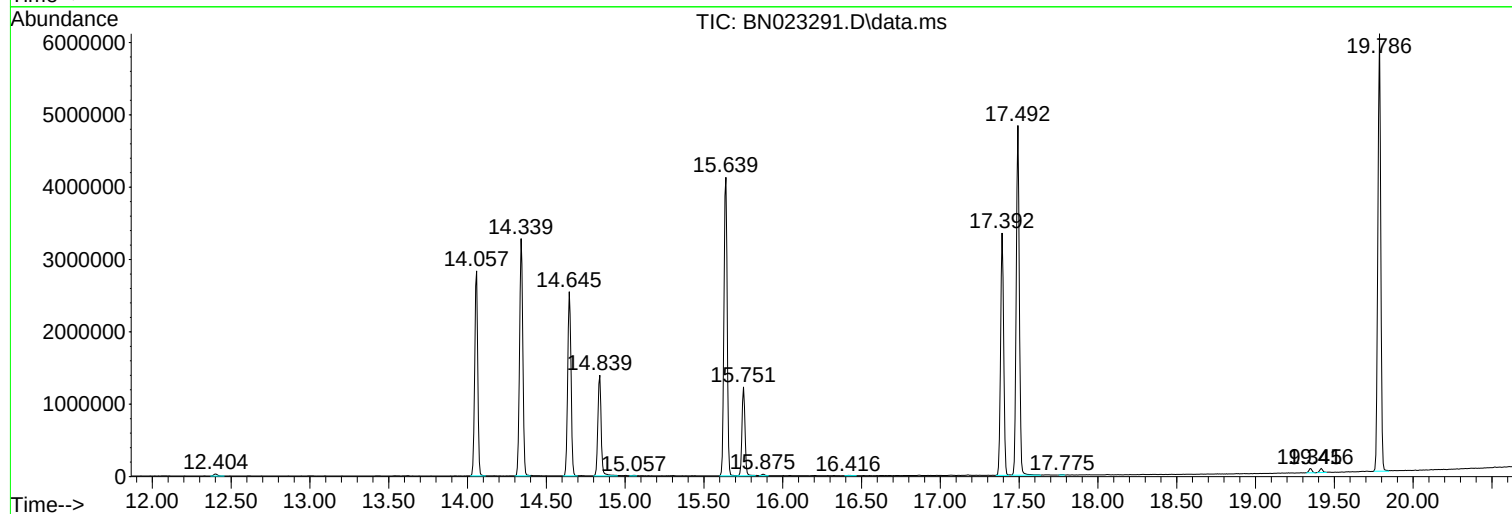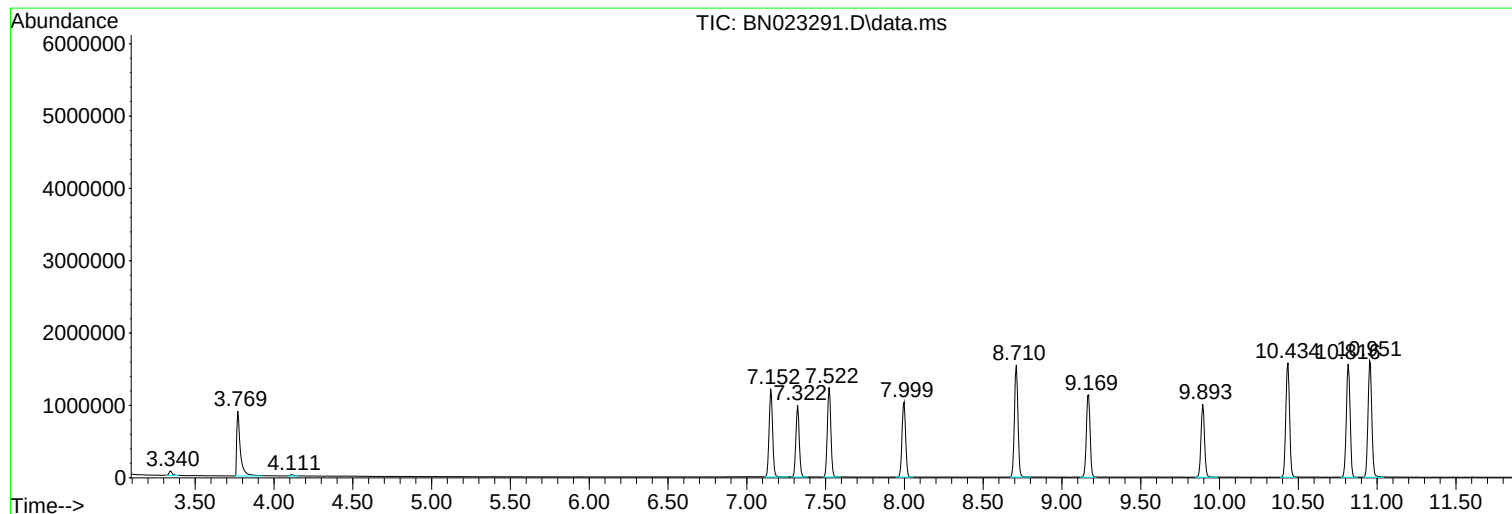

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122022\
Data File : BN023291.D
Acq On : 20 Dec 2022 10:08
Operator : CG/JU
Sample : PB149667BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK667

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN121522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122022\
Data File : BN023291.D
Acq On : 20 Dec 2022 10:08
Operator : CG/JU
Sample : PB149667BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK667

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN121522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc