
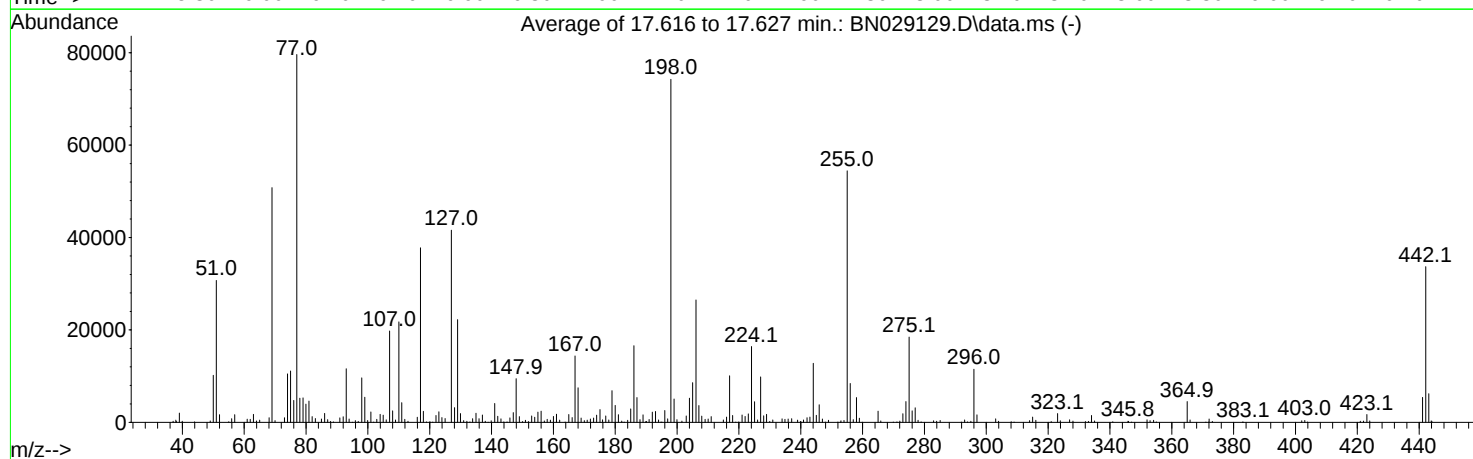


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122023\
Data File : BN029129.D
Acq On : 20 Dec 2023 11:49
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN122023.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Dec 20 18:03:30 2023

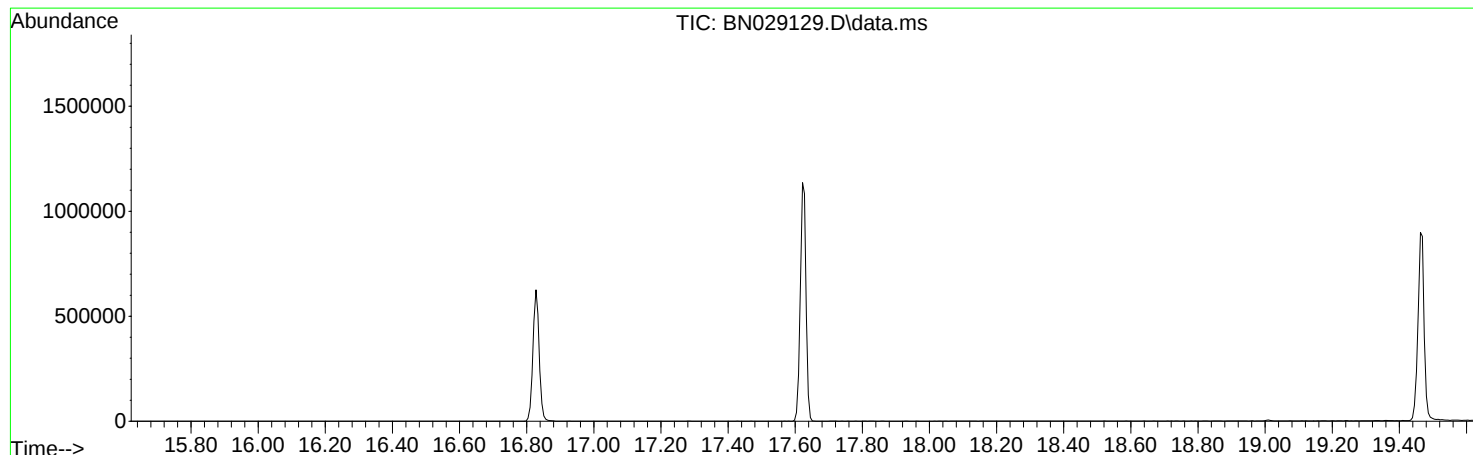




AutoFind: Scans 2470, 2471, 2472; Background Corrected with Scan 2464

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.4	30723	PASS
68	69	0.00	2	1.9	988	PASS
69	198	0.00	100	68.4	50813	PASS
70	69	0.00	2	0.7	369	PASS
127	198	10	80	56.0	41579	PASS
197	198	0.00	2	1.0	779	PASS
198	198	100	100	100.0	74253	PASS
199	198	5	9	6.8	5048	PASS
275	198	10	60	24.9	18466	PASS
365	198	1	100	6.1	4521	PASS
441	198	0.01	100	7.3	5409	PASS
442	442	50	100	100.0	33700	PASS
443	442	15	24	18.5	6218	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122023\
Data File : BN029129.D
Acq On : 20 Dec 2023 11:49
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 21 03:43:58 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 01 23:28:24 2023
Response via : Initial Calibration

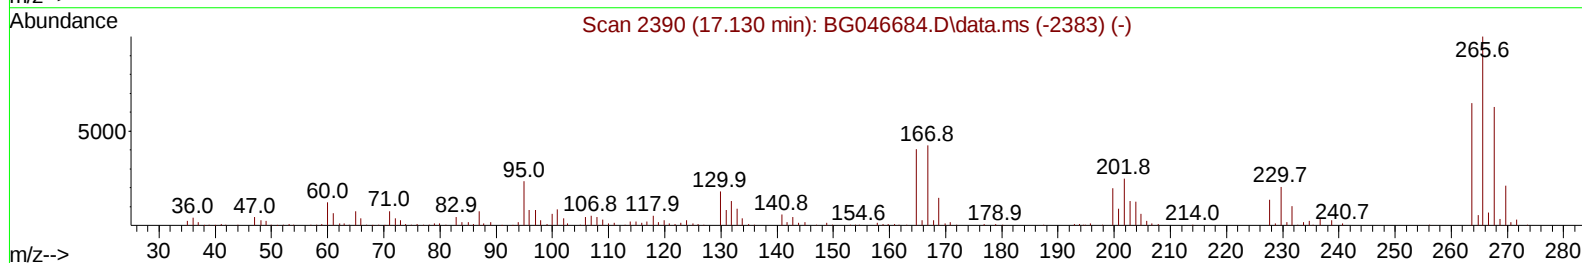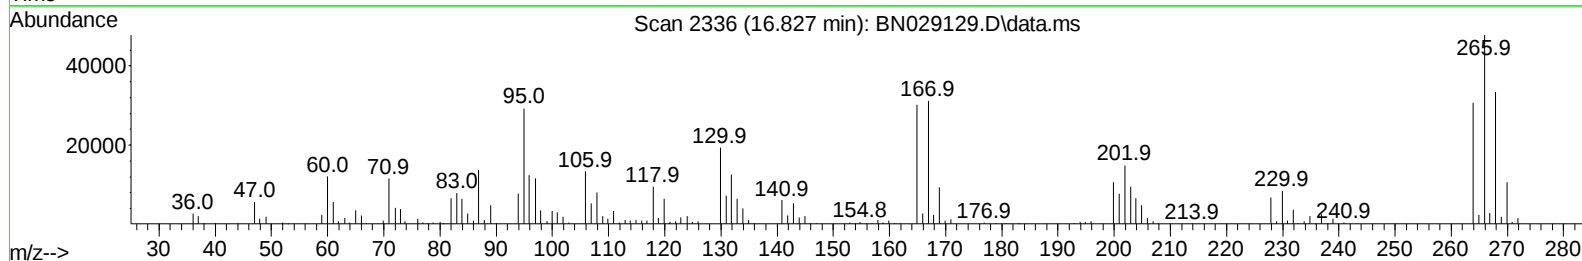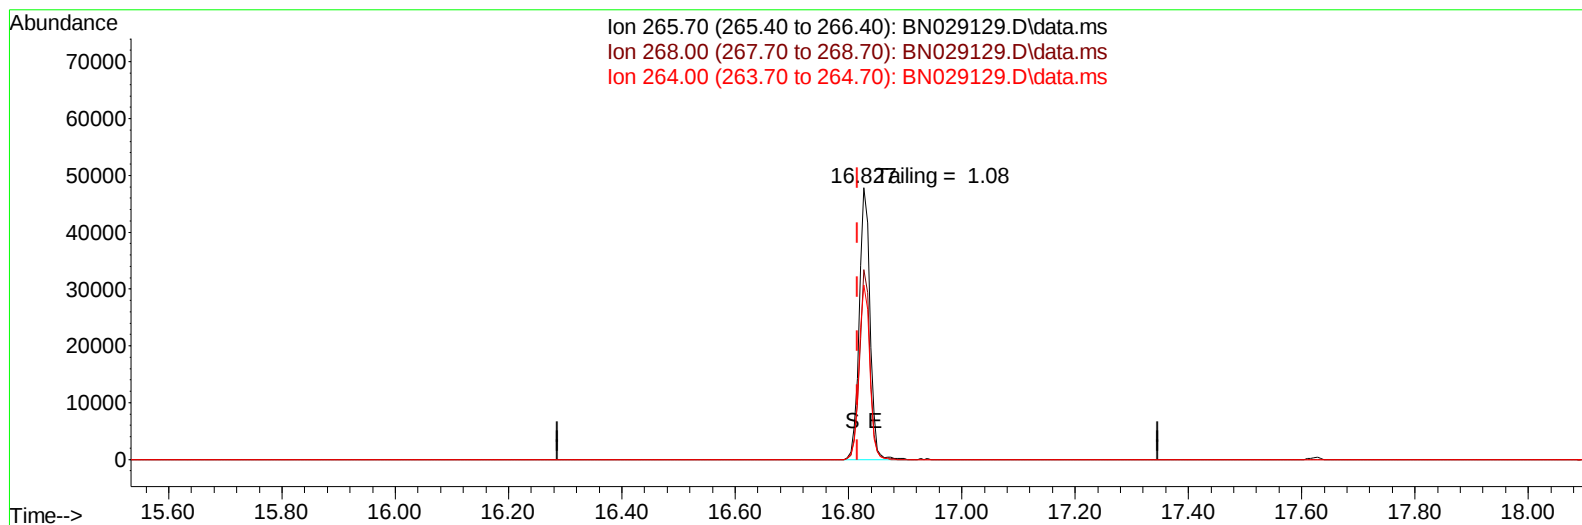

TIC: BN029129.D\data.ms

(70) Pentachlorophenol (C)

16.827min (+ 0.011) 9631.67 ng




response 62586

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	69.94
264.00	61.60	64.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122023\
Data File : BN029129.D
Acq On : 20 Dec 2023 11:49
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 21 03:43:58 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 01 23:28:24 2023
Response via : Initial Calibration

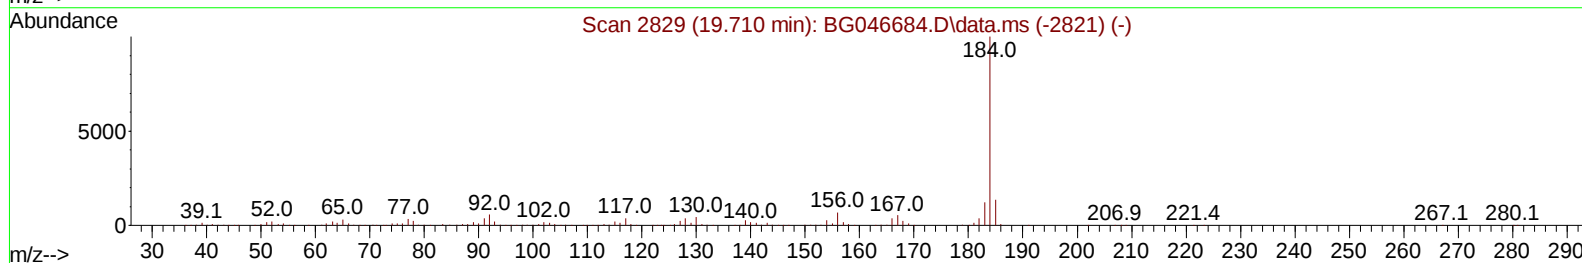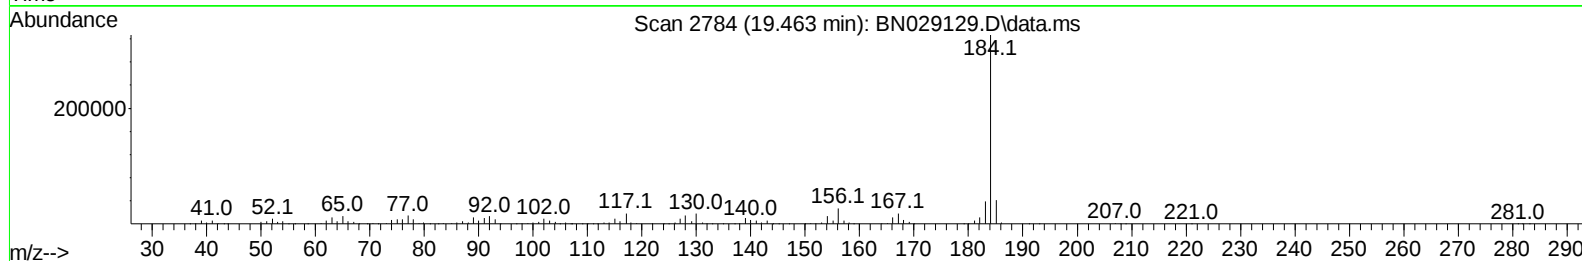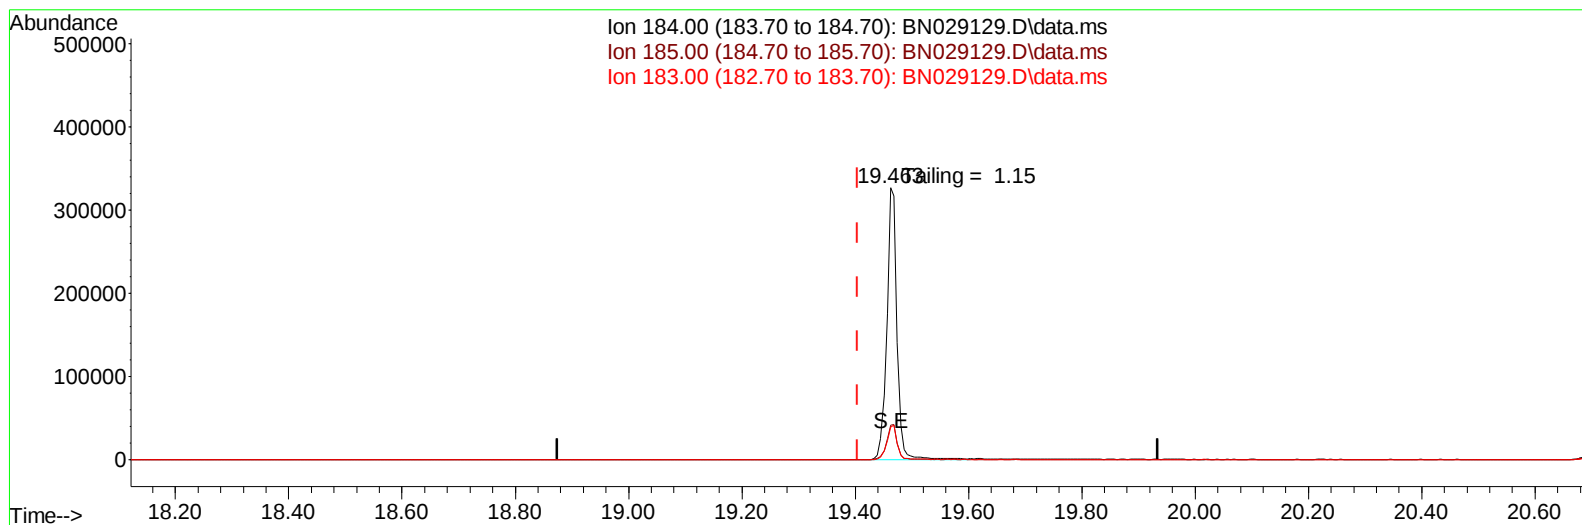

TIC: BN029129.D\data.ms

(77) Benzidine

19.463min (+ 0.059) 0.00 ng

response 408255

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	12.62
183.00	13.20	11.86
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/20/2023	BNA_N	<u>BN029129.D</u>
Compound Name	Response	Retention Time
DDT	220603	20.686
DDD	5693	20.245
DDE	337	19.733
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6030	226633	2.66

Instrument :
BNA_N
ClientSampleId :
DFTPP