

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122122\
 Data File : BN023313.D
 Acq On : 21 Dec 2022 14:00
 Operator : CG/JU
 Sample : PB149668BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Dec 22 03:20:25 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 22 02:28:40 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.994	152	8970	0.400	ng/ul	0.00
4) Naphthalene-d8	10.815	136	28654	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.645	164	16455	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.390	188	37139	0.400	ng/ul	0.00
17) Chrysene-d12	21.581	240	25919	0.400	ng/ul	0.00
23) Perylene-d12	24.030	264	20642	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.345	96	53379	5.477	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.399	152	12519	0.282	ng/ul	0.00
18) Fluoranthene-d10	19.420	212	27774	0.296	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.787	202	4842	0.038	ng/ul#	1
26) Benzo(a)pyrene	23.873	252	6383	0.076	ng/ul#	64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122122\
Data File : BN023313.D
Acq On : 21 Dec 2022 14:00
Operator : CG/JU
Sample : PB149668BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :


Quant Time: Dec 22 03:20:25 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 22 02:28:40 2022
Response via : Initial Calibration

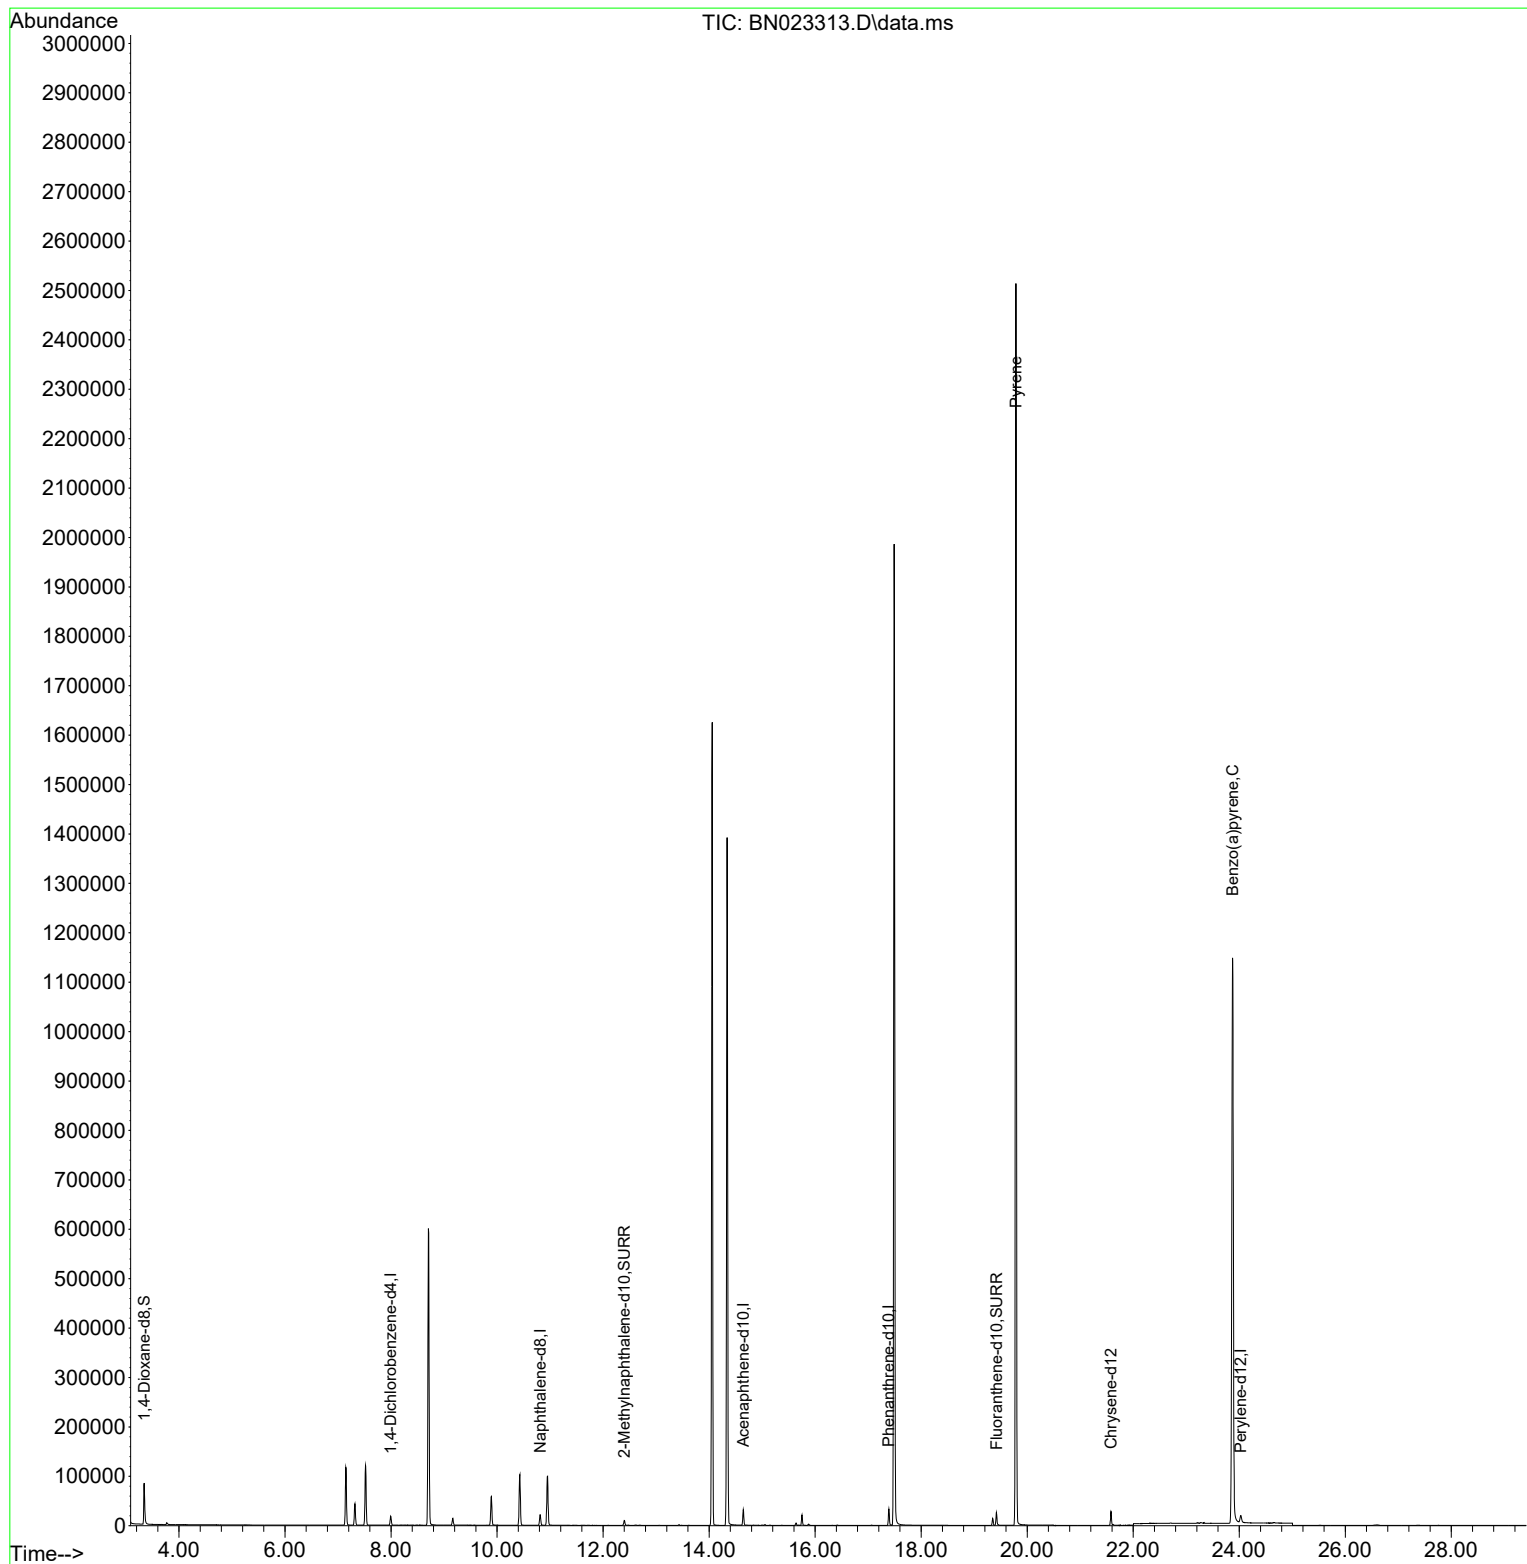



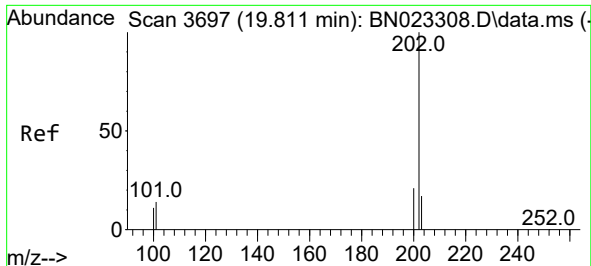


#20
Pyrene
Concen: 0.038 ng/ul
RT: 19.787 min Scan# 30
Delta R.T. -0.024 min
Lab File: BN023313.D
Acq: 21 Dec 2022 14:00

Instrument :
BNA_N
ClientSampleId :

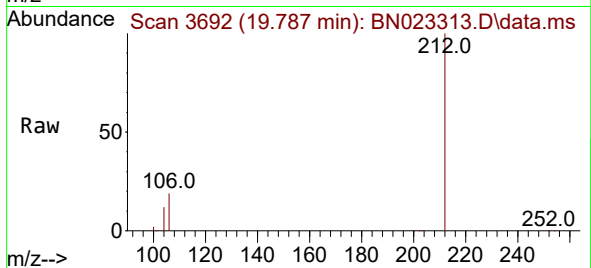

Tgt Ion:202 Resp: 4842
Ion Ratio Lower Upper
202 100
101 159.9 11.3 16.9#
100 1194.1 9.0 13.4#

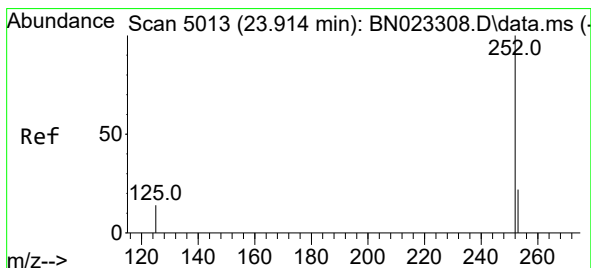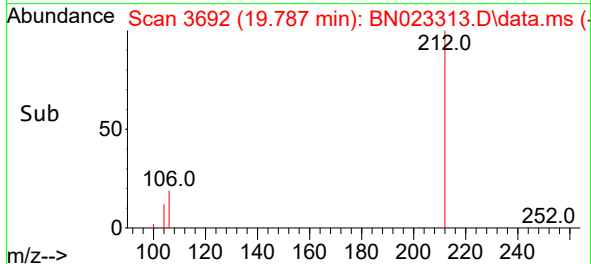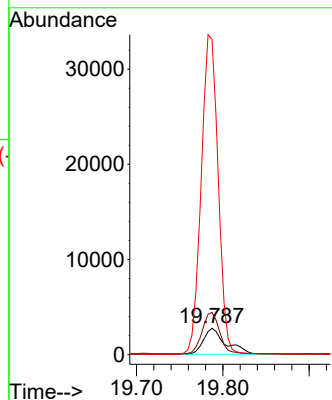

#26
Benzo(a)pyrene
Concen: 0.076 ng/ul
RT: 23.873 min Scan# 4999
Delta R.T. -0.042 min
Lab File: BN023313.D
Acq: 21 Dec 2022 14:00

Tgt Ion:252 Resp: 6383
Ion Ratio Lower Upper
252 100
253 43.1 21.4 32.2#
125 39.1 16.2 24.4#

