

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122122\
 Data File : BN023317.D
 Acq On : 21 Dec 2022 17:25
 Operator : CG/JU
 Sample : PB149668BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Dec 22 03:21:01 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 22 02:28:40 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.998	152	8205	0.400	ng/ul	0.00
4) Naphthalene-d8	10.815	136	25519	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.646	164	14803	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.391	188	34155	0.400	ng/ul	0.00
17) Chrysene-d12	21.578	240	24435	0.400	ng/ul	0.00
23) Perylene-d12	24.028	264	20929	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.348	96	50654	5.682	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.404	152	11495	0.291	ng/ul	0.00
18) Fluoranthene-d10	19.421	212	26276	0.297	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.640	166	3850	0.062	ng/ul#	13
20) Pyrene	19.788	202	3518	0.029	ng/ul#	1
26) Benzo(a)pyrene	23.870	252	6601	0.077	ng/ul#	64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122122\
Data File : BN023317.D
Acq On : 21 Dec 2022 17:25
Operator : CG/JU
Sample : PB149668BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :


Quant Time: Dec 22 03:21:01 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 22 02:28:40 2022
Response via : Initial Calibration

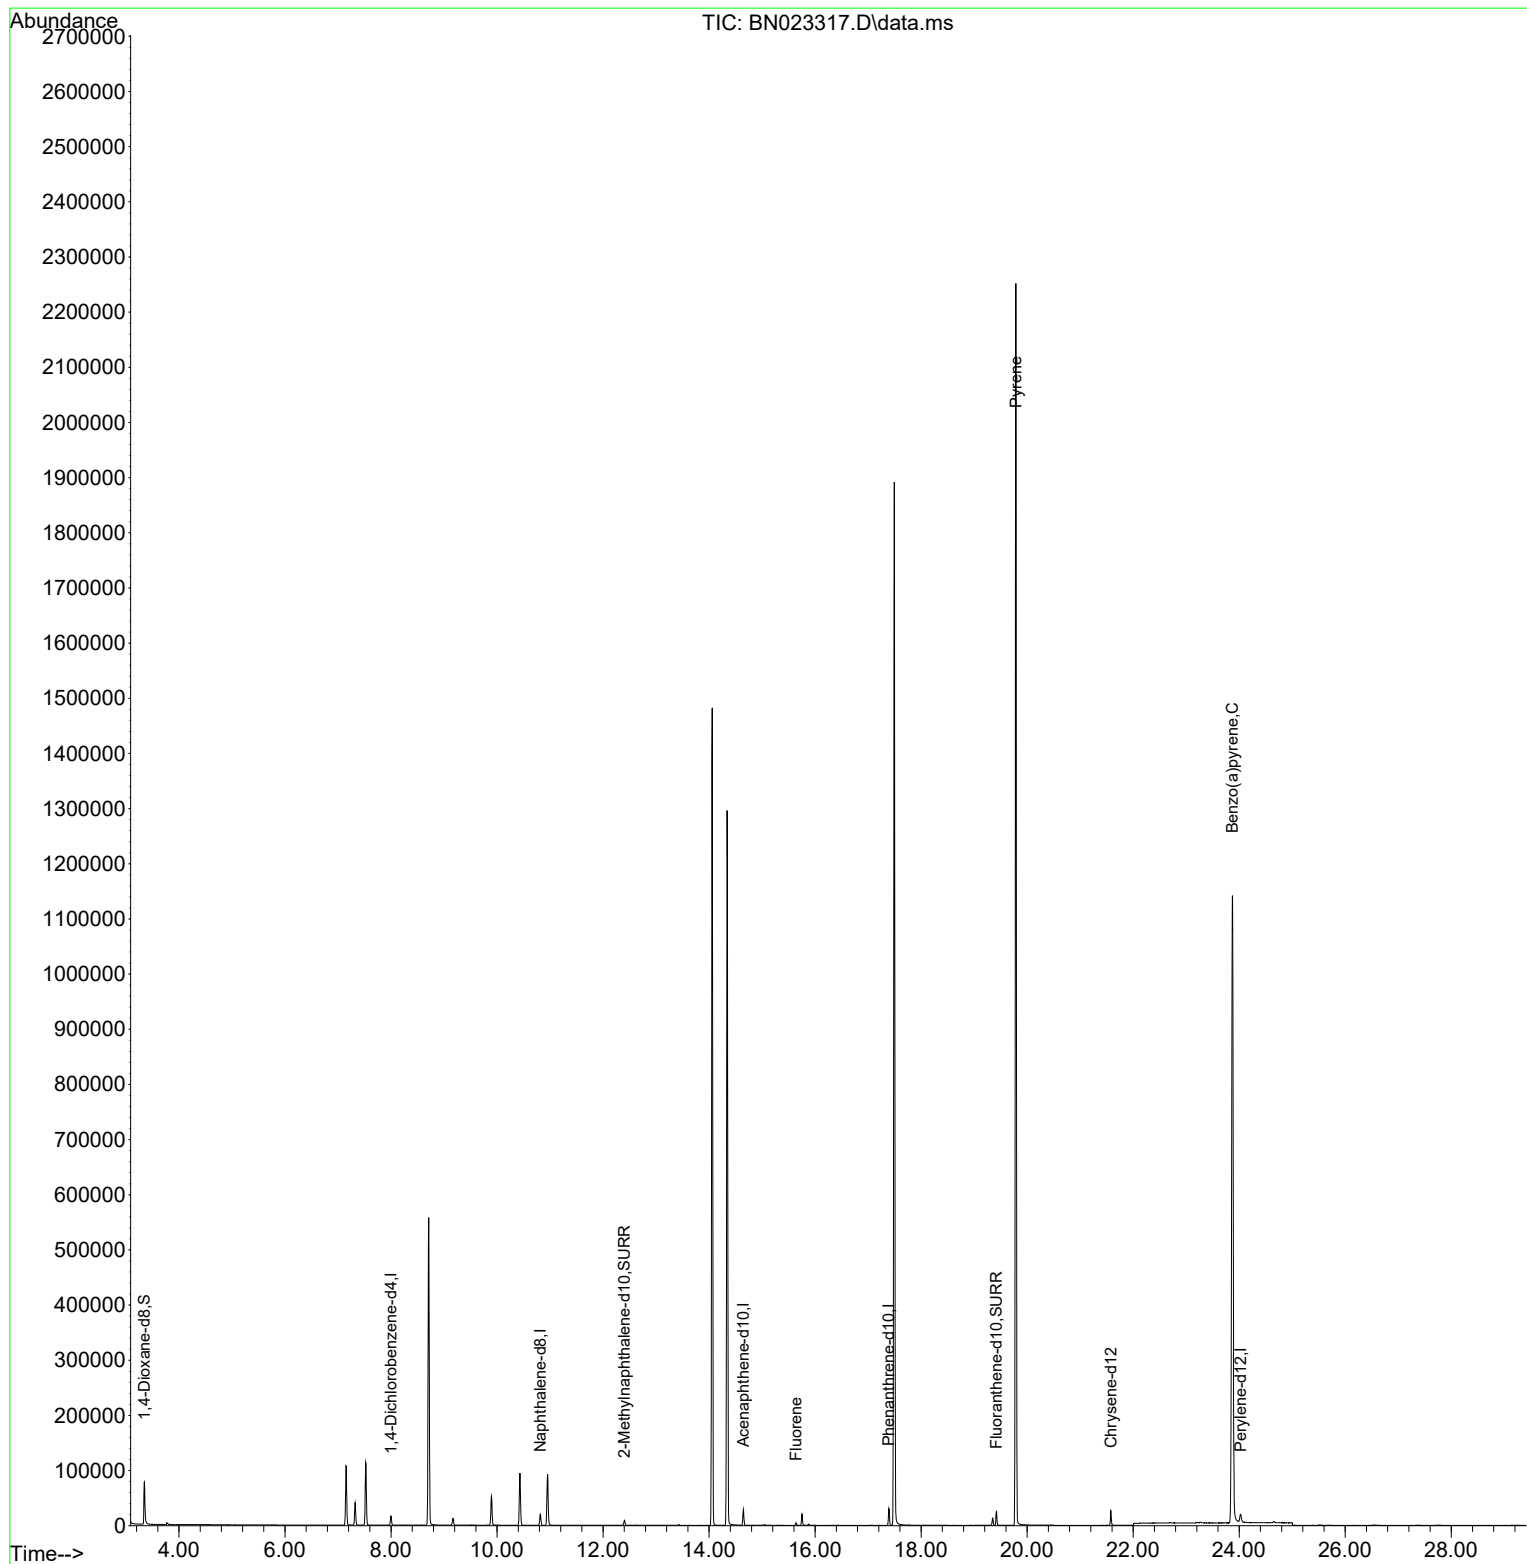



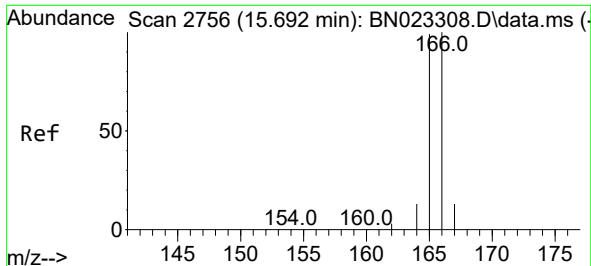


#12
Fluorene
Concen: 0.062 ng/ul
RT: 15.640 min Scan# 21
Delta R.T. -0.051 min
Lab File: BN023317.D
Acq: 21 Dec 2022 17:25

Instrument :
BNA_N
ClientSampleId :



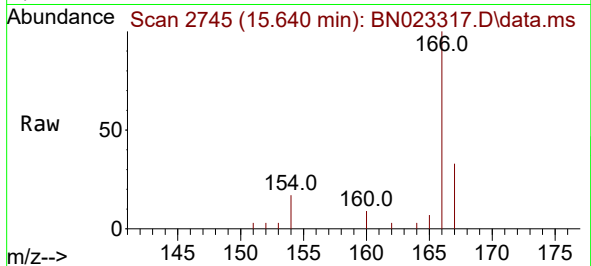



Tgt Ion:166 Resp: 3850
Ion Ratio Lower Upper
166 100
165 6.6 79.1 118.7#
167 32.8 11.0 16.4#

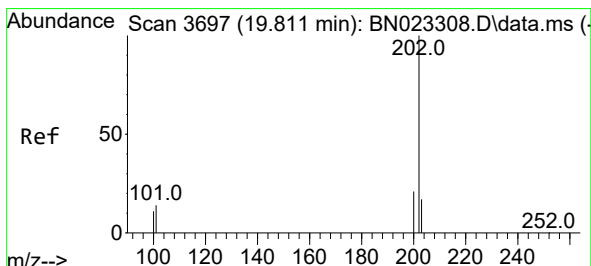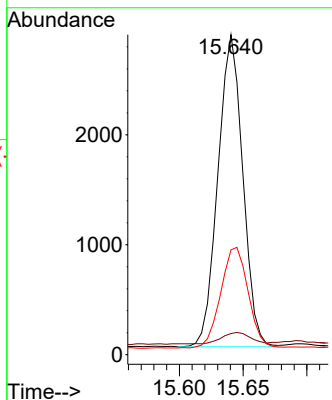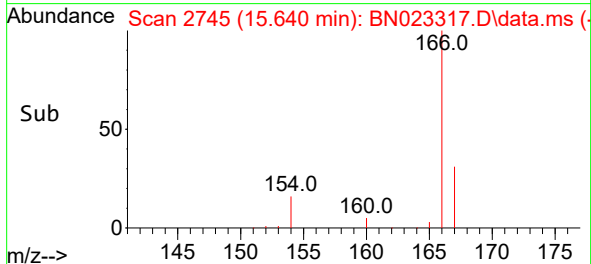

#20
Pyrene
Concen: 0.029 ng/ul
RT: 19.788 min Scan# 3692
Delta R.T. -0.023 min
Lab File: BN023317.D
Acq: 21 Dec 2022 17:25


Tgt Ion:202 Resp: 3518
Ion Ratio Lower Upper
202 100
101 157.1 11.3 16.9#
100 1133.2 9.0 13.4#

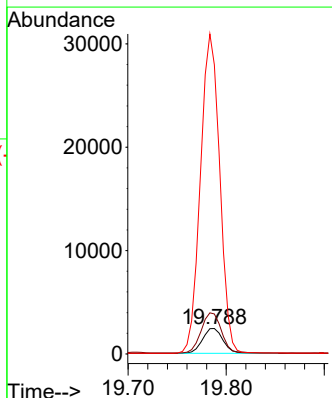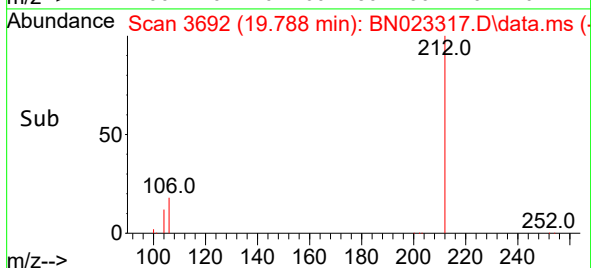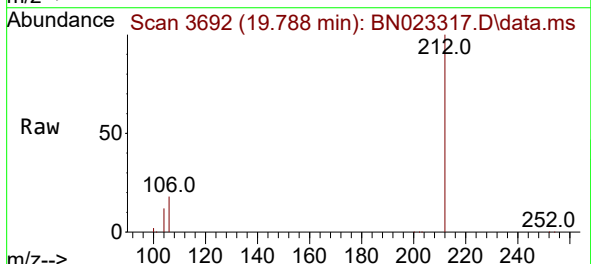

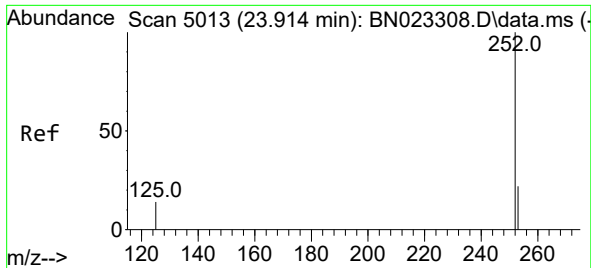

#26
 Benzo(a)pyrene
 Concen: 0.077 ng/ul
 RT: 23.870 min Scan# 4998
 Delta R.T. -0.044 min
 Lab File: BN023317.D
 Acq: 21 Dec 2022 17:25

Instrument :
 BNA_N
 ClientSampleId :

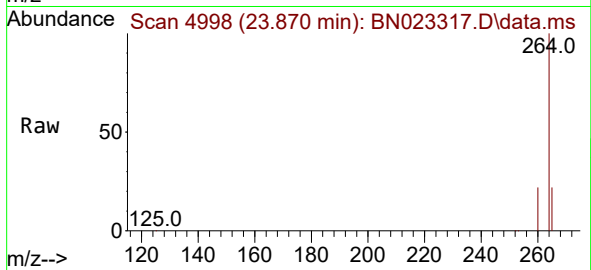

Tgt Ion:252 Resp: 6601
 Ion Ratio Lower Upper
 252 100
 253 43.5 21.4 32.2#
 125 39.4 16.2 24.4#

