

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122122\
 Data File : BN023318.D
 Acq On : 21 Dec 2022 18:02
 Operator : CG/JU
 Sample : N6006-06DL 5X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBXV9DL

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 12/22/2022
 Supervised By :mohammad ahmed 12/22/2022

Quant Time: Dec 22 03:21:07 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 22 02:28:40 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.998	152	5421	0.400	ng/u1	0.00
4) Naphthalene-d8	10.814	136	17654	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.648	164	10081	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.393	188	22994	0.400	ng/u1	0.00
17) Chrysene-d12	21.578	240	18793	0.400	ng/u1	0.00
23) Perylene-d12	24.024	264	14263	0.400	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.344	96	11298	1.918	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.403	152	3051	0.112	ng/u1	0.00
18) Fluoranthene-d10	19.418	212	6878	0.101	ng/u1	0.00
Target Compounds						Qvalue
19) Fluoranthene	19.446	202	196878	2.160	ng/u1	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122122\
Data File : BN023318.D
Acq On : 21 Dec 2022 18:02
Operator : CG/JU
Sample : N6006-06DL 5X
Misc :
ALS Vial : 16 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
DBXV9DL

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 12/22/2022
Supervised By :mohammad ahmed 12/22/2022


Quant Time: Dec 22 03:21:07 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 22 02:28:40 2022
Response via : Initial Calibration

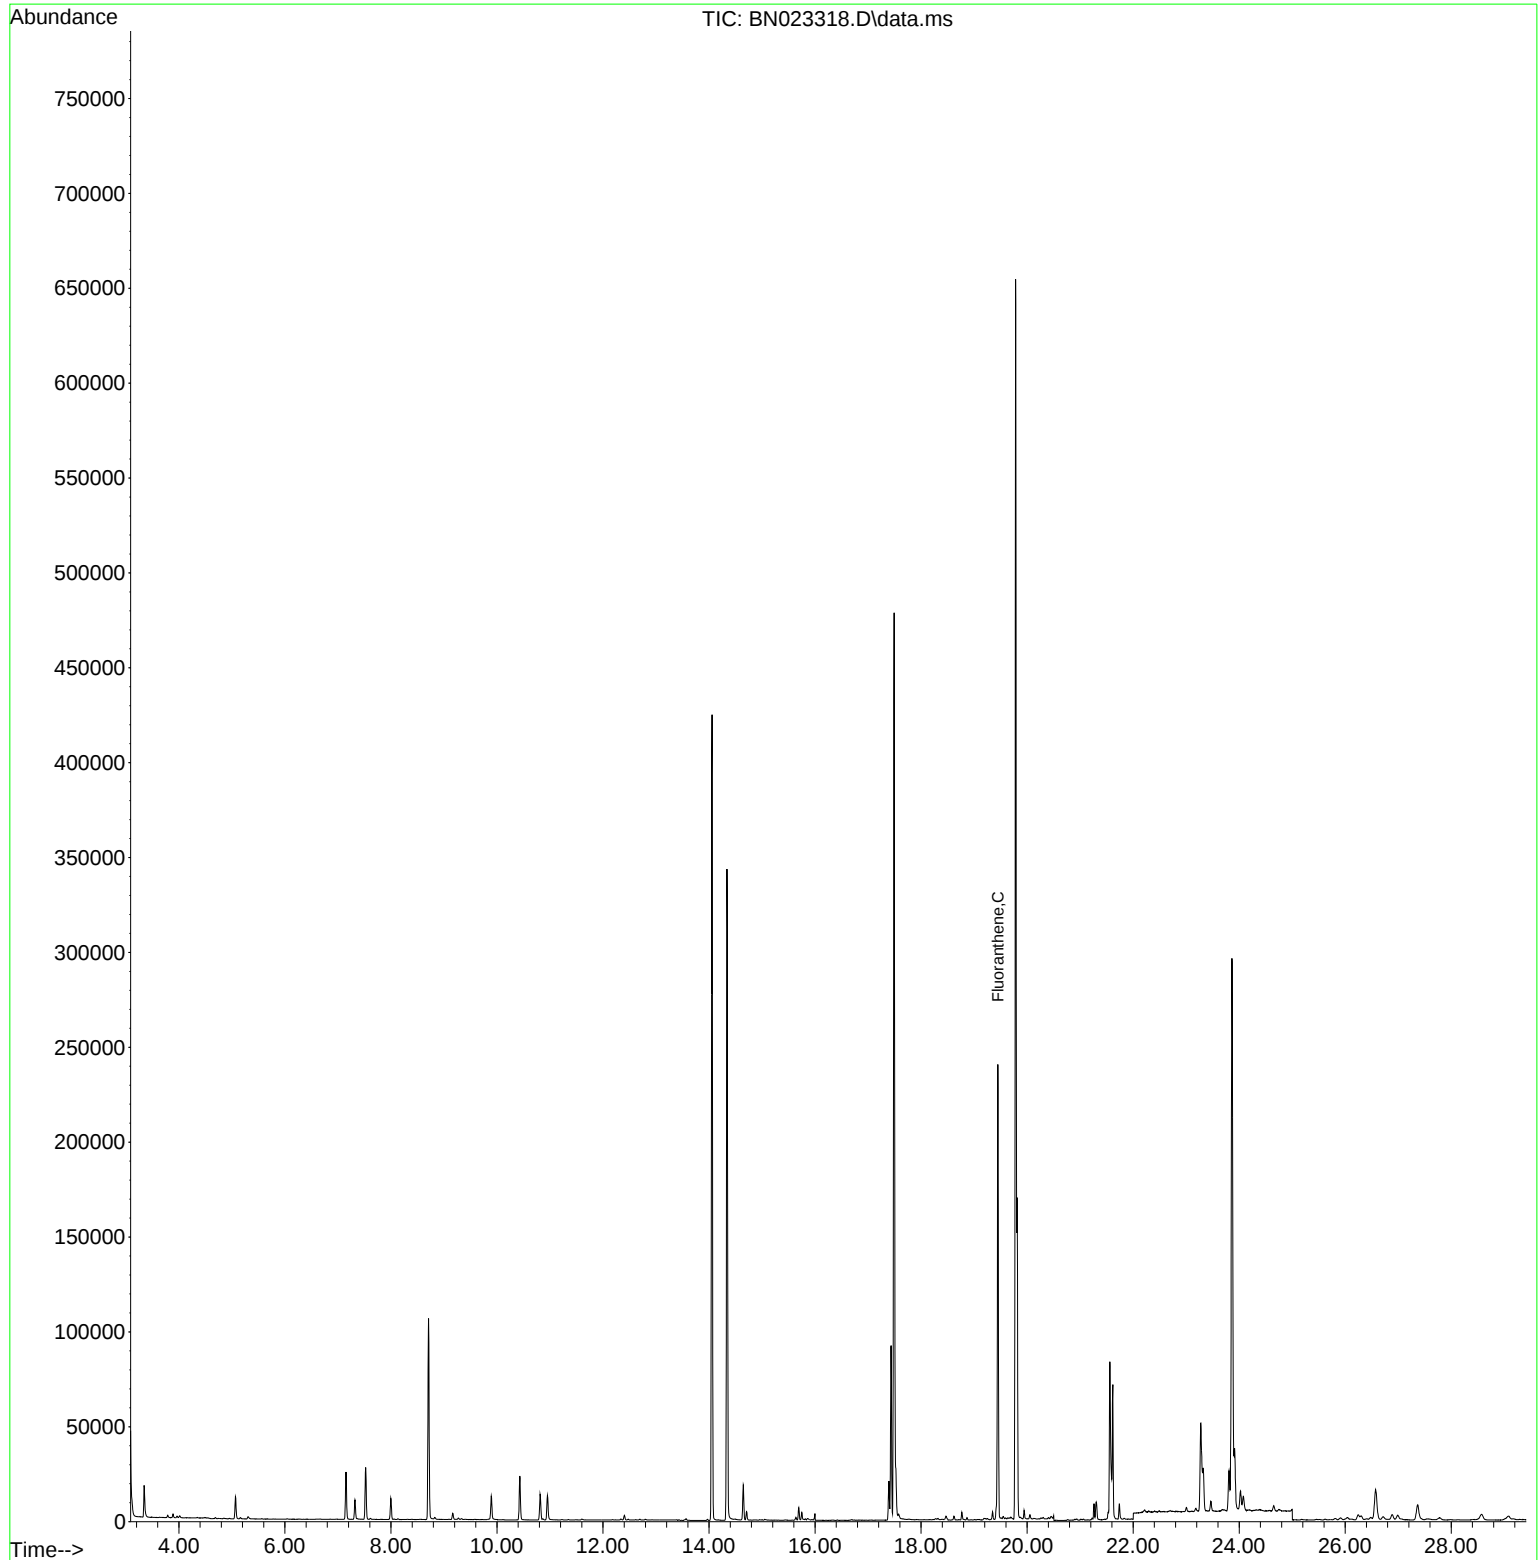

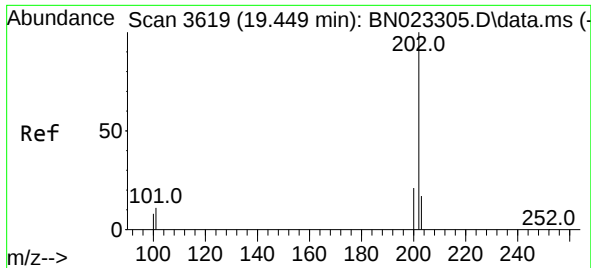

#19
Fluoranthene
Concen: 2.160 ng/ul
RT: 19.446 min Scan# 3619
Delta R.T. -0.003 min
Lab File: BN023318.D
Acq: 21 Dec 2022 18:02

Instrument :
BNA_N
ClientSampleId :
DBXV9DL

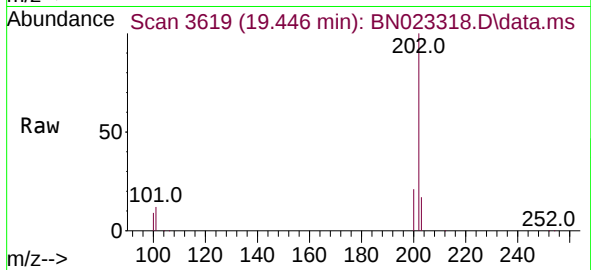

Tgt Ion:202 Resp: 196878
Ion Ratio Lower Upper
202 100
101 12.2 9.4 14.2
100 9.1 7.0 10.6

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 12/22/2022
Supervised By :mohammad ahmed 12/22/2022

