

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122123\
 Data File : BN029156.D
 Acq On : 21 Dec 2023 18:32
 Operator : MA/JU
 Sample : PB157944BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 PB157944BL

Quant Time: Dec 21 23:27:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN122023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 20 18:03:30 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.789	152	879	0.400	ng	0.00
7) Naphthalene-d8	10.584	136	1629	0.400	ng	0.00
13) Acenaphthene-d10	14.425	164	857	0.400	ng	0.00
19) Phenanthrene-d10	17.193	188	1348	0.400	ng	0.01
29) Chrysene-d12	21.393	240	666	0.400	ng	0.00
35) Perylene-d12	23.715	264	878	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.399	112	272	0.129	ng	0.00
5) Phenol-d6	7.009	99	239	0.103	ng	0.00
8) Nitrobenzene-d5	8.982	82	193	0.091	ng	0.02
11) 2-Methylnaphthalene-d10	12.178	152	285	0.115	ng	0.00
14) 2,4,6-Tribromophenol	15.940	330	177	0.236	ng	0.01
15) 2-Fluorobiphenyl	13.068	172	486	0.097	ng	0.01
27) Fluoranthene-d10	19.224	212	337	0.103	ng	0.00
31) Terphenyl-d14	19.833	244	562	0.307	ng	0.00
Target Compounds						
3) n-Nitrosodimethylamine	3.716	42	20	0.035	ng	# 21
20) 4,6-Dinitro-2-methylph...	15.654	198	3	0.067	ng	# 43
34) Bis(2-ethylhexyl)phtha...	21.322	149	104	Below Cal		# 87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122123\
Data File : BN029156.D
Acq On : 21 Dec 2023 18:32
Operator : MA/JU
Sample : PB157944BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB157944BL


Quant Time: Dec 21 23:27:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 20 18:03:30 2023
Response via : Initial Calibration

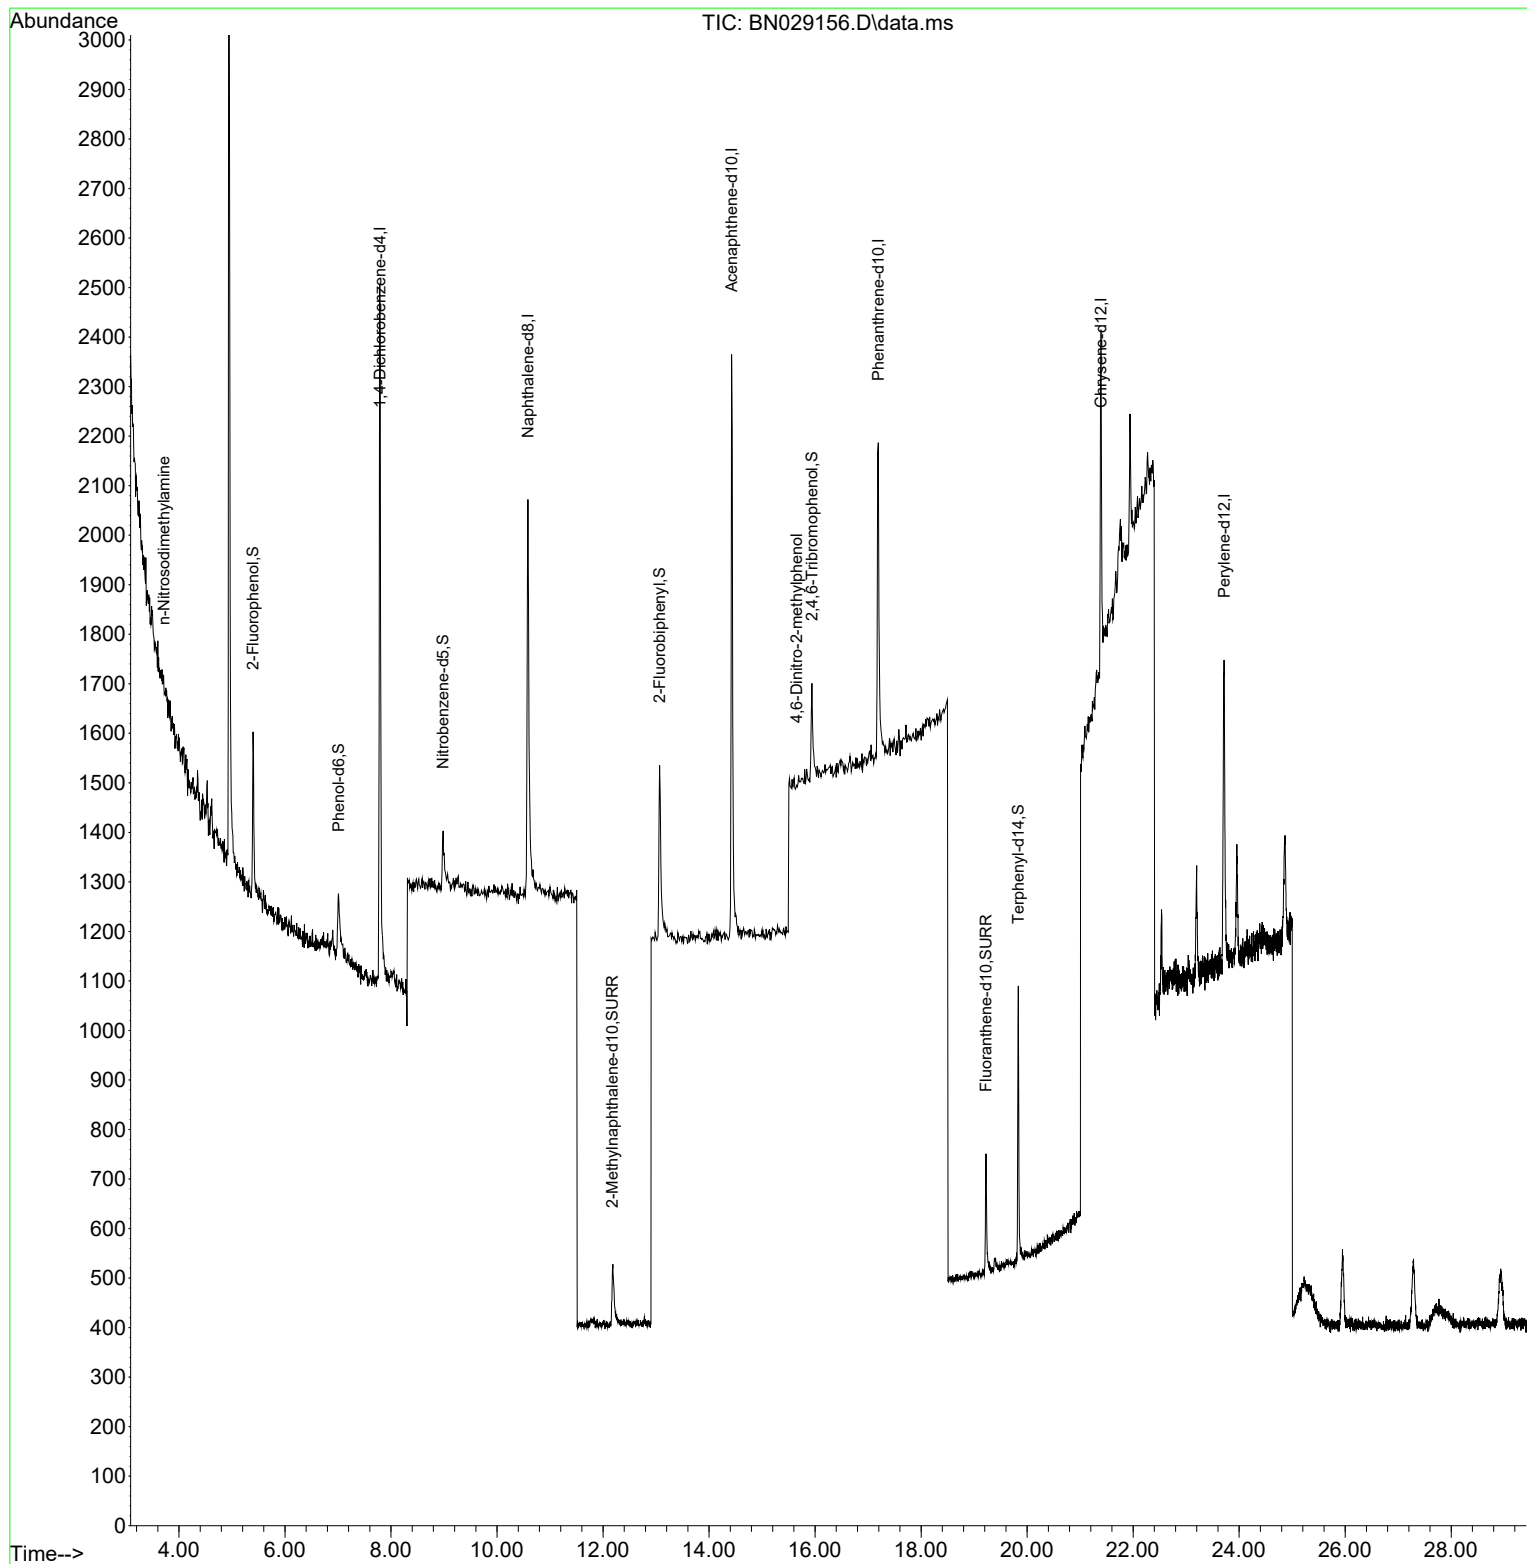



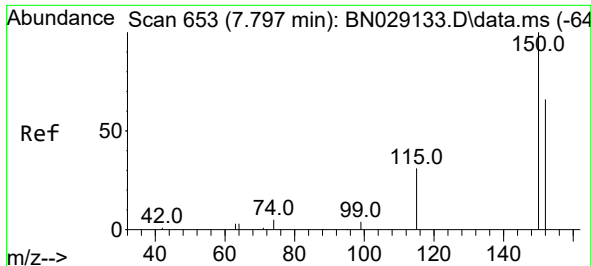


#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.789 min Scan# 61
Delta R.T. -0.008 min
Lab File: BN029156.D
Acq: 21 Dec 2023 18:32

Instrument :
BNA_N
ClientSampleId :
PB157944BL







Tgt Ion:152 Resp: 879
Ion Ratio Lower Upper
152 100
150 147.2 117.6 176.4
115 58.7 44.2 66.2

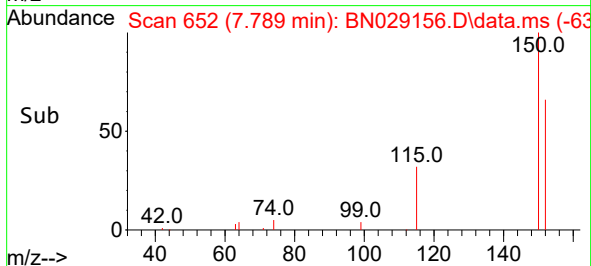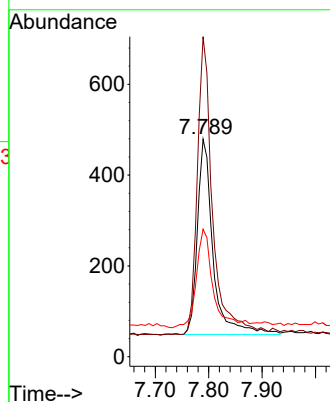

#3
n-Nitrosodimethylamine
Concen: 0.035 ng
RT: 3.716 min Scan# 88
Delta R.T. -0.000 min
Lab File: BN029156.D
Acq: 21 Dec 2023 18:32

Tgt Ion: 42 Resp: 20
Ion Ratio Lower Upper
42 100
74 40.0 103.0 154.4#
44 55.0 3.2 4.8#


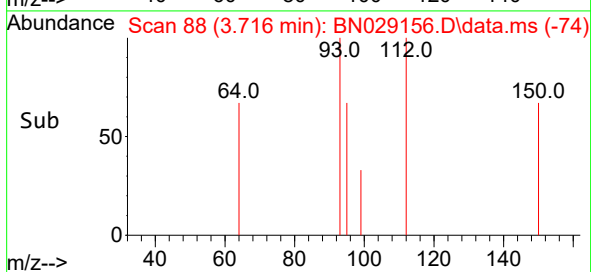
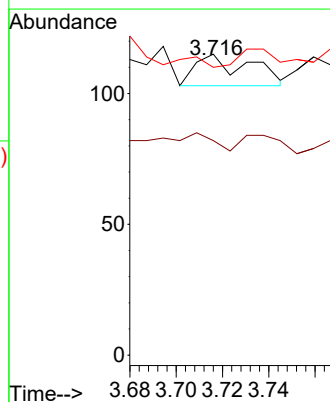
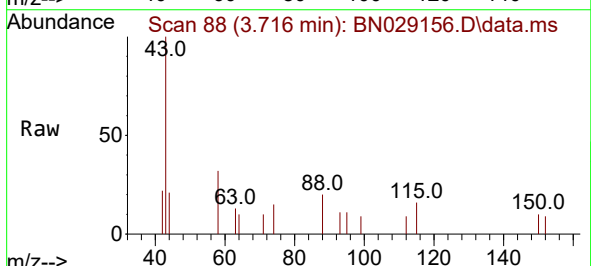


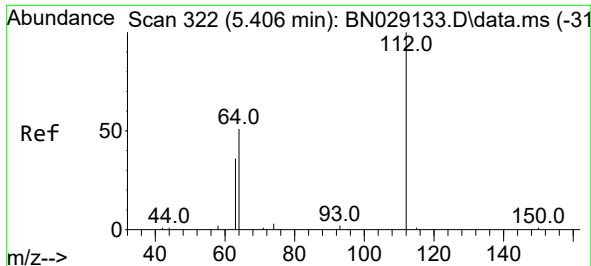

#4
2-Fluorophenol
Concen: 0.129 ng
RT: 5.399 min Scan# 31
Delta R.T. -0.007 min
Lab File: BN029156.D
Acq: 21 Dec 2023 18:32




Instrument :
BNA_N
ClientSampleId :
PB157944BL


Tgt Ion:112 Resp: 272
Ion Ratio Lower Upper
112 100
64 53.3 38.6 58.0
63 37.1 30.0 45.0

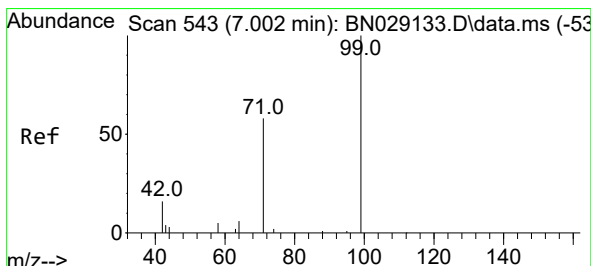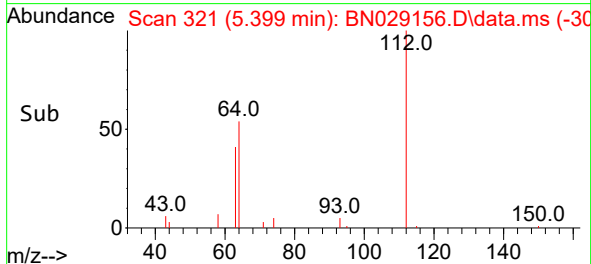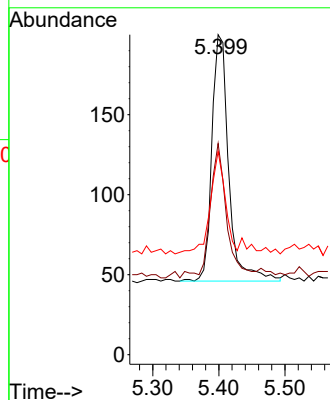

#5
Phenol-d6
Concen: 0.103 ng
RT: 7.009 min Scan# 544
Delta R.T. 0.007 min
Lab File: BN029156.D
Acq: 21 Dec 2023 18:32

Tgt Ion: 99 Resp: 239
Ion Ratio Lower Upper
99 100
42 13.8 13.8 20.6
71 44.8 45.4 68.2#


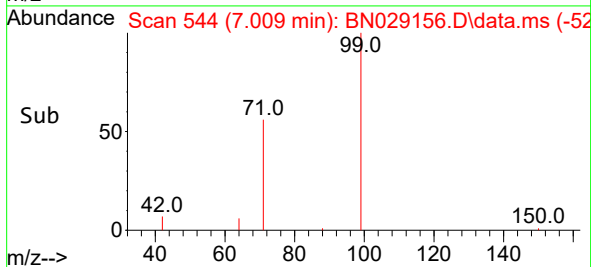
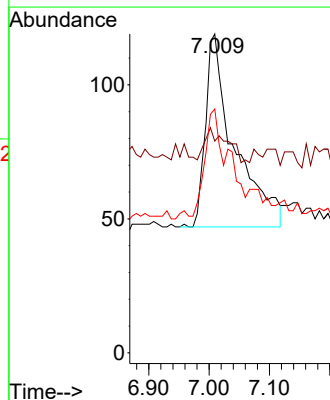
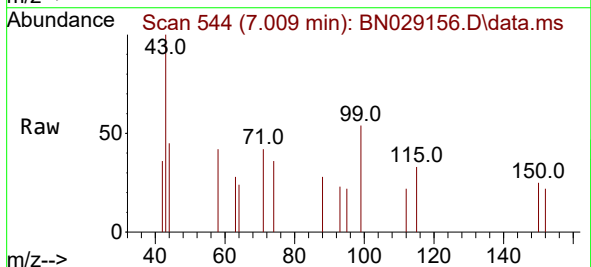


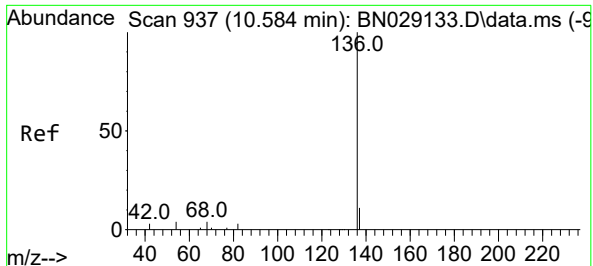

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.584 min Scan# 91
Delta R.T. -0.000 min
Lab File: BN029156.D
Acq: 21 Dec 2023 18:32




Instrument :
BNA_N
ClientSampleId :
PB157944BL


Tgt Ion:	136	Resp:	1629
Ion	Ratio	Lower	Upper
136	100		
137	17.6	13.4	20.0
54	12.4	8.6	13.0
68	11.5	8.0	12.0

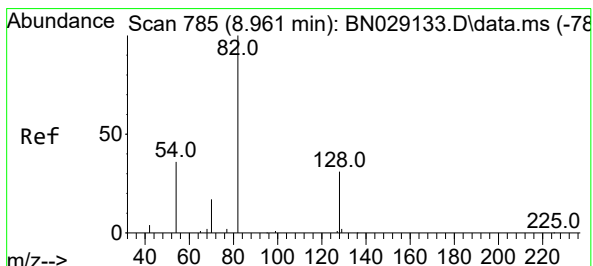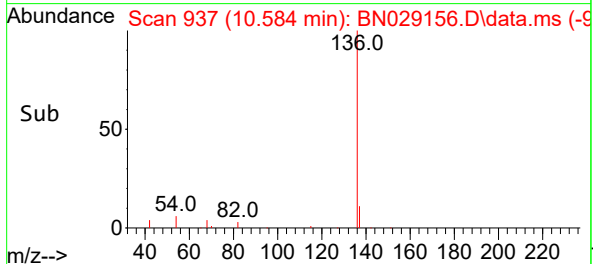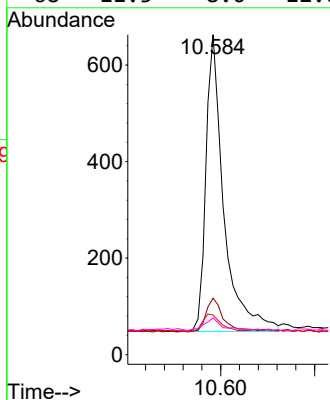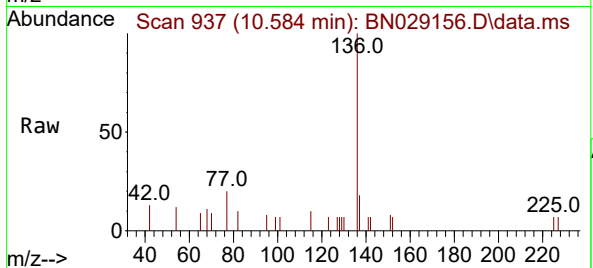

#8
Nitrobenzene-d5
Concen: 0.091 ng
RT: 8.982 min Scan# 787
Delta R.T. 0.021 min
Lab File: BN029156.D
Acq: 21 Dec 2023 18:32

Tgt Ion:	82	Resp:	193
Ion	Ratio	Lower	Upper
82	100		
128	67.0	33.0	49.4#
54	63.2	35.8	53.8#


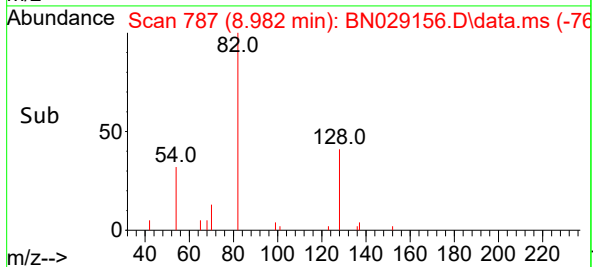
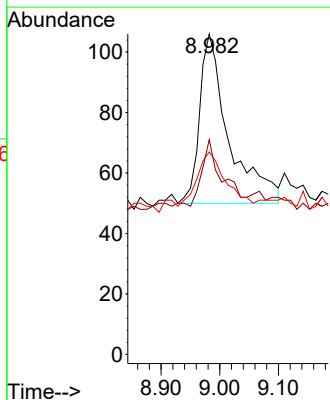
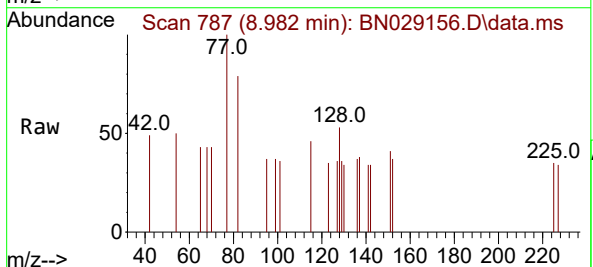


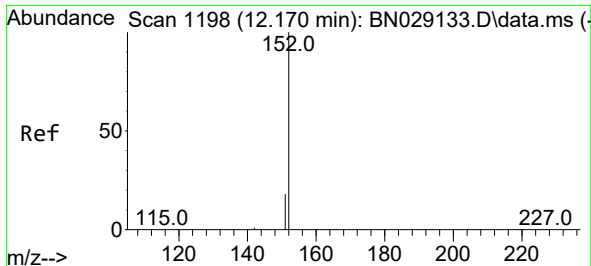

#11
2-Methylnaphthalene-d10
Concen: 0.115 ng
RT: 12.178 min Scan# 1198
Delta R.T. 0.007 min
Lab File: BN029156.D
Acq: 21 Dec 2023 18:32




Instrument :
BNA_N
ClientSampleId :
PB157944BL


Tgt Ion:152 Resp: 285
Ion Ratio Lower Upper
152 100
151 11.2 17.4 26.2#

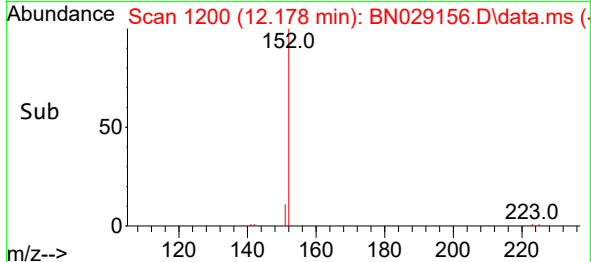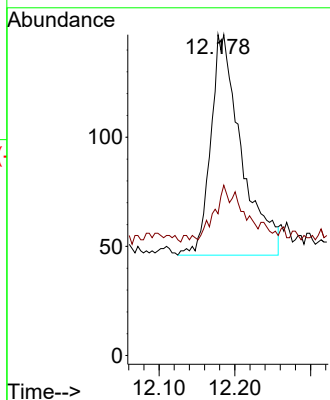

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.425 min Scan# 1535
Delta R.T. -0.000 min
Lab File: BN029156.D
Acq: 21 Dec 2023 18:32

Tgt Ion:164 Resp: 857
Ion Ratio Lower Upper
164 100
162 116.3 85.0 127.4
160 60.5 45.8 68.8


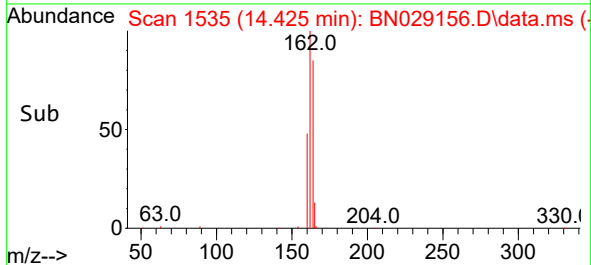
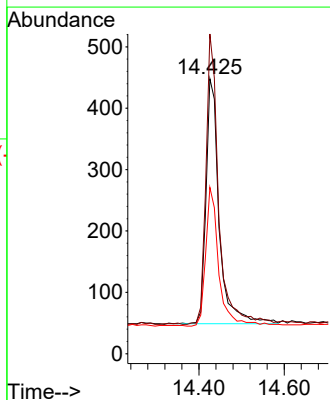
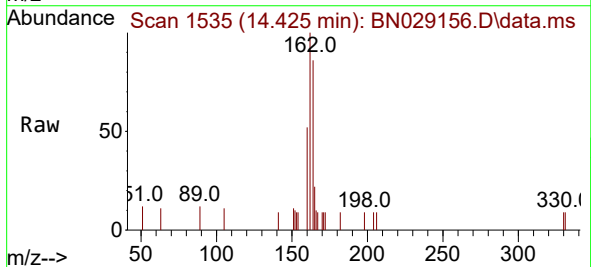


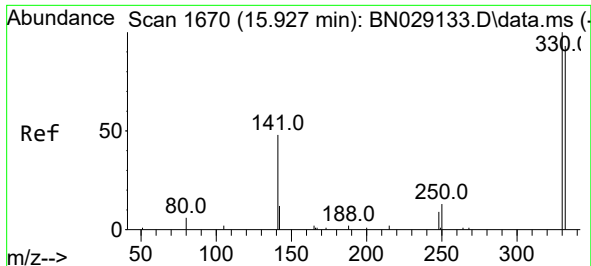

#14
2,4,6-Tribromophenol
Concen: 0.236 ng
RT: 15.940 min Scan# 1671
Delta R.T. 0.012 min
Lab File: BN029156.D
Acq: 21 Dec 2023 18:32




Instrument :
BNA_N
ClientSampleId :
PB157944BL


Tgt Ion:330 Resp: 177
Ion Ratio Lower Upper
330 100
332 86.4 83.4 125.0
141 55.4 43.8 65.8

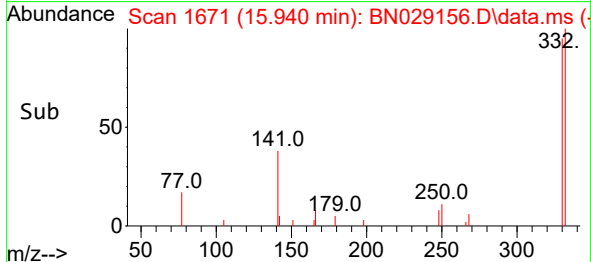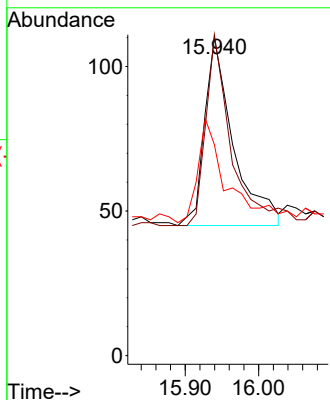

#15
2-Fluorobiphenyl
Concen: 0.097 ng
RT: 13.068 min Scan# 1408
Delta R.T. 0.011 min
Lab File: BN029156.D
Acq: 21 Dec 2023 18:32

Tgt Ion:172 Resp: 486
Ion Ratio Lower Upper
172 100
171 50.6 32.2 48.4#
170 39.9 25.0 37.4#

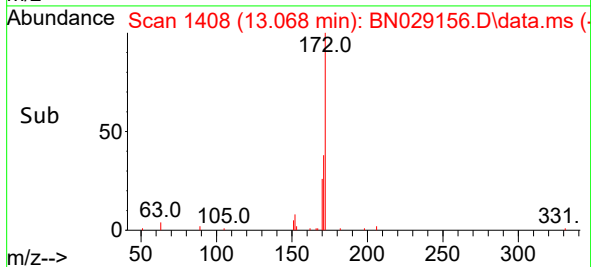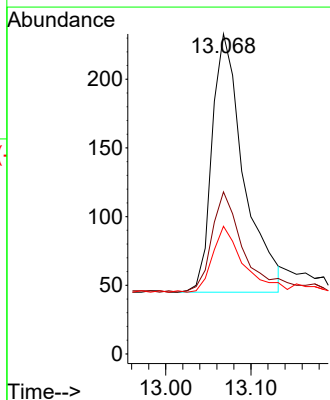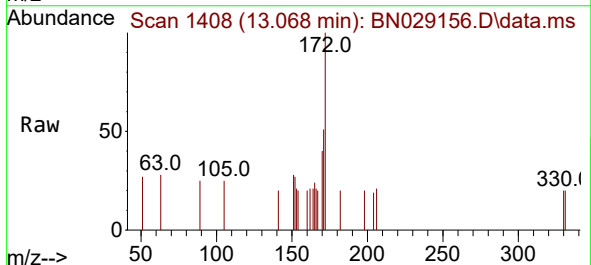



#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.193 min Scan# 1

Delta R.T. 0.012 min

Lab File: BN029156.D

Acq: 21 Dec 2023 18:32

Instrument :

BNA_N

ClientSampleId :

PB157944BL





Tgt Ion:188 Resp: 1348

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 14.7 13.7 20.5

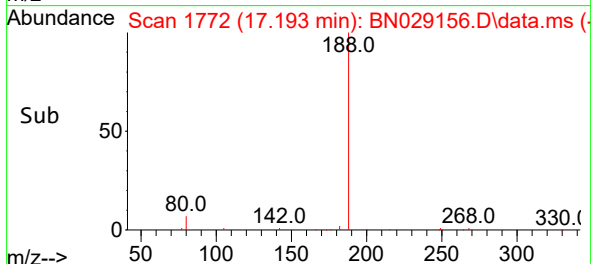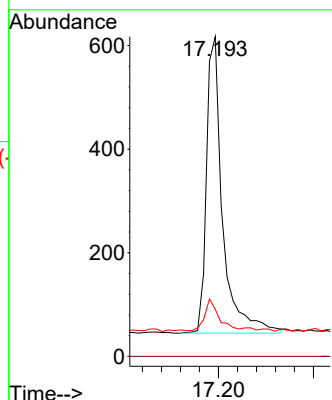

#20

4,6-Dinitro-2-methylphenol

Concen: 0.067 ng

RT: 15.654 min Scan# 1648

Delta R.T. 0.074 min

Lab File: BN029156.D

Acq: 21 Dec 2023 18:32




Tgt Ion:198 Resp: 3


Ion Ratio Lower Upper

198 100

51 121.3 53.6 80.4#

105 125.5 65.6 98.4#

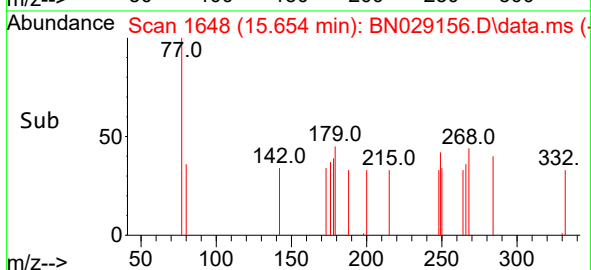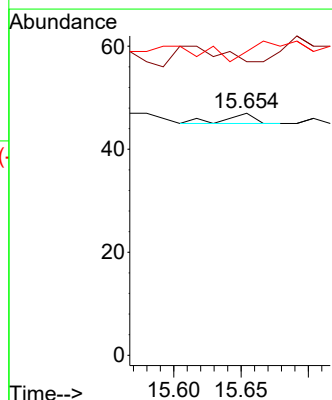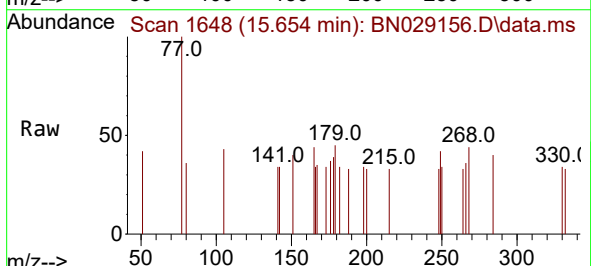

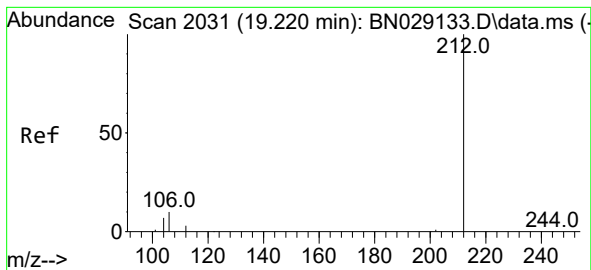

#27

Fluoranthene-d10

Concen: 0.103 ng

RT: 19.224 min Scan# 2031

Delta R.T. 0.005 min

Lab File: BN029156.D

Acq: 21 Dec 2023 18:32

Instrument :

BNA_N

ClientSampleId :

PB157944BL





Tgt Ion:212 Resp: 337

Ion Ratio Lower Upper

212 100

106 9.2 9.6 14.4#

104 7.4 6.5 9.7

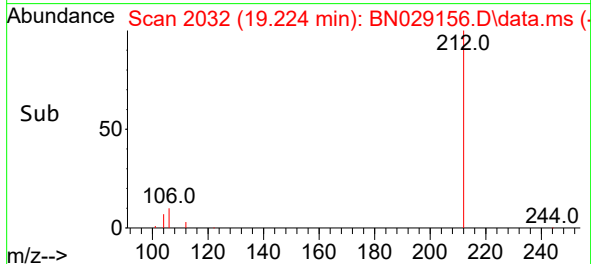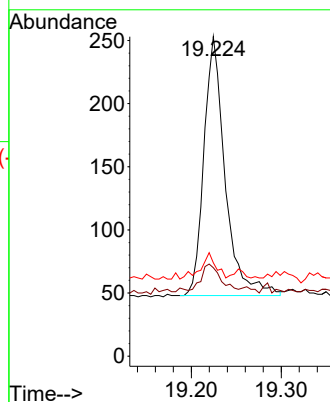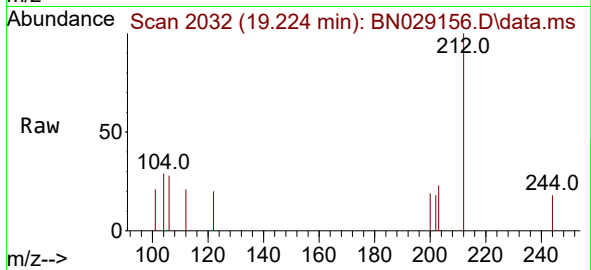

#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.393 min Scan# 2459

Delta R.T. 0.004 min

Lab File: BN029156.D

Acq: 21 Dec 2023 18:32




Tgt Ion:240 Resp: 666


Ion Ratio Lower Upper

240 100

120 25.6 21.4 32.0

236 39.0 33.5 50.3


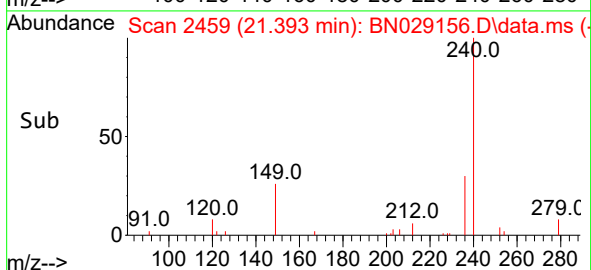
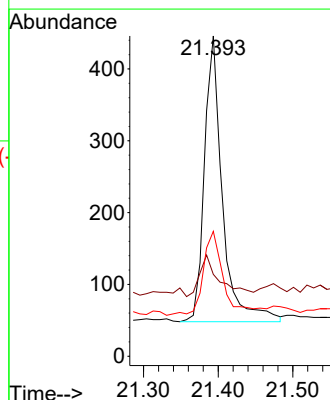
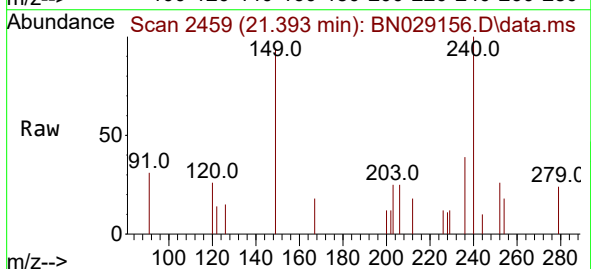


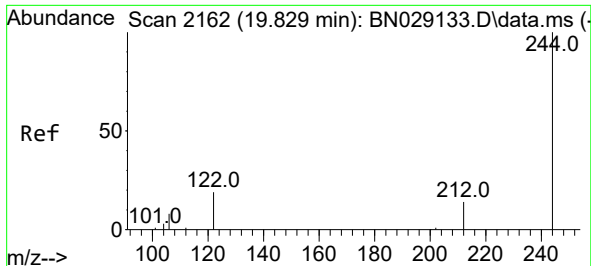

#31
 Terphenyl-d14
 Concen: 0.307 ng
 RT: 19.833 min Scan# 2163
 Delta R.T. 0.005 min
 Lab File: BN029156.D
 Acq: 21 Dec 2023 18:32




Instrument :
 BNA_N
 ClientSampleId :
 PB157944BL


Tgt Ion:244 Resp: 562
 Ion Ratio Lower Upper
 244 100
 212 23.9 19.0 28.6
 122 27.1 22.5 33.7

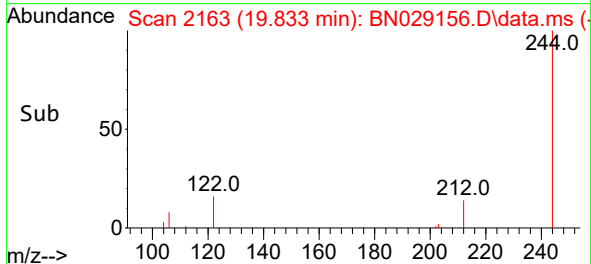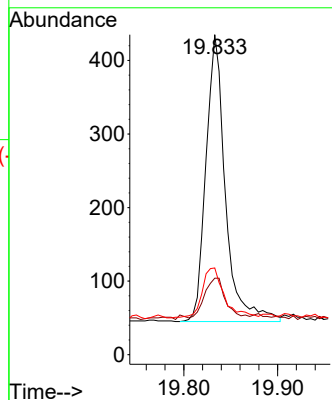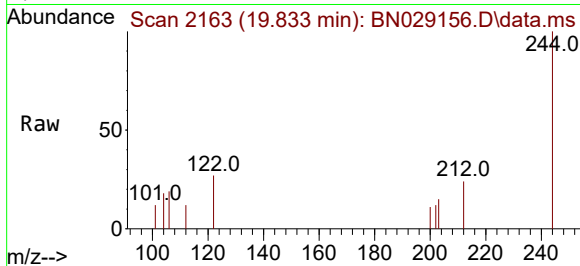

#34
 Bis(2-ethylhexyl)phthalate
 Concen: Below Cal
 RT: 21.322 min Scan# 2451
 Delta R.T. 0.013 min
 Lab File: BN029156.D
 Acq: 21 Dec 2023 18:32


Tgt Ion:149 Resp: 104
 Ion Ratio Lower Upper
 149 100
 167 31.7 20.2 30.2#
 279 0.0 2.5 3.7#

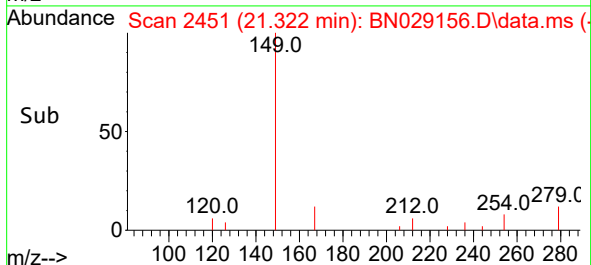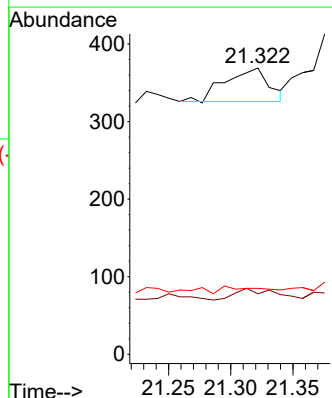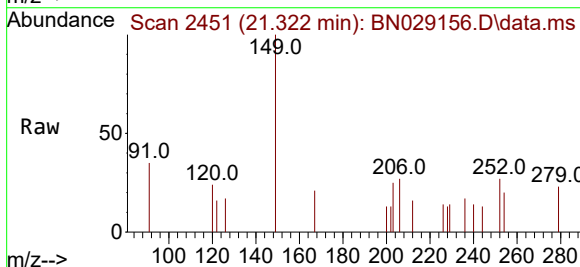

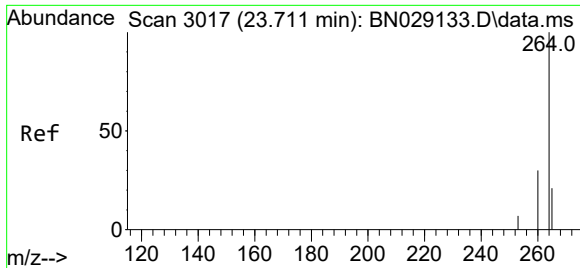

#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.715 min Scan# 30
 Delta R.T. 0.004 min
 Lab File: BN029156.D
 Acq: 21 Dec 2023 18:32

Instrument :
 BNA_N
 ClientSampleId :
 PB157944BL

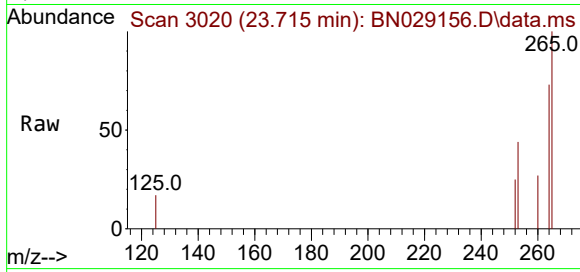

Tgt Ion:264 Resp: 878
 Ion Ratio Lower Upper
 264 100
 260 36.7 31.0 46.6
 265 137.6 105.3 157.9

