
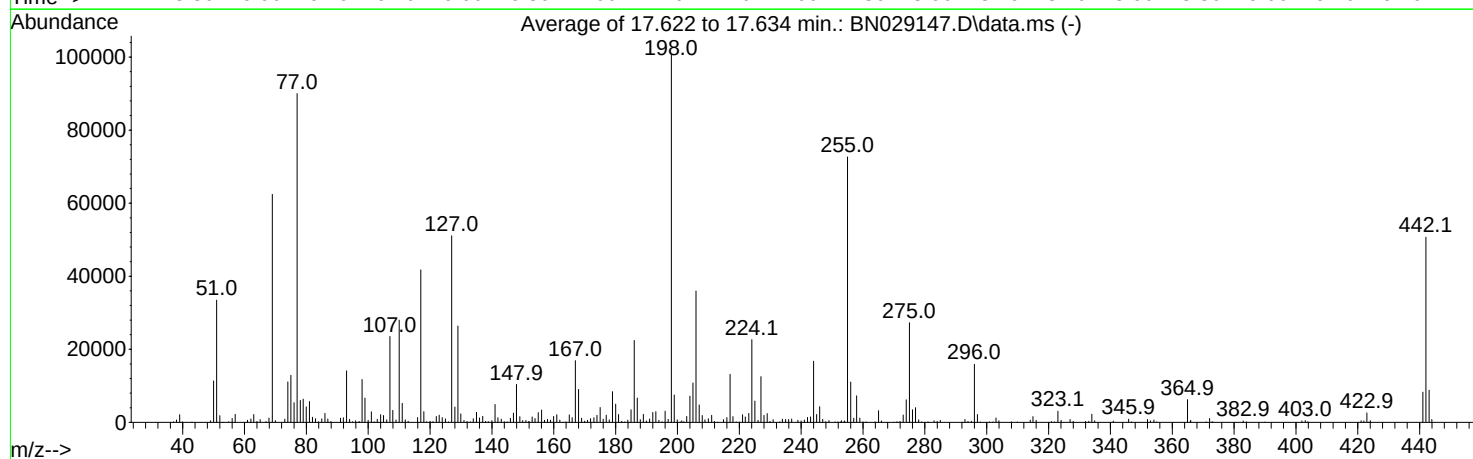


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122123\
Data File : BN029147.D
Acq On : 21 Dec 2023 13:12
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN122023.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Dec 20 18:03:30 2023

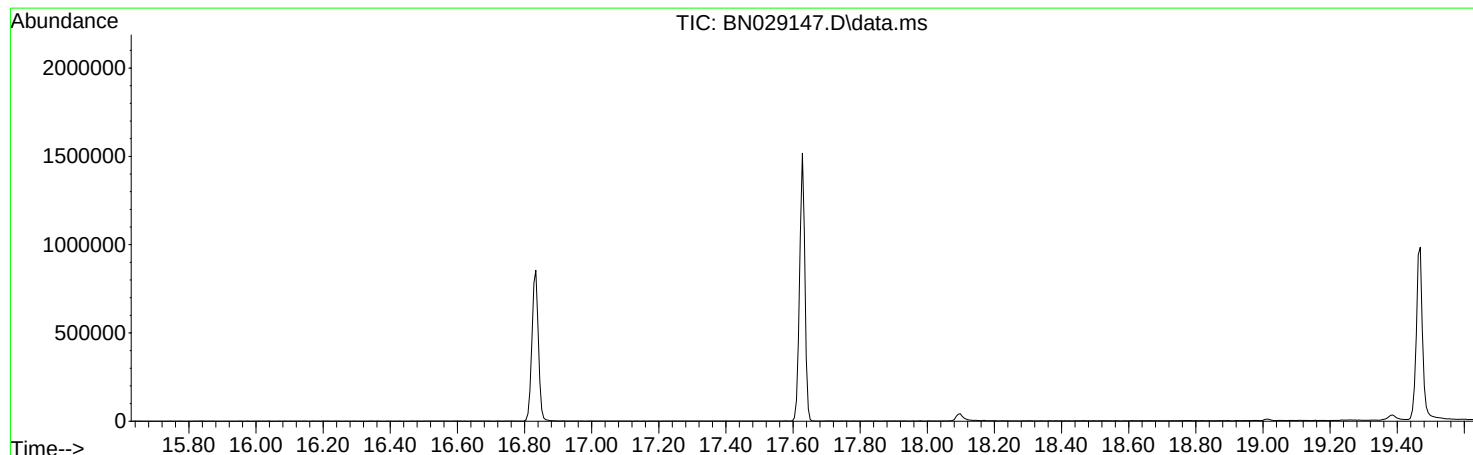




AutoFind: Scans 2471, 2472, 2473; Background Corrected with Scan 2464

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.2	33459	PASS
68	69	0.00	2	1.9	1195	PASS
69	198	0.00	100	62.0	62400	PASS
70	69	0.00	2	0.8	468	PASS
127	198	10	80	50.7	51064	PASS
197	198	0.00	2	0.8	831	PASS
198	198	100	100	100.0	100707	PASS
199	198	5	9	7.4	7472	PASS
275	198	10	60	27.1	27307	PASS
365	198	1	100	6.2	6226	PASS
441	198	0.01	100	8.2	8261	PASS
442	442	50	100	100.0	50688	PASS
443	442	15	24	17.4	8824	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122123\
Data File : BN029147.D
Acq On : 21 Dec 2023 13:12
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 22 01:48:45 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 01 23:28:24 2023
Response via : Initial Calibration

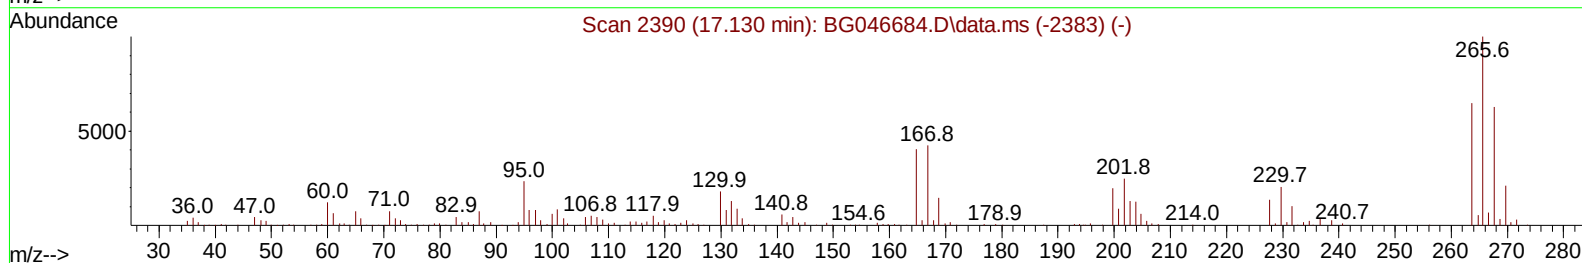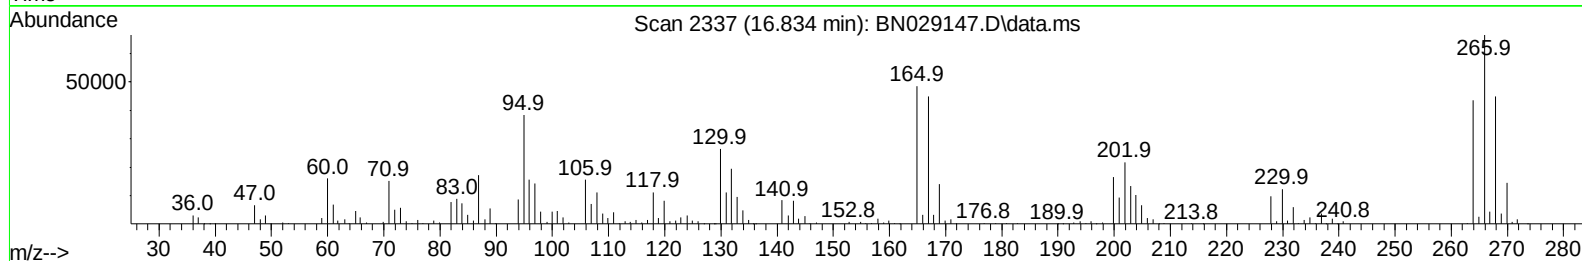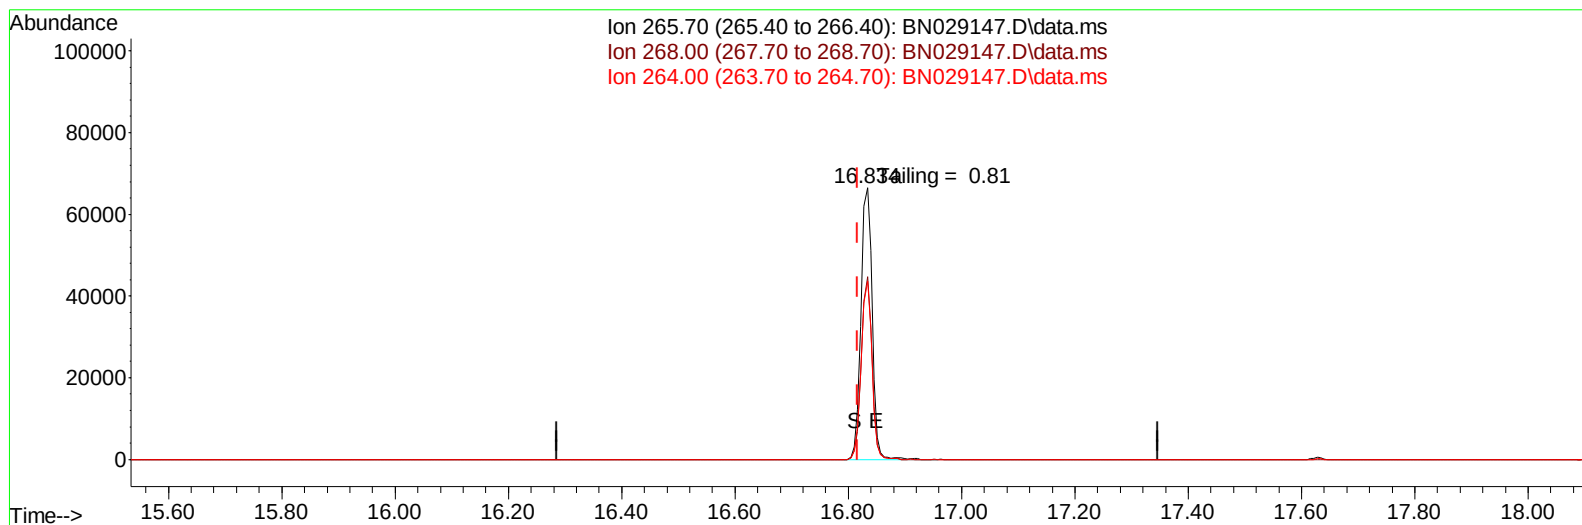

TIC: BN029147.D\data.ms

(70) Pentachlorophenol (C)

16.834min (+ 0.018) 11838.39 ng




response 90675

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	67.44
264.00	61.60	65.67
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122123\
Data File : BN029147.D
Acq On : 21 Dec 2023 13:12
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 22 01:48:45 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 01 23:28:24 2023
Response via : Initial Calibration

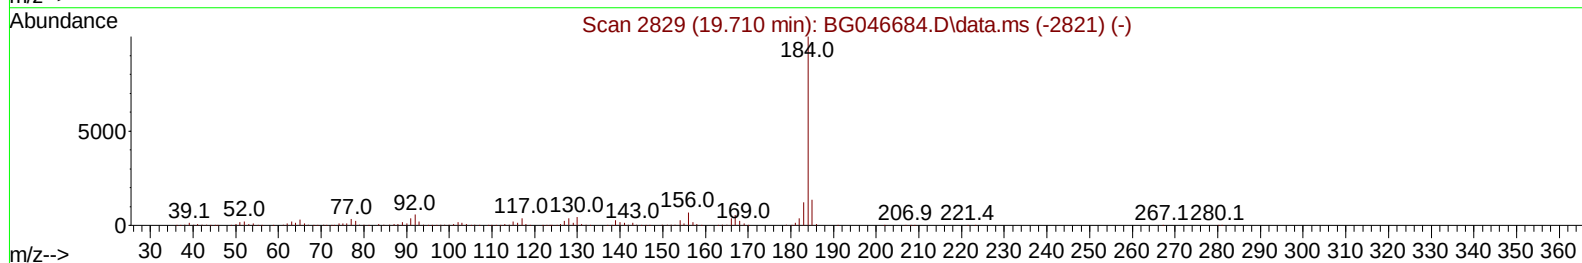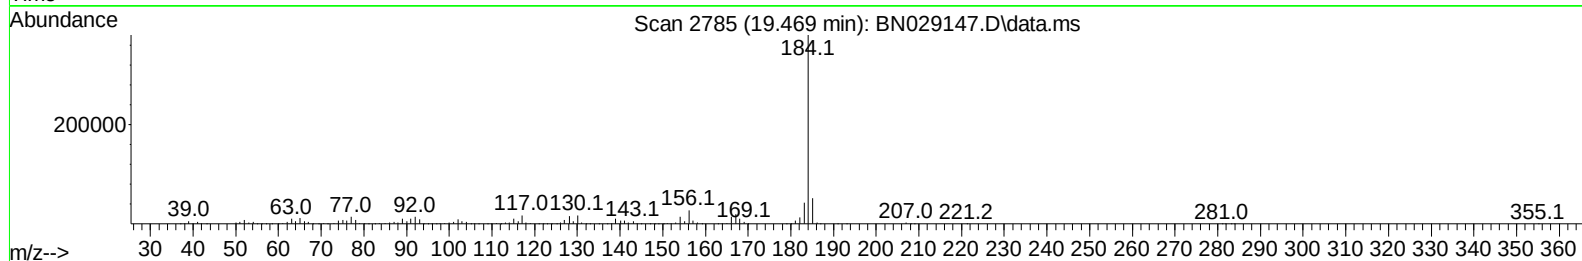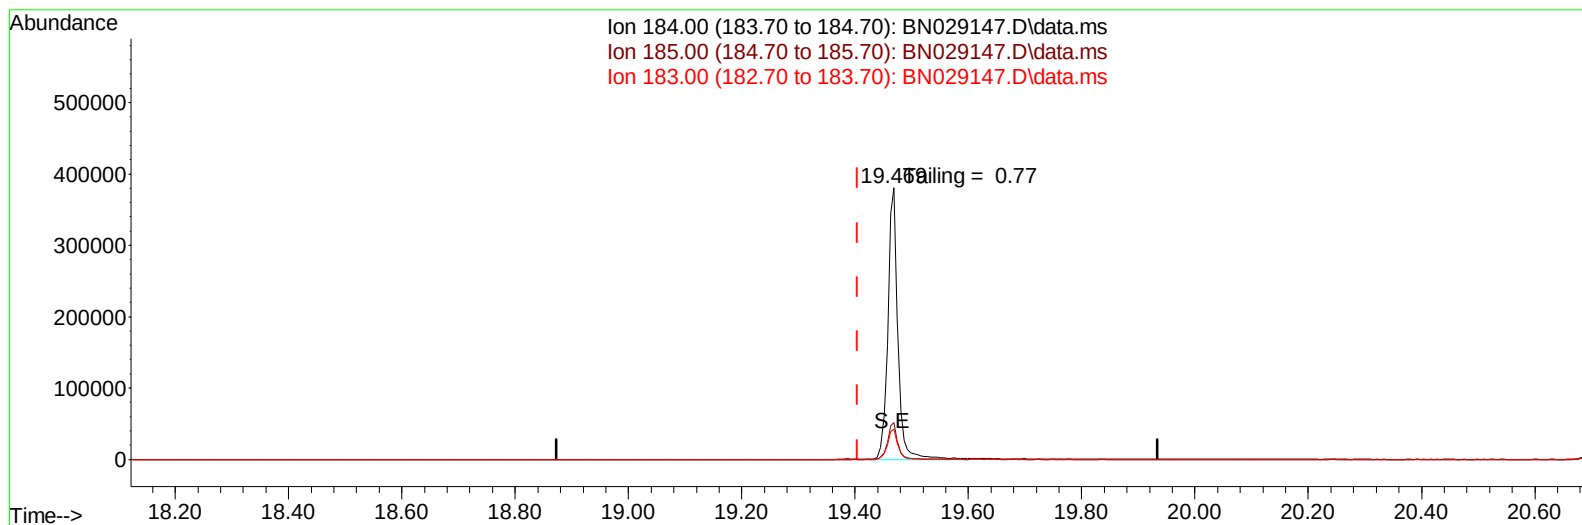

TIC: BN029147.D\data.ms

(77) Benzidine

19.469min (+ 0.065) 0.00 ng

response 469449

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.48
183.00	13.20	11.34
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/21/2023	BNA_N	<u>BN029147.D</u>
Compound Name	Response	Retention Time
DDT	297578	20.686
DDD	13686	20.245
DDE	61	19.733
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13747	311325	4.42

Instrument :
BNA_N
ClientSampleId :
DFTPP