
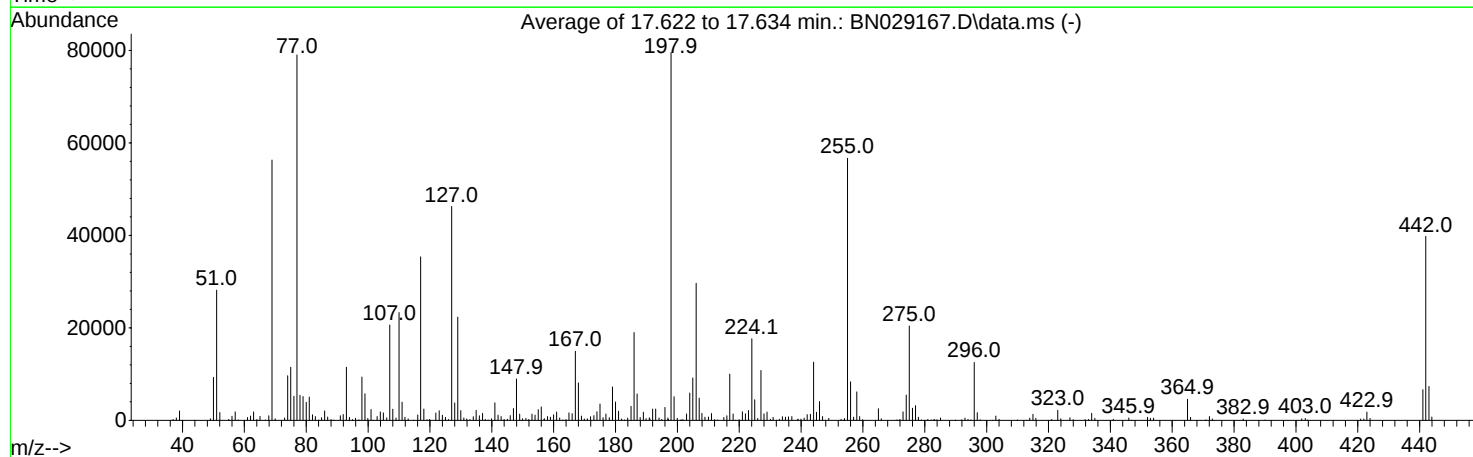


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122123\
Data File : BN029167.D
Acq On : 22 Dec 2023 01:06
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN122023.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Dec 20 18:03:30 2023

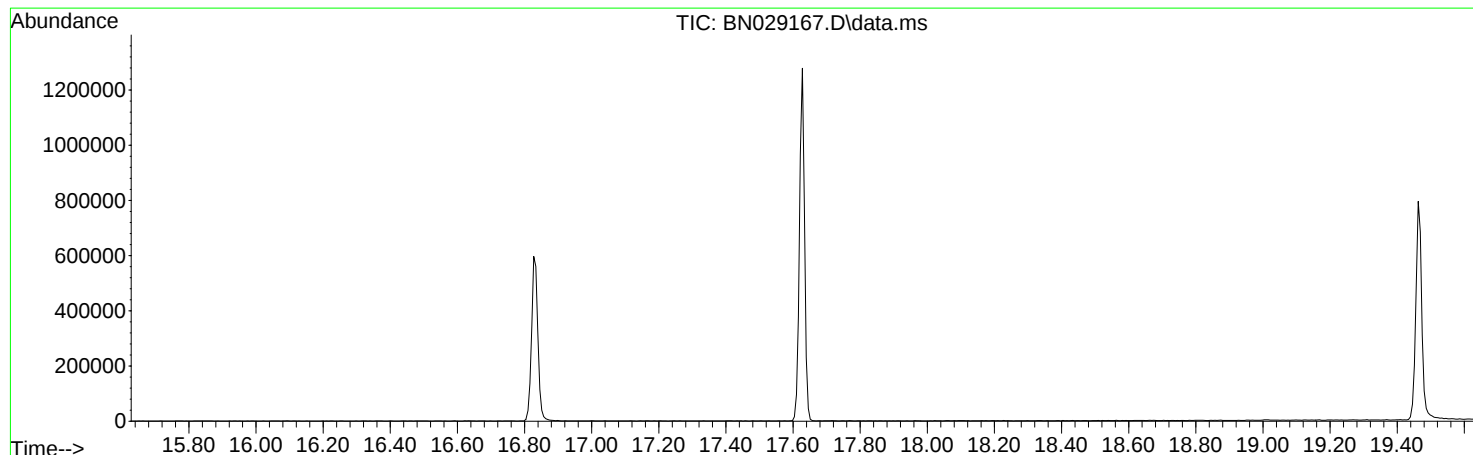




AutoFind: Scans 2471, 2472, 2473; Background Corrected with Scan 2465

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.4	28160	PASS
68	69	0.00	2	1.8	1000	PASS
69	198	0.00	100	70.8	56299	PASS
70	69	0.00	2	0.6	333	PASS
127	198	10	80	58.1	46253	PASS
197	198	0.00	2	0.6	511	PASS
198	198	100	100	100.0	79544	PASS
199	198	5	9	6.5	5135	PASS
275	198	10	60	25.7	20424	PASS
365	198	1	100	5.8	4579	PASS
441	198	0.01	100	8.4	6648	PASS
442	442	50	100	100.0	39784	PASS
443	442	15	24	18.5	7355	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122123\
Data File : BN029167.D
Acq On : 22 Dec 2023 01:06
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 22 04:24:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 01 23:28:24 2023
Response via : Initial Calibration

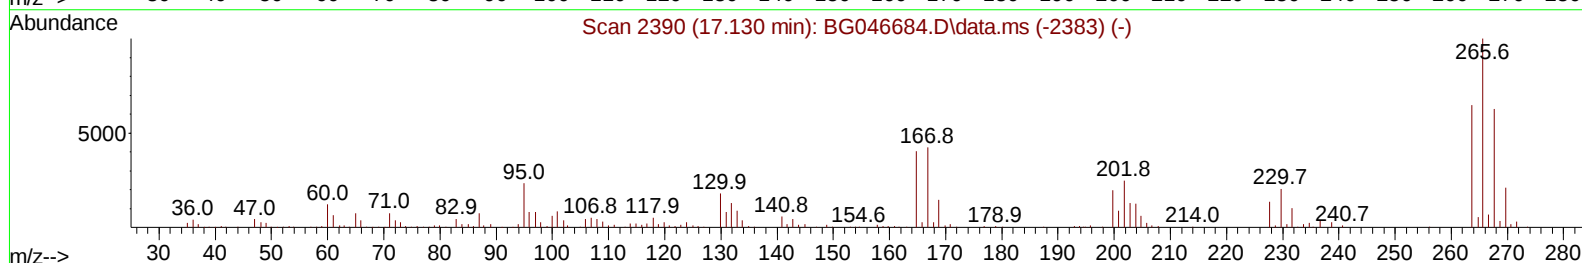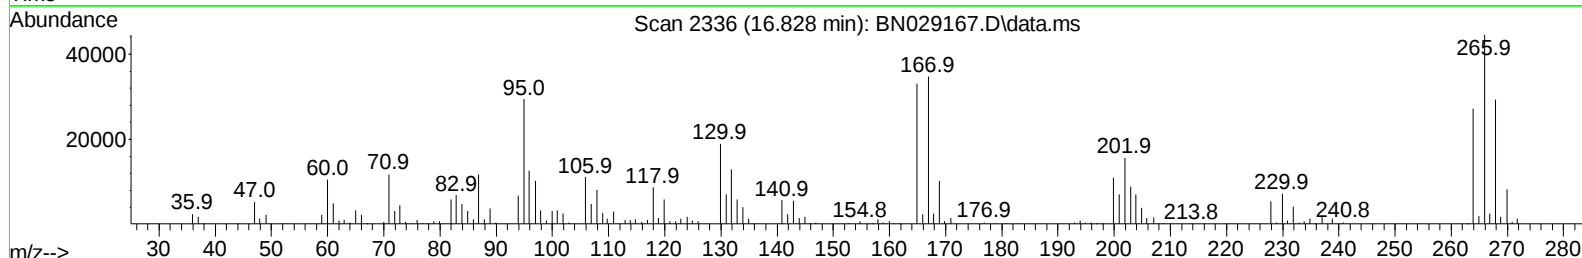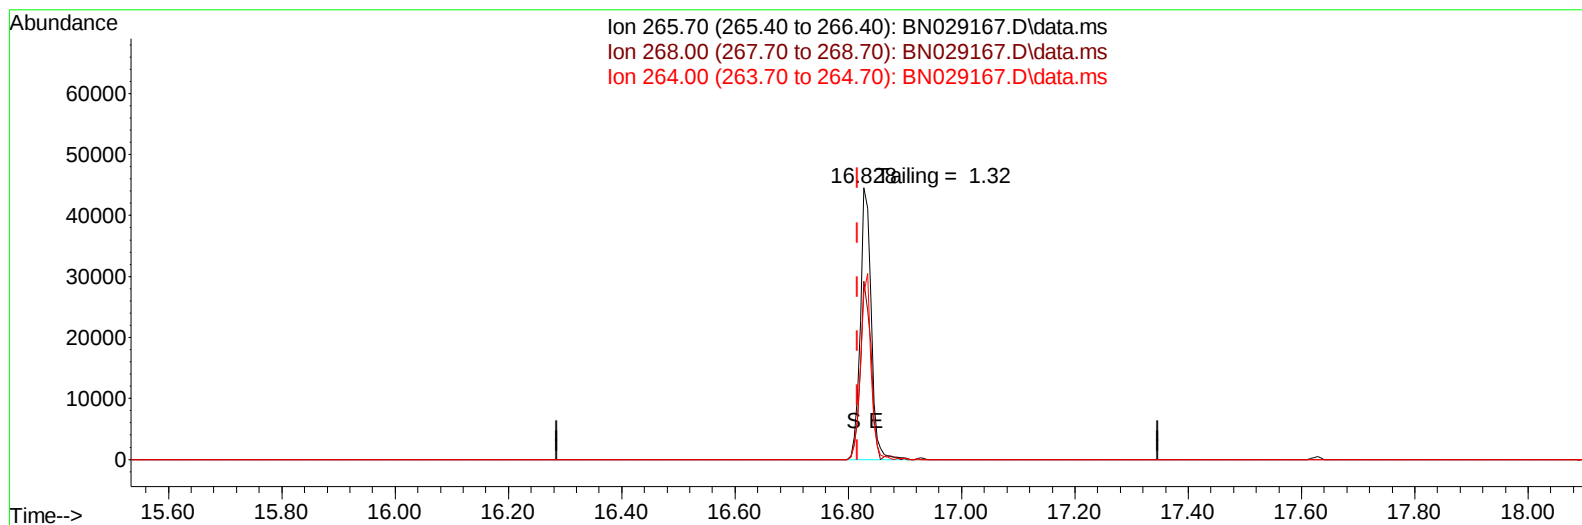

TIC: BN029167.D\data.ms

(70) Pentachlorophenol (C)

16.828min (+ 0.012) 9996.85 ng




response 58918

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.79
264.00	61.60	61.08
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122123\
Data File : BN029167.D
Acq On : 22 Dec 2023 01:06
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 22 04:24:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 01 23:28:24 2023
Response via : Initial Calibration

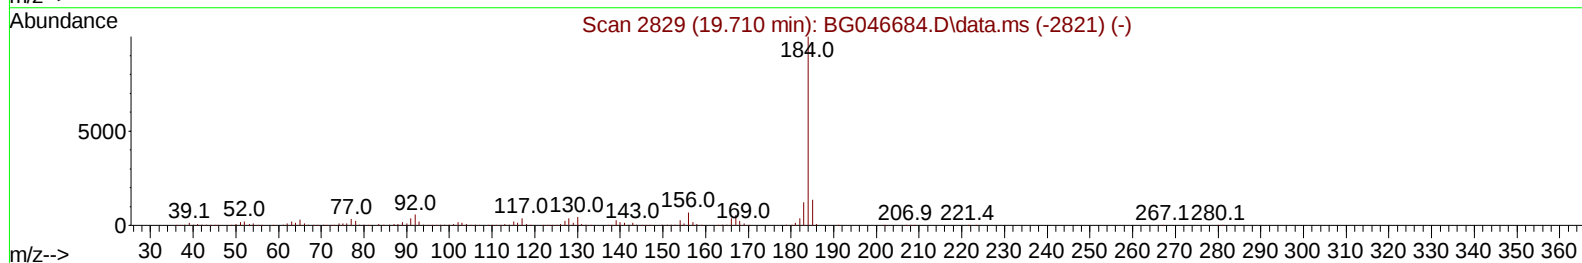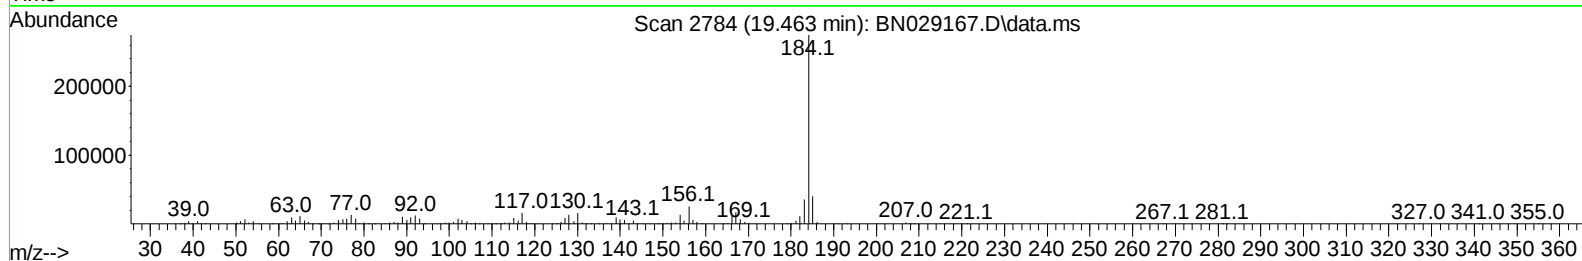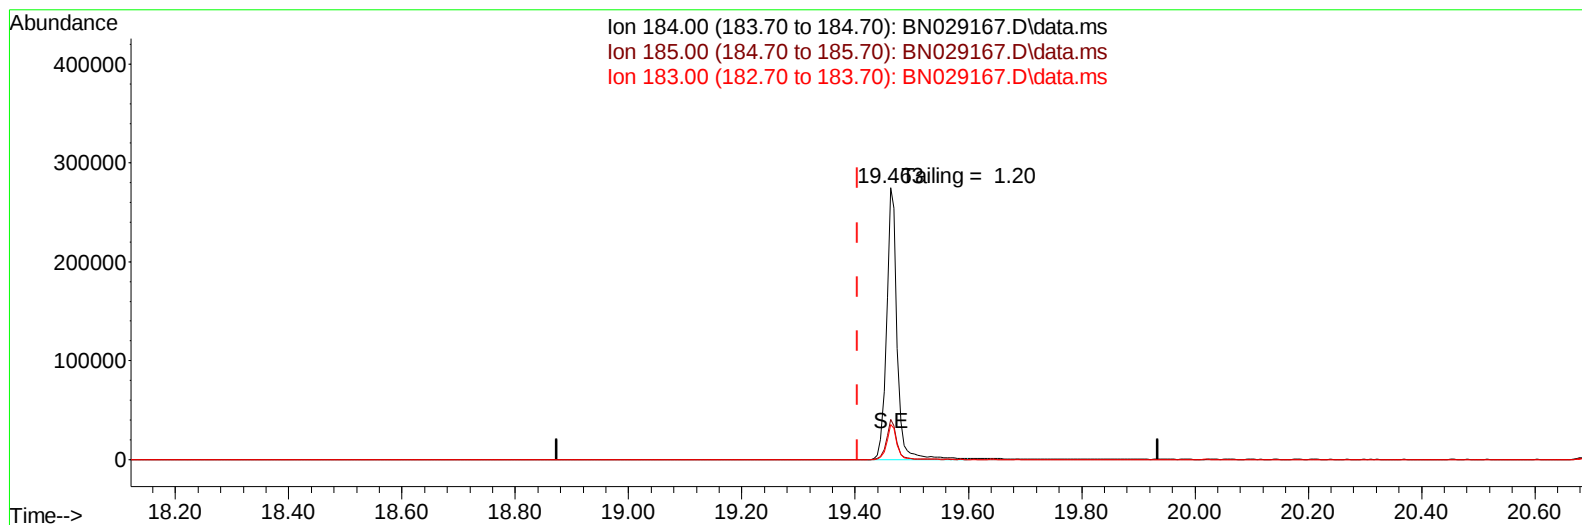

TIC: BN029167.D\data.ms

(77) Benzidine

19.463min (+ 0.059) 0.00 ng

response 355423

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.74
183.00	13.20	12.86
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/21/2023	BNA_N	<u>BN029167.D</u>
Compound Name	Response	Retention Time
DDT	179996	20.686
DDD	7815	20.245
DDE	0	19.733
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7815	187811	4.16

Instrument :
BNA_N
ClientSampleId :
DFTPP