

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122220\
 Data File : BN013262.D
 Acq On : 22 Dec 2020 08:35
 Operator : CG/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4

Quant Time: Dec 22 10:47:33 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN121620.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 22 10:46:43 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.330	152	729	0.40	ng	0.00
7) Naphthalene-d8	10.099	136	2589	0.40	ng	# 0.00
13) Acenaphthene-d10	13.991	164	1675	0.40	ng	0.00
19) Phenanthrene-d10	16.763	188	3834	0.40	ng	# 0.00
29) Chrysene-d12	20.995	240	3896	0.40	ng	# 0.00
36) Perylene-d12	23.085	264	4582	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	4.954	112	1100	0.37	ng	0.00
5) Phenol-d6	6.541	99	1082	0.36	ng	0.00
8) Nitrobenzene-d5	8.502	82	795	0.30	ng	0.00
11) 2-Methylnaphthalene-d10	11.706	152	2192	0.48	ng	0.00
14) 2,4,6-Tribromophenol	15.526	330	336	0.32	ng	0.00
15) 2-Fluorobiphenyl	12.608	172	2153	0.31	ng	0.00
27) Fluoranthene-d10	18.816	212	5692	0.45	ng	0.00
31) Terphenyl-d14	19.432	244	3163	0.32	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	2.925	88	611	0.48	ng	# 90
3) n-Nitrosodimethylamine	3.263	42	709	0.34	ng	# 79
6) bis(2-Chloroethyl)ether	6.782	93	718	0.38	ng	95
9) Naphthalene	10.150	128	2496	0.31	ng	# 93
10) Hexachlorobutadiene	10.416	225	559	0.33	ng	# 99
12) 2-Methylnaphthalene	11.786	142	1635	0.30	ng	97
16) Acenaphthylene	13.712	152	2745	0.31	ng	100
17) Acenaphthene	14.054	154	1755	0.31	ng	90
18) Fluorene	15.069	166	2370	0.32	ng	100
20) 4,6-Dinitro-2-methylph...	15.222	198	171	0.35	ng	# 1
21) 4-Bromophenyl-phenylether	16.021	248	140	0.19	ng	# 87
22) Hexachlorobenzene	16.070	284	812	0.31	ng	94
23) Atrazine	16.264	200	651	0.28	ng	# 88
24) Pentachlorophenol	16.435	266	302	0.27	ng	97
25) Phenanthrene	16.812	178	3774	0.30	ng	99
26) Anthracene	16.897	178	3144	0.28	ng	99
28) Fluoranthene	18.846	202	4676	0.31	ng	98
30) Pyrene	19.213	202	4755	0.31	ng	100
32) Benzo(a)anthracene	20.984	228	4367	0.32	ng	98
33) Chrysene	21.038	228	4435	0.31	ng	98
34) Bis(2-ethylhexyl)phtha...	20.921	149	2461	0.09	ng	96
35) Indeno(1,2,3-cd)pyrene	25.122	276	6909	0.34	ng	98
37) Benzo(b)fluoranthene	22.473	252	5403	0.33	ng	# 82
38) Benzo(k)fluoranthene	22.514	252	5772	0.31	ng	# 93
39) Benzo(a)pyrene	23.000	252	5378	0.33	ng	# 86
40) Dibenzo(a,h)anthracene	25.132	278	5716	0.33	ng	# 92
41) Benzo(g,h,i)perylene	25.741	276	6097	0.33	ng	# 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122220\
Data File : BN013262.D
Acq On : 22 Dec 2020 08:35
Operator : CG/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Quant Time: Dec 22 10:47:33 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN121620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 22 10:46:43 2020
Response via : Initial Calibration







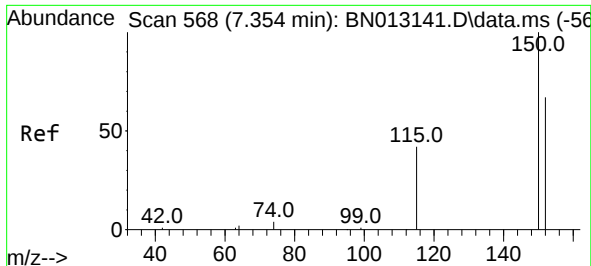

#1
1,4-Dichlorobenzene-d4
Concen: 0.40 ng
RT: 7.330 min Scan# 565
Delta R.T. -0.000 min
Lab File: BN013262.D
Acq: 22 Dec 2020 08:35




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:152 Resp: 729
Ion Ratio Lower Upper
152 100
150 144.0 116.6 174.8
115 71.9 52.9 79.3

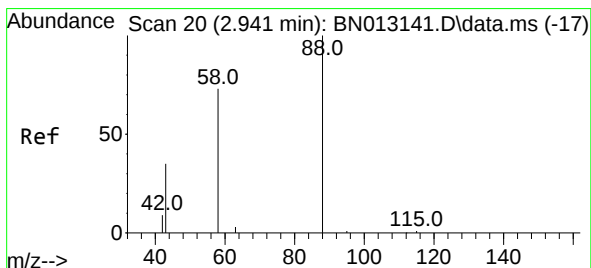

#2
1,4-Dioxane
Concen: 0.48 ng
RT: 2.925 min Scan# 18
Delta R.T. 0.000 min
Lab File: BN013262.D
Acq: 22 Dec 2020 08:35

Tgt Ion: 88 Resp: 611
Ion Ratio Lower Upper
88 100
58 74.3 59.4 89.2
43 22.7 32.3 48.5#









#3
n-Nitrosodimethylamine
Concen: 0.34 ng
RT: 3.263 min Scan# 60
Delta R.T. 0.000 min
Lab File: BN013262.D
Acq: 22 Dec 2020 08:35




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion: 42 Resp: 709
Ion Ratio Lower Upper
42 100
74 99.7 64.4 96.6#
44 0.0 2.8 4.2#



#4
2-Fluorophenol
Concen: 0.37 ng
RT: 4.954 min Scan# 270
Delta R.T. 0.000 min
Lab File: BN013262.D
Acq: 22 Dec 2020 08:35

Tgt Ion: 112 Resp: 1100
Ion Ratio Lower Upper
112 100
64 68.1 49.5 74.3
63 40.2 32.0 48.0









#5
Phenol-d6
Concen: 0.36 ng
RT: 6.541 min Scan# 467
Delta R.T. 0.000 min
Lab File: BN013262.D
Acq: 22 Dec 2020 08:35




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:	99	Resp:	1082
Ion	Ratio	Lower	Upper
99	100		
42	29.3	22.4	33.6
71	42.8	37.8	56.6



#6
bis(2-Chloroethyl)ether
Concen: 0.38 ng
RT: 6.782 min Scan# 497
Delta R.T. 0.000 min
Lab File: BN013262.D
Acq: 22 Dec 2020 08:35

Tgt Ion:	93	Resp:	718
Ion	Ratio	Lower	Upper
93	100		
63	75.9	63.1	94.7
95	27.7	26.1	39.1









#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.099 min Scan# 828
Delta R.T. 0.000 min
Lab File: BN013262.D
Acq: 22 Dec 2020 08:35




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:136	Resp:	2589
Ion Ratio	Lower	Upper
136	100	
137	15.0	10.6 15.8
54	12.7	8.6 12.8
68	9.6	5.7 8.5#



#8
Nitrobenzene-d5
Concen: 0.30 ng
RT: 8.502 min Scan# 702
Delta R.T. 0.000 min
Lab File: BN013262.D
Acq: 22 Dec 2020 08:35

Tgt Ion: 82	Resp:	795
Ion Ratio	Lower	Upper
82	100	
128	46.2	30.6 46.0#
54	69.5	48.3 72.5









#9
Naphthalene
Concen: 0.31 ng
RT: 10.150 min Scan# 832
Delta R.T. 0.000 min
Lab File: BN013262.D
Acq: 22 Dec 2020 08:35




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:128 Resp: 2496
Ion Ratio Lower Upper
128 100
129 15.7 9.8 14.8#
127 17.6 12.2 18.4



#10
Hexachlorobutadiene
Concen: 0.33 ng
RT: 10.416 min Scan# 853
Delta R.T. 0.000 min
Lab File: BN013262.D
Acq: 22 Dec 2020 08:35

Tgt Ion:225 Resp: 559
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 64.4 51.0 76.6









#11
2-Methylnaphthalene-d10
Concen: 0.48 ng
RT: 11.706 min Scan# 984
Delta R.T. 0.000 min
Lab File: BN013262.D
Acq: 22 Dec 2020 08:35




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:152 Resp: 2192
Ion Ratio Lower Upper
152 100
151 20.2 16.7 25.1



#12
2-Methylnaphthalene
Concen: 0.30 ng
RT: 11.786 min Scan# 1002
Delta R.T. 0.000 min
Lab File: BN013262.D
Acq: 22 Dec 2020 08:35

Tgt Ion:142 Resp: 1635
Ion Ratio Lower Upper
142 100
141 88.8 69.4 104.2
115 48.3 35.7 53.5









#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 13.991 min Scan# 1281
Delta R.T. 0.000 min
Lab File: BN013262.D
Acq: 22 Dec 2020 08:35




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:164 Resp: 1675
Ion Ratio Lower Upper
164 100
162 106.2 80.6 120.8
160 52.7 39.5 59.3



#14
2,4,6-Tribromophenol
Concen: 0.32 ng
RT: 15.526 min Scan# 1402
Delta R.T. 0.000 min
Lab File: BN013262.D
Acq: 22 Dec 2020 08:35

Tgt Ion:330 Resp: 336
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 44.0 34.4 51.6









#15
2-Fluorobiphenyl
Concen: 0.31 ng
RT: 12.608 min Scan# 1172
Delta R.T. 0.000 min
Lab File: BN013262.D
Acq: 22 Dec 2020 08:35




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:	172	Resp:	2153
Ion Ratio	Lower	Upper	
172	100		
171	39.9	28.2	42.4
170	27.1	20.0	30.0



#16
Acenaphthylene
Concen: 0.31 ng
RT: 13.712 min Scan# 1259
Delta R.T. 0.000 min
Lab File: BN013262.D
Acq: 22 Dec 2020 08:35

Tgt Ion:	152	Resp:	2745
Ion Ratio	Lower	Upper	
152	100		
151	19.6	15.8	23.8
153	13.4	10.6	16.0









#17
Acenaphthene
Concen: 0.31 ng
RT: 14.054 min Scan# 1286
Delta R.T. 0.000 min
Lab File: BN013262.D
Acq: 22 Dec 2020 08:35




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:154 Resp: 1755
Ion Ratio Lower Upper
154 100
153 117.1 83.6 125.4
152 59.5 43.9 65.9



#18
Fluorene
Concen: 0.32 ng
RT: 15.069 min Scan# 1366
Delta R.T. 0.000 min
Lab File: BN013262.D
Acq: 22 Dec 2020 08:35

Tgt Ion:166 Resp: 2370
Ion Ratio Lower Upper
166 100
165 98.6 78.6 118.0
167 13.2 10.7 16.1









#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 16.763 min Scan# 1502
Delta R.T. 0.000 min
Lab File: BN013262.D
Acq: 22 Dec 2020 08:35




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:188 Resp: 3834
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 10.7 5.0 7.4#



#20
4,6-Dinitro-2-methylphenol
Concen: 0.35 ng
RT: 15.222 min Scan# 1378
Delta R.T. 0.000 min
Lab File: BN013262.D
Acq: 22 Dec 2020 08:35

Tgt Ion:198 Resp: 171
Ion Ratio Lower Upper
198 100
51 157.6 43.5 65.3#
105 91.8 27.2 40.8#









#21
4-Bromophenyl-phenylether
Concen: 0.19 ng
RT: 16.021 min Scan# 1441
Delta R.T. 0.000 min
Lab File: BN013262.D
Acq: 22 Dec 2020 08:35




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:248 Resp: 140
Ion Ratio Lower Upper
248 100
250 101.4 77.3 115.9
141 92.9 57.8 86.8#



#22
Hexachlorobenzene
Concen: 0.31 ng
RT: 16.070 min Scan# 1445
Delta R.T. 0.000 min
Lab File: BN013262.D
Acq: 22 Dec 2020 08:35

Tgt Ion:284 Resp: 812
Ion Ratio Lower Upper
284 100
142 35.1 32.0 48.0
249 31.8 27.0 40.6









#23
Atrazine
 Concen: 0.28 ng
 RT: 16.264 min Scan# 1461
 Delta R.T. 0.000 min
 Lab File: BN013262.D
 Acq: 22 Dec 2020 08:35




Instrument :
 BNA_N
ClientSampled :
 SSTDCCC0.4


Tgt Ion:	200	Resp:	651
Ion Ratio	Lower	Upper	
200	100		
173	34.6	22.8	34.2#
215	55.8	38.1	57.1



#24
Pentachlorophenol
 Concen: 0.27 ng
 RT: 16.435 min Scan# 1475
 Delta R.T. 0.000 min
 Lab File: BN013262.D
 Acq: 22 Dec 2020 08:35

Tgt Ion:	266	Resp:	302
Ion Ratio	Lower	Upper	
266	100		
264	67.5	50.9	76.3
268	65.9	51.5	77.3









#25
Phenanthrene
Concen: 0.30 ng
RT: 16.812 min Scan# 1506
Delta R.T. 0.000 min
Lab File: BN013262.D
Acq: 22 Dec 2020 08:35




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:178 Resp: 3774
Ion Ratio Lower Upper
178 100
176 19.1 14.8 22.2
179 15.9 12.4 18.6



#26
Anthracene
Concen: 0.28 ng
RT: 16.897 min Scan# 1513
Delta R.T. 0.000 min
Lab File: BN013262.D
Acq: 22 Dec 2020 08:35

Tgt Ion:178 Resp: 3144
Ion Ratio Lower Upper
178 100
176 18.6 14.8 22.2
179 16.0 12.5 18.7









#27
Fluoranthene-d10
Concen: 0.45 ng
RT: 18.816 min Scan# 1766
Delta R.T. 0.000 min
Lab File: BN013262.D
Acq: 22 Dec 2020 08:35




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:212 Resp: 5692
Ion Ratio Lower Upper
212 100
106 9.5 6.8 10.2
104 5.5 4.1 6.1



#28
Fluoranthene
Concen: 0.31 ng
RT: 18.846 min Scan# 1772
Delta R.T. 0.000 min
Lab File: BN013262.D
Acq: 22 Dec 2020 08:35

Tgt Ion:202 Resp: 4676
Ion Ratio Lower Upper
202 100
101 8.1 5.8 8.6
203 16.6 13.7 20.5





#29

Chrysene-d12

Concen: 0.40 ng

RT: 20.995 min Scan# 2099





Delta R.T. 0.000 min

Lab File: BN013262.D

Acq: 22 Dec 2020 08:35

Tgt Ion:240	Resp:	3896
Ion Ratio	Lower	Upper
240	100	
120	11.0	5.3 7.9#
236	28.3	21.8 32.8

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4



#30

Pyrene

Concen: 0.31 ng




RT: 19.213 min Scan# 1846


Delta R.T. 0.000 min

Lab File: BN013262.D

Acq: 22 Dec 2020 08:35

Tgt Ion:202	Resp:	4755
Ion Ratio	Lower	Upper
202	100	
200	20.8	16.6 24.8
203	17.5	13.8 20.8









#31
 Terphenyl-d14
 Concen: 0.32 ng
 RT: 19.432 min Scan# 1890
 Delta R.T. 0.000 min
 Lab File: BN013262.D
 Acq: 22 Dec 2020 08:35




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4


Tgt Ion:244 Resp: 3163
 Ion Ratio Lower Upper
 244 100
 212 10.9 7.3 10.9#
 122 13.2 7.3 10.9#



#32
 Benzo(a)anthracene
 Concen: 0.32 ng
 RT: 20.984 min Scan# 2098
 Delta R.T. 0.000 min
 Lab File: BN013262.D
 Acq: 22 Dec 2020 08:35

Tgt Ion:228 Resp: 4367
 Ion Ratio Lower Upper
 228 100
 226 27.3 22.3 33.5
 229 21.4 15.7 23.5





#33

Chrysene

Concen: 0.31 ng

RT: 21.038 min Scan# 2103

Delta R.T. 0.000 min

Lab File: BN013262.D

Acq: 22 Dec 2020 08:35





Tgt Ion:228 Resp: 4435

Ion Ratio Lower Upper

228 100

226 30.5 24.2 36.2

229 21.3 15.7 23.5



#34

Bis(2-ethylhexyl)phthalate

Concen: 0.09 ng

RT: 20.921 min Scan# 2092

Delta R.T. 0.000 min

Lab File: BN013262.D

Acq: 22 Dec 2020 08:35




Tgt Ion:149 Resp: 2461


Ion Ratio Lower Upper

149 100

167 26.7 23.2 34.8

279 4.7 3.9 5.9









#35
Indeno(1,2,3-cd)pyrene
Concen: 0.34 ng
RT: 25.122 min Scan# 3025
Delta R.T. 0.000 min
Lab File: BN013262.D
Acq: 22 Dec 2020 08:35




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:276 Resp: 6909
Ion Ratio Lower Upper
276 100
138 16.3 13.3 19.9
277 23.5 20.2 30.4



#36
Perylene-d12
Concen: 0.40 ng
RT: 23.085 min Scan# 2430
Delta R.T. 0.000 min
Lab File: BN013262.D
Acq: 22 Dec 2020 08:35

Tgt Ion:264 Resp: 4582
Ion Ratio Lower Upper
264 100
260 25.9 19.8 29.6
265 63.2 51.4 77.0









#37
Benzo(b)fluoranthene
Concen: 0.33 ng
RT: 22.473 min Scan# 2251
Delta R.T. 0.000 min
Lab File: BN013262.D
Acq: 22 Dec 2020 08:35




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:252 Resp: 5403
Ion Ratio Lower Upper
252 100
253 30.1 20.1 30.1#
125 23.0 7.2 10.8#



#38
Benzo(k)fluoranthene
Concen: 0.31 ng
RT: 22.514 min Scan# 2263
Delta R.T. 0.000 min
Lab File: BN013262.D
Acq: 22 Dec 2020 08:35

Tgt Ion:252 Resp: 5772
Ion Ratio Lower Upper
252 100
253 28.3 19.8 29.8
125 11.3 7.1 10.7#





#39

Benzo(a)pyrene

Concen: 0.33 ng

RT: 23.000 min Scan# 2405

Delta R.T. 0.000 min

Lab File: BN013262.D

Acq: 22 Dec 2020 08:35





Tgt Ion:	252	Resp:	5378
Ion Ratio	Lower	Upper	
252	100		
253	32.2	21.3	31.9#
125	18.7	8.3	12.5#

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4



#40

Dibenzo(a,h)anthracene

Concen: 0.33 ng




RT: 25.132 min Scan# 3028


Delta R.T. 0.000 min

Lab File: BN013262.D

Acq: 22 Dec 2020 08:35


Tgt Ion:	278	Resp:	5716
Ion Ratio	Lower	Upper	
278	100		
139	15.8	9.3	13.9#
279	30.2	21.6	32.4





#41
Benzo(g,h,i)perylene
Concen: 0.33 ng
RT: 25.741 min Scan# 3206
Delta R.T. 0.000 min
Lab File: BN013262.D
Acq: 22 Dec 2020 08:35

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4



Tgt Ion: 276 Resp: 6097
Ion Ratio Lower Upper
276 100
277 27.0 19.8 29.8
138 18.2 11.7 17.5#

