
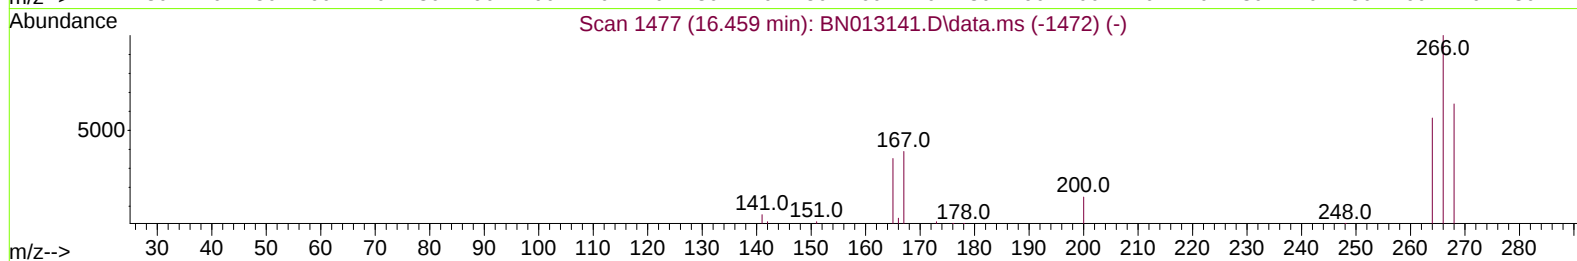
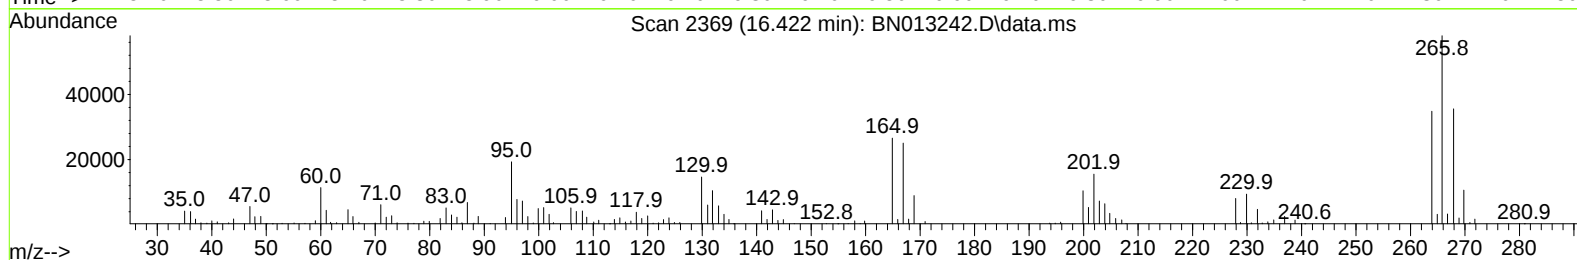


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122220\
 Data File : BN013242.D
 Acq On : 21 Dec 2020 18:04
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 22 04:35:38 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN121620.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 18 16:11:20 2020
 Response via : Initial Calibration

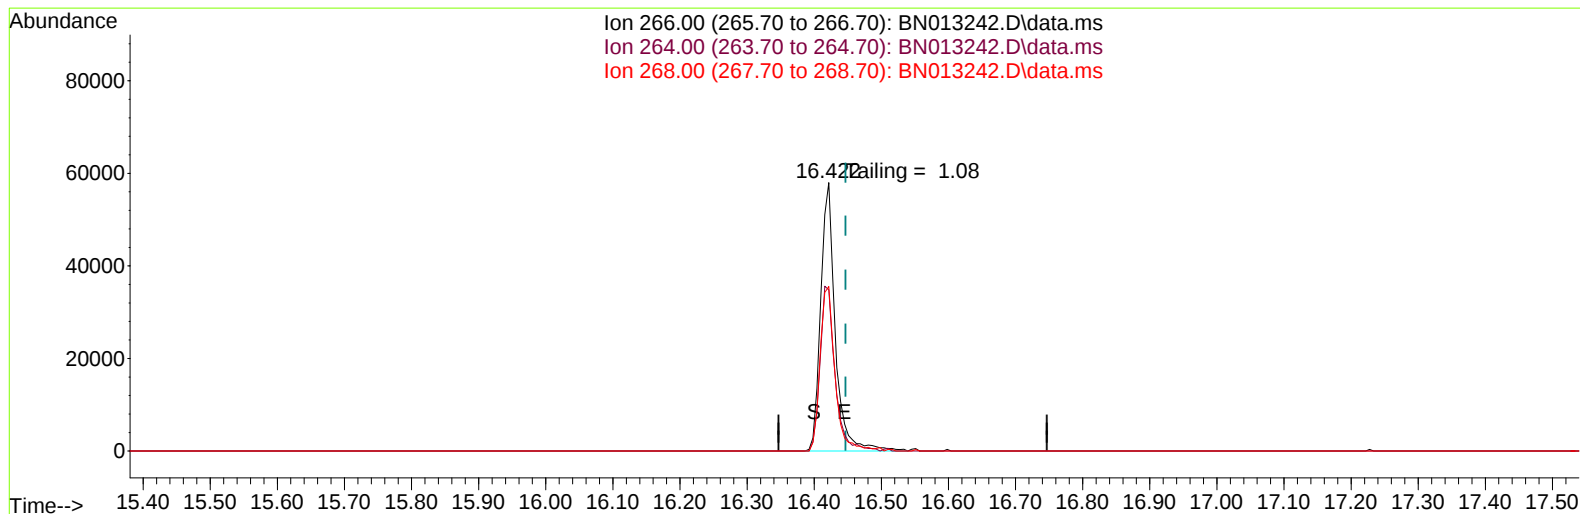

TIC: BN013242.D\data.ms

(24) Pentachlorophenol

16.422min (-0.025) 0.00 ng

response 87652

Ion	Exp%	Act%
266.00	100.00	100.00
264.00	63.60	62.68
268.00	64.40	63.23
0.00	0.00	0.00