
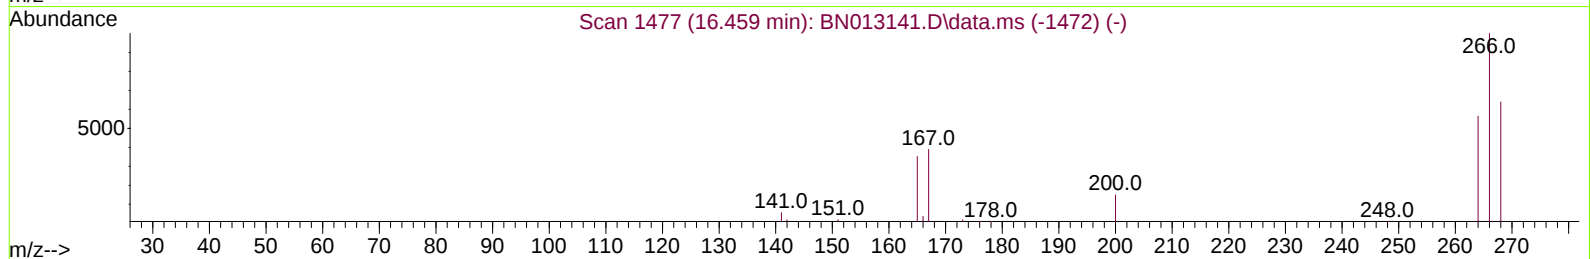
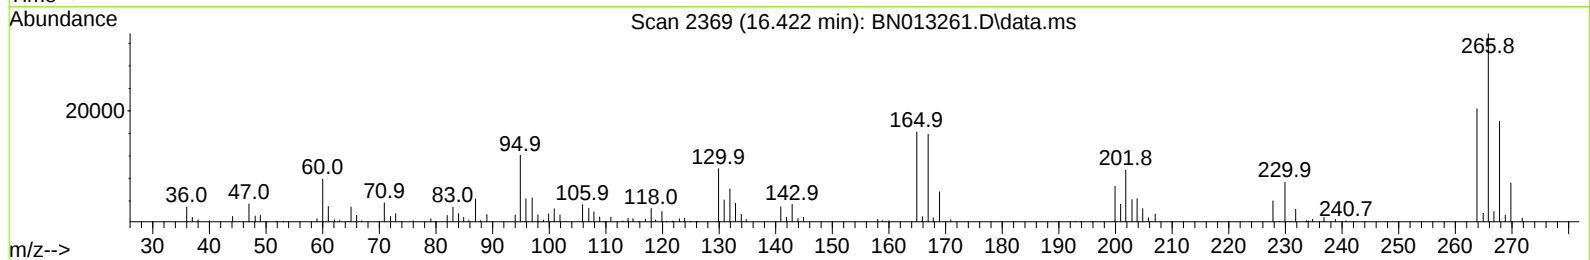


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122220\
Data File : BN013261.D
Acq On : 22 Dec 2020 06:42
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 23 03:34:37 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN121620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 22 10:46:43 2020
Response via : Initial Calibration

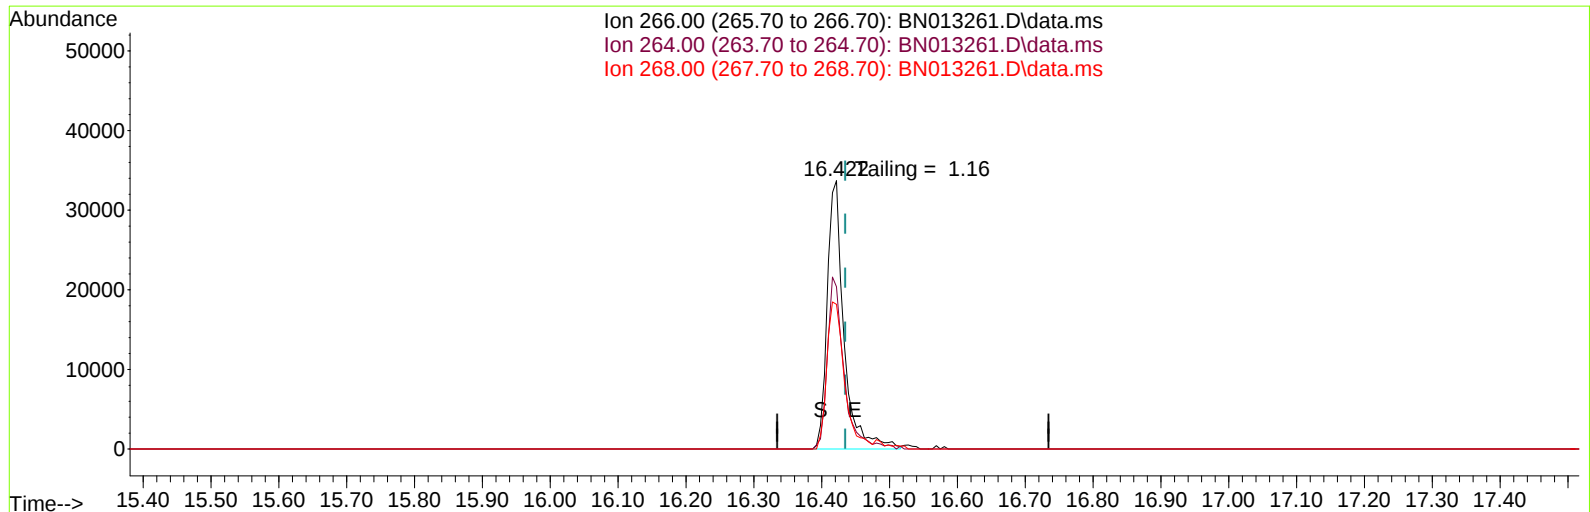

TIC: BN013261.D\data.ms

(24) Pentachlorophenol

16.422min (-0.013) 0.00 ng

response 57574

Ion	Exp%	Act%
266.00	100.00	100.00
264.00	63.60	63.92
268.00	64.40	57.90
0.00	0.00	0.00