

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122220\
 Data File : BN013260.D
 Acq On : 22 Dec 2020 05:30
 Operator : CG/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC

Quant Time: Dec 22 06:04:27 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN121620.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 18 16:11:20 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.330	152	812	0.40	ng	-0.02
7) Naphthalene-d8	10.099	136	2478	0.40	ng	#-0.01
13) Acenaphthene-d10	13.991	164	1637	0.40	ng	-0.01
19) Phenanthrene-d10	16.763	188	3746	0.40	ng	#-0.01
29) Chrysene-d12	20.995	240	3804	0.40	ng	#-0.01
36) Perylene-d12	23.085	264	4505	0.40	ng	-0.01
System Monitoring Compounds						
4) 2-Fluorophenol	4.954	112	1065	0.32	ng	0.00
5) Phenol-d6	6.541	99	1129	0.33	ng	0.00
8) Nitrobenzene-d5	8.502	82	951	0.37	ng	-0.03
11) 2-Methylnaphthalene-d10	11.711	152	2100	0.48	ng	-0.01
14) 2,4,6-Tribromophenol	15.526	330	329	0.32	ng	-0.01
15) 2-Fluorobiphenyl	12.621	172	2074	0.30	ng	-0.01
27) Fluoranthene-d10	18.811	212	5623	0.46	ng	0.00
31) Terphenyl-d14	19.432	244	3044	0.32	ng	-0.01
Target Compounds						Qvalue
2) 1,4-Dioxane	2.933	88	604	0.43	ng	# 88
3) n-Nitrosodimethylamine	3.271	42	666	0.28	ng	# 77
6) bis(2-Chloroethyl)ether	6.790	93	628	0.30	ng	# 84
9) Naphthalene	10.150	128	2443	0.32	ng	# 94
10) Hexachlorobutadiene	10.416	225	518	0.32	ng	# 99
12) 2-Methylnaphthalene	11.786	142	1618	0.31	ng	95
16) Acenaphthylene	13.712	152	2603	0.30	ng	99
17) Acenaphthene	14.067	154	1724	0.32	ng	92
18) Fluorene	15.069	166	2268	0.32	ng	100
20) 4,6-Dinitro-2-methylph...	15.222	198	163	0.34	ng	# 1
21) 4-Bromophenyl-phenylether	16.021	248	139	0.19	ng	# 81
22) Hexachlorobenzene	16.070	284	786	0.31	ng	95
23) Atrazine	16.264	200	624	0.28	ng	# 90
24) Pentachlorophenol	16.447	266	311	0.29	ng	97
25) Phenanthrene	16.812	178	3701	0.30	ng	100
26) Anthracene	16.897	178	3150	0.29	ng	99
28) Fluoranthene	18.846	202	4598	0.31	ng	99
30) Pyrene	19.213	202	4670	0.32	ng	99
32) Benzo(a)anthracene	20.985	228	3919	0.29	ng	98
33) Chrysene	21.027	228	4751	0.33	ng	98
34) Bis(2-ethylhexyl)phtha...	20.921	149	2386	0.09	ng	97
35) Indeno(1,2,3-cd)pyrene	25.122	276	6559	0.33	ng	97
37) Benzo(b)fluoranthene	22.469	252	5172	0.33	ng	# 84
38) Benzo(k)fluoranthene	22.510	252	5717	0.31	ng	# 92
39) Benzo(a)pyrene	22.993	252	5158	0.33	ng	# 83
40) Dibenzo(a,h)anthracene	25.132	278	5467	0.32	ng	# 90
41) Benzo(g,h,i)perylene	25.741	276	5980	0.33	ng	# 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122220\
Data File : BN013260.D
Acq On : 22 Dec 2020 05:30
Operator : CG/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Quant Time: Dec 22 06:04:27 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN121620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 18 16:11:20 2020
Response via : Initial Calibration




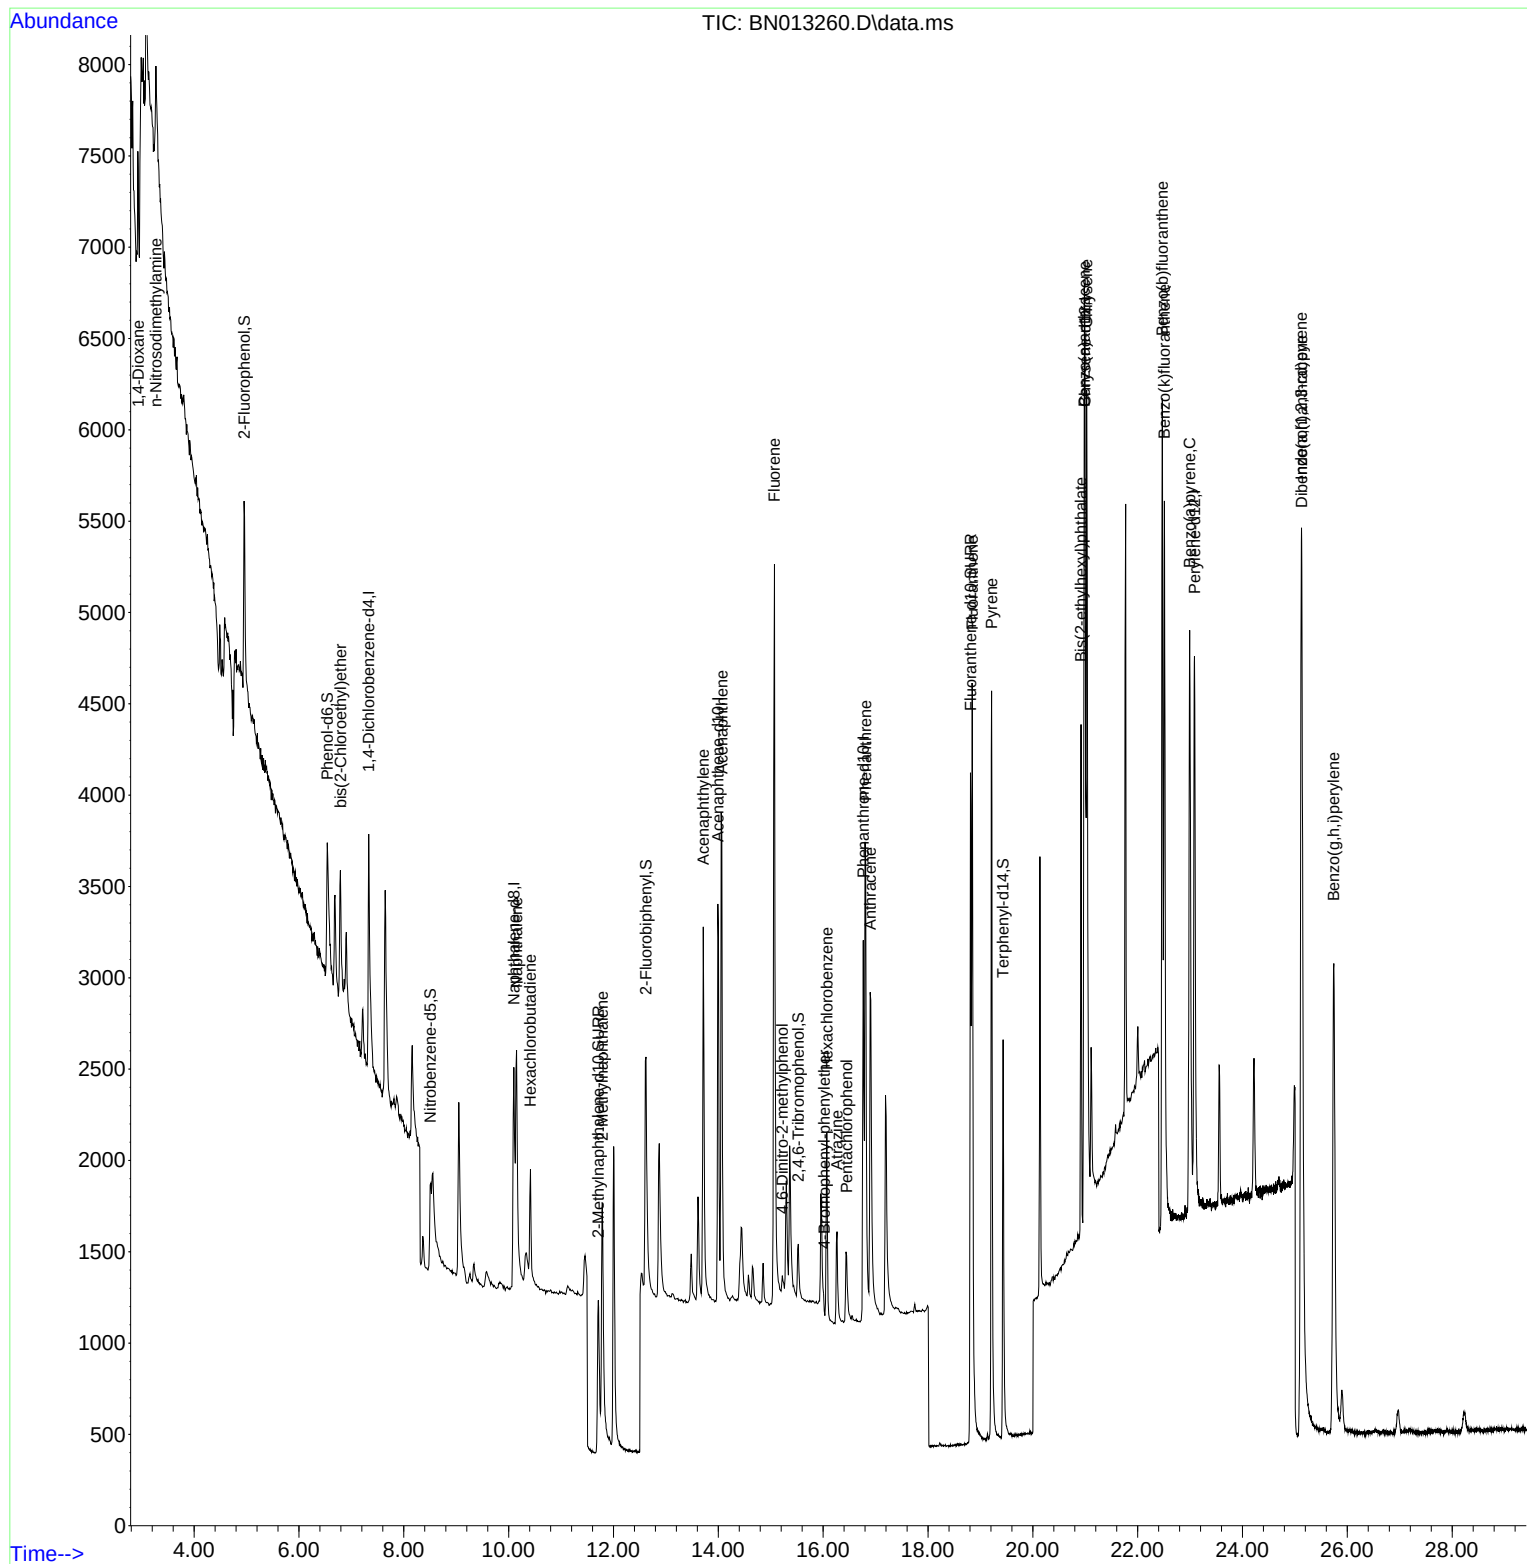


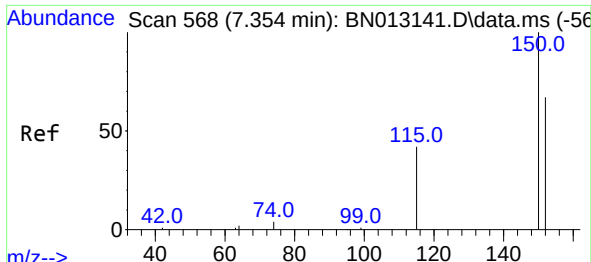

#1
1,4-Dichlorobenzene-d4
Concen: 0.40 ng
RT: 7.330 min Scan# 565
Delta R.T. -0.016 min
Lab File: BN013260.D
Acq: 22 Dec 2020 05:30




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:152 Resp: 812
Ion Ratio Lower Upper
152 100
150 150.6 116.6 174.8
115 75.5 52.9 79.3

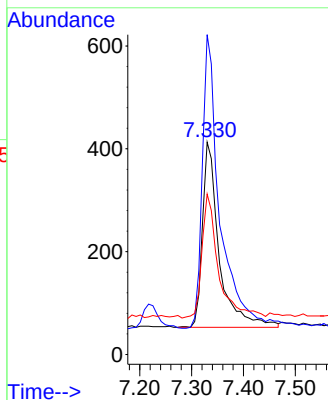

#2
1,4-Dioxane
Concen: 0.43 ng
RT: 2.933 min Scan# 19
Delta R.T. 0.000 min
Lab File: BN013260.D
Acq: 22 Dec 2020 05:30

Tgt Ion: 88 Resp: 604
Ion Ratio Lower Upper
88 100
58 68.5 59.4 89.2
43 27.3 32.3 48.5#


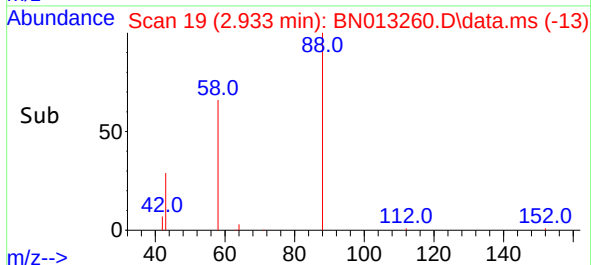
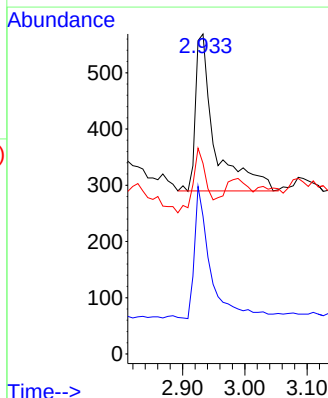
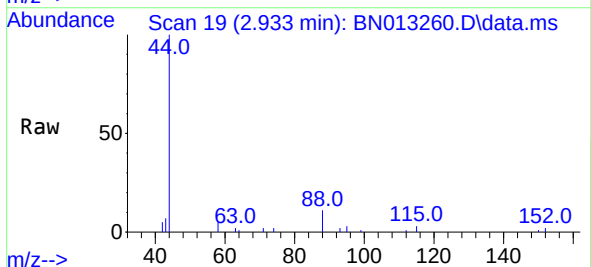




#3
n-Nitrosodimethylamine
Concen: 0.28 ng
RT: 3.271 min Scan# 61
Delta R.T. -0.008 min
Lab File: BN013260.D
Acq: 22 Dec 2020 05:30




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion: 42 Resp: 666
Ion Ratio Lower Upper
42 100
74 101.4 64.4 96.6#
44 0.0 2.8 4.2#

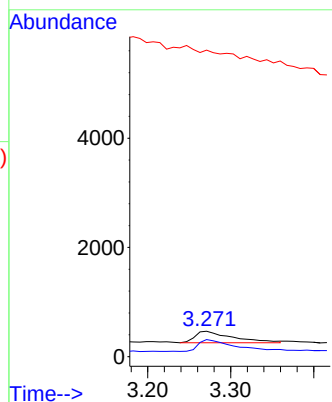

#4
2-Fluorophenol
Concen: 0.32 ng
RT: 4.954 min Scan# 270
Delta R.T. -0.008 min
Lab File: BN013260.D
Acq: 22 Dec 2020 05:30

Tgt Ion: 112 Resp: 1065
Ion Ratio Lower Upper
112 100
64 64.9 49.5 74.3
63 37.6 32.0 48.0

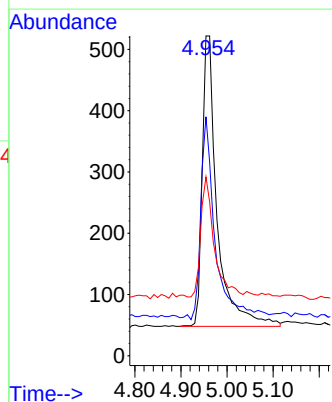







#5
Phenol-d6
Concen: 0.33 ng
RT: 6.541 min Scan# 467
Delta R.T. -0.008 min
Lab File: BN013260.D
Acq: 22 Dec 2020 05:30

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion: 99 Resp: 1129




Ion	Ratio	Lower	Upper
99	100		
42	27.5	22.4	33.6
71	42.7	37.8	56.6




#6
bis(2-Chloroethyl)ether
Concen: 0.30 ng
RT: 6.790 min Scan# 498
Delta R.T. -0.008 min
Lab File: BN013260.D
Acq: 22 Dec 2020 05:30

Tgt Ion: 93 Resp: 628

Ion	Ratio	Lower	Upper
93	100		
63	93.3	63.1	94.7
95	40.9	26.1	39.1









#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.099 min Scan# 828
Delta R.T. -0.013 min
Lab File: BN013260.D
Acq: 22 Dec 2020 05:30




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:	136	Resp:	2478
Ion	Ratio	Lower	Upper
136	100		
137	15.3	10.6	15.8
54	13.6	8.6	12.8#
68	9.7	5.7	8.5#

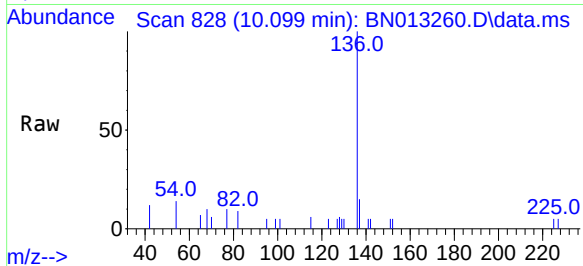

#8
Nitrobenzene-d5
Concen: 0.37 ng
RT: 8.502 min Scan# 702
Delta R.T. -0.025 min
Lab File: BN013260.D
Acq: 22 Dec 2020 05:30

Tgt Ion:	82	Resp:	951
Ion	Ratio	Lower	Upper
82	100		
128	43.1	30.6	46.0
54	72.1	48.3	72.5




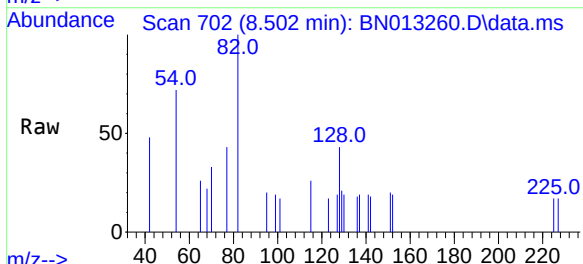


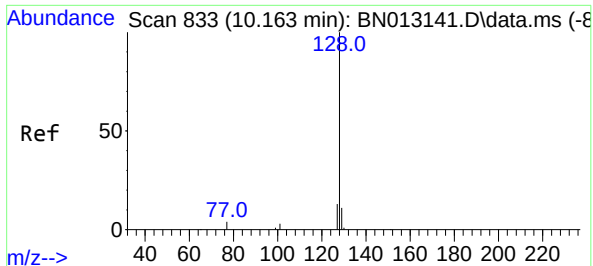

#9
Naphthalene
Concen: 0.32 ng
RT: 10.150 min Scan# 832
Delta R.T. -0.013 min
Lab File: BN013260.D
Acq: 22 Dec 2020 05:30




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:	128	Resp:	2443
Ion Ratio	Lower	Upper	
128	100		
129	14.9	9.8	14.8#
127	17.9	12.2	18.4

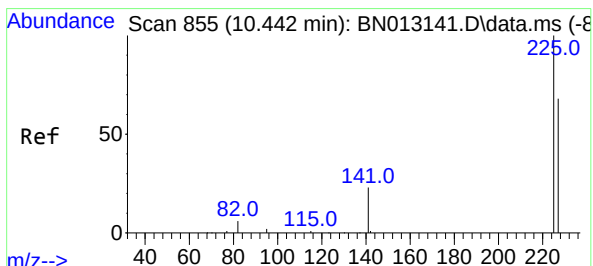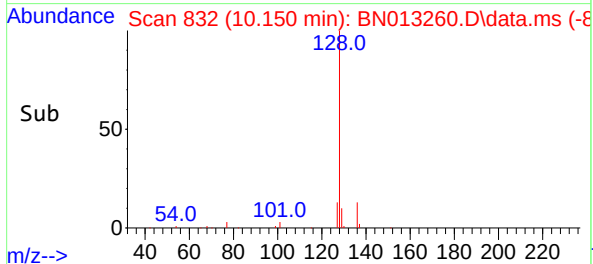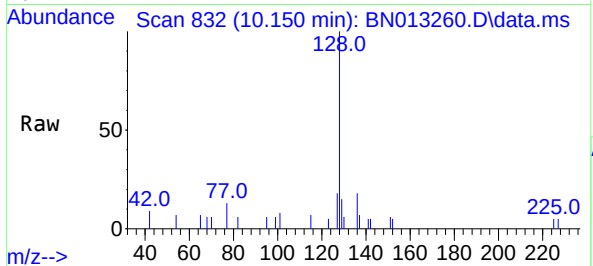

#10
Hexachlorobutadiene
Concen: 0.32 ng
RT: 10.416 min Scan# 853
Delta R.T. 0.000 min
Lab File: BN013260.D
Acq: 22 Dec 2020 05:30

Tgt Ion:	225	Resp:	518
Ion Ratio	Lower	Upper	
225	100		
223	0.0	0.0	0.0
227	64.9	51.0	76.6


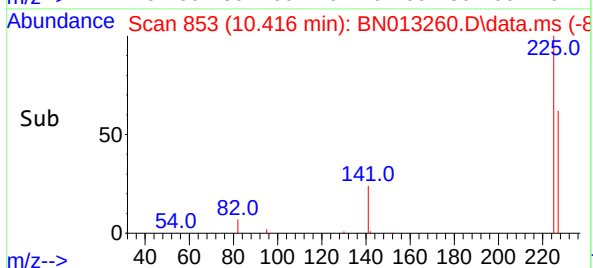
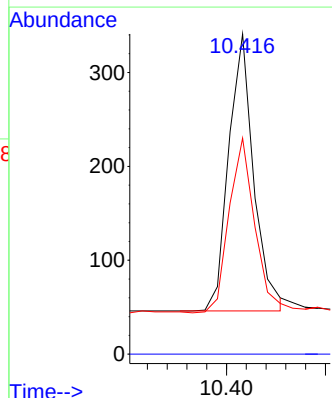
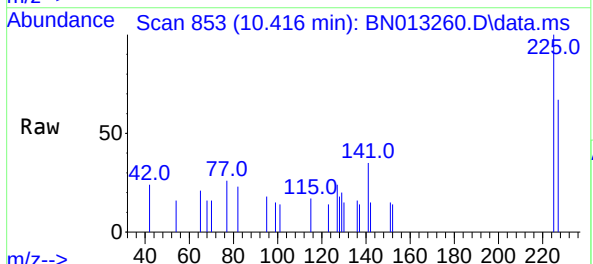


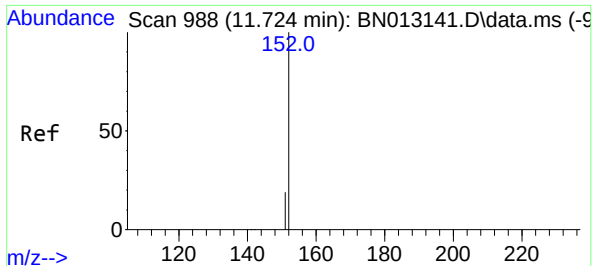

#11
2-Methylnaphthalene-d10
Concen: 0.48 ng
RT: 11.711 min Scan# 985
Delta R.T. -0.013 min
Lab File: BN013260.D
Acq: 22 Dec 2020 05:30




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:152 Resp: 2100
Ion Ratio Lower Upper
152 100
151 19.4 16.7 25.1

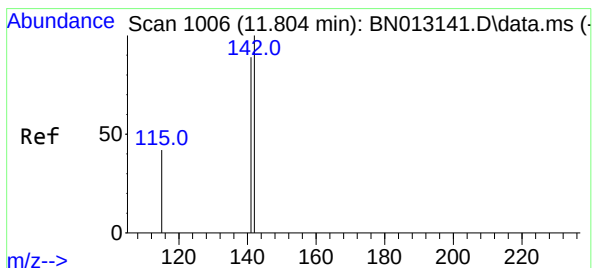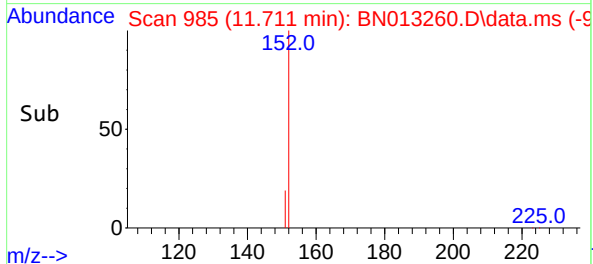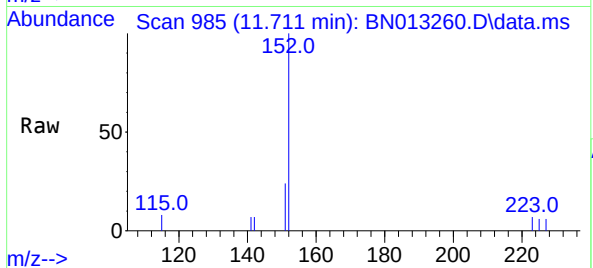

#12
2-Methylnaphthalene
Concen: 0.31 ng
RT: 11.786 min Scan# 1002
Delta R.T. -0.018 min
Lab File: BN013260.D
Acq: 22 Dec 2020 05:30

Tgt Ion:142 Resp: 1618
Ion Ratio Lower Upper
142 100
141 89.9 69.4 104.2
115 50.6 35.7 53.5

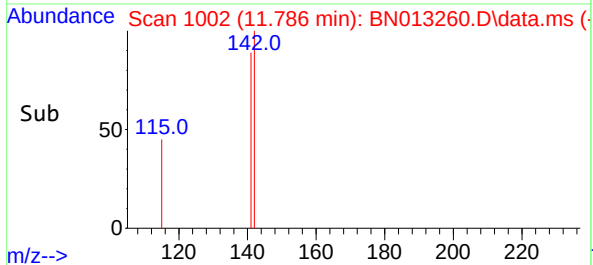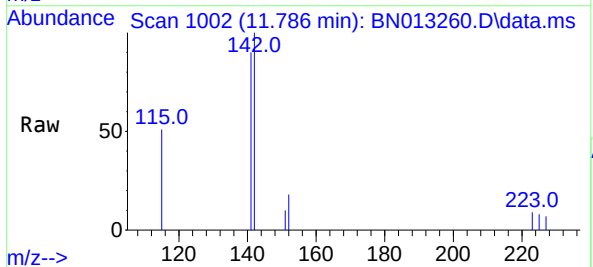







#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 13.991 min Scan# 1281
Delta R.T. -0.013 min
Lab File: BN013260.D
Acq: 22 Dec 2020 05:30

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion:164 Resp: 1637




Ion	Ratio	Lower	Upper
164	100		
162	104.8	80.6	120.8
160	52.7	39.5	59.3

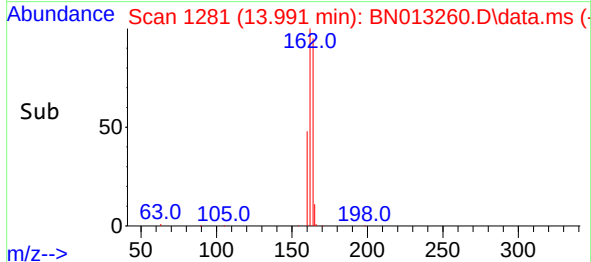


#14
2,4,6-Tribromophenol
Concen: 0.32 ng
RT: 15.526 min Scan# 1402
Delta R.T. -0.013 min
Lab File: BN013260.D
Acq: 22 Dec 2020 05:30

Tgt Ion:330 Resp: 329

Ion	Ratio	Lower	Upper
330	100		
332	0.0	0.0	0.0
141	38.0	34.4	51.6


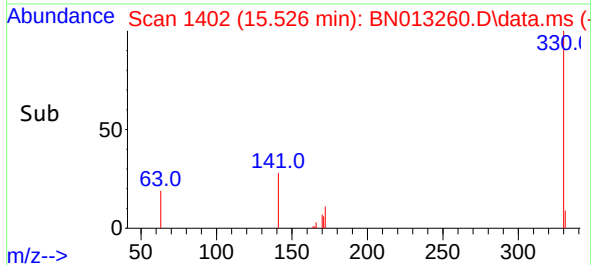

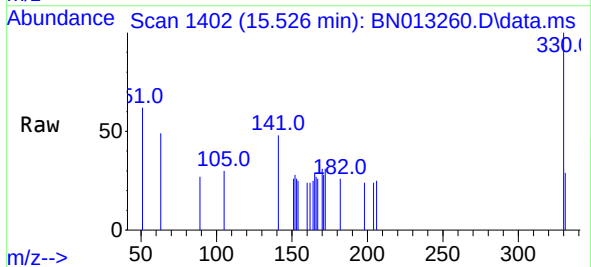




#15
2-Fluorobiphenyl
Concen: 0.30 ng
RT: 12.621 min Scan# 1173
Delta R.T. -0.013 min
Lab File: BN013260.D
Acq: 22 Dec 2020 05:30




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:	172	Resp:	2074
Ion	Ratio	Lower	Upper
172	100		
171	38.4	28.2	42.4
170	27.7	20.0	30.0

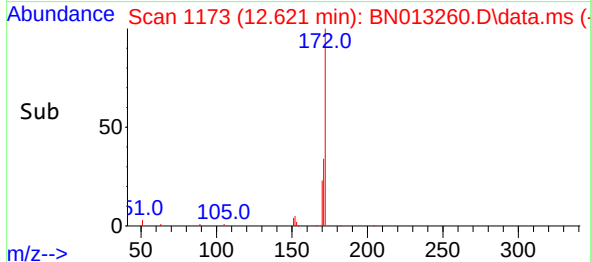

#16
Acenaphthylene
Concen: 0.30 ng
RT: 13.712 min Scan# 1259
Delta R.T. -0.013 min
Lab File: BN013260.D
Acq: 22 Dec 2020 05:30

Tgt Ion:	152	Resp:	2603
Ion	Ratio	Lower	Upper
152	100		
151	19.9	15.8	23.8
153	13.8	10.6	16.0


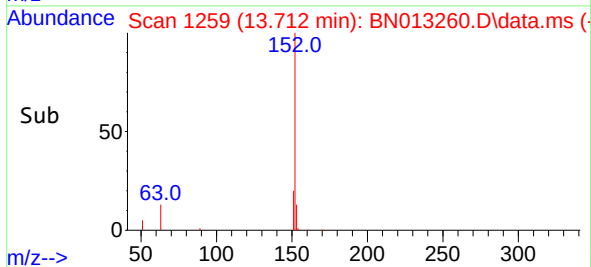

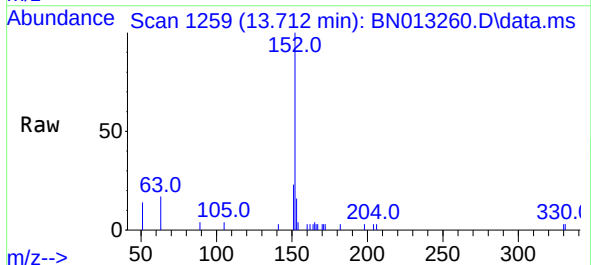




#17
Acenaphthene
Concen: 0.32 ng
RT: 14.067 min Scan# 1287
Delta R.T. 0.000 min
Lab File: BN013260.D
Acq: 22 Dec 2020 05:30




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:154 Resp: 1724
Ion Ratio Lower Upper
154 100
153 115.5 83.6 125.4
152 57.8 43.9 65.9

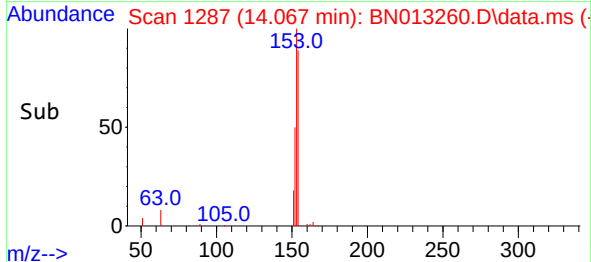

#18
Fluorene
Concen: 0.32 ng
RT: 15.069 min Scan# 1366
Delta R.T. 0.000 min
Lab File: BN013260.D
Acq: 22 Dec 2020 05:30

Tgt Ion:166 Resp: 2268
Ion Ratio Lower Upper
166 100
165 98.0 78.6 118.0
167 13.4 10.7 16.1









#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 16.763 min Scan# 1502
Delta R.T. -0.012 min
Lab File: BN013260.D
Acq: 22 Dec 2020 05:30




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:188 Resp: 3746
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 10.7 5.0 7.4#

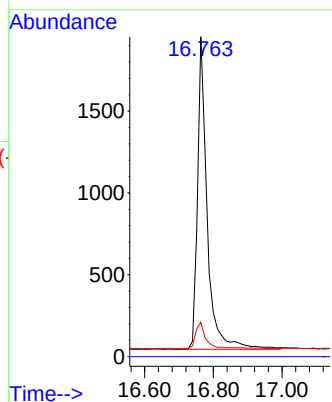

#20
4,6-Dinitro-2-methylphenol
Concen: 0.34 ng
RT: 15.222 min Scan# 1378
Delta R.T. -0.038 min
Lab File: BN013260.D
Acq: 22 Dec 2020 05:30

Tgt Ion:198 Resp: 163
Ion Ratio Lower Upper
198 100
51 170.6 43.5 65.3#
105 84.7 27.2 40.8#






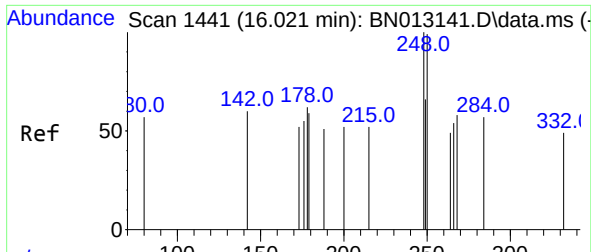


#21
4-Bromophenyl-phenylether
Concen: 0.19 ng
RT: 16.021 min Scan# 1441
Delta R.T. 0.000 min
Lab File: BN013260.D
Acq: 22 Dec 2020 05:30

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion:248 Resp: 139




Ion	Ratio	Lower	Upper
248	100		
250	102.9	77.3	115.9
141	101.5	57.8	86.8#

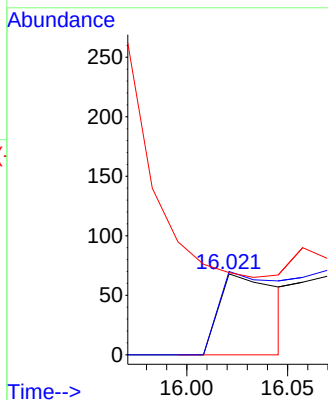


#22
Hexachlorobenzene
Concen: 0.31 ng
RT: 16.070 min Scan# 1445
Delta R.T. -0.012 min
Lab File: BN013260.D
Acq: 22 Dec 2020 05:30

Tgt Ion:284 Resp: 786

Ion	Ratio	Lower	Upper
284	100		
142	36.6	32.0	48.0
249	31.6	27.0	40.6


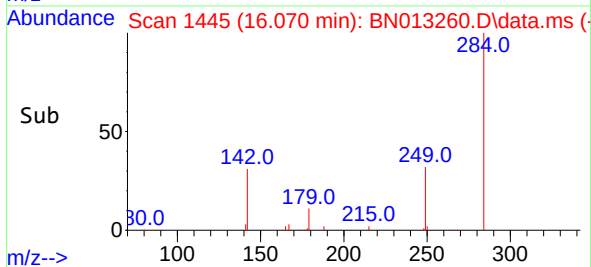
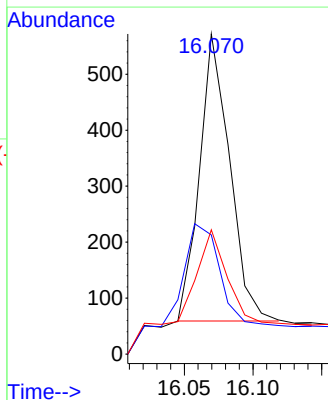
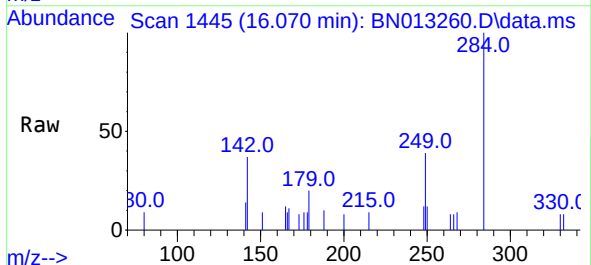




#23
Atrazine
Concen: 0.28 ng
RT: 16.264 min Scan# 1461
Delta R.T. -0.012 min
Lab File: BN013260.D
Acq: 22 Dec 2020 05:30




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:200 Resp: 624
Ion Ratio Lower Upper
200 100
173 34.2 22.8 34.2#
215 54.1 38.1 57.1

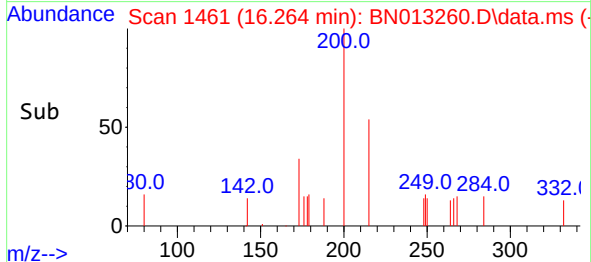

#24
Pentachlorophenol
Concen: 0.29 ng
RT: 16.447 min Scan# 1476
Delta R.T. 0.000 min
Lab File: BN013260.D
Acq: 22 Dec 2020 05:30

Tgt Ion:266 Resp: 311
Ion Ratio Lower Upper
266 100
264 62.4 50.9 76.3
268 60.5 51.5 77.3


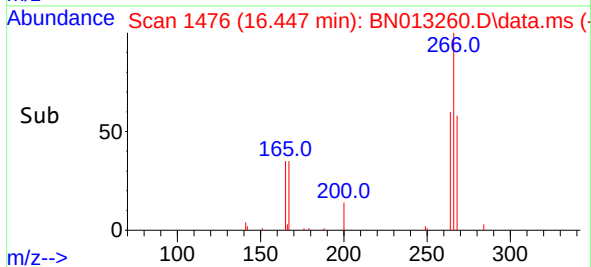

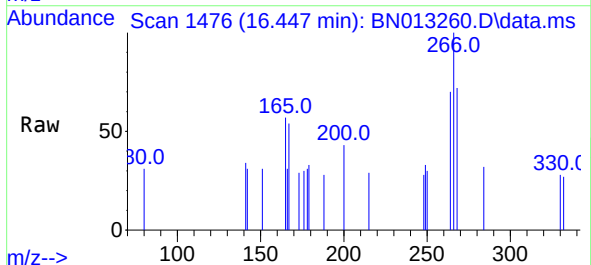




#25
Phenanthrene
Concen: 0.30 ng
RT: 16.812 min Scan# 1506
Delta R.T. 0.000 min
Lab File: BN013260.D
Acq: 22 Dec 2020 05:30




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:178	Resp:	3701	
Ion	Ratio	Lower	Upper
178	100		
176	18.5	14.8	22.2
179	15.1	12.4	18.6



#26
Anthracene
Concen: 0.29 ng
RT: 16.897 min Scan# 1513
Delta R.T. -0.024 min
Lab File: BN013260.D
Acq: 22 Dec 2020 05:30

Tgt Ion:178	Resp:	3150	
Ion	Ratio	Lower	Upper
178	100		
176	18.6	14.8	22.2
179	16.0	12.5	18.7









#27
Fluoranthene-d10
Concen: 0.46 ng
RT: 18.811 min Scan# 1765
Delta R.T. -0.010 min
Lab File: BN013260.D
Acq: 22 Dec 2020 05:30




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:212 Resp: 5623
Ion Ratio Lower Upper
212 100
106 9.1 6.8 10.2
104 5.8 4.1 6.1



#28
Fluoranthene
Concen: 0.31 ng
RT: 18.846 min Scan# 1772
Delta R.T. -0.010 min
Lab File: BN013260.D
Acq: 22 Dec 2020 05:30

Tgt Ion:202 Resp: 4598
Ion Ratio Lower Upper
202 100
101 7.9 5.8 8.6
203 17.3 13.7 20.5









#29
Chrysene-d12
Concen: 0.40 ng
RT: 20.995 min Scan# 2099
Delta R.T. -0.011 min
Lab File: BN013260.D
Acq: 22 Dec 2020 05:30




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:240 Resp: 3804
Ion Ratio Lower Upper
240 100
120 9.5 5.3 7.9#
236 28.1 21.8 32.8



#30
Pyrene
Concen: 0.32 ng
RT: 19.213 min Scan# 1846
Delta R.T. -0.010 min
Lab File: BN013260.D
Acq: 22 Dec 2020 05:30

Tgt Ion:202 Resp: 4670
Ion Ratio Lower Upper
202 100
200 20.6 16.6 24.8
203 18.5 13.8 20.8









#31
Terphenyl-d14
Concen: 0.32 ng
RT: 19.432 min Scan# 1890
Delta R.T. -0.015 min
Lab File: BN013260.D
Acq: 22 Dec 2020 05:30




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:244 Resp: 3044
Ion Ratio Lower Upper
244 100
212 10.4 7.3 10.9
122 11.7 7.3 10.9#



#32
Benzo(a)anthracene
Concen: 0.29 ng
RT: 20.985 min Scan# 2098
Delta R.T. -0.011 min
Lab File: BN013260.D
Acq: 22 Dec 2020 05:30

Tgt Ion:228 Resp: 3919
Ion Ratio Lower Upper
228 100
226 27.8 22.3 33.5
229 21.9 15.7 23.5







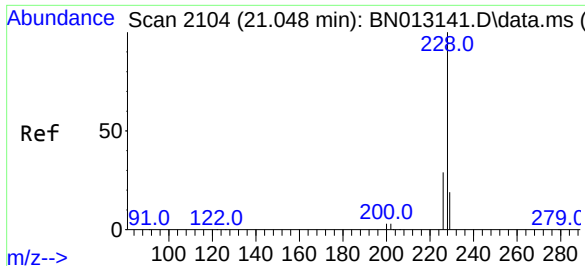

#33
Chrysene
Concen: 0.33 ng
RT: 21.027 min Scan# 2102
Delta R.T. -0.011 min
Lab File: BN013260.D
Acq: 22 Dec 2020 05:30




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:228	Resp:	4751
Ion Ratio	Lower	Upper
228	100	
226	31.5	24.2 36.2
229	20.7	15.7 23.5

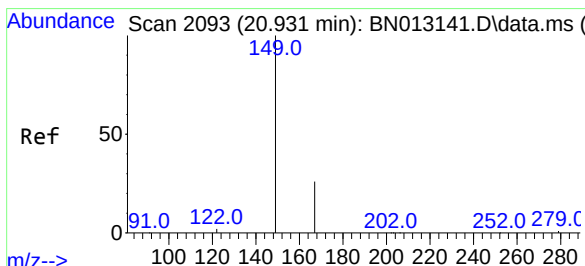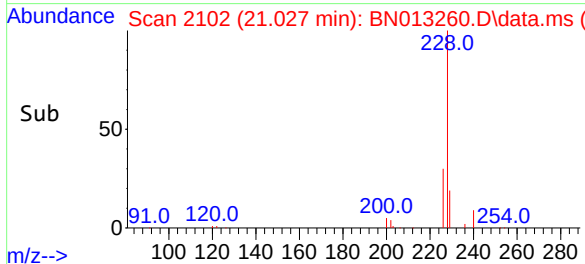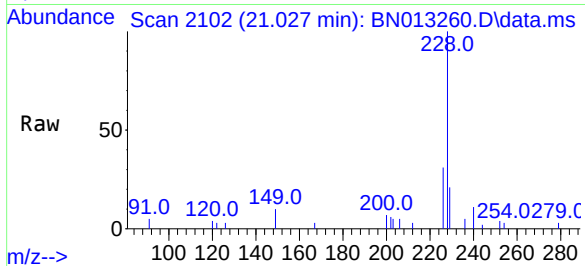

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.09 ng
RT: 20.921 min Scan# 2092
Delta R.T. 0.000 min
Lab File: BN013260.D
Acq: 22 Dec 2020 05:30

Tgt Ion:149	Resp:	2386
Ion Ratio	Lower	Upper
149	100	
167	27.5	23.2 34.8
279	4.5	3.9 5.9


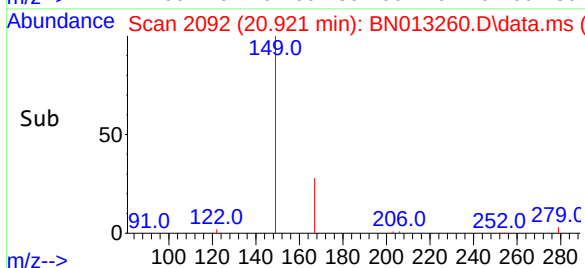
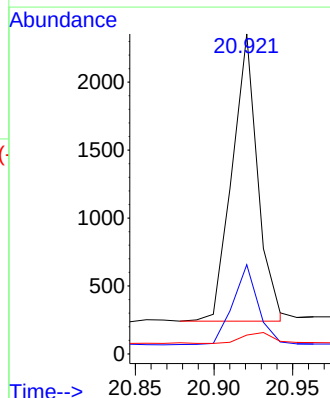
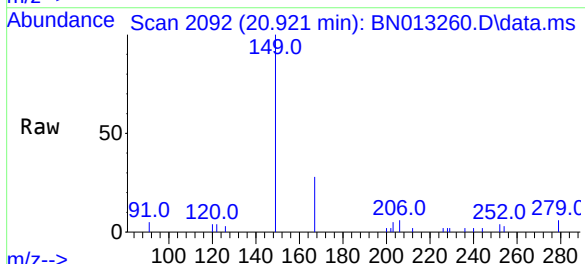




#35
Indeno(1,2,3-cd)pyrene
Concen: 0.33 ng
RT: 25.122 min Scan# 3025
Delta R.T. -0.010 min
Lab File: BN013260.D
Acq: 22 Dec 2020 05:30




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:276 Resp: 6559
Ion Ratio Lower Upper
276 100
138 16.1 13.3 19.9
277 22.8 20.2 30.4

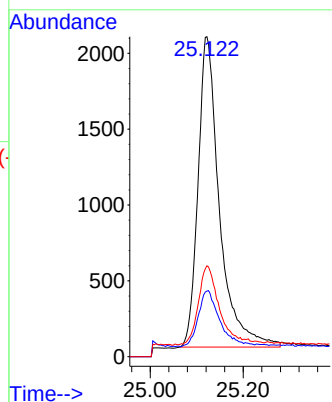

#36
Perylene-d12
Concen: 0.40 ng
RT: 23.085 min Scan# 2430
Delta R.T. -0.010 min
Lab File: BN013260.D
Acq: 22 Dec 2020 05:30

Tgt Ion:264 Resp: 4505
Ion Ratio Lower Upper
264 100
260 26.0 19.8 29.6
265 65.6 51.4 77.0




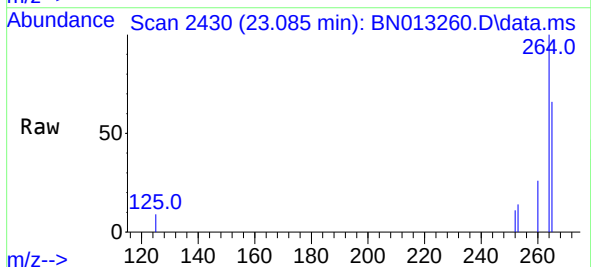




#37
Benzo(b)fluoranthene
Concen: 0.33 ng
RT: 22.469 min Scan# 2250
Delta R.T. -0.010 min
Lab File: BN013260.D
Acq: 22 Dec 2020 05:30




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:252 Resp: 5172
Ion Ratio Lower Upper
252 100
253 30.1 20.1 30.1#
125 21.2 7.2 10.8#

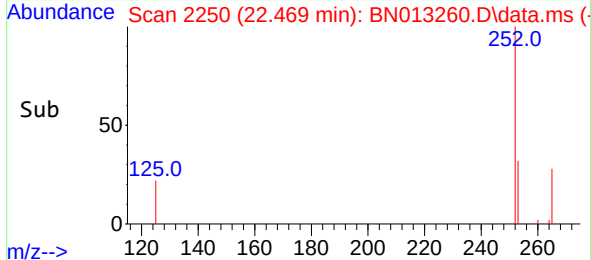

#38
Benzo(k)fluoranthene
Concen: 0.31 ng
RT: 22.510 min Scan# 2262
Delta R.T. -0.007 min
Lab File: BN013260.D
Acq: 22 Dec 2020 05:30

Tgt Ion:252 Resp: 5717
Ion Ratio Lower Upper
252 100
253 28.7 19.8 29.8
125 11.9 7.1 10.7#

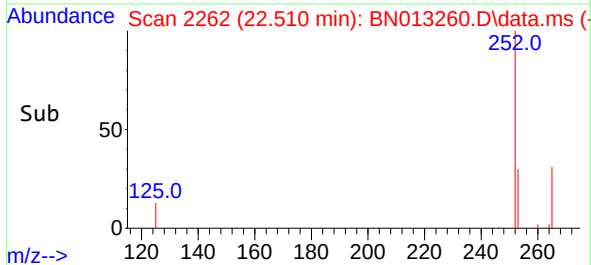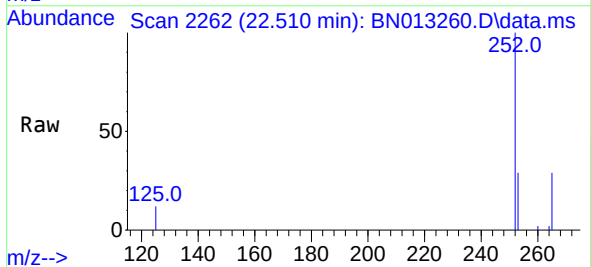



#39

Benzo(a)pyrene

Concen: 0.33 ng

RT: 22.993 min Scan# 2403

Delta R.T. -0.014 min

Lab File: BN013260.D

Acq: 22 Dec 2020 05:30





Tgt Ion:	252	Resp:	5158
Ion Ratio	Lower	Upper	
252	100		
253	32.9	21.3	31.9#
125	21.6	8.3	12.5#

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4EC



#40

Dibenzo(a,h)anthracene

Concen: 0.32 ng




RT: 25.132 min Scan# 3028


Delta R.T. -0.020 min

Lab File: BN013260.D

Acq: 22 Dec 2020 05:30

Tgt Ion:	278	Resp:	5467
Ion Ratio	Lower	Upper	
278	100		
139	16.1	9.3	13.9#
279	31.9	21.6	32.4

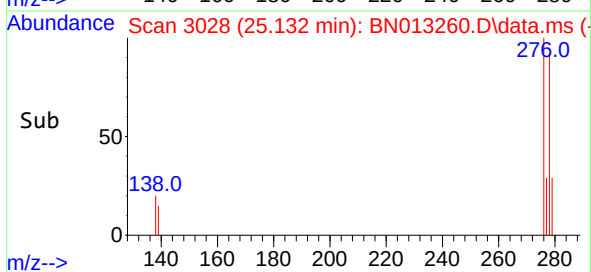

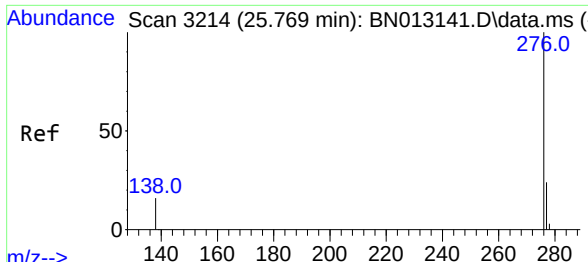

#41
Benzo(g,h,i)perylene
Concen: 0.33 ng
RT: 25.741 min Scan# 3206
Delta R.T. -0.007 min
Lab File: BN013260.D
Acq: 22 Dec 2020 05:30

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion:276 Resp: 5980
Ion Ratio Lower Upper
276 100
277 26.1 19.8 29.8
138 18.5 11.7 17.5#

