
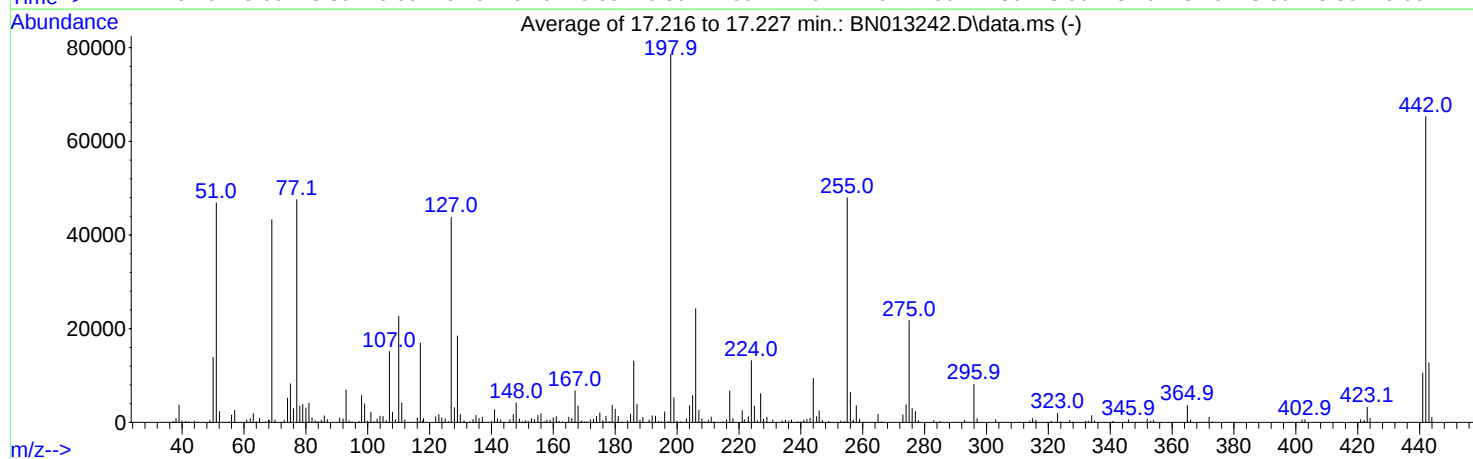


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122220\
 Data File : BN013242.D
 Acq On : 21 Dec 2020 18:04
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN121620.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 22 10:46:43 2020

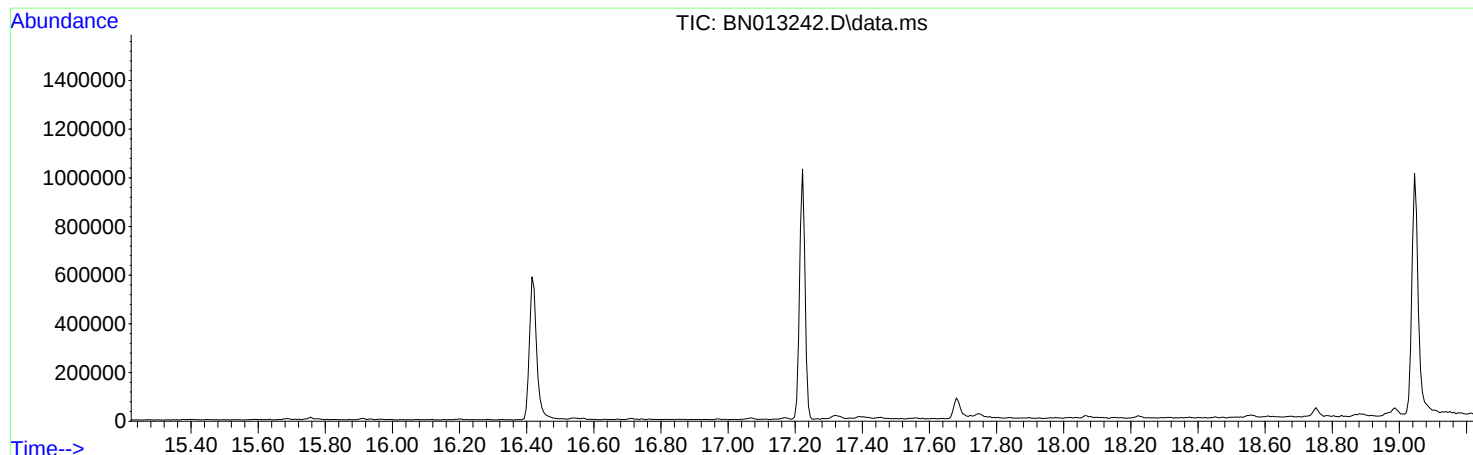

AutoFind: Scans 2504, 2505, 2506; Background Corrected with Scan 2498

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	59.7	46877	PASS
68	69	0.00	2	1.3	565	PASS
69	198	0.00	100	55.1	43265	PASS
70	69	0.00	2	1.2	502	PASS
127	198	10	80	55.7	43779	PASS
197	198	0.00	2	0.3	212	PASS
198	198	100	100	100.0	78536	PASS
199	198	5	9	6.7	5260	PASS
275	198	10	60	27.7	21755	PASS
365	198	1	100	4.6	3638	PASS
441	198	0.01	100	13.5	10568	PASS
442	442	50	100	100.0	65285	PASS
443	442	15	24	19.5	12712	PASS