


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122220\
 Data File : BN013261.D
 Acq On : 22 Dec 2020 06:42
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN121620.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 22 10:46:43 2020

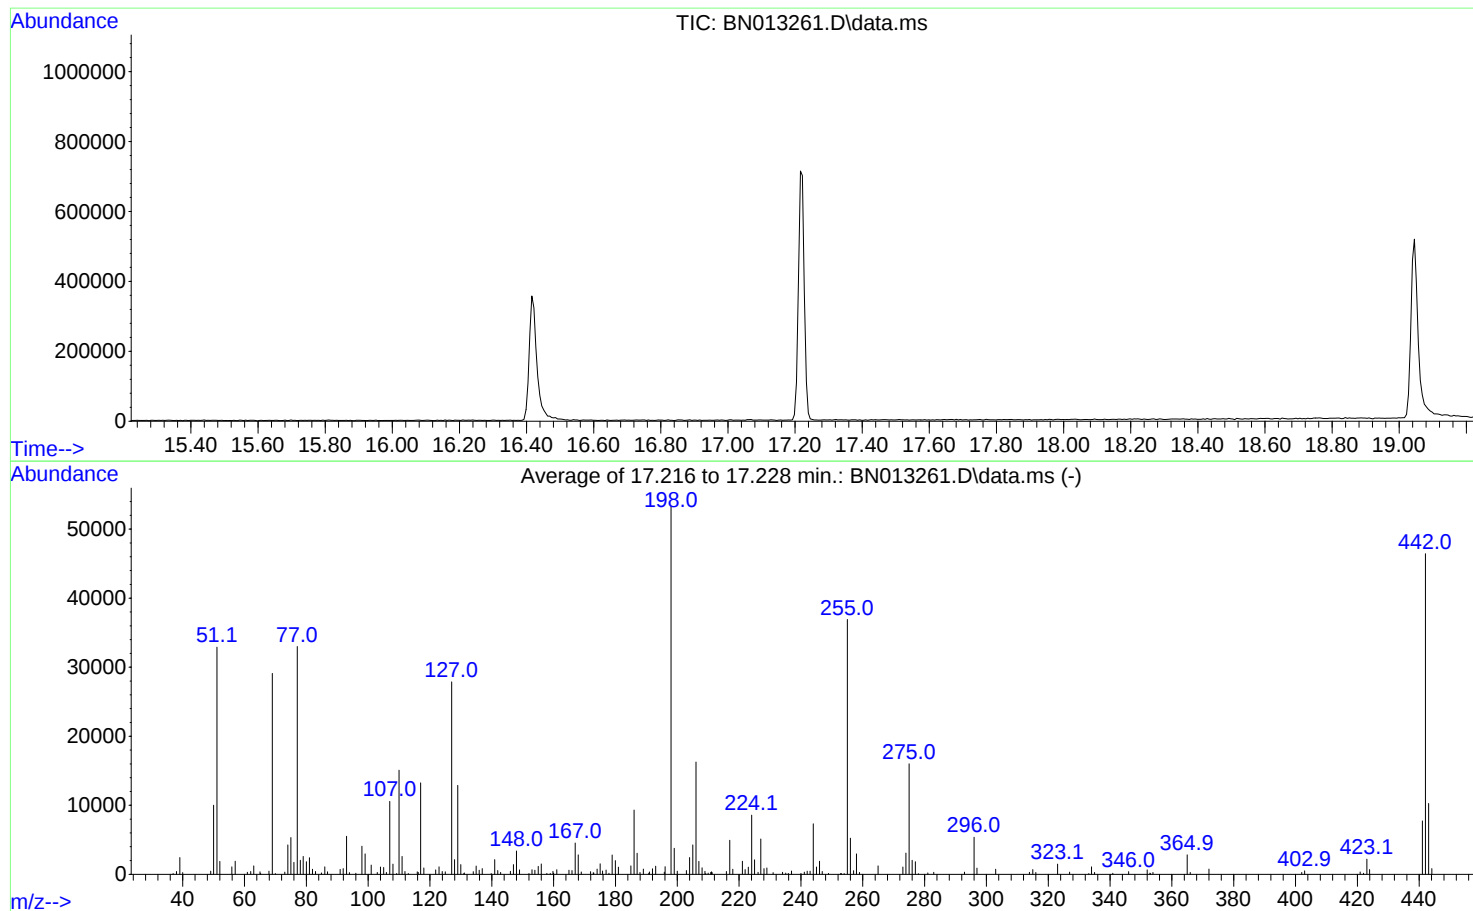

AutoFind: Scans 2504, 2505, 2506; Background Corrected with Scan 2498

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	61.8	32901	PASS
68	69	0.00	2	1.6	475	PASS
69	198	0.00	100	54.6	29099	PASS
70	69	0.00	2	0.4	116	PASS
127	198	10	80	52.3	27869	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	53277	PASS
199	198	5	9	7.1	3786	PASS
275	198	10	60	30.1	16025	PASS
365	198	1	100	5.3	2839	PASS
441	198	0.01	100	14.5	7735	PASS
442	442	50	100	100.0	46437	PASS
443	442	15	24	22.1	10278	PASS