

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122222\
 Data File : BN023346.D
 Acq On : 22 Dec 2022 19:20
 Operator : CG/JU
 Sample : PB149668BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK668

Quant Time: Dec 22 23:54:46 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 22 02:28:40 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.998	152	6309	0.400	ng/ul	0.00
4) Naphthalene-d8	10.815	136	21050	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.645	164	12619	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.394	188	29783	0.400	ng/ul	0.00
17) Chrysene-d12	21.578	240	23177	0.400	ng/ul	0.00
23) Perylene-d12	24.025	264	19246	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.345	96	36704	5.354	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.405	152	9675	0.297	ng/ul	0.00
18) Fluoranthene-d10	19.420	212	24069	0.287	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.640	166	3160	0.060	ng/ul#	14
20) Pyrene	19.787	202	3064	0.027	ng/ul#	1
26) Benzo(a)pyrene	23.870	252	5484	0.070	ng/ul#	54


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122222\
Data File : BN023346.D
Acq On : 22 Dec 2022 19:20
Operator : CG/JU
Sample : PB149668BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK668

Quant Time: Dec 22 23:54:46 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 22 02:28:40 2022
Response via : Initial Calibration




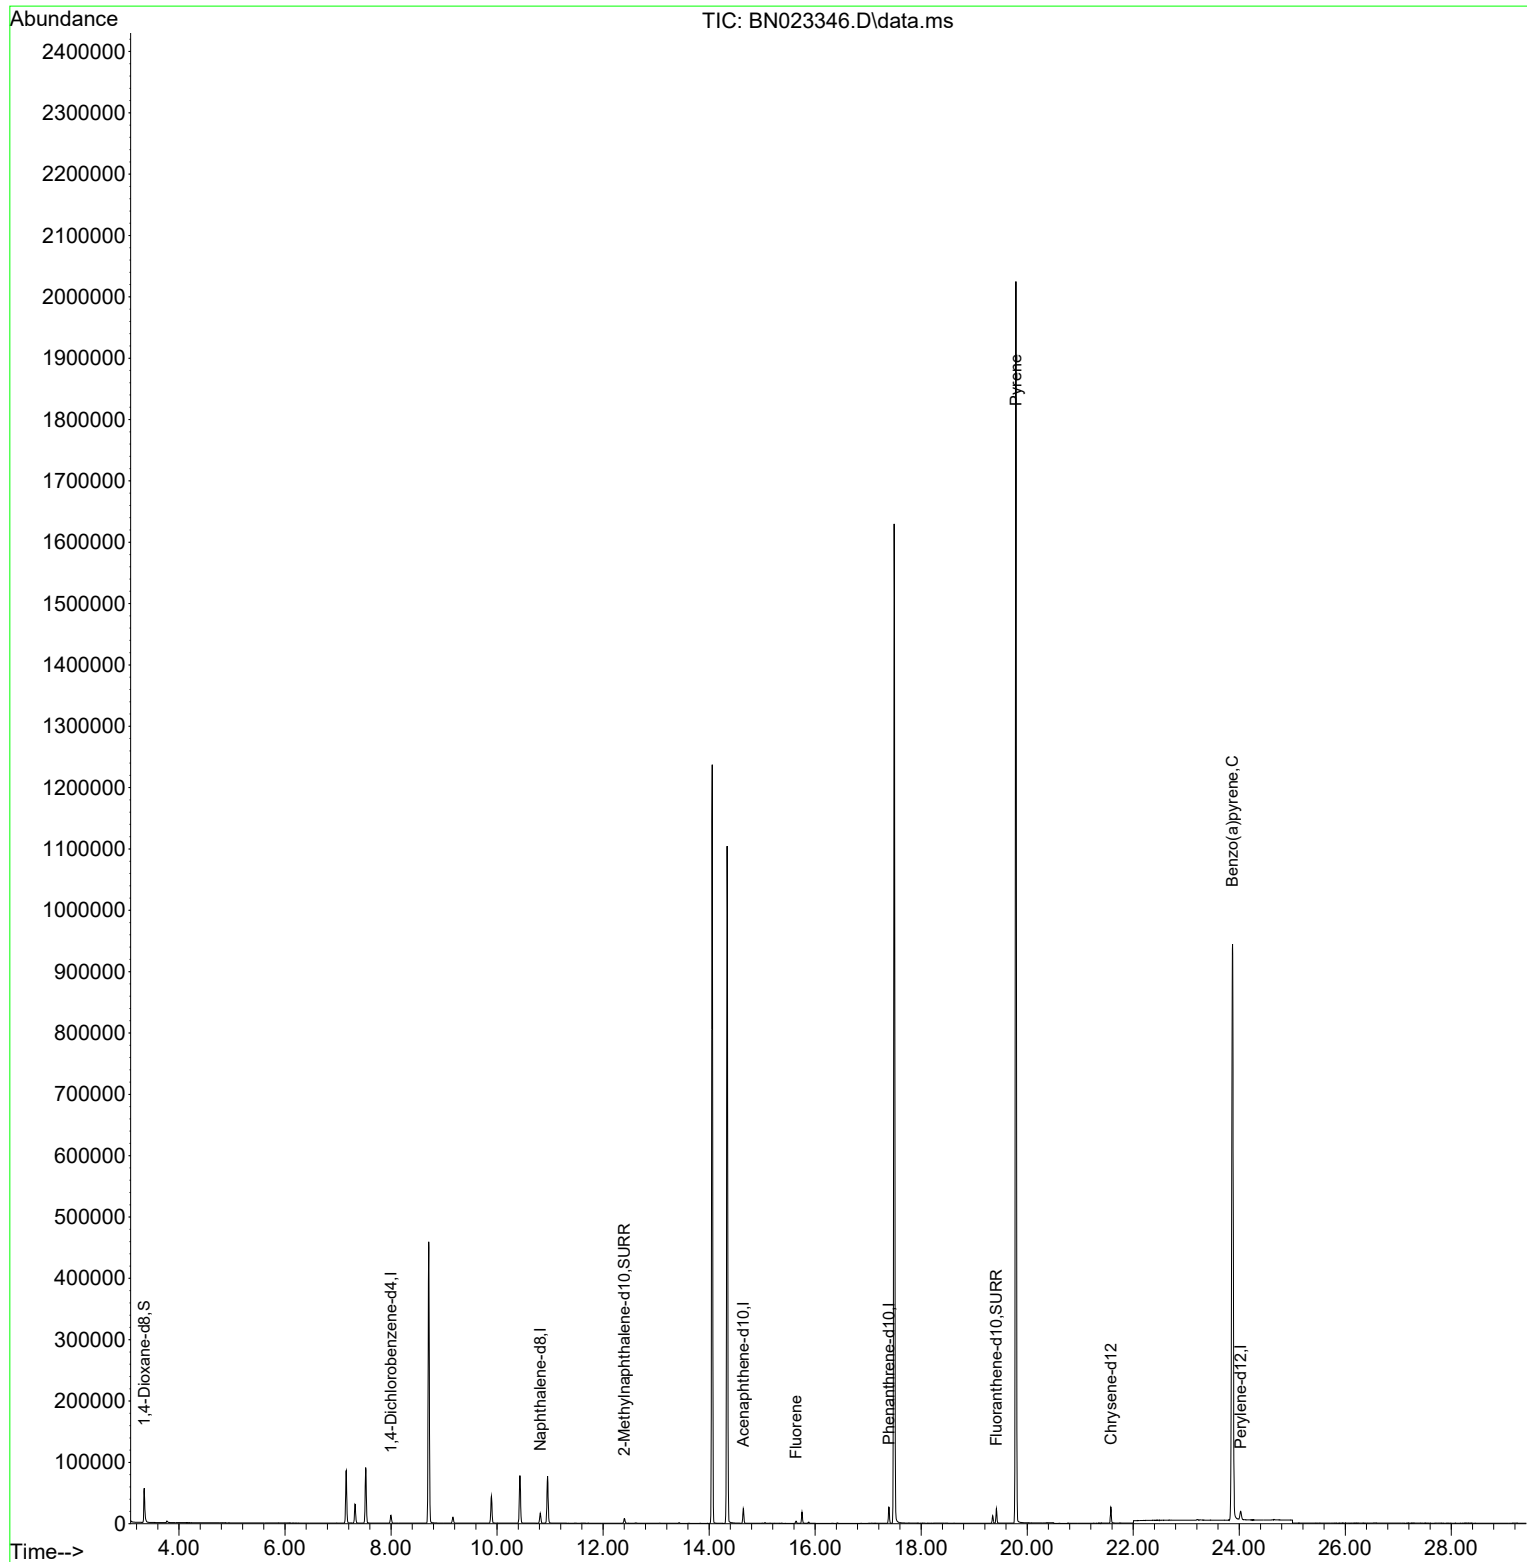


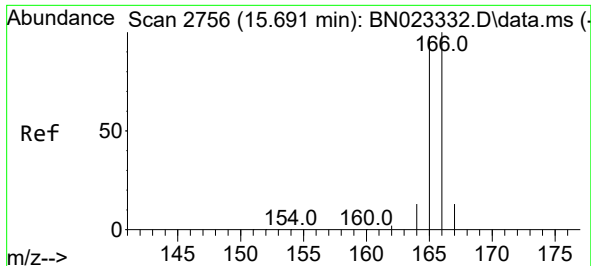

#12
Fluorene
Concen: 0.060 ng/ul
RT: 15.640 min Scan# 21
Delta R.T. -0.052 min
Lab File: BN023346.D
Acq: 22 Dec 2022 19:20




Instrument :
BNA_N
ClientSampleId :
SBLK668


Tgt Ion:166 Resp: 3160
Ion Ratio Lower Upper
166 100
165 8.1 79.1 118.7#
167 33.2 11.0 16.4#

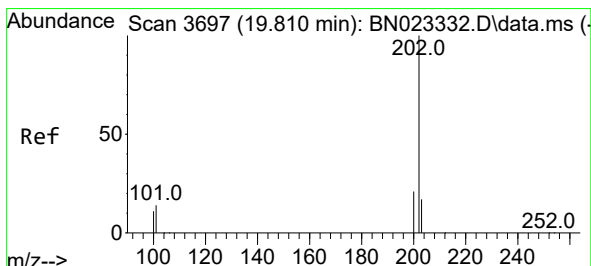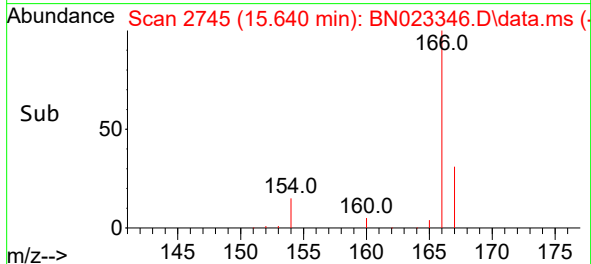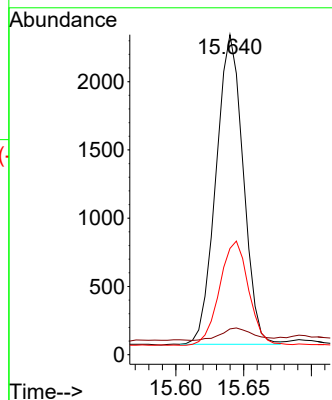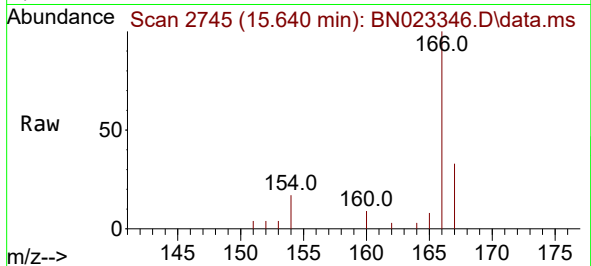

#20
Pyrene
Concen: 0.027 ng/ul
RT: 19.787 min Scan# 3692
Delta R.T. -0.024 min
Lab File: BN023346.D
Acq: 22 Dec 2022 19:20


Tgt Ion:202 Resp: 3064
Ion Ratio Lower Upper
202 100
101 155.1 11.3 16.9#
100 1128.4 9.0 13.4#

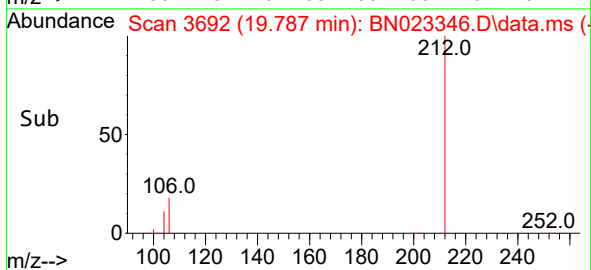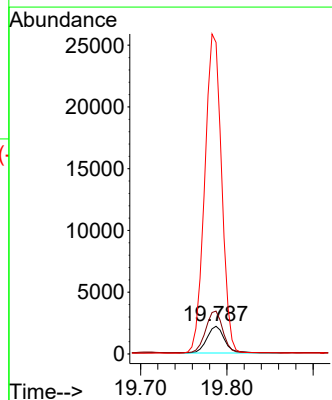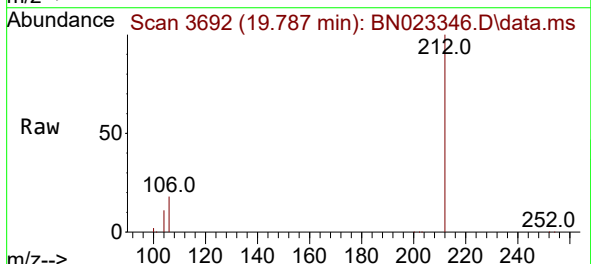

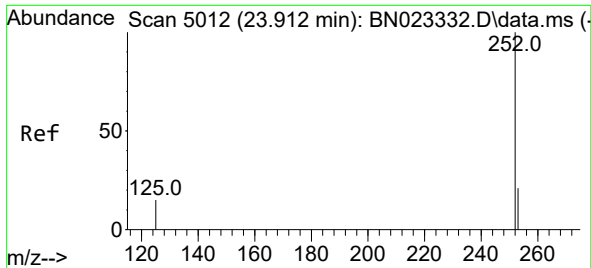

#26
Benzo(a)pyrene
Concen: 0.070 ng/ul
RT: 23.870 min Scan# 4998
Delta R.T. -0.045 min
Lab File: BN023346.D
Acq: 22 Dec 2022 19:20

Instrument :
BNA_N
ClientSampleId :
SBLK668

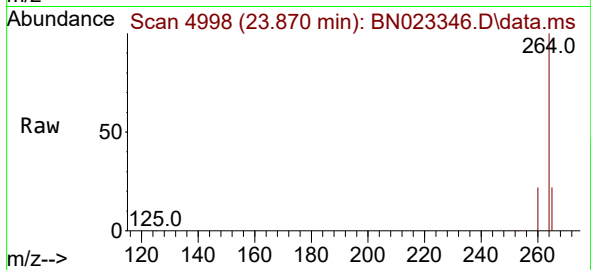

Tgt Ion:252 Resp: 5484
Ion Ratio Lower Upper
252 100
253 48.3 21.4 32.2#
125 44.5 16.2 24.4#

