
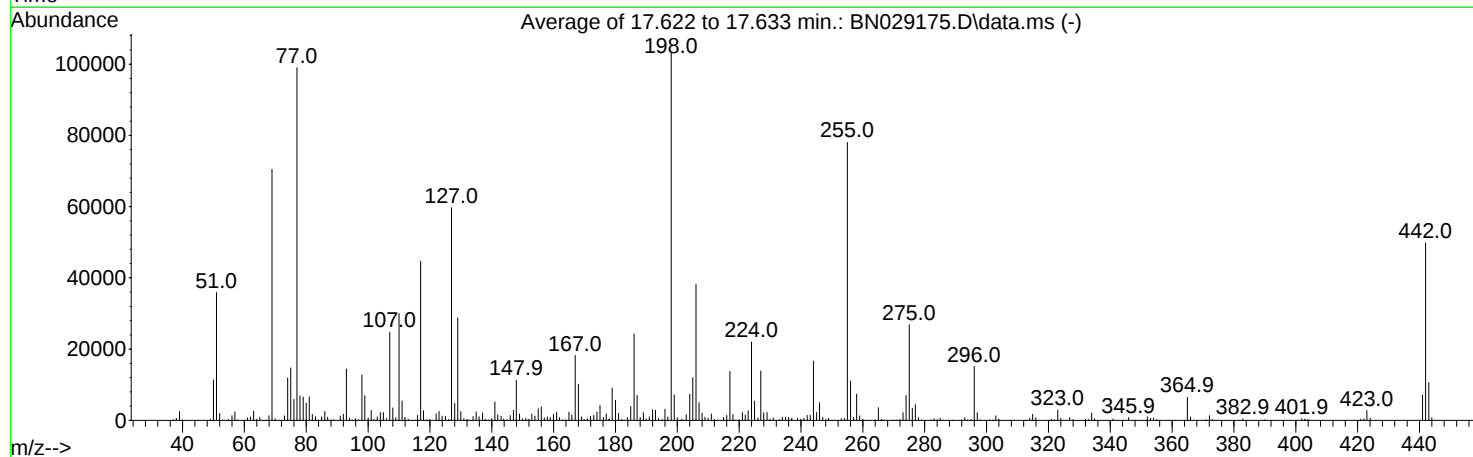


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122223\
Data File : BN029175.D
Acq On : 22 Dec 2023 10:43
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN122223.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Dec 23 03:51:02 2023

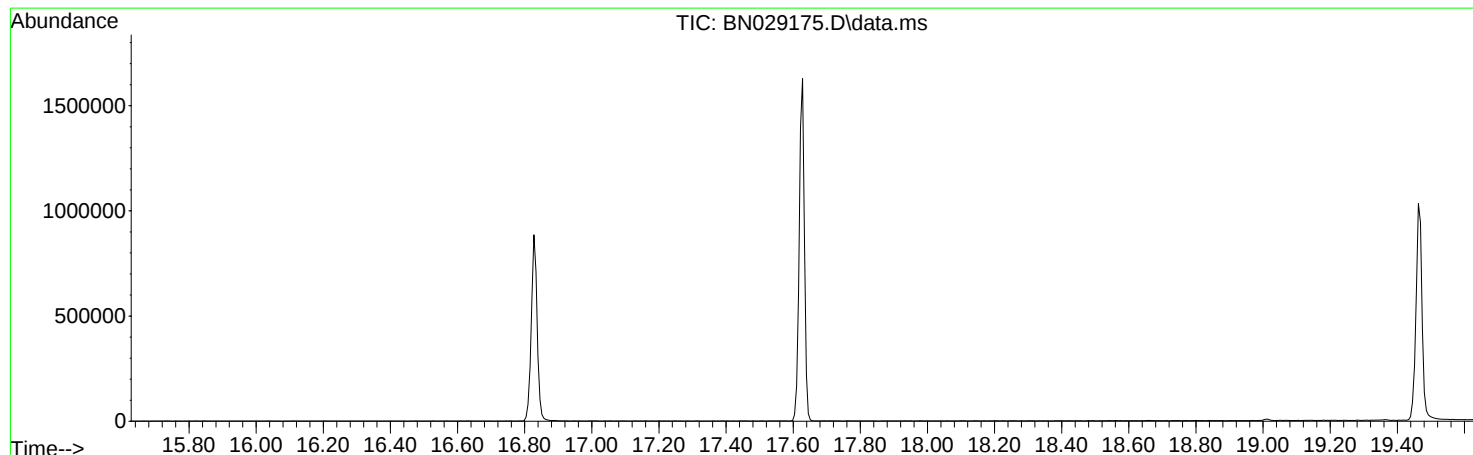




AutoFind: Scans 2471, 2472, 2473; Background Corrected with Scan 2464

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.8	35909	PASS
68	69	0.00	2	1.9	1319	PASS
69	198	0.00	100	68.3	70488	PASS
70	69	0.00	2	0.6	415	PASS
127	198	10	80	57.8	59701	PASS
197	198	0.00	2	0.9	978	PASS
198	198	100	100	100.0	103264	PASS
199	198	5	9	6.9	7125	PASS
275	198	10	60	26.0	26880	PASS
365	198	1	100	6.3	6482	PASS
441	198	0.01	100	6.9	7130	PASS
442	442	50	100	100.0	49821	PASS
443	442	15	24	21.2	10581	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122223\
 Data File : BN029175.D
 Acq On : 22 Dec 2023 10:43
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Dec 23 05:19:52 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 01 23:28:24 2023
 Response via : Initial Calibration

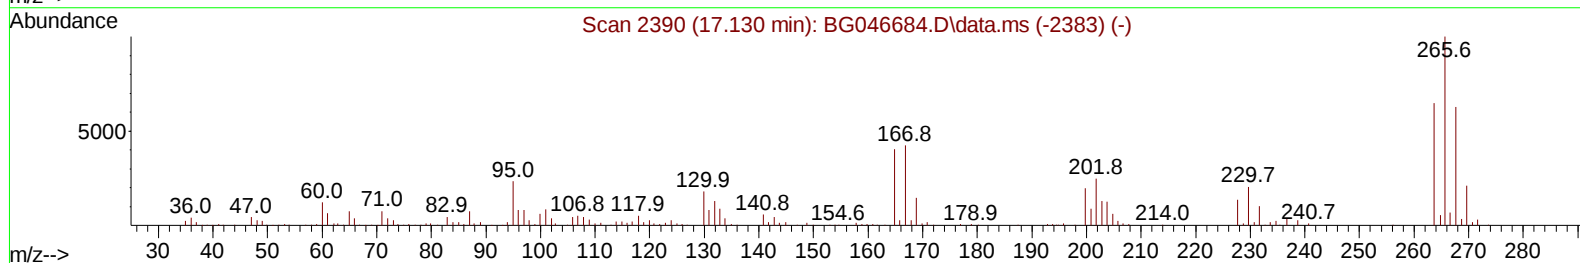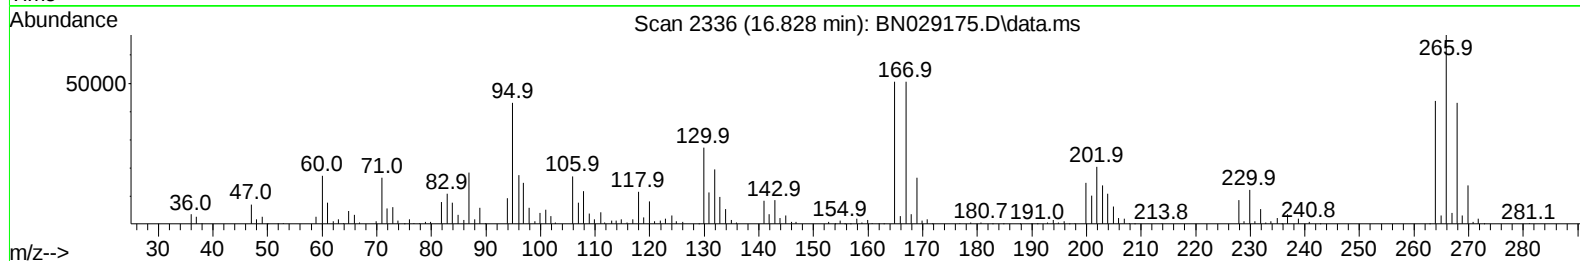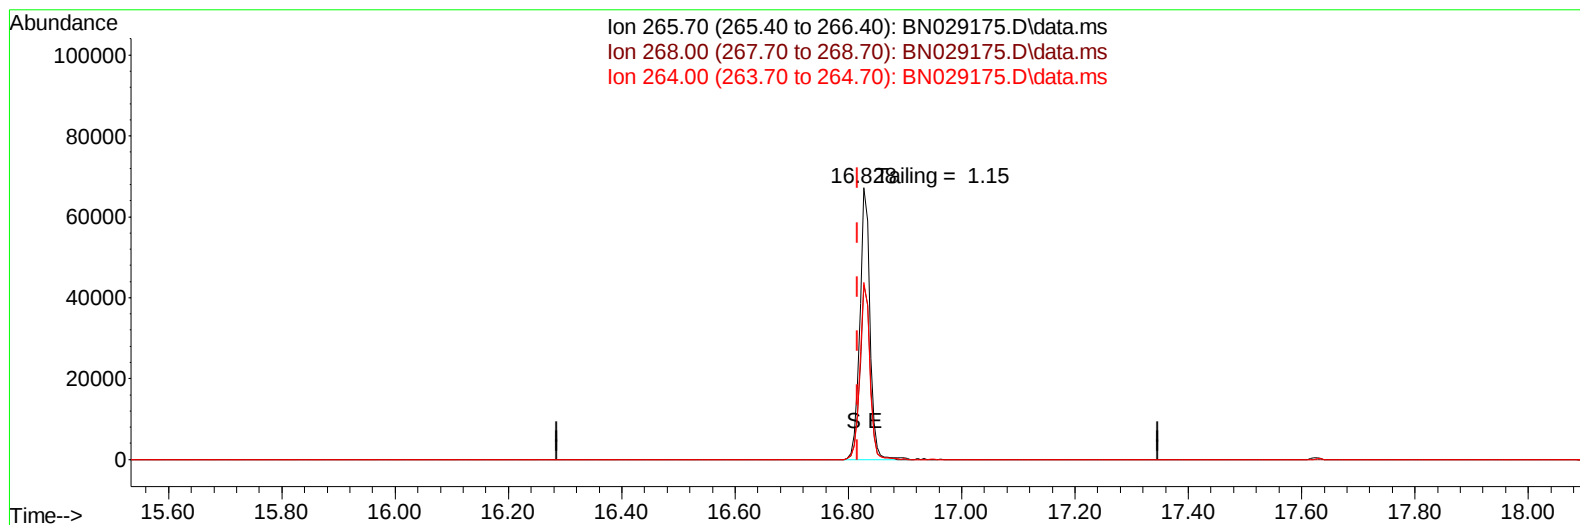

TIC: BN029175.D\data.ms

(70) Pentachlorophenol (C)

16.828min (+ 0.012) 10062.15 ng




response 81650

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.28
264.00	61.60	65.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122223\
 Data File : BN029175.D
 Acq On : 22 Dec 2023 10:43
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Dec 23 05:19:52 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 01 23:28:24 2023
 Response via : Initial Calibration

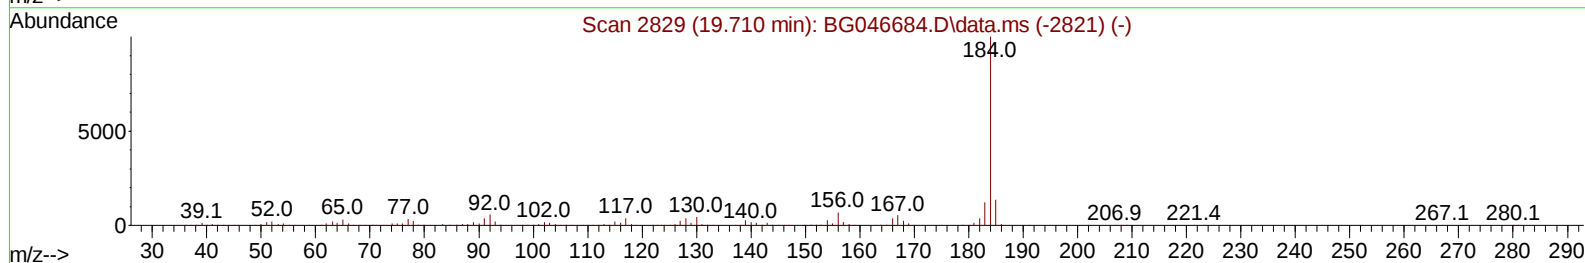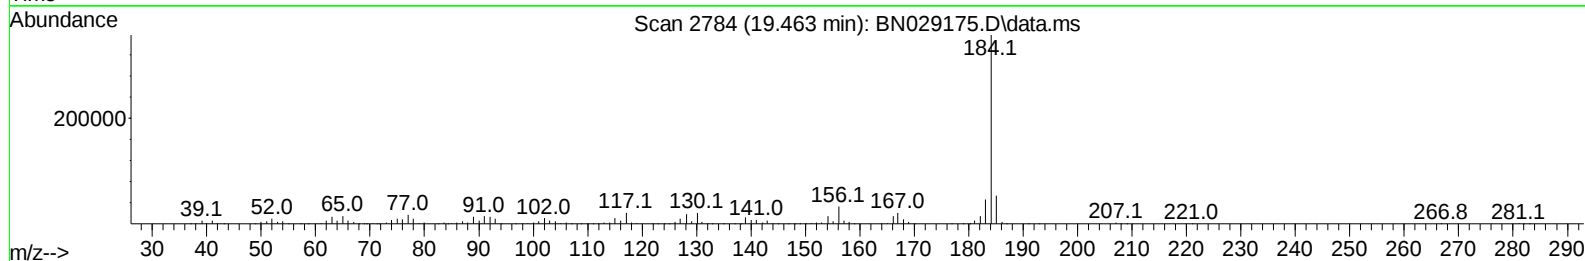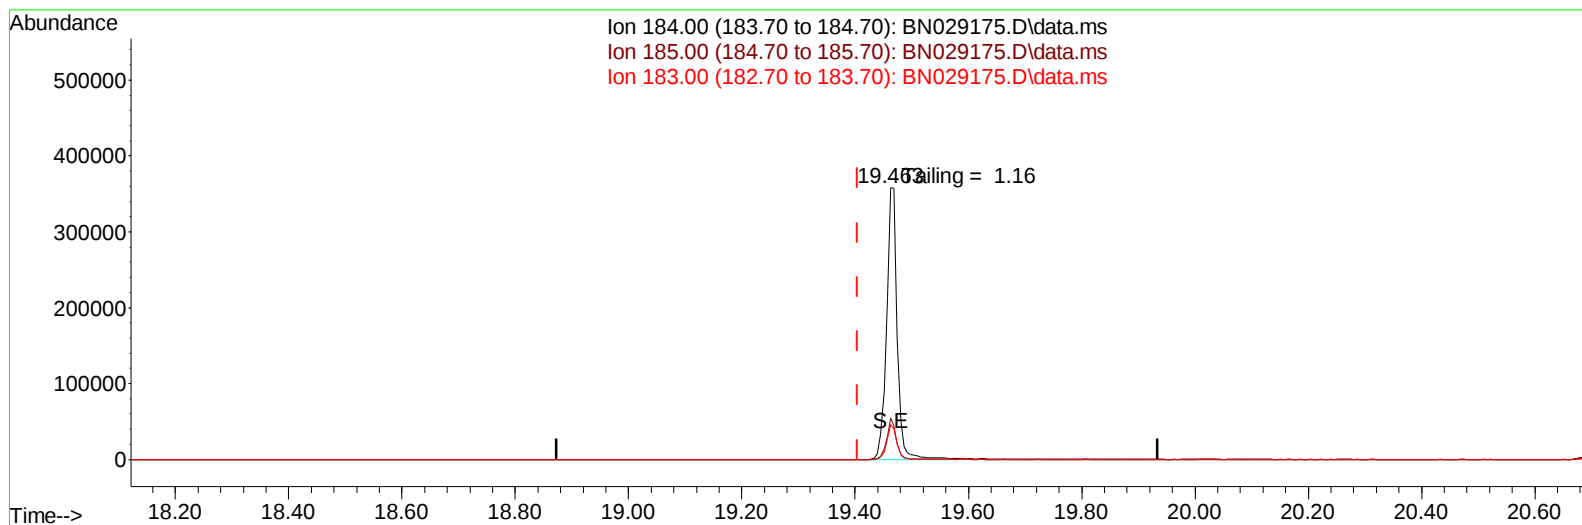

TIC: BN029175.D\data.ms

(77) Benzidine

19.463min (+ 0.059) 0.00 ng

response 470617

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.13
183.00	13.20	12.84
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/22/2023	BNA_N	<u>BN029175.D</u>
Compound Name	Response	Retention Time
DDT	236812	20.686
DDD	9015	20.245
DDE	139	19.727
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9154	245966	3.72

Instrument :
BNA_N
ClientSampleId :
DFTPP