
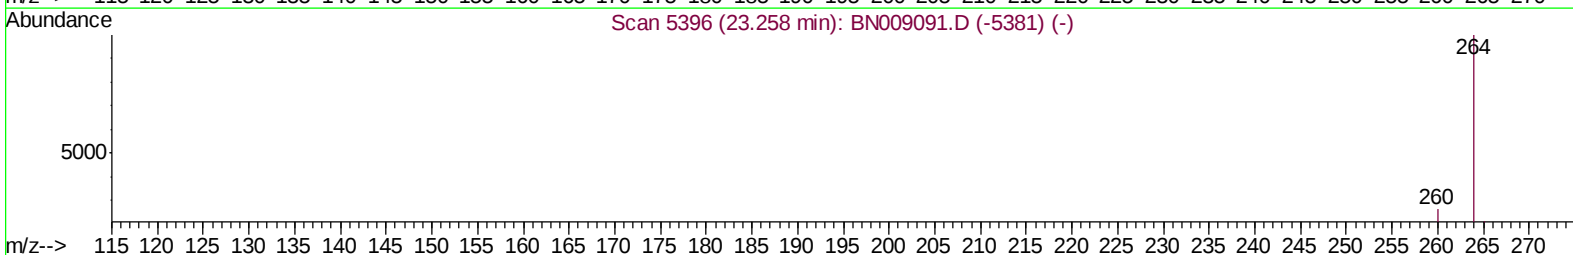
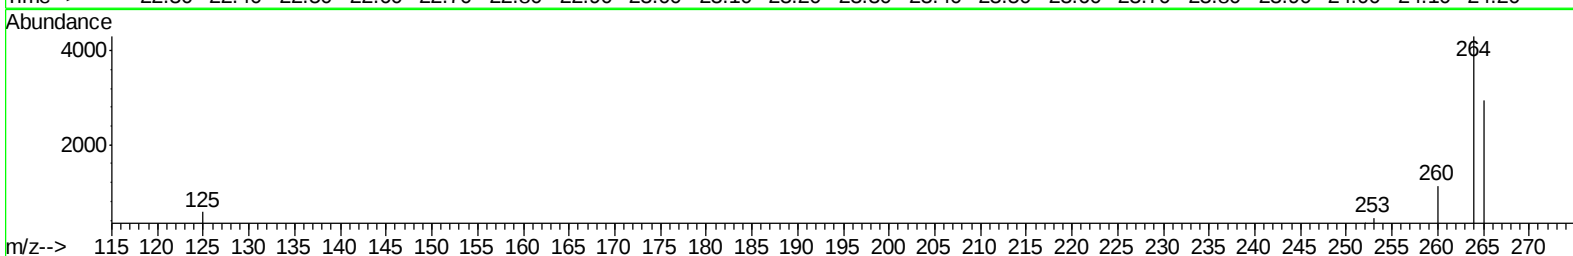


Data File : BN009097.D
Acq On : 23 Dec 2019 21:14
Operator : JU
Sample : K6202-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Quant Time: Dec 24 02:58:07 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN121619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 24 02:43:36 2019
Response via : Initial Calibration

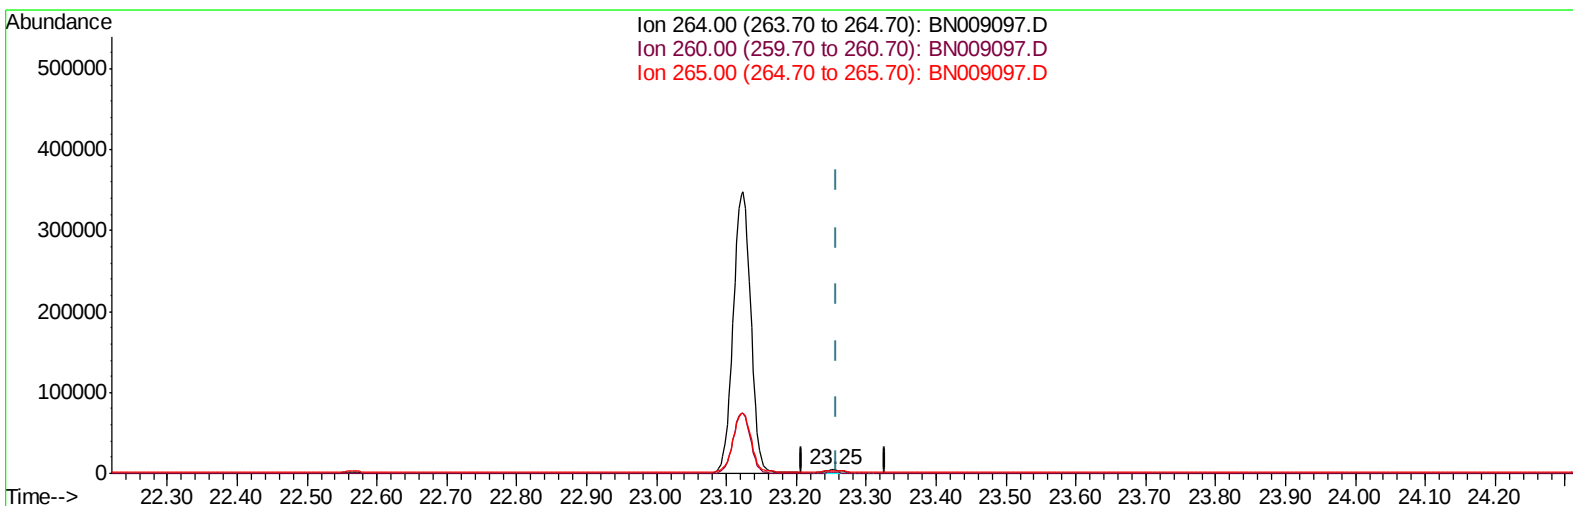

TIC: BN009097.D

(20) Perylene-d12 (I)

23.253min (-0.006) 0.40ng/ul

response 7437

Ion	Exp%	Act%
264.00	100	100
260.00	26.70	26.34
265.00	61.20	68.45
0.00	0.00	0.00