

Data File : BN009093.D
Acq On : 23 Dec 2019 18:50
Operator : JU
Sample : PB125488BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK88

Quant Time: Dec 24 02:46:08 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN121619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 24 02:43:36 2019
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.54	152	3184	0.40	ng/ul	0.00
2) Naphthalene-d8	10.29	136	11891	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.16	164	7052	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-16.91
16) Chrysene-d12	21.12	240	8529	0.40	ng/ul	0.00
20) Perylene-d12	23.26	264	8207	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.89	152	7314	0.35	ng/ul	0.00
14) Fluoranthene-d10	18.94	212	14588	0.00	ng/ul	0.00
Target Compounds						
9) Fluorene	15.17	166	2390	0.070	ng/ul#	13
17) Pyrene	19.32	202	1922	0.044	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN009093.D
Acq On : 23 Dec 2019 18:50
Operator : JU
Sample : PB125488BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK88

Quant Time: Dec 24 02:46:08 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN121619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 24 02:43:36 2019
Response via : Initial Calibration

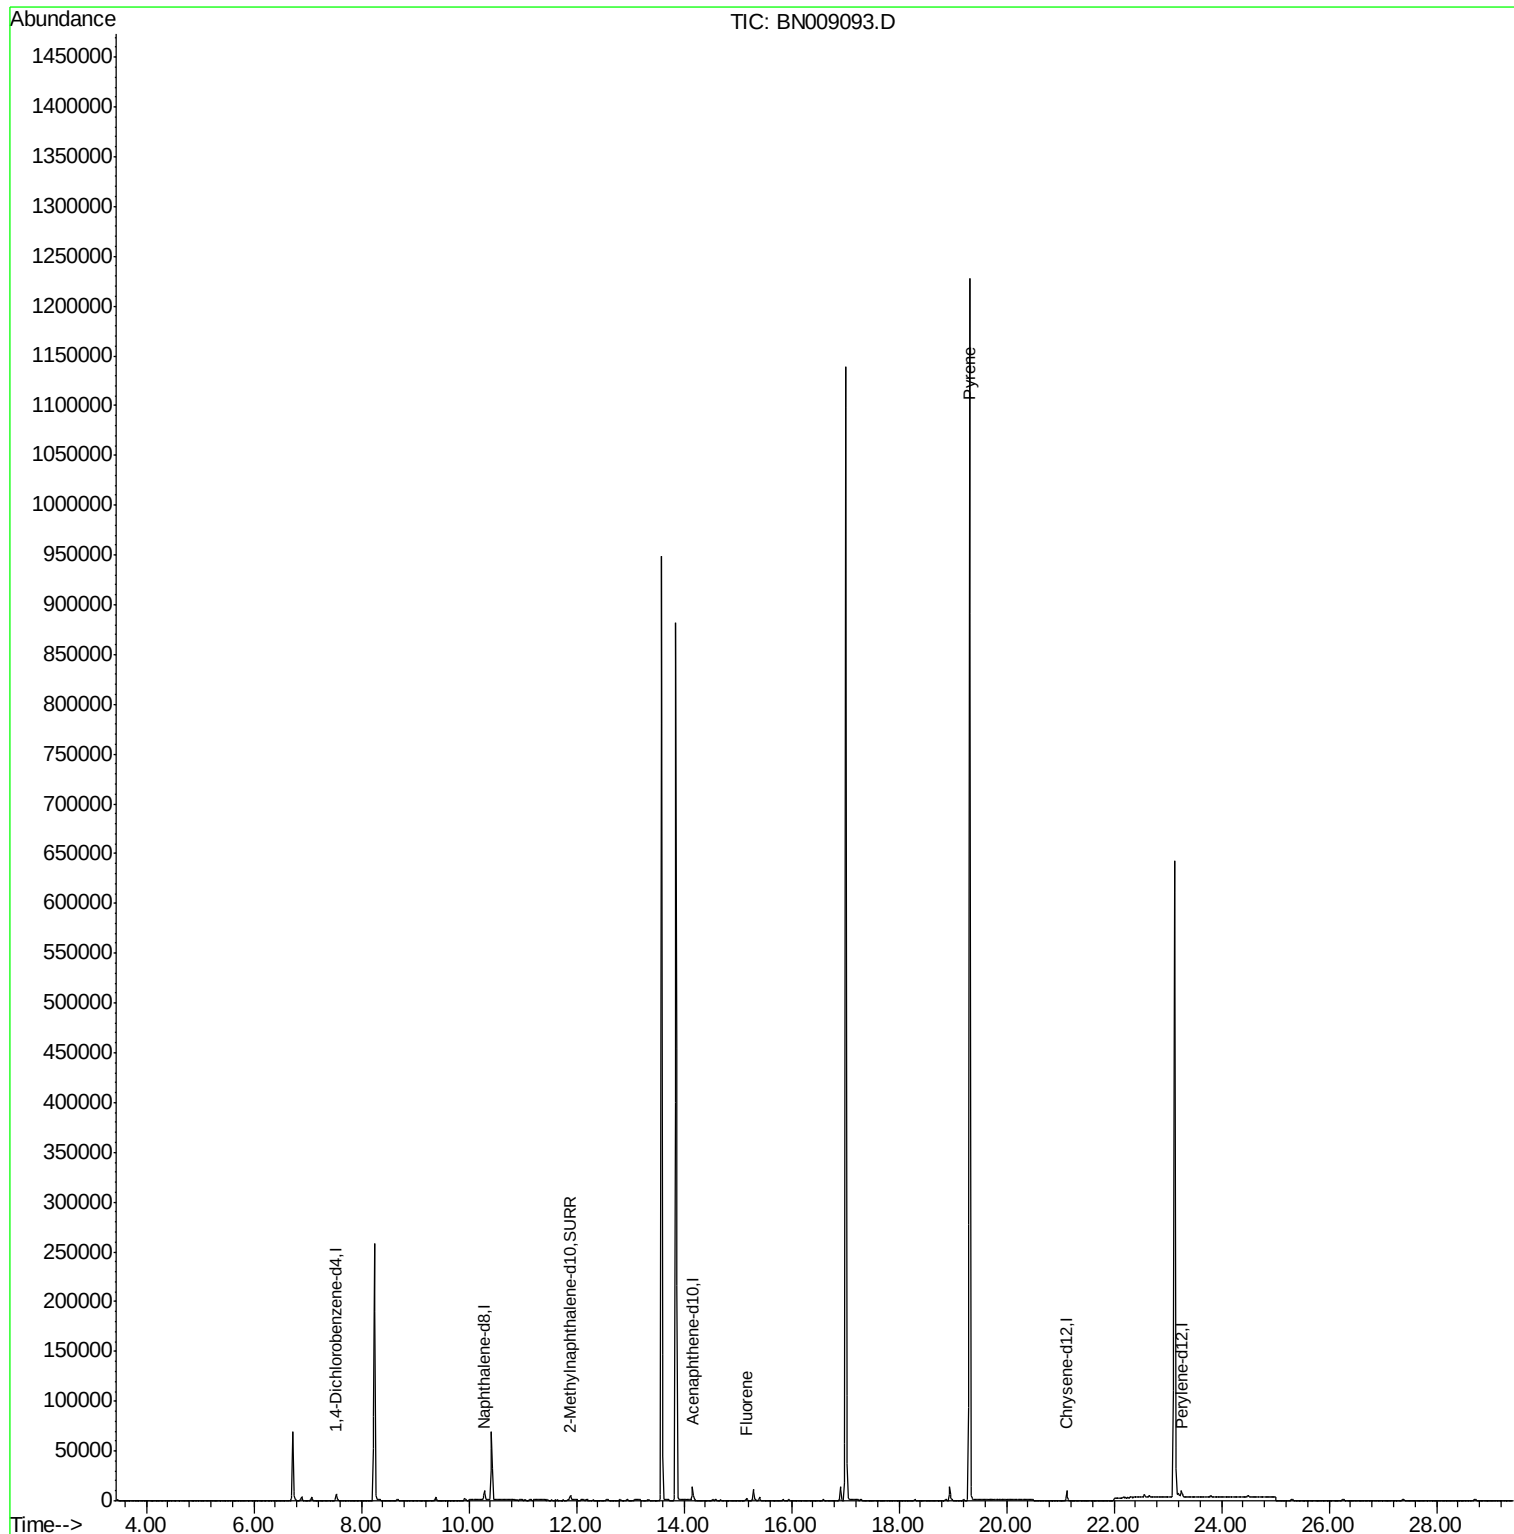

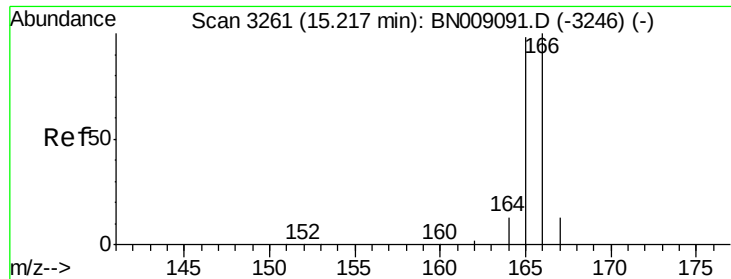

#9

Fluorene

Concen: 0.070 ng/ul

RT: 15.17 min Scan# 3250

Delta R.T. -0.05 min

Lab File: BN009093.D

Acq: 23 Dec 2019 18:50

Instrument :

BNA_N

ClientSampleId :

SBLK88


Tgt Ion:166 Resp: 2390

Ion Ratio Lower Upper




166 100

165 7.2 78.2 117.4#

167 34.1 11.0 16.6#

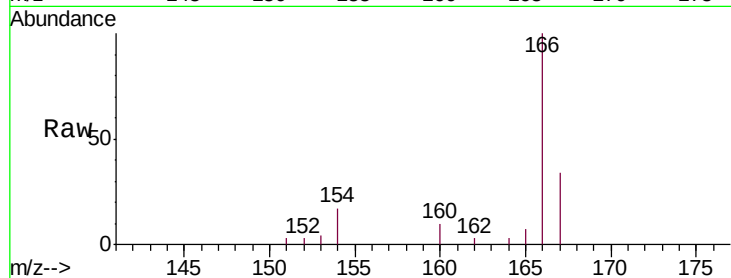

Abundance Ion 166.00 (165.70 to 166.70): E
Ion 165.00 (164.70 to 165.70): E
Ion 167.00 (166.70 to 167.70): E

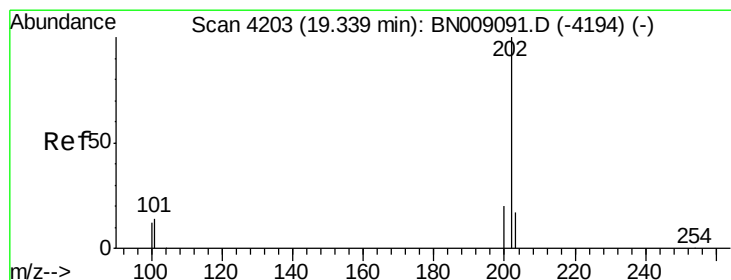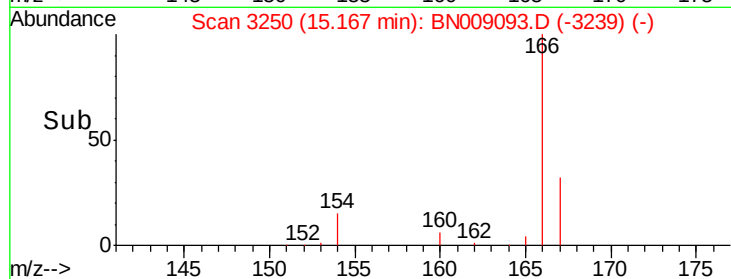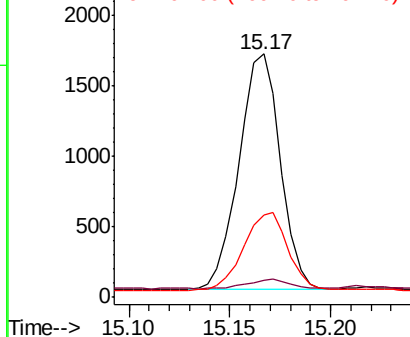

#17

Pyrene

Concen: 0.044 ng/ul

RT: 19.32 min Scan# 4198

Delta R.T. -0.02 min

Lab File: BN009093.D

Acq: 23 Dec 2019 18:50


Tgt Ion:202 Resp: 1922

Ion Ratio Lower Upper

202 100

101 170.8 10.9 16.3#

100 1102.9 9.0 13.6#

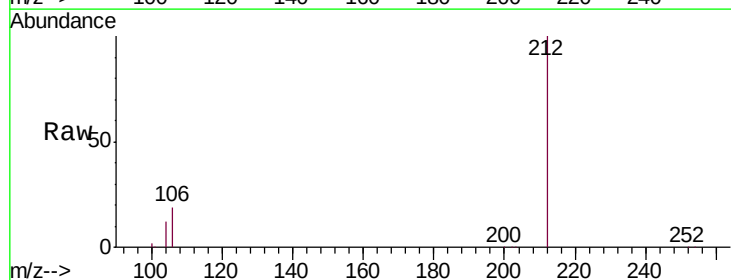

Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 100.00 (99.70 to 100.70): B

