

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN122319\
Quantitation Report (Not Reviewed)

Data File : BN009100.D
Acq On : 23 Dec 2019 23:01
Operator : JU
Sample : K6202-13
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0C12

Quant Time: Dec 24 02:48:04 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN121619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 24 02:43:36 2019
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.54	152	3259	0.40	ng/ul	0.00
2) Naphthalene-d8	10.28	136	12451	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.16	164	7132	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-16.91
16) Chrysene-d12	21.12	240	8472	0.40	ng/ul	0.00
20) Perylene-d12	23.25	264	7819	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.89	152	5598	0.25	ng/ul	0.00
14) Fluoranthene-d10	18.94	212	11729	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	19.31	202	1840	0.043	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN009100.D
Acq On : 23 Dec 2019 23:01
Operator : JU
Sample : K6202-13
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0C12

Quant Time: Dec 24 02:48:04 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN121619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 24 02:43:36 2019
Response via : Initial Calibration

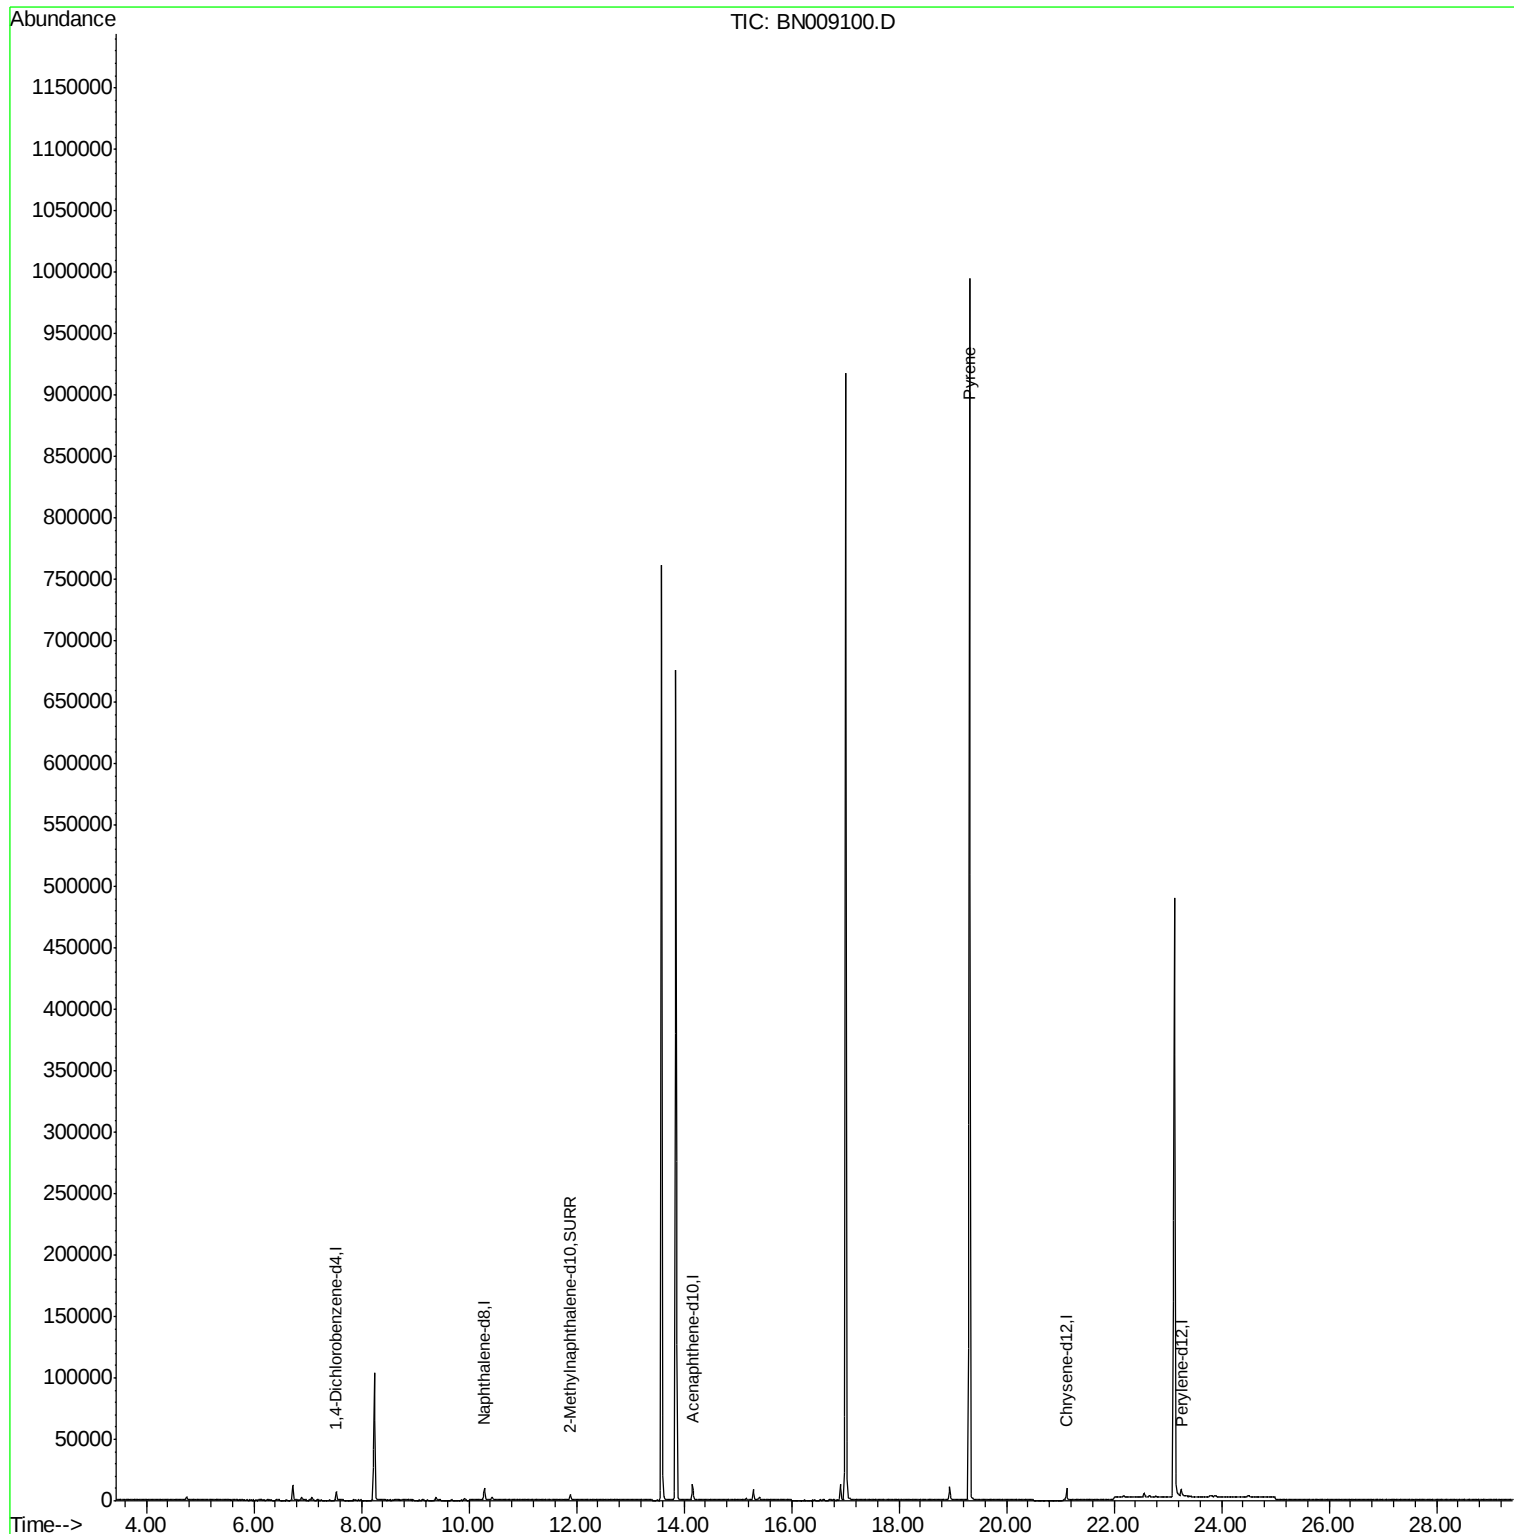

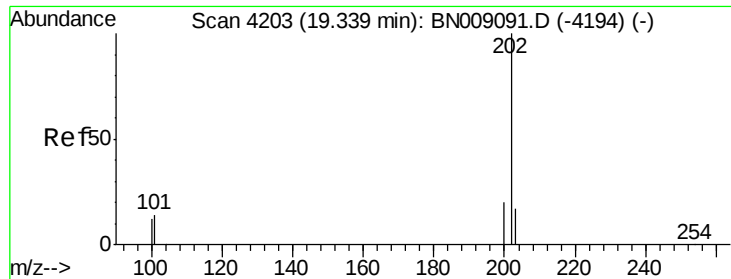

#17

Pyrene

Concen: 0.043 ng/ul

RT: 19.31 min Scan# 4197

Delta R.T. -0.03 min

Lab File: BN009100.D


Acq: 23 Dec 2019 23:01

Instrument :

BNA_N

ClientSampleId :

C0C12

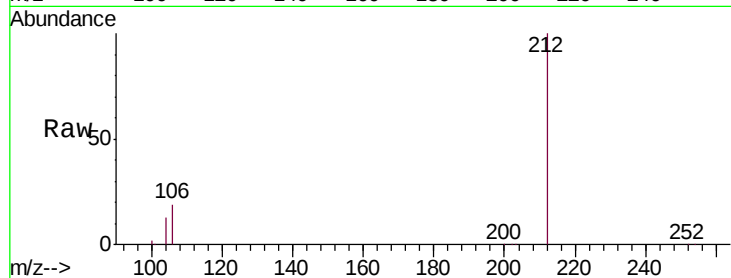

Tgt Ion: 202 Resp: 1840

Ion Ratio Lower Upper

202 100

101 172.0 10.9 16.3#

100 1154.3 9.0 13.6#

