

Data File : BN009107.D
Acq On : 24 Dec 2019 03:12
Operator : JU
Sample : K6253-07
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0C24

Quant Time: Dec 24 05:32:10 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN121619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 24 02:43:36 2019
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.53	152	3469	0.40	ng/ul	0.00
2) Naphthalene-d8	10.28	136	12867	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.16	164	7109	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-16.91
16) Chrysene-d12	21.11	240	7586	0.40	ng/ul	0.00
20) Perylene-d12	23.25	264	7772	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.89	152	5733	0.25	ng/ul	0.00
14) Fluoranthene-d10	18.94	212	10123	0.00	ng/ul	0.00
Target Compounds						
9) Fluorene	15.16	166	1781	0.051	ng/ul#	14
17) Pyrene	19.31	202	1324	0.034	ng/ul#	1
23) Benzo(a)pyrene	23.12	252	2309	0.073	ng/ul#	47


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN009107.D
Acq On : 24 Dec 2019 03:12
Operator : JU
Sample : K6253-07
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0C24

Quant Time: Dec 24 05:32:10 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN121619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 24 02:43:36 2019
Response via : Initial Calibration




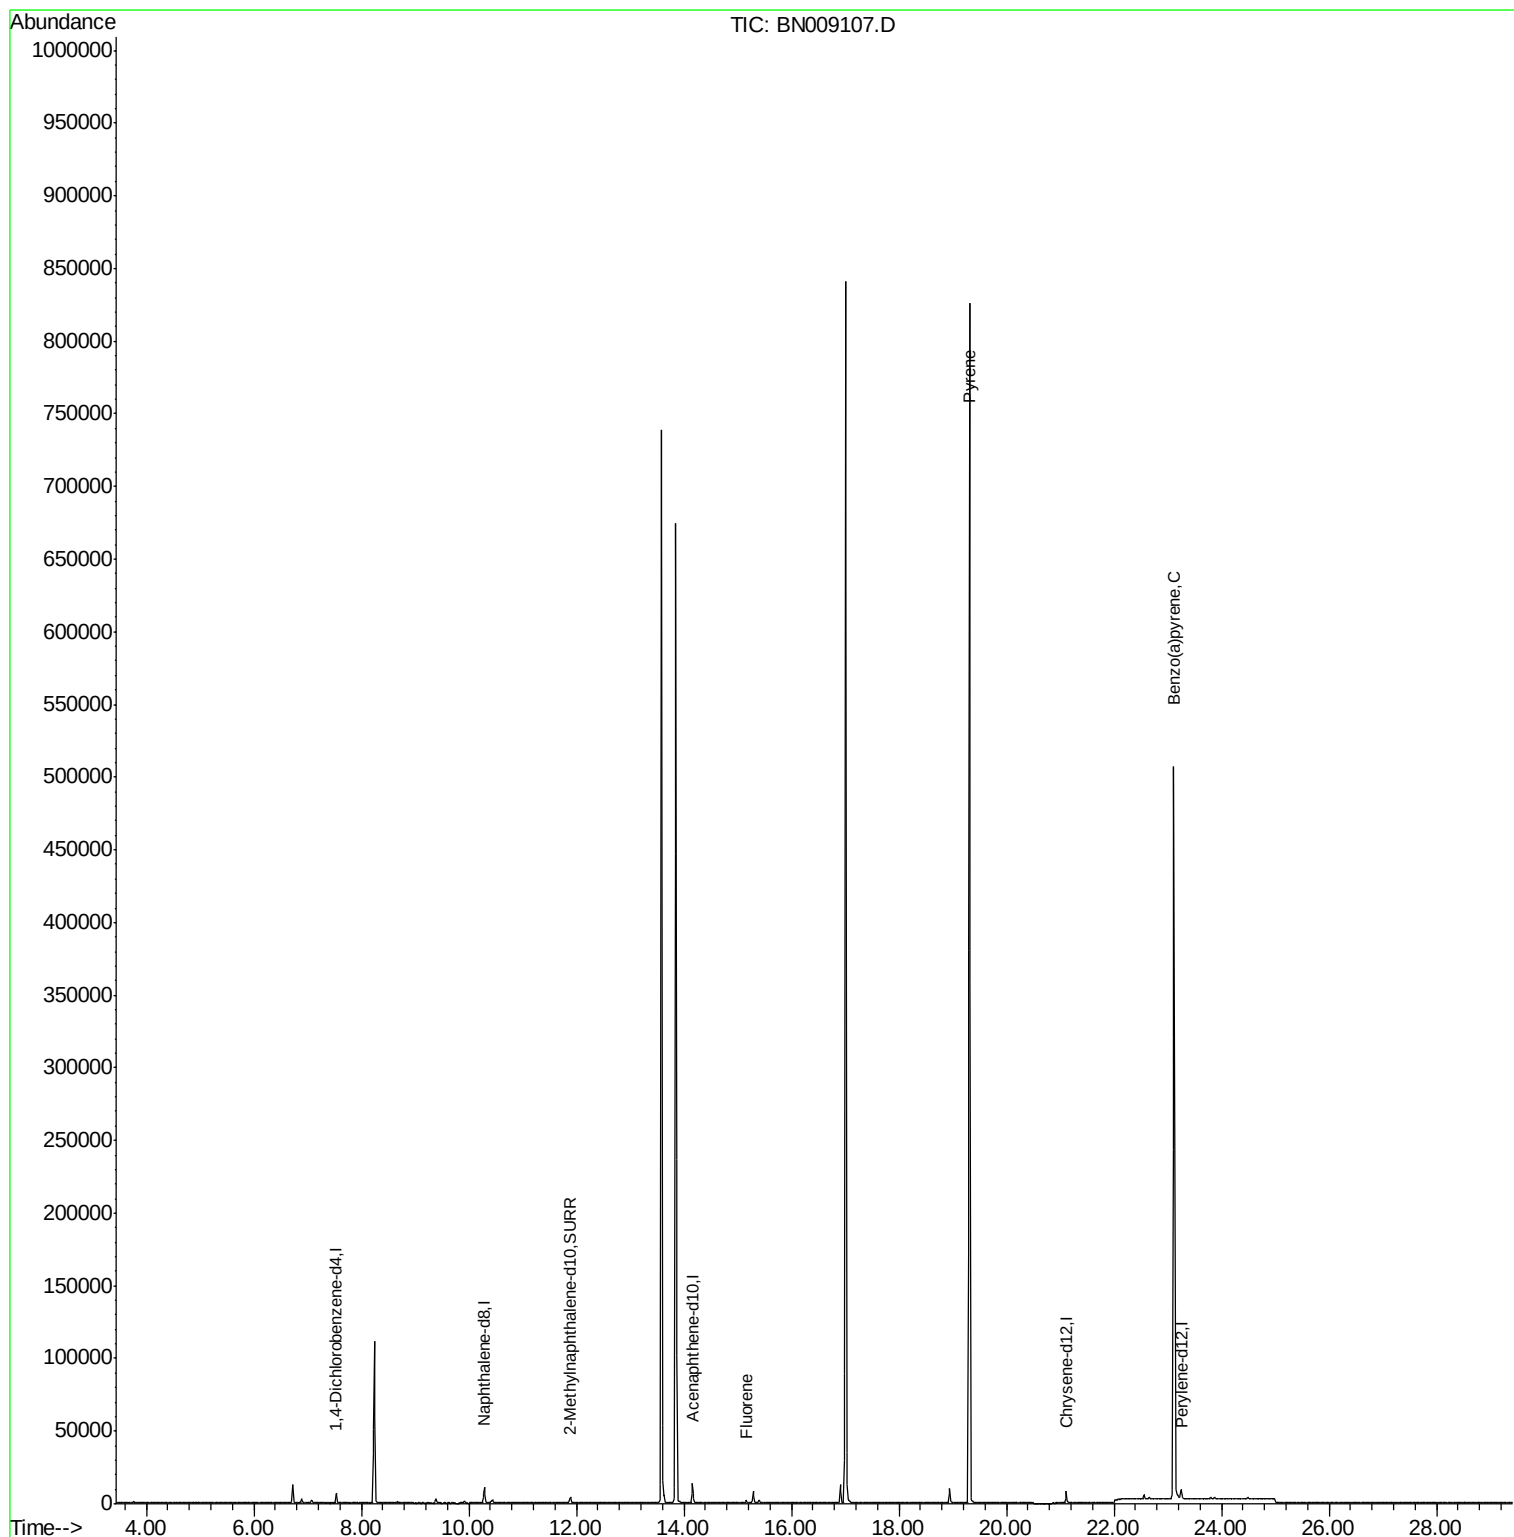


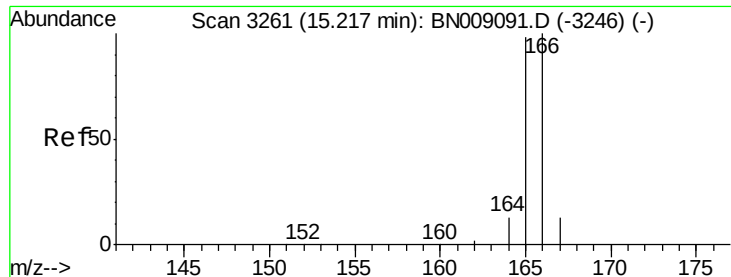

#9
Fluorene
 Concen: 0.051 ng/ul
 RT: 15.16 min Scan# 3249
 Delta R.T. -0.06 min
 Lab File: BN009107.D
 Acq: 24 Dec 2019 03:12




Instrument :
 BNA_N
 ClientSampleId :
 C0C24


Tgt Ion:166 Resp: 1781
 Ion Ratio Lower Upper
 166 100
 165 8.0 78.2 117.4#
 167 34.7 11.0 16.6#

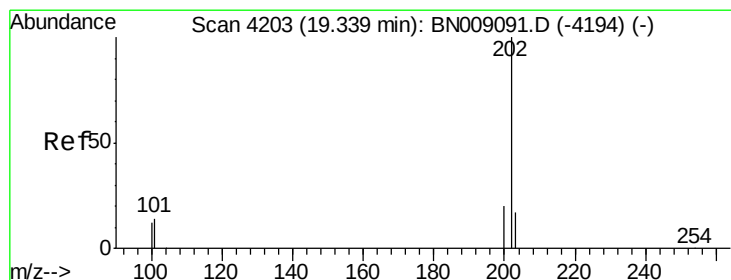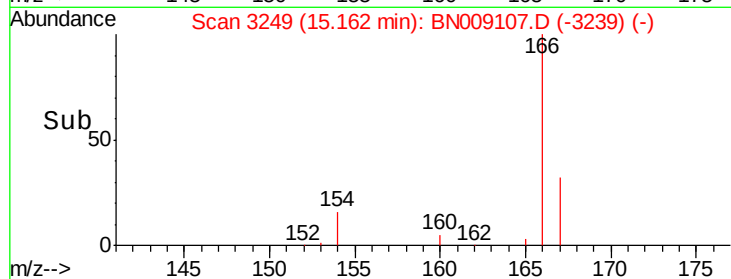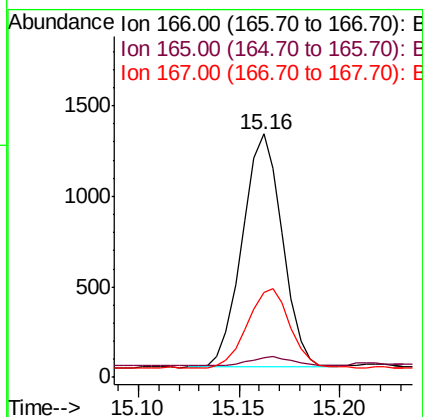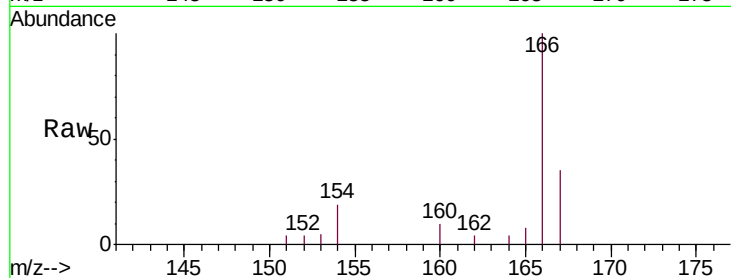

#17
Pyrene
 Concen: 0.034 ng/ul
 RT: 19.31 min Scan# 4197
 Delta R.T. -0.03 min
 Lab File: BN009107.D
 Acq: 24 Dec 2019 03:12

Tgt Ion:202 Resp: 1324
 Ion Ratio Lower Upper
 202 100
 101 169.8 10.9 16.3#
 100 1100.2 9.0 13.6#

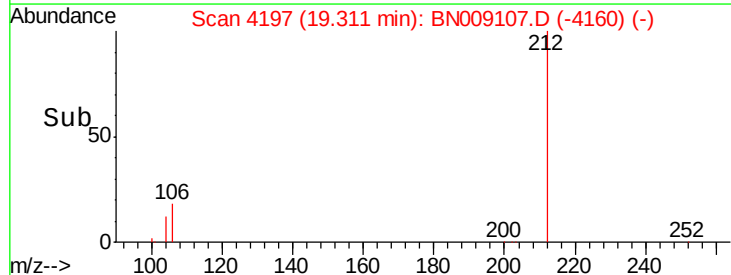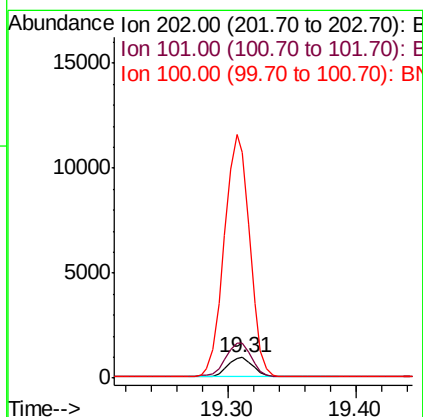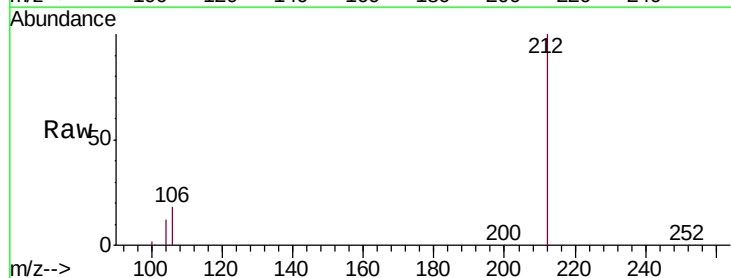

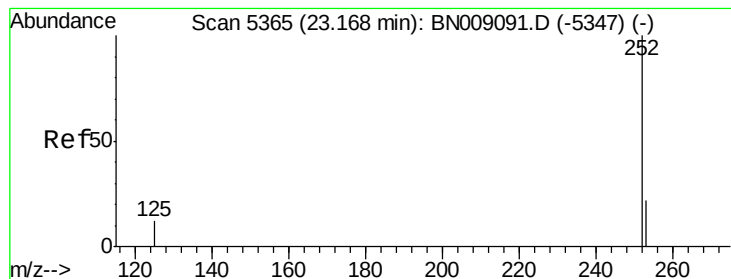

#23

Benzo(a)pyrene

Concen: 0.073 ng/ul

RT: 23.12 min Scan# 5347

Delta R.T. -0.05 min

Lab File: BN009107.D


Acq: 24 Dec 2019 03:12

Instrument :

BNA_N

ClientSampleId :

C0C24

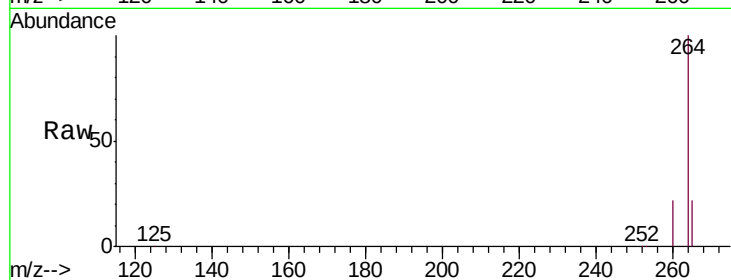

Tgt Ion: 252 Resp: 2309

Ion Ratio Lower Upper

252 100

253 47.3 20.2 30.4#

125 45.0 13.2 19.8#

