

Data File : BN009110.D
Acq On : 24 Dec 2019 05:35
Operator : JU
Sample : PB125607BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK07

Quant Time: Dec 24 06:51:38 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN121619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 24 06:49:13 2019
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.53	152	3381	0.40	ng/ul	0.00
2) Naphthalene-d8	10.28	136	12840	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.16	164	7316	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-16.91
16) Chrysene-d12	21.12	240	7856	0.40	ng/ul	0.00
20) Perylene-d12	23.26	264	7664	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.89	152	7033	0.31	ng/ul	0.00
14) Fluoranthene-d10	18.94	212	12961	0.00	ng/ul	0.00
Target Compounds						
					Qvalue	
9) Fluorene	15.16	166	2219	0.062	ng/ul#	13
17) Pyrene	19.31	202	1693	0.042	ng/ul#	1
23) Benzo(a)pyrene	23.12	252	2735	0.087	ng/ul#	54


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN009110.D
Acq On : 24 Dec 2019 05:35
Operator : JU
Sample : PB125607BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK07

Quant Time: Dec 24 06:51:38 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN121619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 24 06:49:13 2019
Response via : Initial Calibration




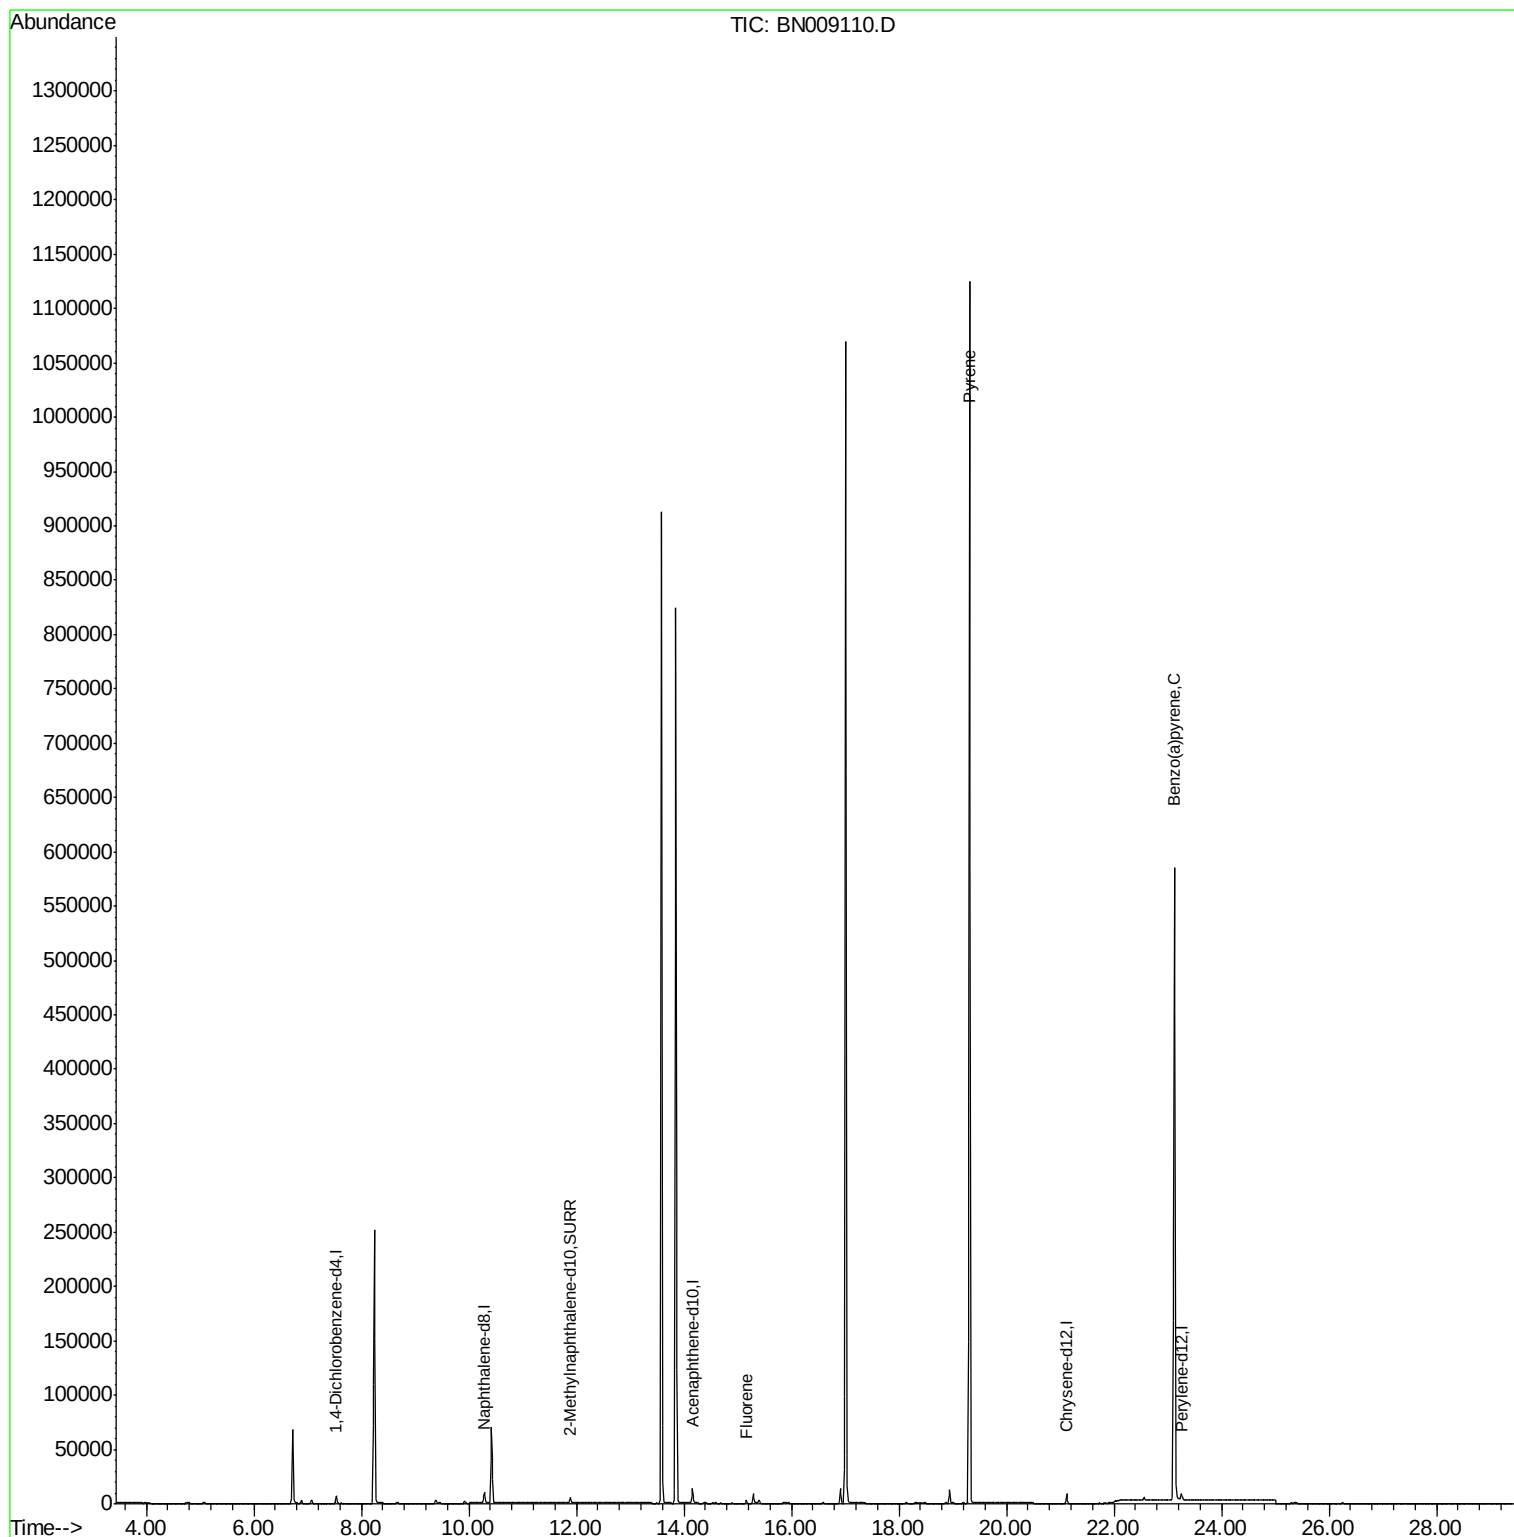


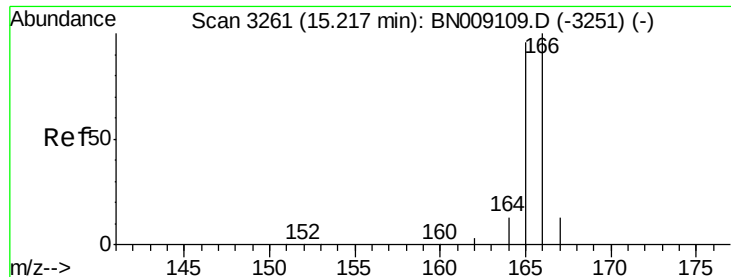

#9
Fluorene
 Concen: 0.062 ng/ul
 RT: 15.16 min Scan# 3249
 Delta R.T. -0.06 min
 Lab File: BN009110.D
 Acq: 24 Dec 2019 05:35




Instrument :
 BNA_N
 ClientSampleId :
 SBLK07


Tgt Ion:166 Resp: 2219
 Ion Ratio Lower Upper
 166 100
 165 6.9 78.2 117.4#
 167 34.1 11.0 16.6#

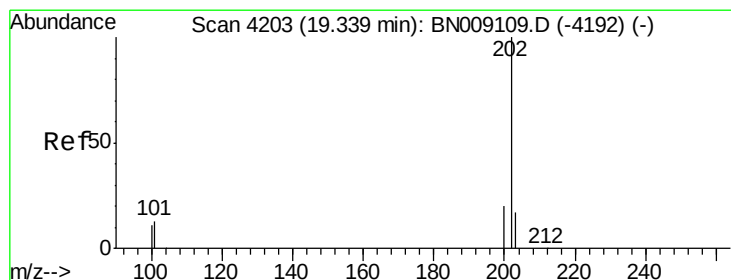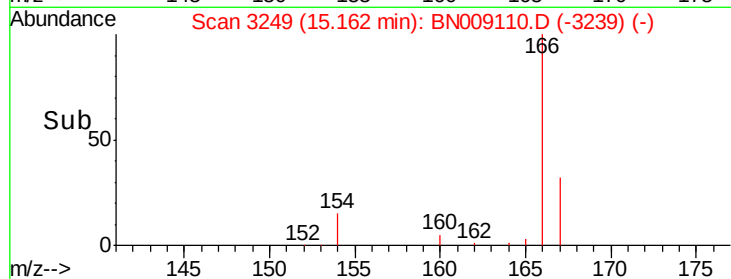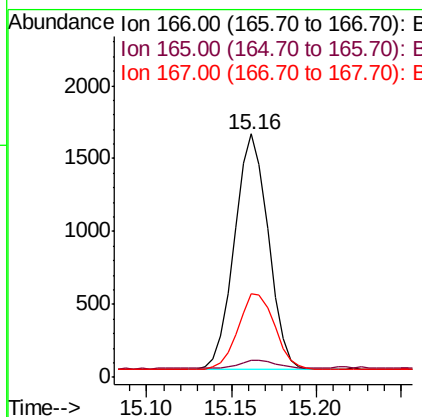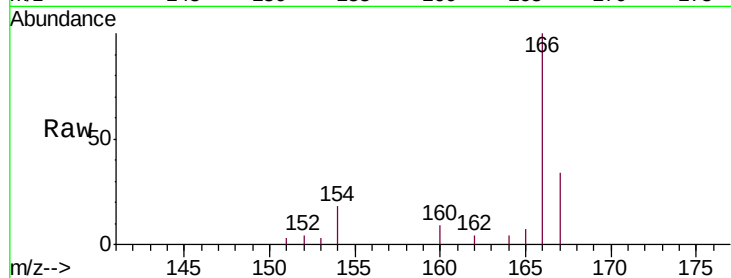

#17
Pyrene
 Concen: 0.042 ng/ul
 RT: 19.31 min Scan# 4197
 Delta R.T. -0.03 min
 Lab File: BN009110.D
 Acq: 24 Dec 2019 05:35

Tgt Ion:202 Resp: 1693
 Ion Ratio Lower Upper
 202 100
 101 171.0 10.9 16.3#
 100 1170.4 9.0 13.6#

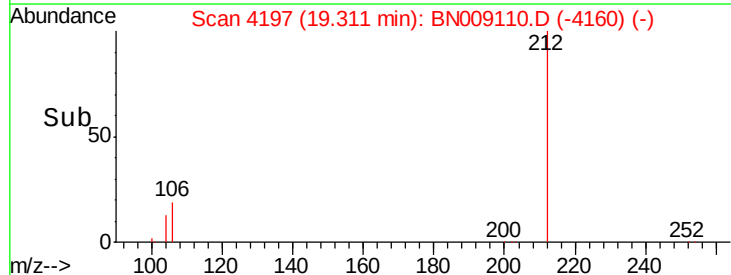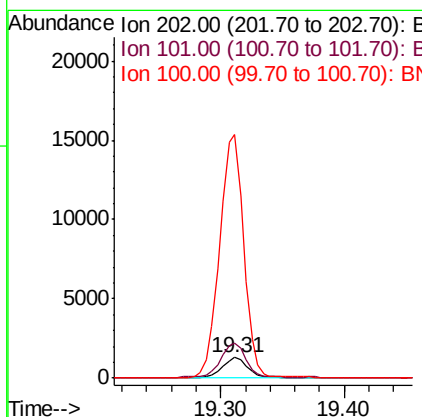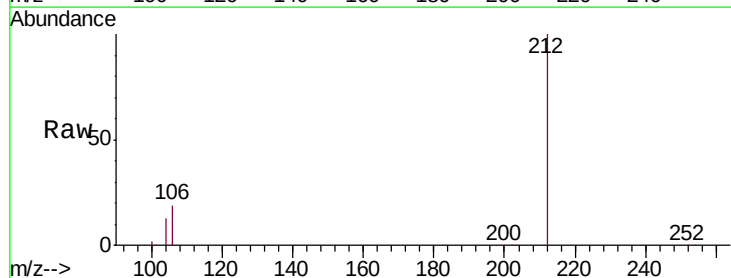

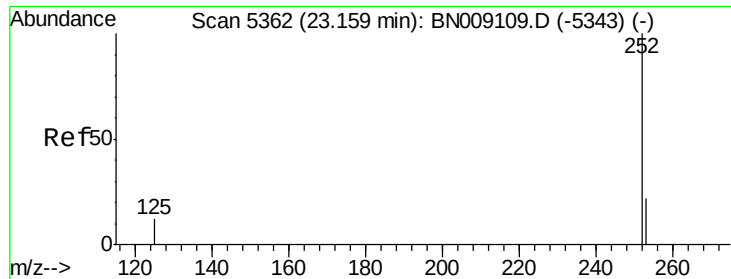

#23

Benzo(a)pyrene

Concen: 0.087 ng/ul

RT: 23.12 min Scan# 5349

Delta R.T. -0.04 min

Lab File: BN009110.D


Acq: 24 Dec 2019 05:35

Instrument :

BNA_N

ClientSampleId :

SBLK07

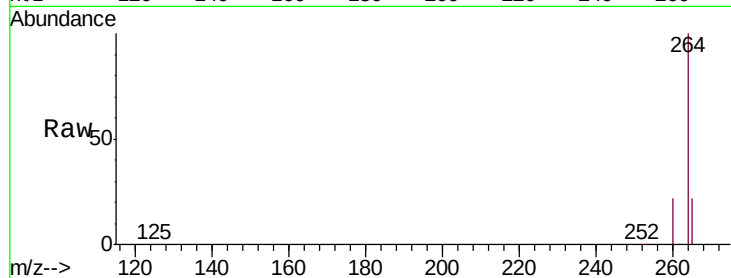


Tgt Ion: 252 Resp: 2735

Ion Ratio Lower Upper

252 100

253 43.1 20.2 30.4#

125 43.8 13.2 19.8#

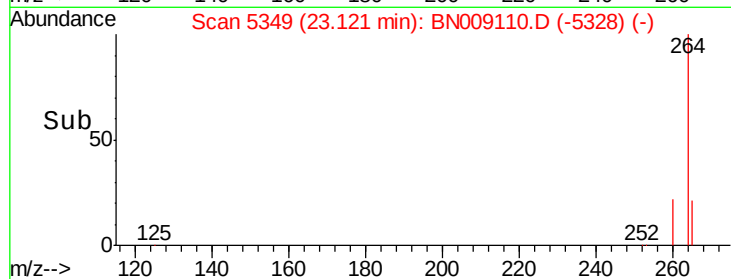

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

