


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN122319\
Data File : BN009088.D
Acq On : 23 Dec 2019 15:50
Operator : JU
Sample : PB125405BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK05

Manual Integrations
APPROVED

mohammad
12/24/2019 2:59:30 PM

Quant Time: Dec 23 17:11:24 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN121619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 20 23:31:06 2019
Response via : Initial Calibration

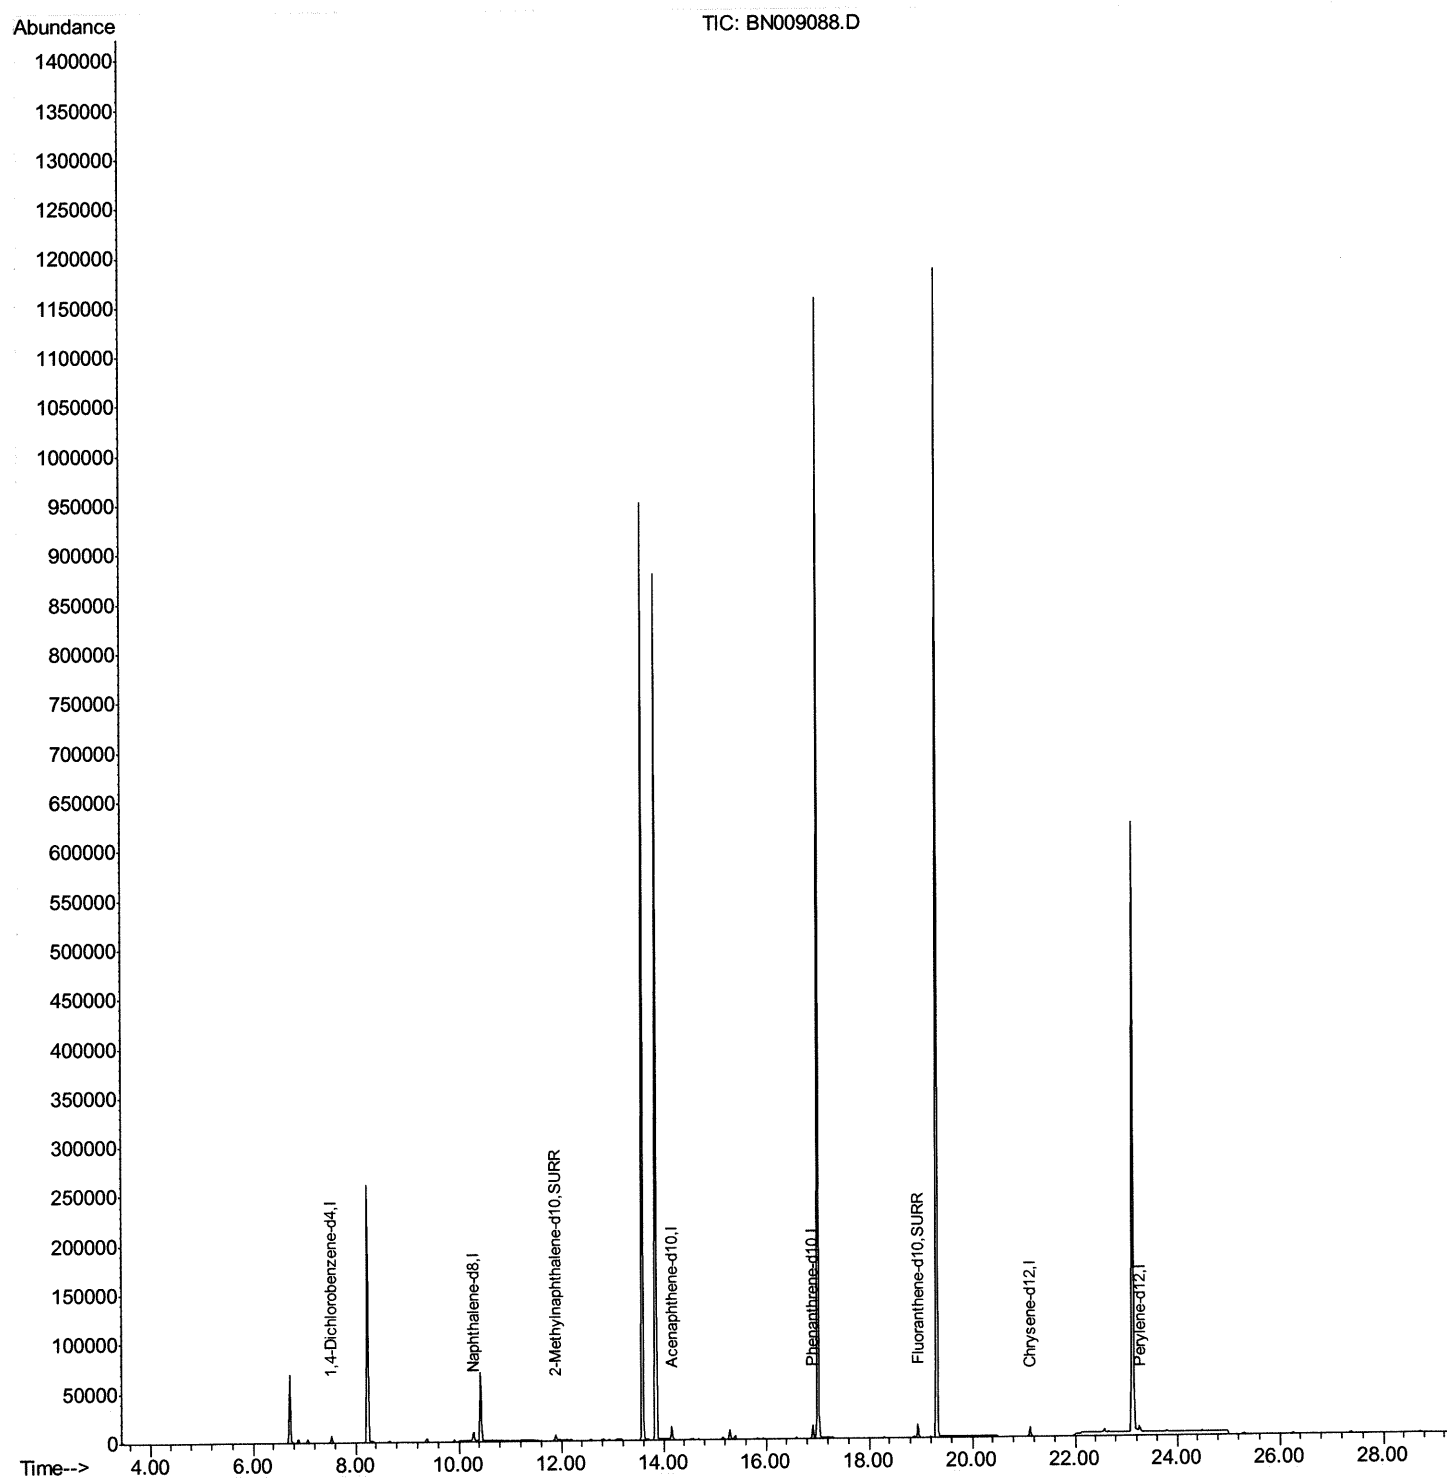

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN122319\
 Data File : BN009088.D
 Acq On : 23 Dec 2019 15:50
 Operator : JU
 Sample : PB125405BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK05

Manual Integrations
 APPROVED

mohammad
 12/24/2019 2:59:30 PM

Quant Time: Dec 23 17:10:40 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN121619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 20 23:31:06 2019
 Response via : Initial Calibration

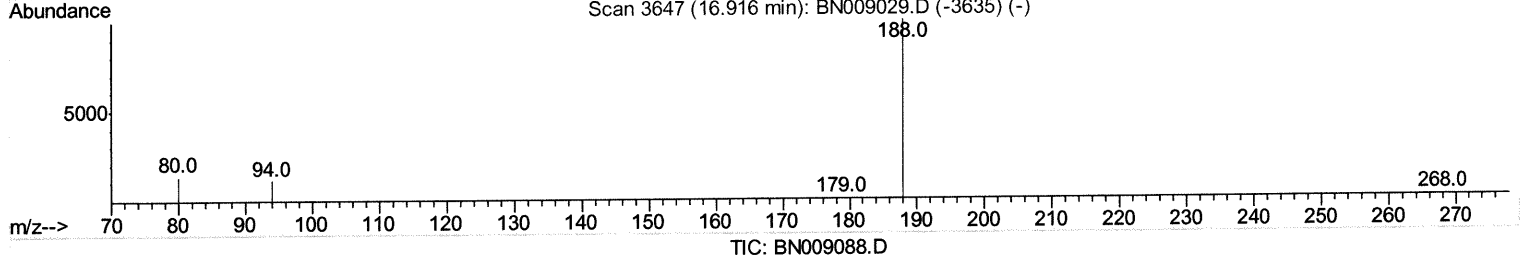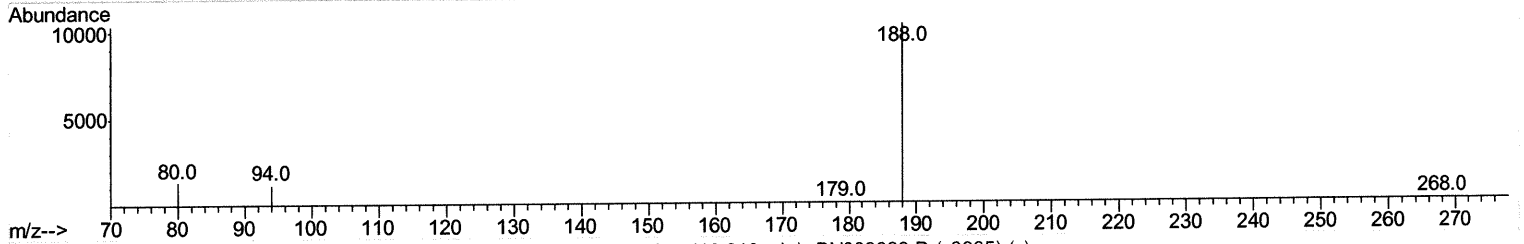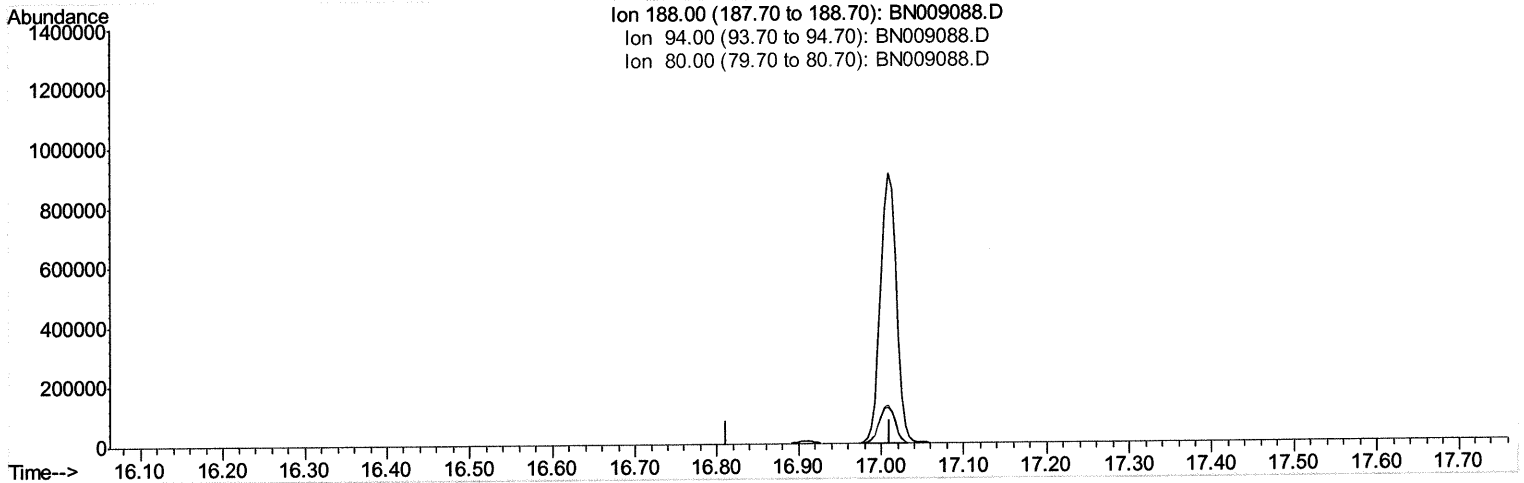

(10) Phenanthrene-d10 (I)

16.911min (-16.911) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.60	0.00#
80.00	13.70	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN122319\
 Data File : BN009088.D
 Acq On : 23 Dec 2019 15:50
 Operator : JU
 Sample : PB125405BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK05

Manual Integrations
 APPROVED

mohammad
 12/24/2019 2:59:30 PM

Quant Time: Dec 23 17:10:40 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN121619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 20 23:31:06 2019
 Response via : Initial Calibration

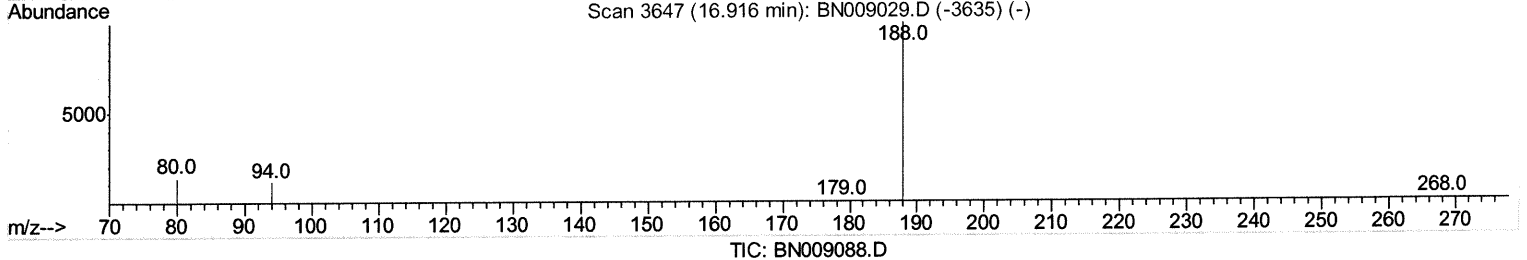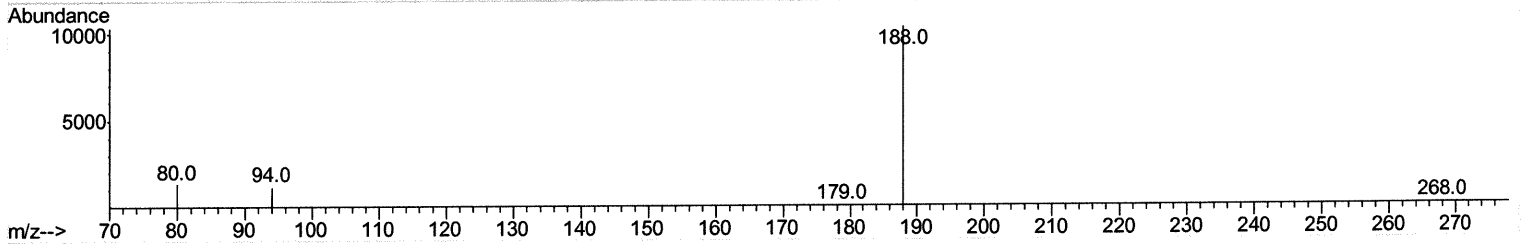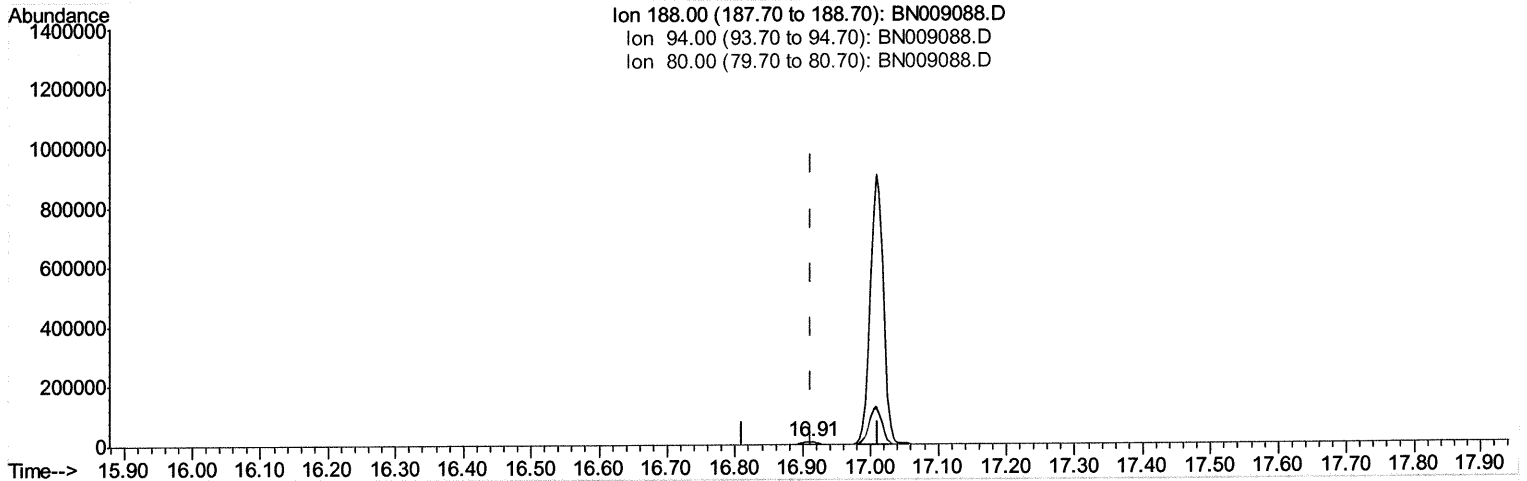

TIC: BN009088.D

(10) Phenanthrene-d10 (I)

16.912min (+0.000) 0.40ng/ul m JU/2/26/19

response 14479

Ion	Exp%	Act%
188.00	100	100
94.00	11.60	11.69
80.00	13.70	13.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN122319\
Data File : BN009088.D
Acq On : 23 Dec 2019 15:50
Operator : JU
Sample : PB125405BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK05

Manual Integrations
APPROVED

mohammad
12/24/2019 2:59:30 PM

Quant Time: Dec 23 17:11:24 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN121619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 20 23:31:06 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.53	152	3133	0.40	ng/ul	0.00
2) Naphthalene-d8	10.28	136	12088	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.16	164	6969	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.91	188	14479m >	0.40	ng/ul >	0.00
16) Chrysene-d12	21.12	240	8430	0.40	ng/ul	0.00
20) Perylene-d12	23.26	264	7760	0.40	ng/ul	0.00

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	11.88	152	7405	0.34	ng/ul	0.00
14) Fluoranthene-d10	18.94	212	14328	0.34	ng/ul	0.00

Target Compounds Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

JU 12/24/19