

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN122319\
Quantitation Report (QT Reviewed)


Data File : BN009092.D
Acq On : 23 Dec 2019 18:14
Operator : JU
Sample : PB125433BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK33

Manual Integrations
APPROVED

mohammad
12/24/2019 2:59:35 PM

Quant Time: Dec 24 02:51:45 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN121619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 24 02:43:36 2019
Response via : Initial Calibration

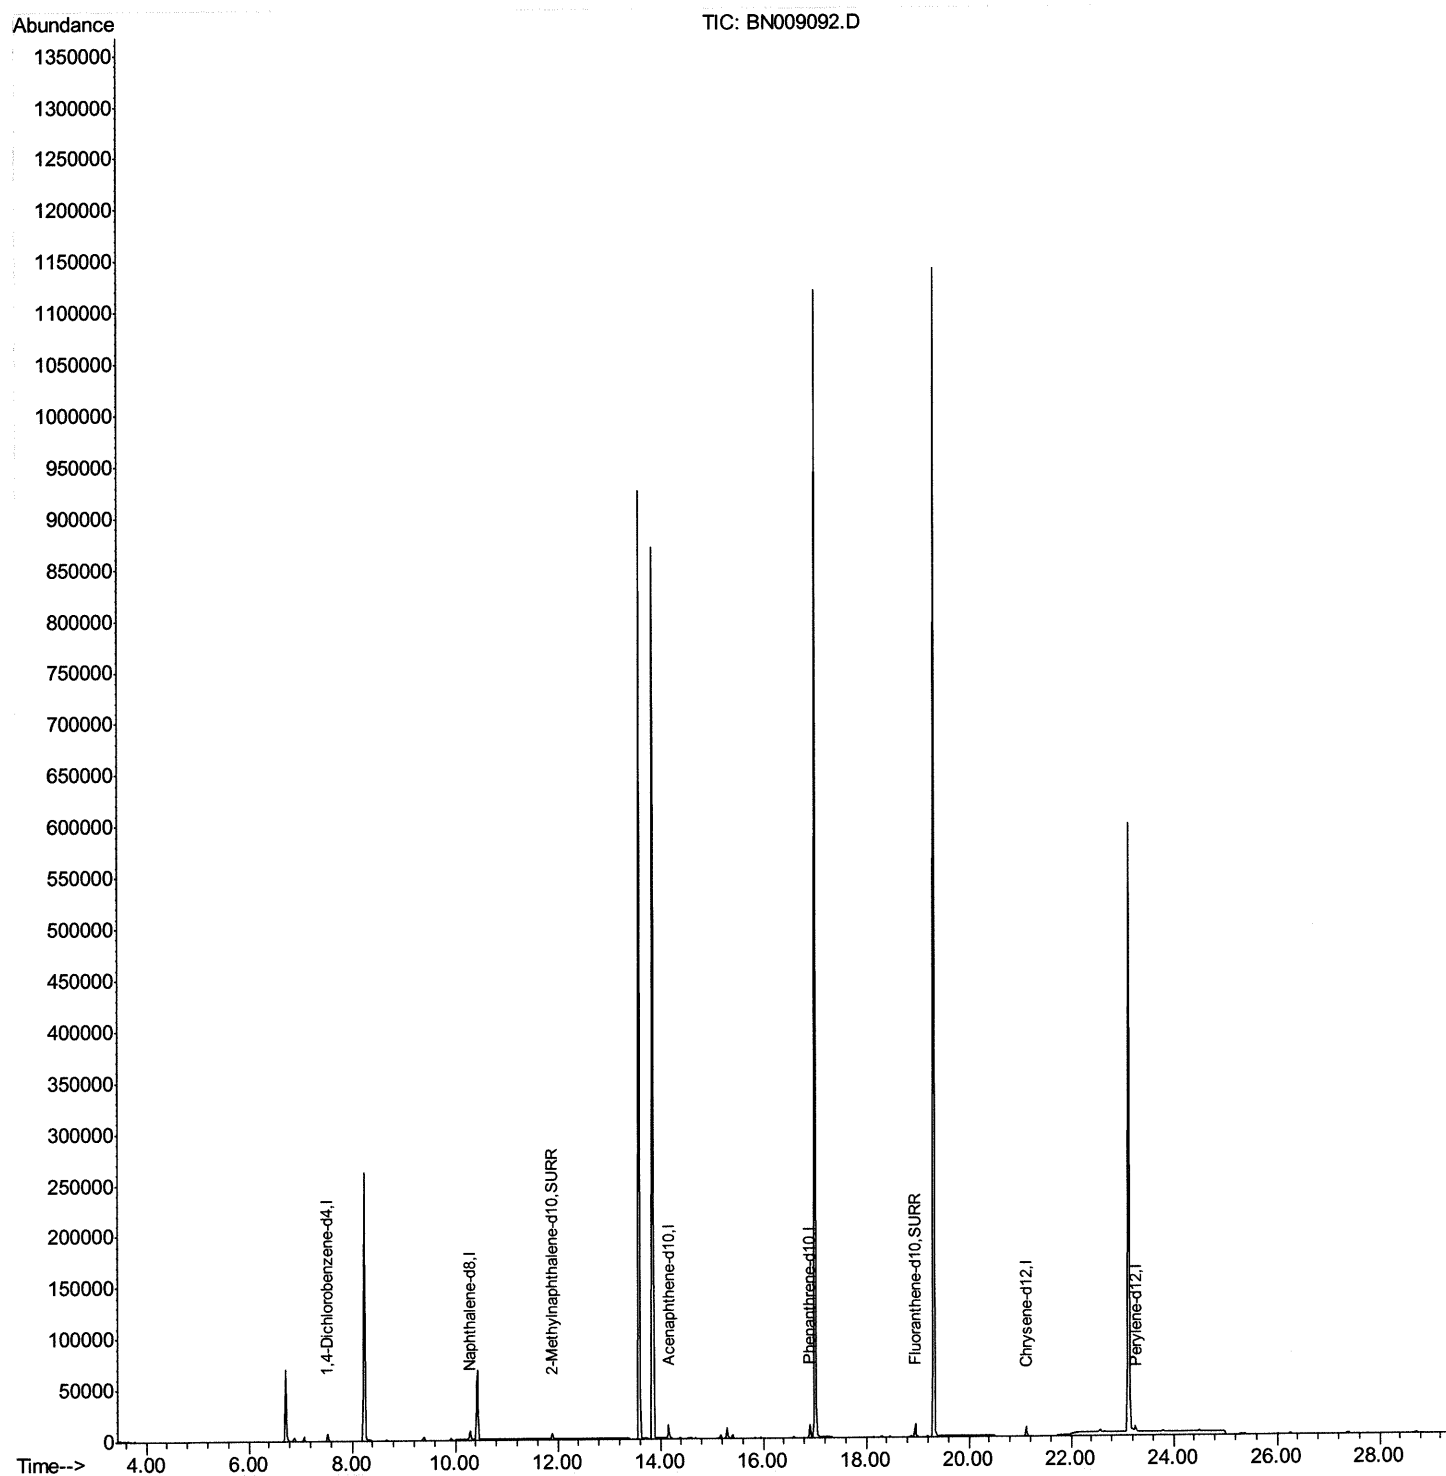

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN122319\
Quantitation Report (Qedit)




Data File : BN009092.D
Acq On : 23 Dec 2019 18:14
Operator : JU
Sample : PB125433BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK33

Manual Integrations
APPROVED

mohammad
12/24/2019 2:59:35 PM

Quant Time: Dec 24 02:46:04 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN121619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 24 02:43:36 2019
Response via : Initial Calibration

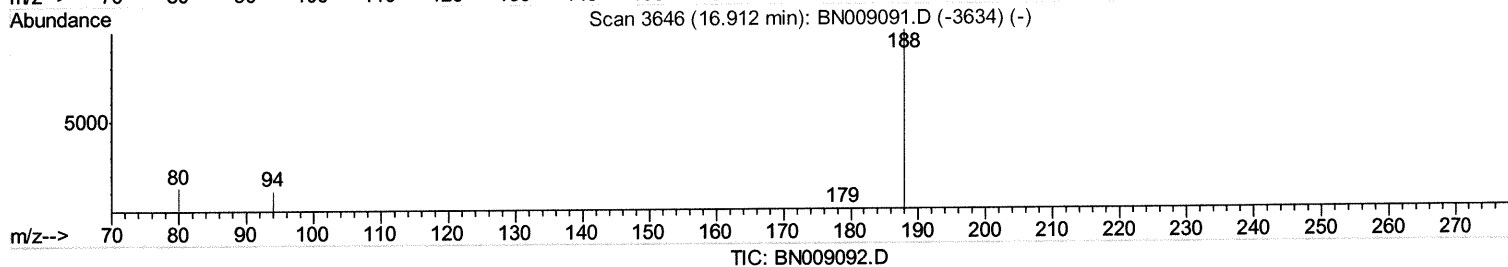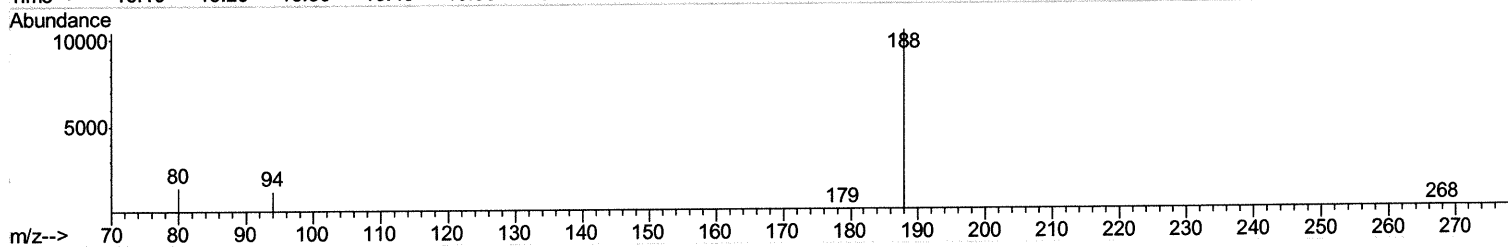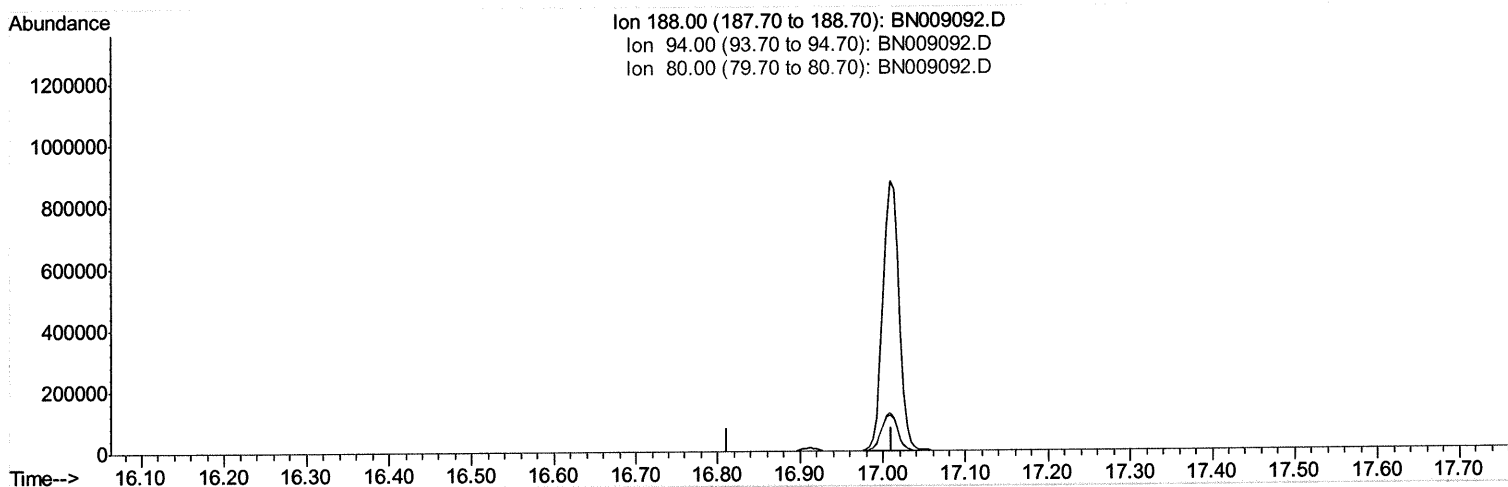

(10) Phenanthrene-d10 (I)

16.912min (-16.912) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.60	0.00#
80.00	13.70	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN122319\
Quantitation Report (Qedit)




Data File : BN009092.D
Acq On : 23 Dec 2019 18:14
Operator : JU
Sample : PB125433BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK33

Manual Integrations
APPROVED

mohammad
12/24/2019 2:59:35 PM

Quant Time: Dec 24 02:46:04 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN121619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 24 02:43:36 2019
Response via : Initial Calibration

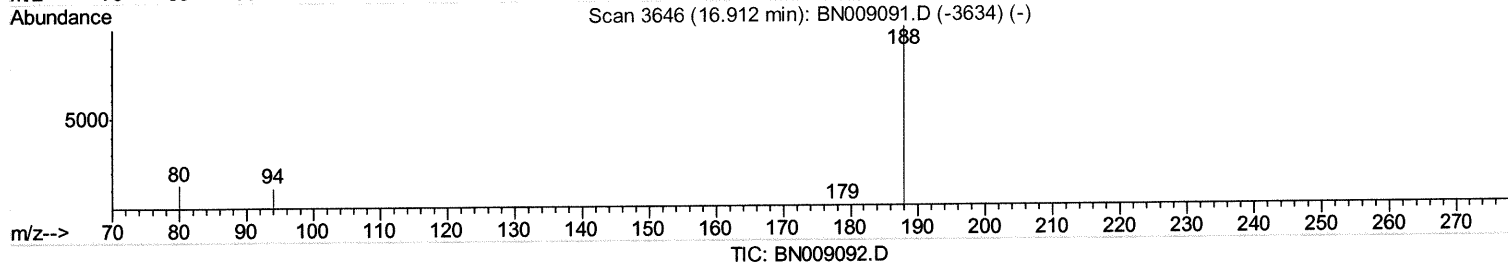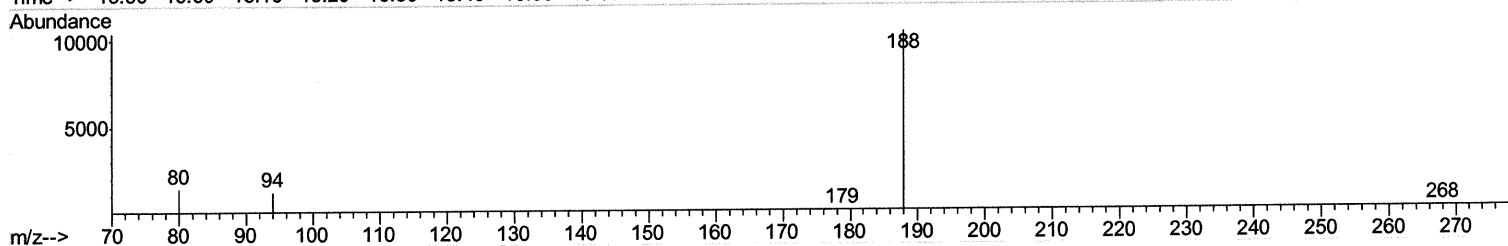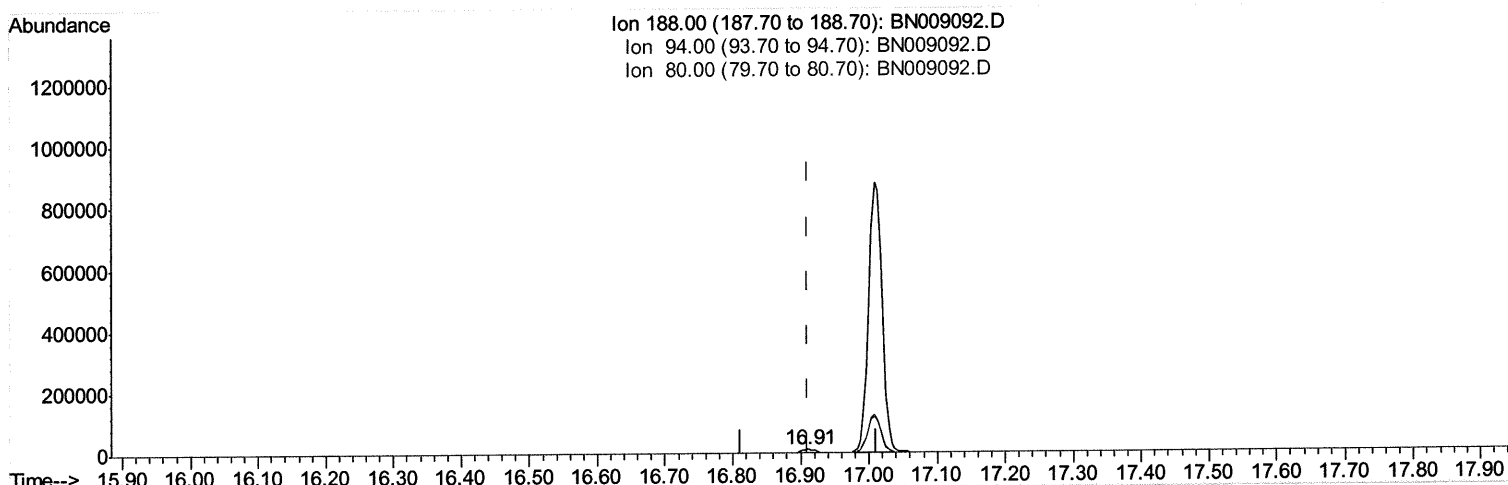

(10) Phenanthrene-d10 (I)

16.912min (-0.000) 0.40ng/ul m JU 12/26/19

response 14066

Ion	Exp%	Act%
188.00	100	100
94.00	11.60	11.65
80.00	13.70	13.55
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN122319\
Quantitation Report (Qedit)




Data File : BN009092.D
Acq On : 23 Dec 2019 18:14
Operator : JU
Sample : PB125433BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK33

Manual Integrations
APPROVED

mohammad
12/24/2019 2:59:35 PM

Quant Time: Dec 24 02:50:59 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN121619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 24 02:43:36 2019
Response via : Initial Calibration

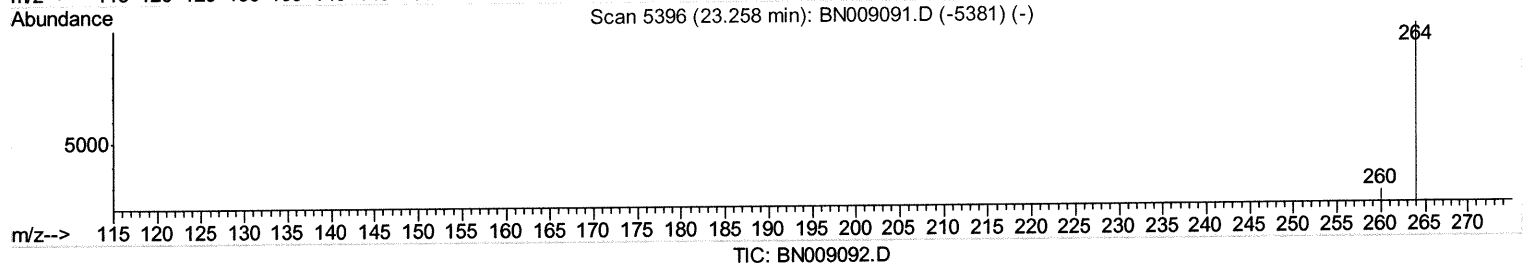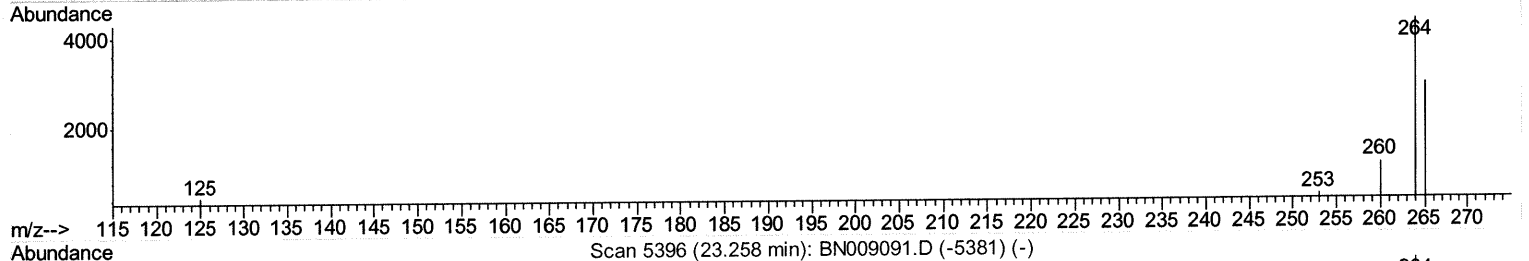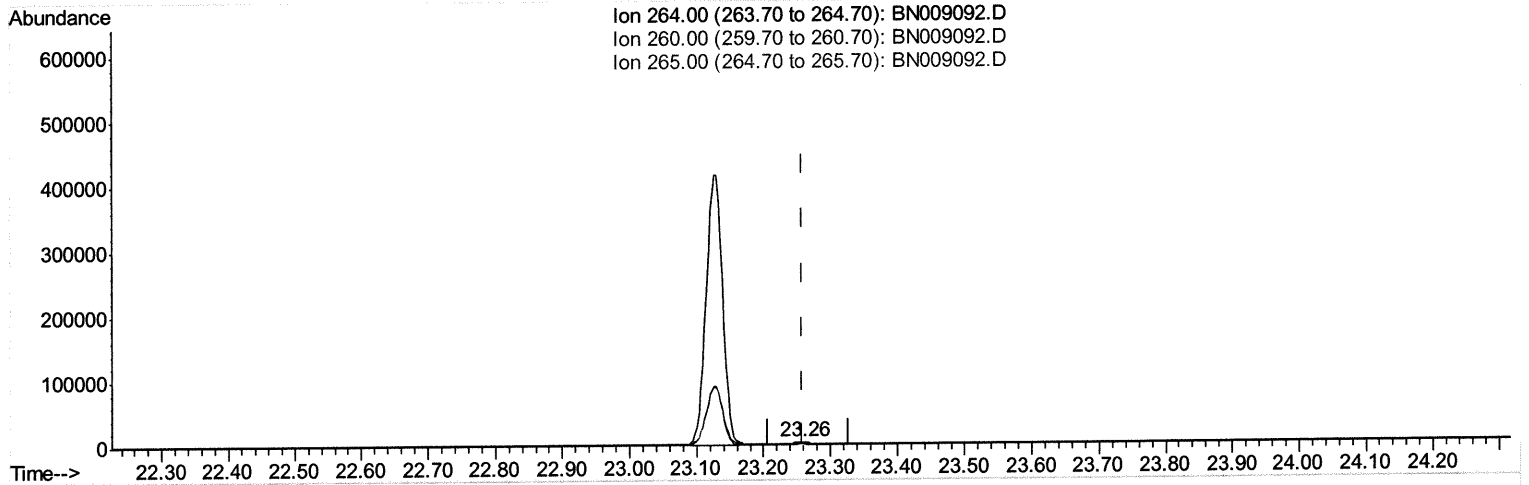

(20) Perylene-d12 (I)

23.258min (-0.000) 0.40ng/ul

response 7407

Ion	Exp%	Act%
264.00	100	100
260.00	26.70	26.34
265.00	61.20	67.27
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN122319\
Quantitation Report (Qedit)




Data File : BN009092.D
Acq On : 23 Dec 2019 18:14
Operator : JU
Sample : PB125433BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK33

Manual Integrations
APPROVED

mohammad
12/24/2019 2:59:35 PM

Quant Time: Dec 24 02:50:59 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN121619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 24 02:43:36 2019
Response via : Initial Calibration

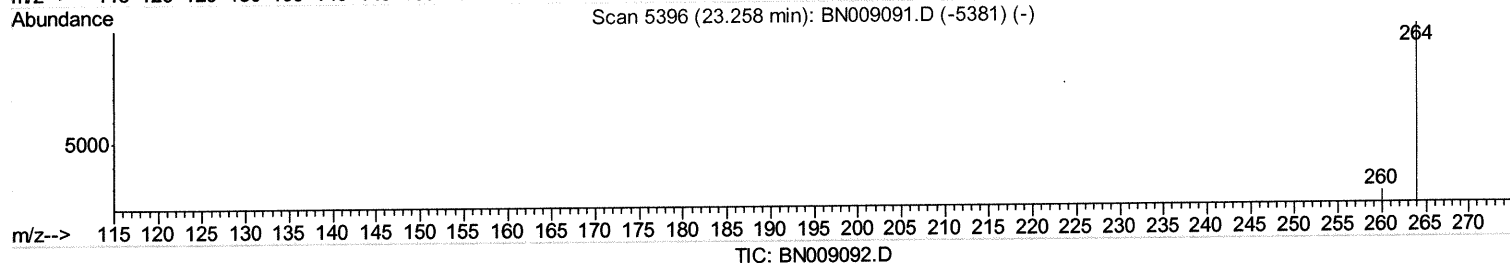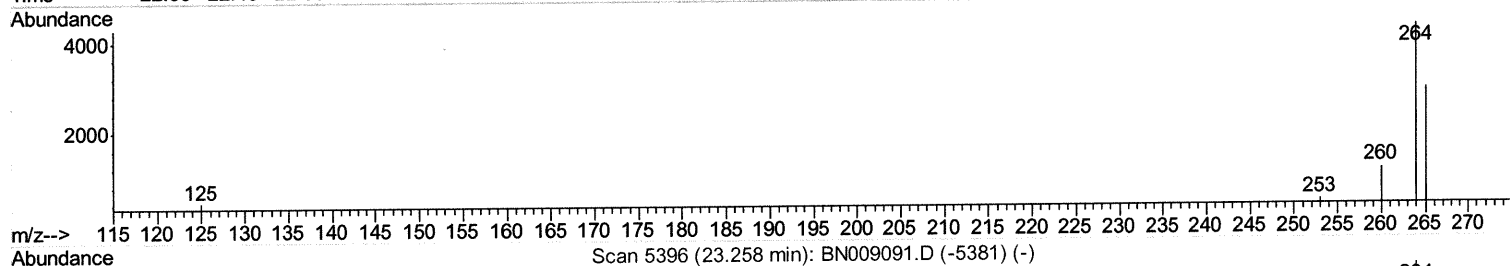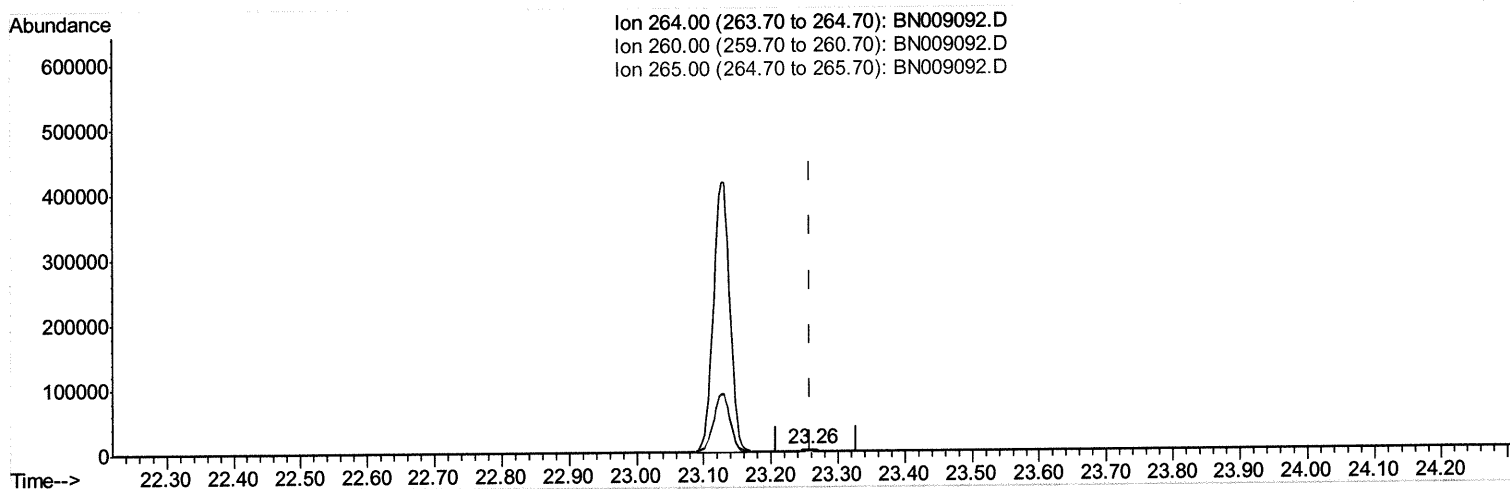

(20) Perylene-d12 (I)

23.258min (-0.000) 0.40ng/ul m

JU 12/26/19

response 6256

Ion	Exp%	Act%
264.00	100	100
260.00	26.70	26.34
265.00	61.20	67.27
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN122319\
 Quantitation Report (QT Reviewed)
 Data File : BN009092.D
 Acq On : 23 Dec 2019 18:14
 Operator : JU
 Sample : PB125433BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK33

Manual Integrations
 APPROVED

mohammad
 12/24/2019 2:59:35 PM

Quant Time: Dec 24 02:51:45 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN121619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 24 02:43:36 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.54	152	3113	0.40	ng/ul	0.00
2) Naphthalene-d8	10.28	136	11849	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.16	164	6900	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.91	188	14066m >	0.40	ng/ul	> 0.00
16) Chrysene-d12	21.12	240	7786	0.40	ng/ul	0.00
20) Perylene-d12	23.26	264	6256m >	0.40	ng/ul	> 0.00

Ju 12/26/19

Ju 12/26/19

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	11.89	152	7328	0.35	ng/ul	0.00
14) Fluoranthene-d10	18.95	212	13614	0.33	ng/ul	0.00

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed