

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN122319\
Quantitation Report (QT Reviewed)


Data File : BN009093.D
Acq On : 23 Dec 2019 18:50
Operator : JU
Sample : PB125488BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK88

Manual Integrations
APPROVED

mohammad
12/24/2019 2:59:38 PM

Quant Time: Dec 24 02:53:03 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN121619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 24 02:43:36 2019
Response via : Initial Calibration

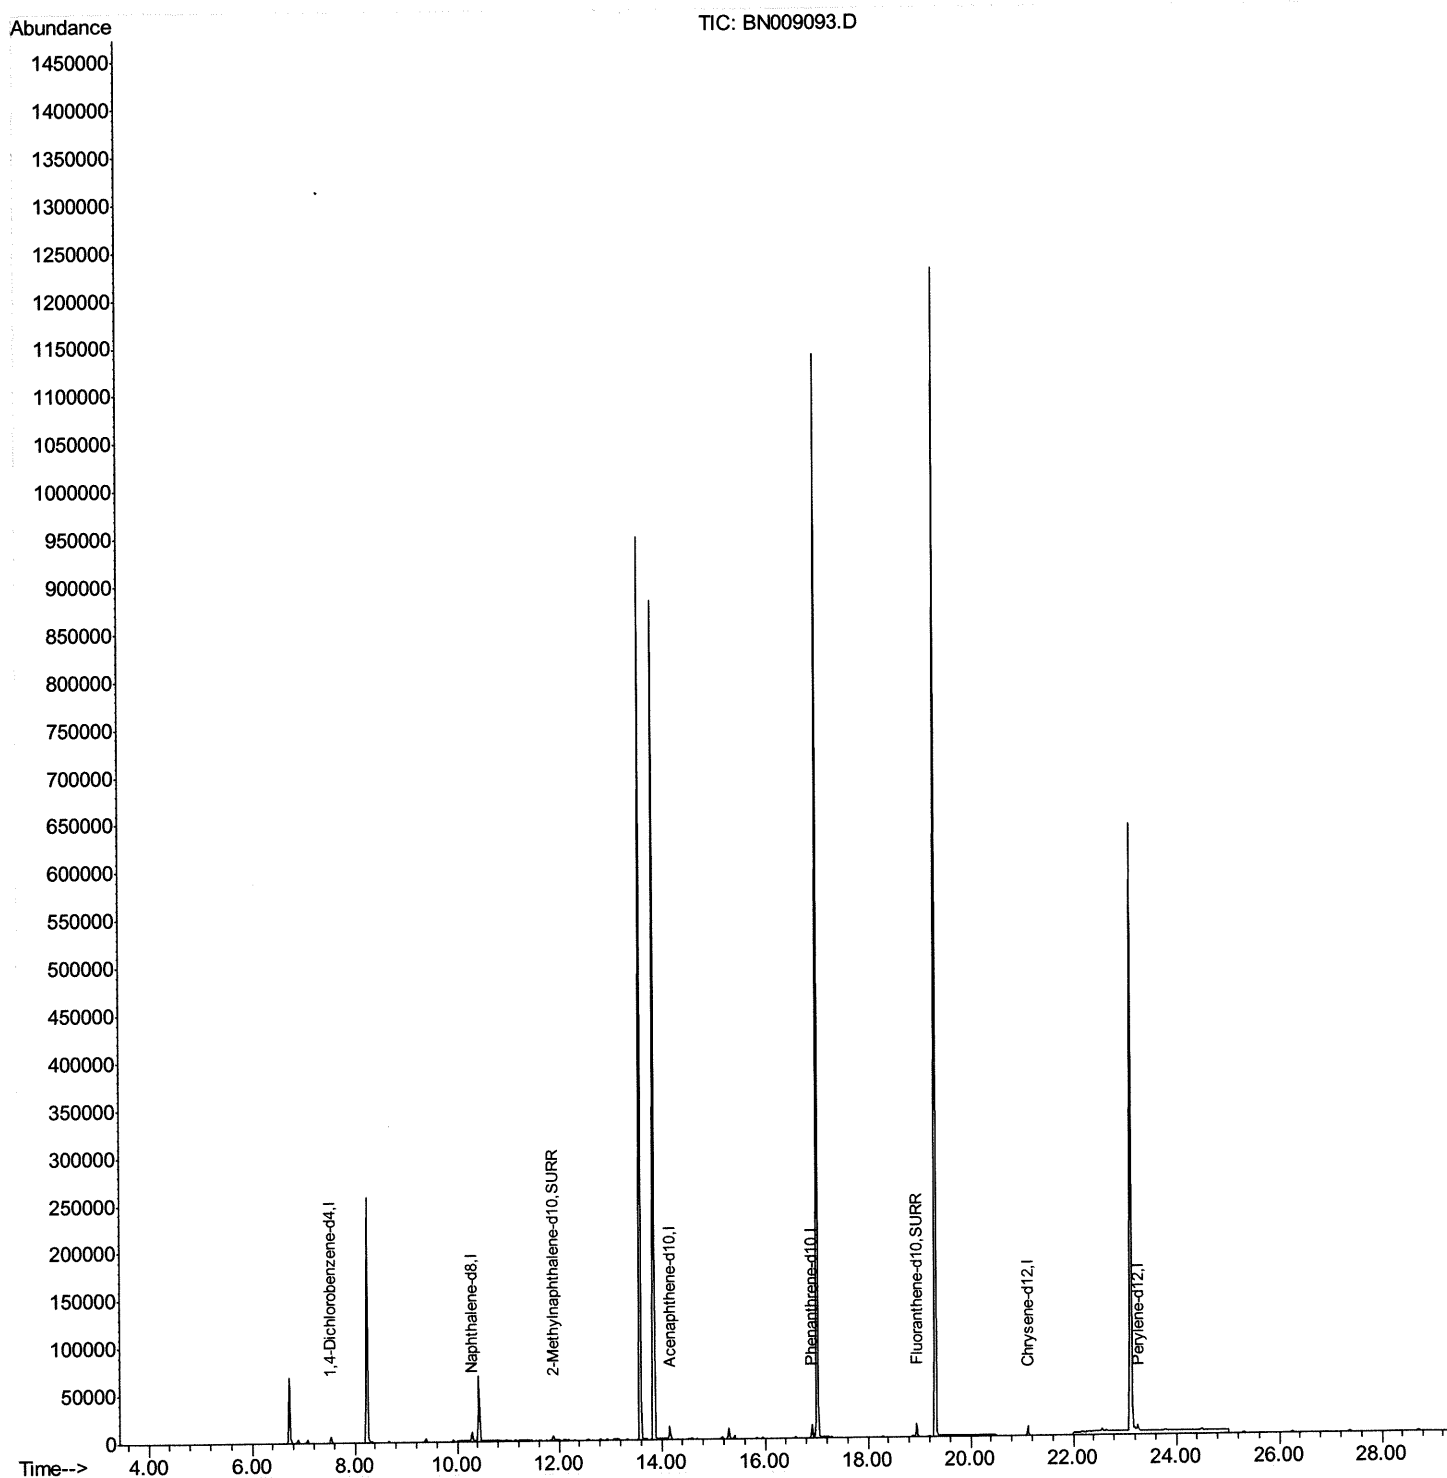

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN122319\
Quantitation Report (Qedit)




Data File : BN009093.D
Acq On : 23 Dec 2019 18:50
Operator : JU
Sample : PB125488BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK88

Manual Integrations
APPROVED

mohammad
12/24/2019 2:59:38 PM

Quant Time: Dec 24 02:46:08 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN121619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 24 02:43:36 2019
Response via : Initial Calibration

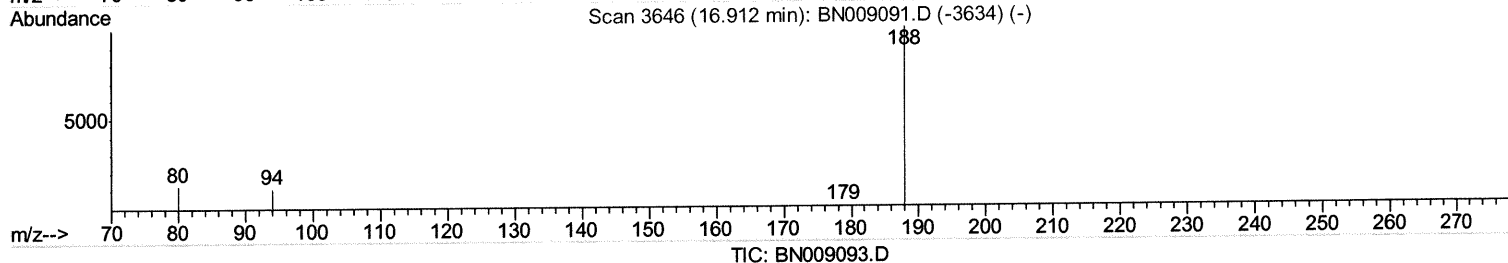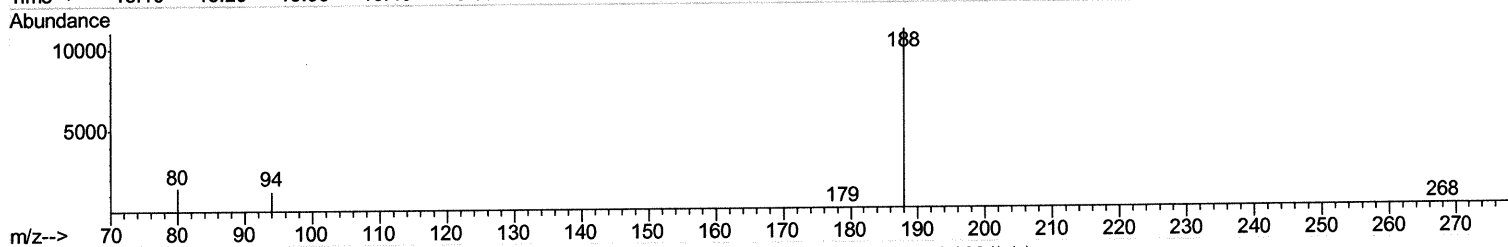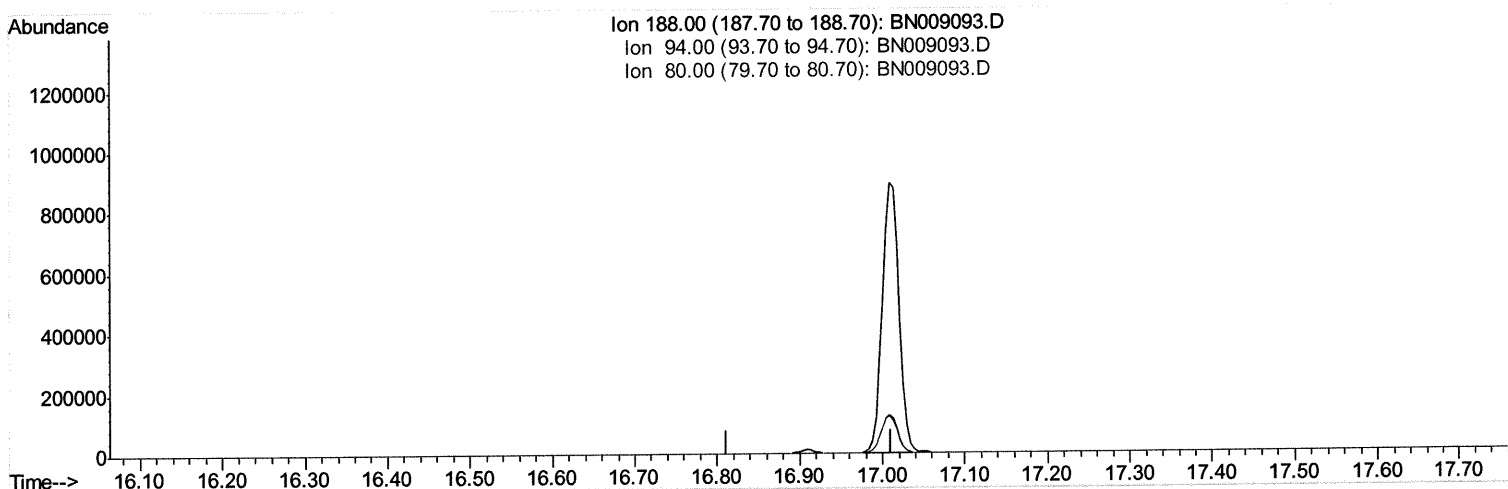

(10) Phenanthrene-d10 (I)

16.912min (-16.912) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.60	0.00#
80.00	13.70	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN122319\
Quantitation Report (Qedit)




Data File : BN009093.D
Acq On : 23 Dec 2019 18:50
Operator : JU
Sample : PB125488BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK88

Manual Integrations
APPROVED

mohammad
12/24/2019 2:59:38 PM

Quant Time: Dec 24 02:46:08 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN121619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 24 02:43:36 2019
Response via : Initial Calibration

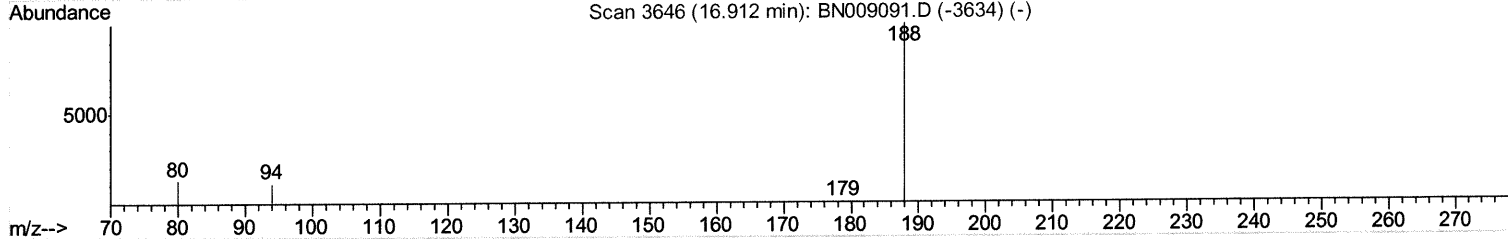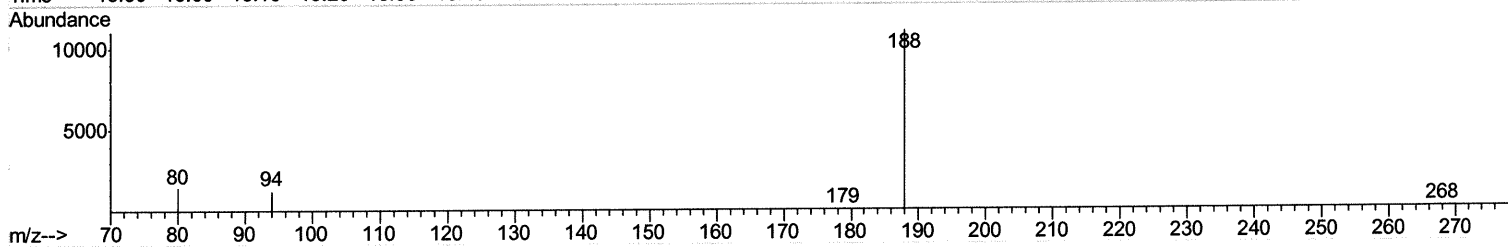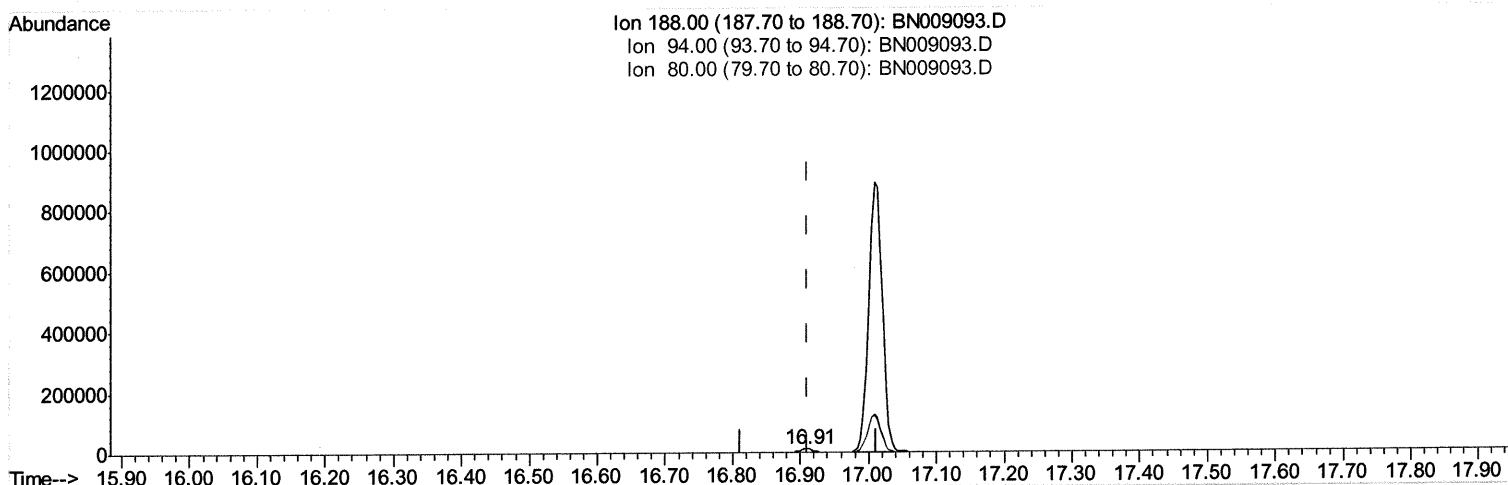

TIC: BN009093.D

(10) Phenanthrene-d10 (I)

16.912min (+0.000) 0.40ng/ul m *JU 12/26/19*

response 14791

Ion	Exp%	Act%
188.00	100	100
94.00	11.60	11.56
80.00	13.70	13.09
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN122319\
Quantitation Report (QT Reviewed)

Data File : BN009093.D
Acq On : 23 Dec 2019 18:50
Operator : JU
Sample : PB125488BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK88

Manual Integrations
APPROVED

mohammad
12/24/2019 2:59:38 PM

Quant Time: Dec 24 02:53:03 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN121619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 24 02:43:36 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.54	152	3184	0.40	ng/ul	0.00
2) Naphthalene-d8	10.29	136	11891	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.16	164	7052	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.91	188	14791m >	0.40	ng/ul >	0.00
16) Chrysene-d12	21.12	240	8529	0.40	ng/ul	0.00
20) Perylene-d12	23.26	264	8207	0.40	ng/ul	0.00

J4 12/26/19

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	11.89	152	7314	0.35	ng/ul	0.00
14) Fluoranthene-d10	18.94	212	14588	0.33	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed