


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN122319\
Data File : BN009121.D
Acq On : 24 Dec 2019 12:09
Operator : JU
Sample : K6276-04
Misc :
ALS Vial : 37 Sample Multiplier: 1

Quant Time: Dec 24 12:48:11 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN121619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 24 06:49:13 2019
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
C0C44

Manual Integrations
APPROVED

mohammad
12/24/2019 3:00:54 PM

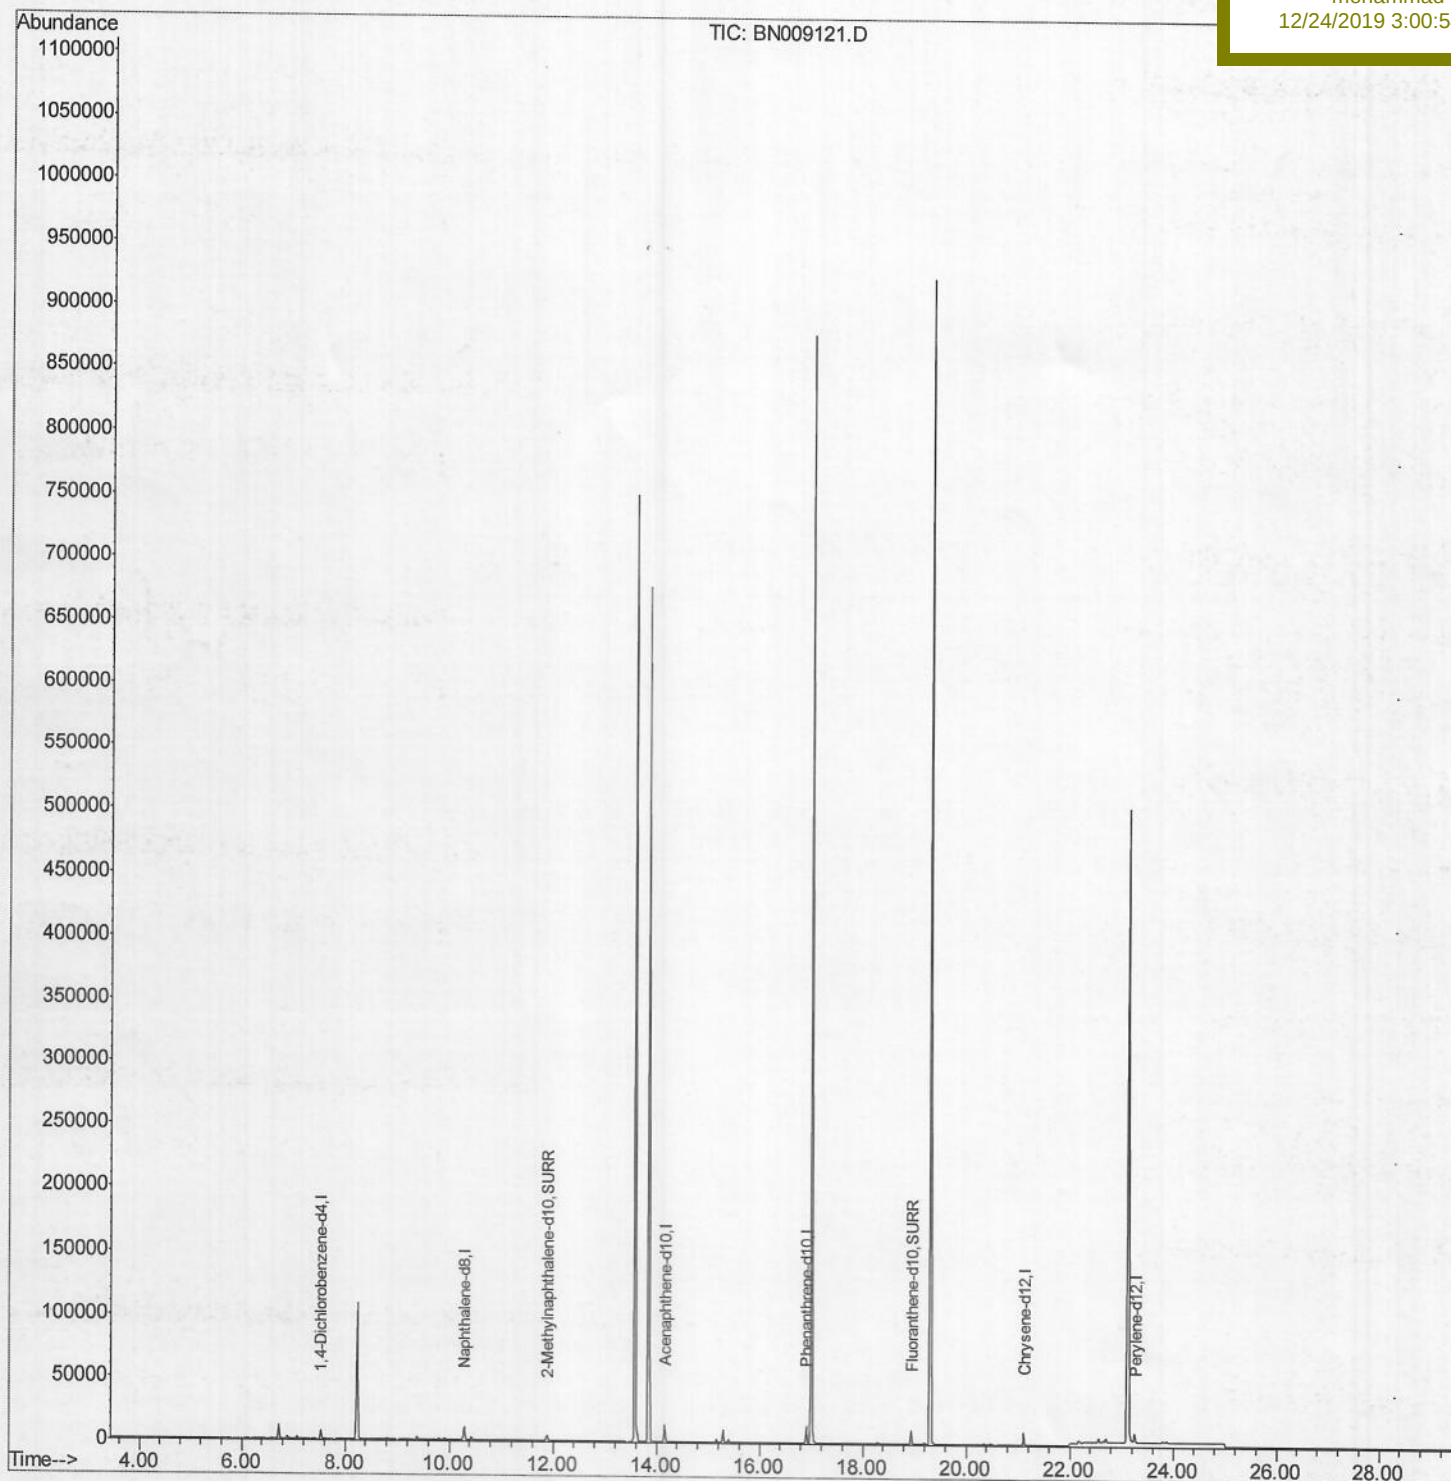

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN122319\

Data File : BN009121.D

Acq On : 24 Dec 2019 12:09

Operator : JU

Sample : K6276-04

Misc :

ALS Vial : 37 Sample Multiplier: 1

Quant Time: Dec 24 12:46:49 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN121619.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Dec 24 06:49:13 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :




C0C44

Manual Integrations

APPROVED

mohammad

12/24/2019 3:00:54 PM

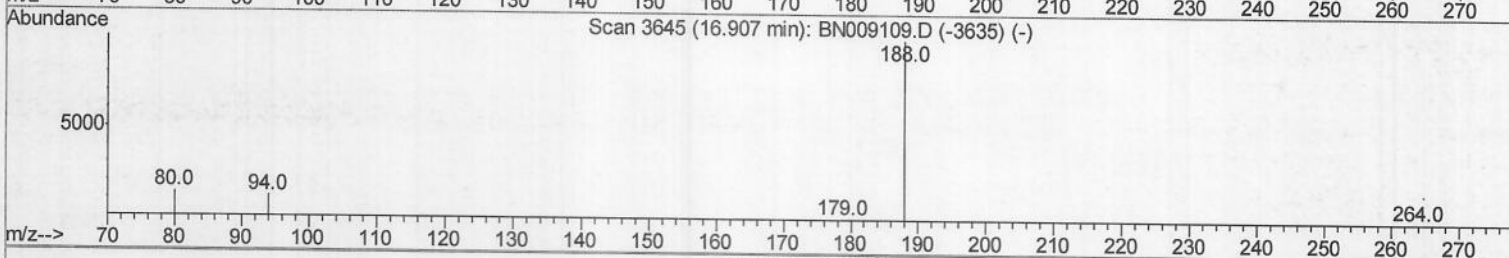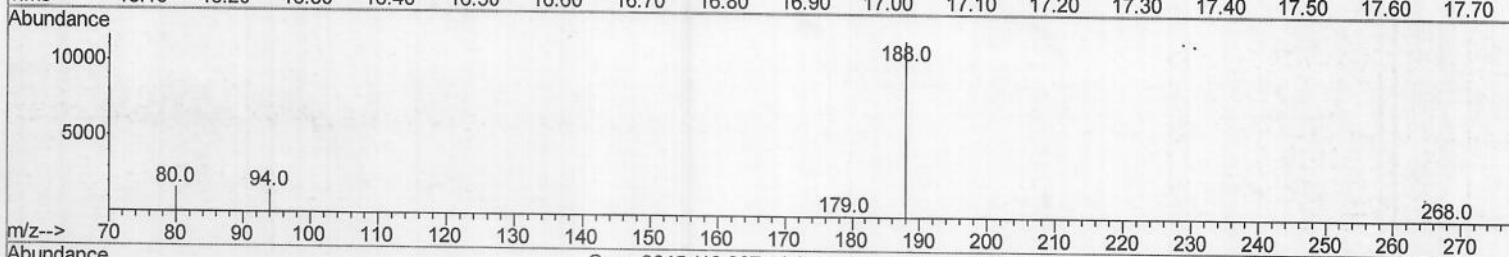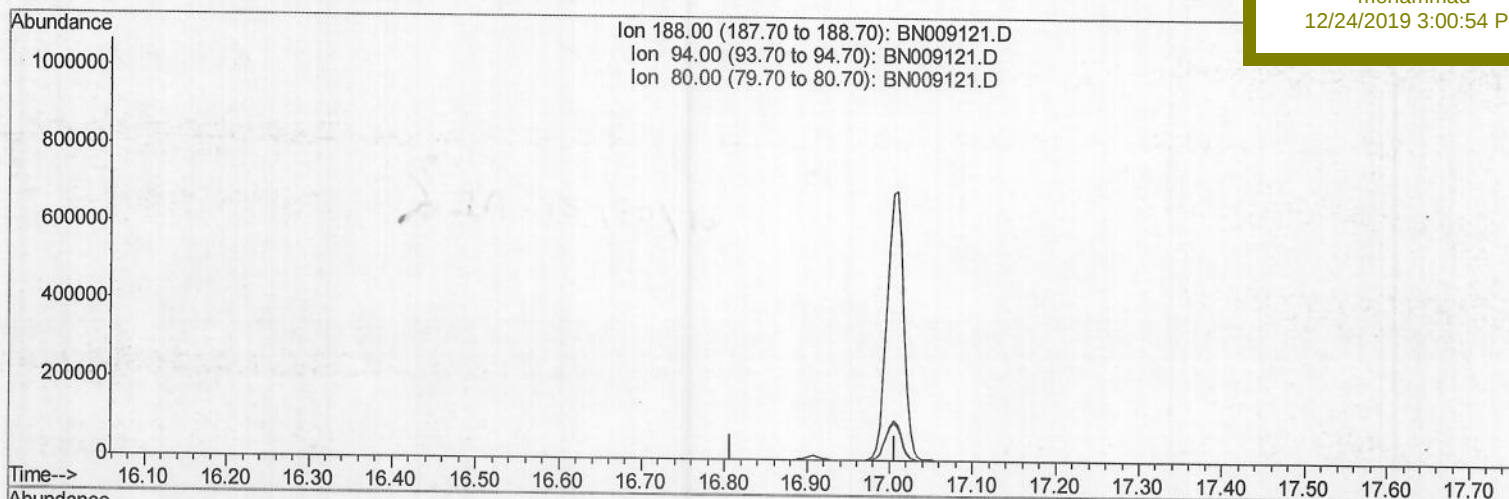

TIC: BN009121.D

(10) Phenanthrene-d10 (I)

16.907min (-16.907) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.60	0.00#
80.00	13.70	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN122319\

Data File : BN009121.D

Acq On : 24 Dec 2019 12:09

Operator : JU

Sample : K6276-04

Misc :

ALS Vial : 37 Sample Multiplier: 1

Quant Time: Dec 24 12:46:49 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN121619.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Dec 24 06:49:13 2019

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :




C0C44

Manual Integrations

APPROVED

mohammad

12/24/2019 3:00:54 PM

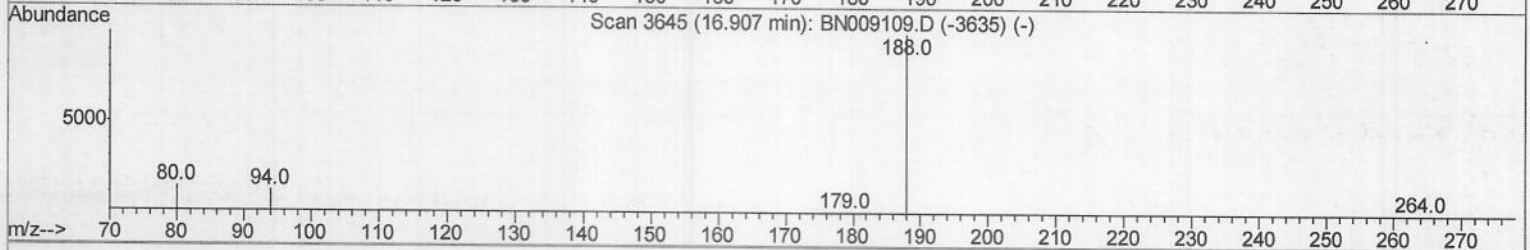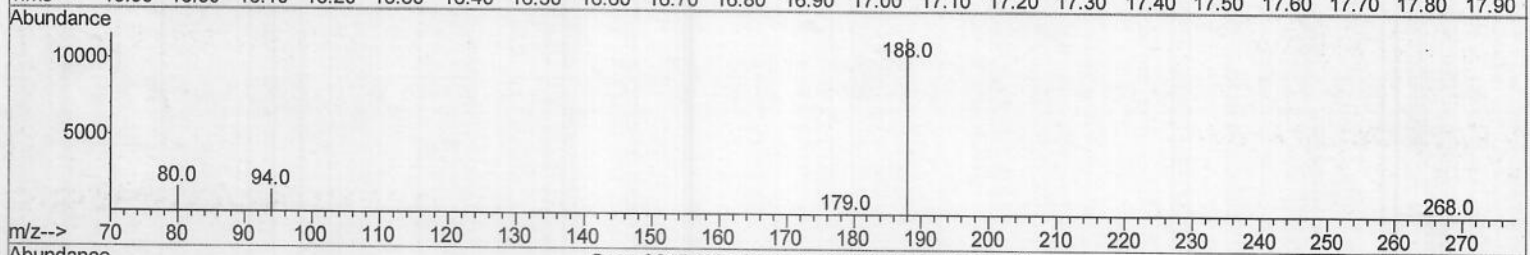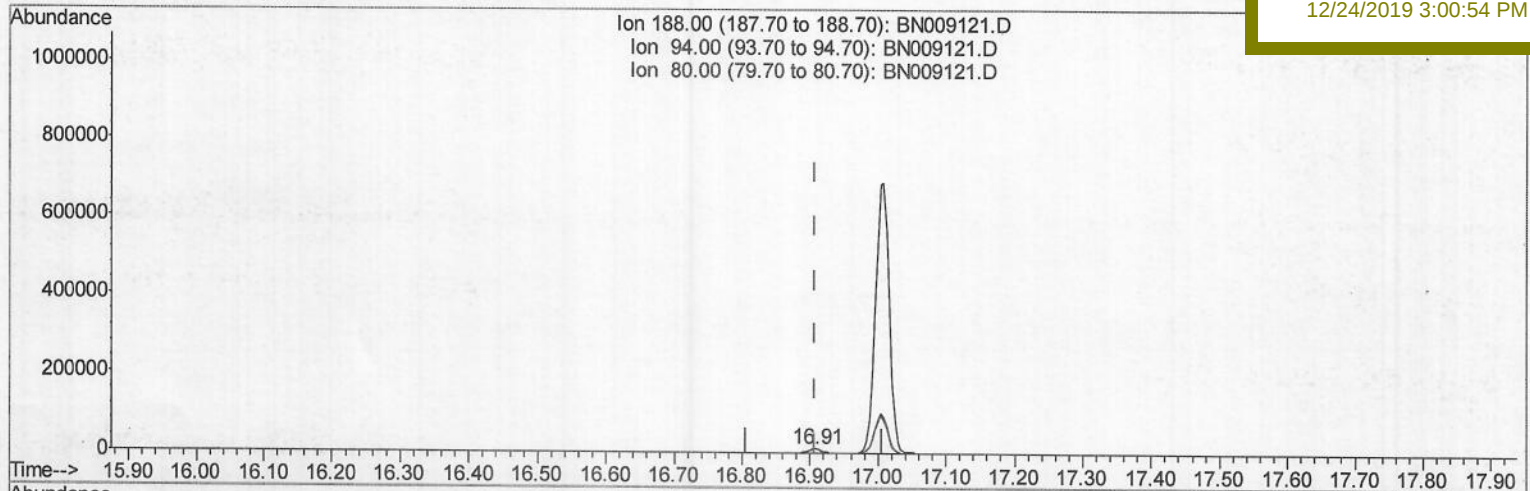

TIC: BN009121.D

(10) Phenanthrene-d10 (I)

16.907min (+0.000) 0.40ng/ul m

response 15590

Ion	Exp%	Act%
188.00	100	100
94.00	11.60	12.40
80.00	13.70	13.74
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN122319\
Data File : BN009121.D
Acq On : 24 Dec 2019 12:09
Operator : JU
Sample : K6276-04
Misc :
ALS Vial : 37 Sample Multiplier: 1

Quant Time: Dec 24 12:48:11 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN121619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 24 06:49:13 2019
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
C0C44

Manual Integrations
APPROVED

mohammad
12/24/2019 3:00:54 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.53	152	3506	0.40	ng/ul	0.00
2) Naphthalene-d8	10.28	136	13546	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.16	164	7722	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.91	188	15590m	0.40	ng/ul	0.00
16) Chrysene-d12	21.11	240	8695	0.40	ng/ul	0.00
20) Perylene-d12	23.25	264	8284	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.88	152	5352	0.22	ng/ul	0.00
14) Fluoranthene-d10	18.94	212	12142	0.26	ng/ul	0.00

Target Compounds

Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

JU 12/31/19