

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN122319\
 Data File : BN009116.D
 Acq On : 24 Dec 2019 09:09
 Operator : JU
 Sample : K6254-07
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0C21

Quant Time: Dec 24 10:57:16 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN121619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 24 06:49:13 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.53	152	3905	0.40	ng/ul	0.00
2) Naphthalene-d8	10.28	136	14503	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.16	164	7659	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.91	188	14215	0.40	ng/ul	0.00
16) Chrysene-d12	21.12	240	8255	0.40	ng/ul	0.00
20) Perylene-d12	23.25	264	8577	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.88	152	2640	0.10	ng/ul	0.00
14) Fluoranthene-d10	18.94	212	4574	0.11	ng/ul	0.00
Target Compounds						
12) Phenanthrene	16.95	178	1226	0.025	ng/ul#	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN122319\
Data File : BN009116.D
Acq On : 24 Dec 2019 09:09
Operator : JU
Sample : K6254-07
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0C21

Quant Time: Dec 24 10:57:16 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN121619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 24 06:49:13 2019
Response via : Initial Calibration

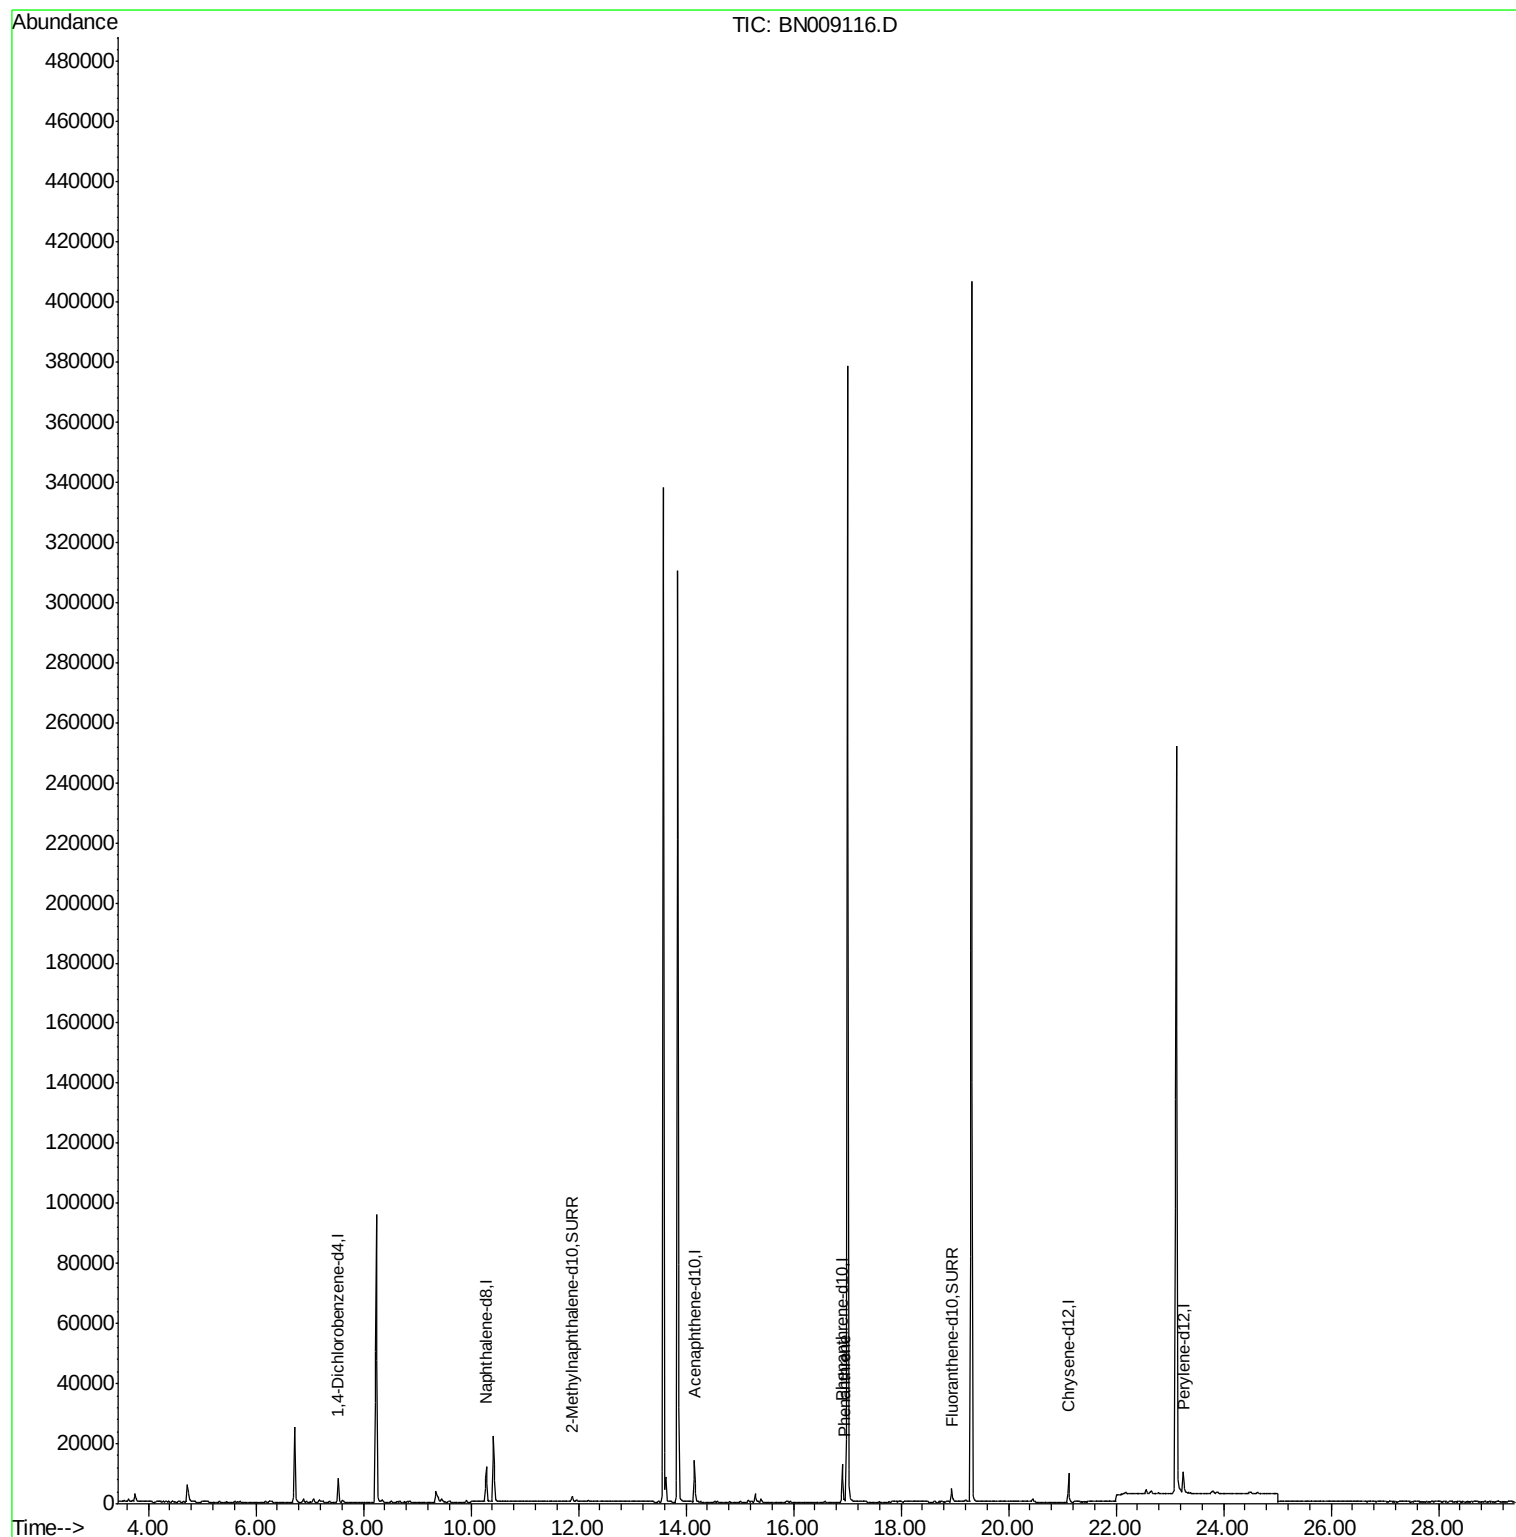

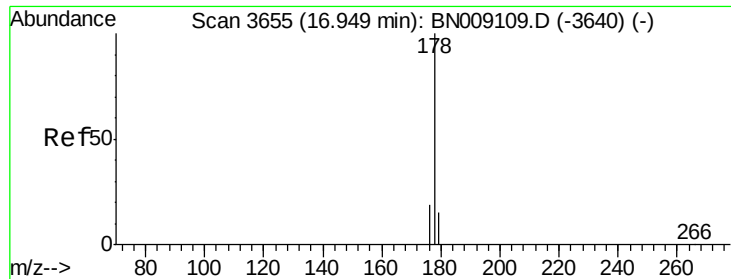

#12

Phenanthrene

Concen: 0.025 ng/ul

RT: 16.95 min Scan# 3654

Delta R.T. -0.00 min

Lab File: BN009116.D

Acq: 24 Dec 2019 09:09

Instrument :

BNA_N

ClientSampleId :

C0C21



Tot Ion:178 Resp: 1226

Ion Ratio Lower Upper

178 100

179 24.1 12.3 18.5#

176 24.3 15.1 22.7#

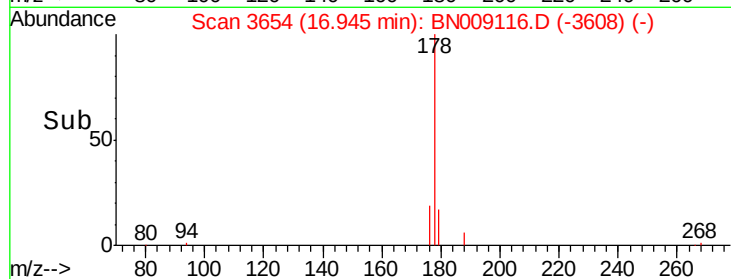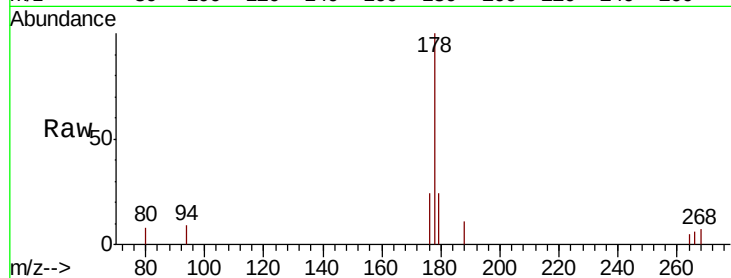

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

