

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN122319\
 Data File : BN009122.D
 Acq On : 24 Dec 2019 12:44
 Operator : JU
 Sample : K6254-07
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0C21

Quant Time: Dec 24 13:15:40 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN121619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 24 06:49:13 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.53	152	3639	0.40	ng/ul	0.00
2) Naphthalene-d8	10.28	136	14162	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.16	164	8095	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.91	188	16893	0.40	ng/ul	0.00
16) Chrysene-d12	21.11	240	9554	0.40	ng/ul	0.00
20) Perylene-d12	23.25	264	8674	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.88	152	3802	0.15	ng/ul	0.00
14) Fluoranthene-d10	18.94	212	8108	0.16	ng/ul	0.00
Target Compounds						
					Ovalue	
12) Phenanthrene	16.95	178	1500	0.026	ng/ul#	89
17) Pyrene	19.33	202	1096	0.022	ng/ul#	72


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN122319\
Data File : BN009122.D
Acq On : 24 Dec 2019 12:44
Operator : JU
Sample : K6254-07
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0C21

Quant Time: Dec 24 13:15:40 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN121619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 24 06:49:13 2019
Response via : Initial Calibration

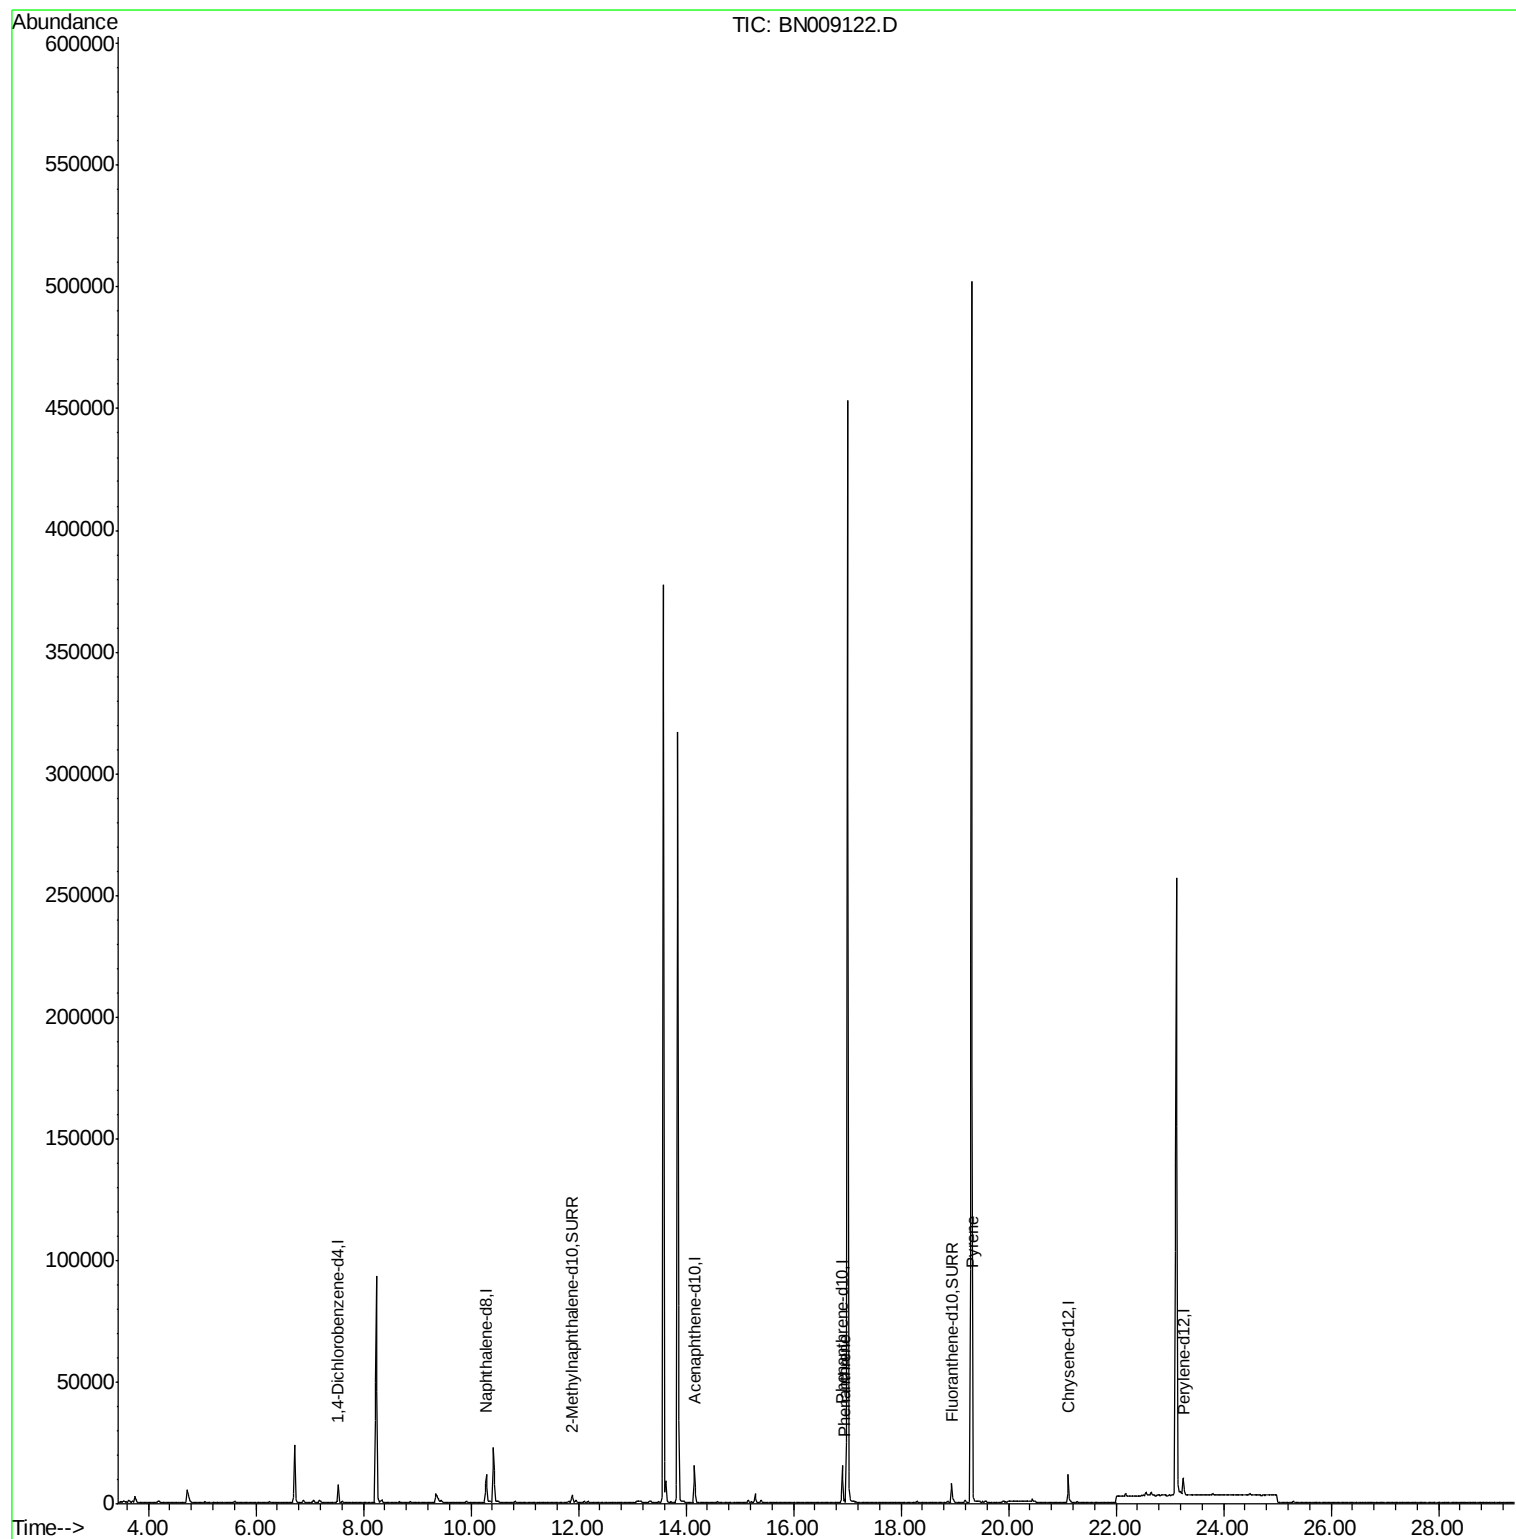

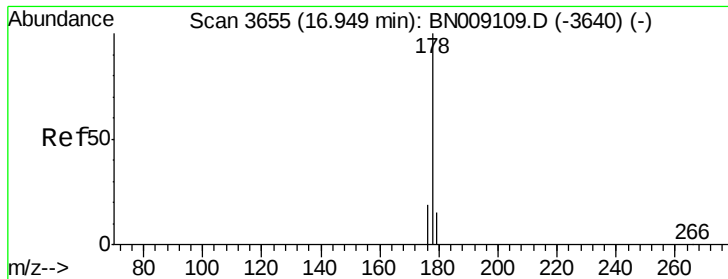

#12

Phenanthrene

Concen: 0.026 ng/ul

RT: 16.95 min Scan# 3655

Delta R.T. -0.00 min

Lab File: BN009122.D

Acq: 24 Dec 2019 12:44

Instrument :

BNA_N

ClientSampleId :

C0C21


Tot Ion:178 Resp: 1500

Ion Ratio Lower Upper

178 100

179 21.0 12.3 18.5#




176 22.7 15.1 22.7#

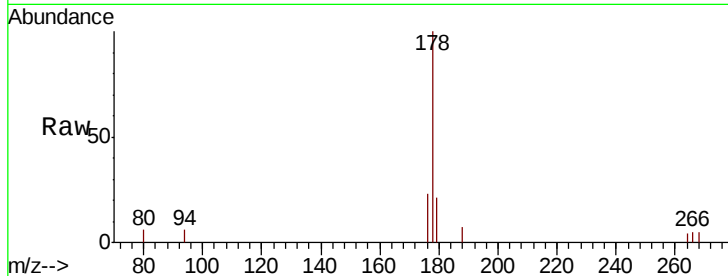

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

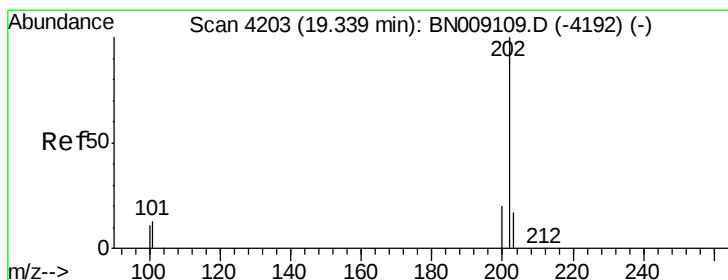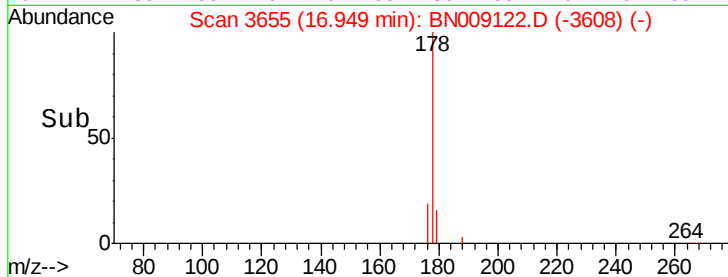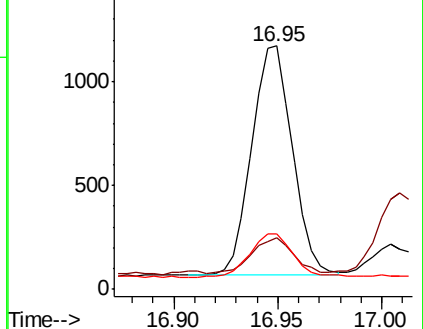

#17

Pyrene

Concen: 0.022 ng/ul

RT: 19.33 min Scan# 4202

Delta R.T. -0.00 min

Lab File: BN009122.D

Acq: 24 Dec 2019 12:44


Tgt Ion:202 Resp: 1096

Ion Ratio Lower Upper

202 100

101 22.9 10.9 16.3#

100 24.0 9.0 13.6#

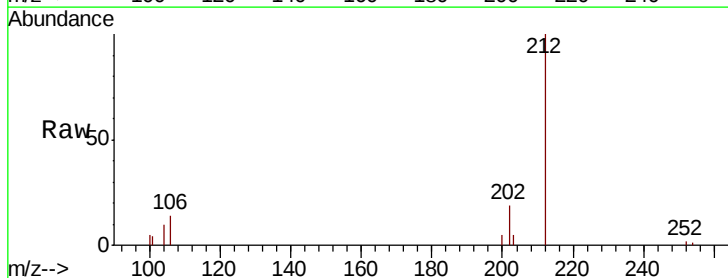

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

