
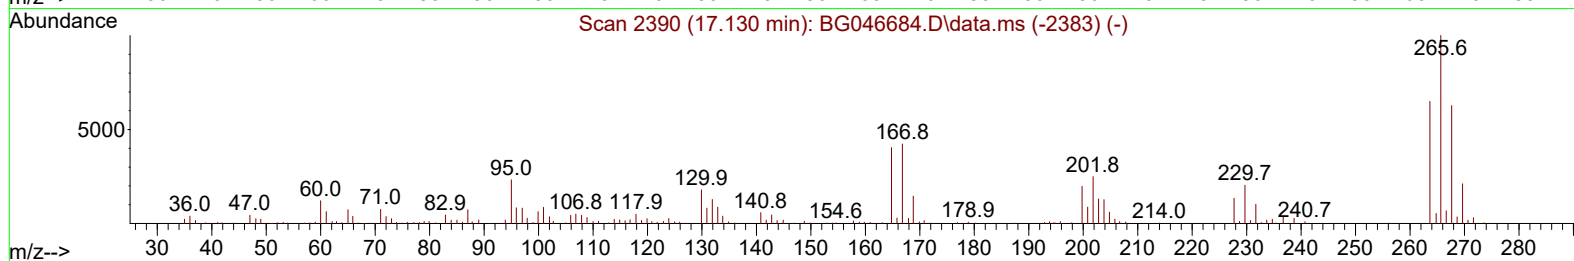
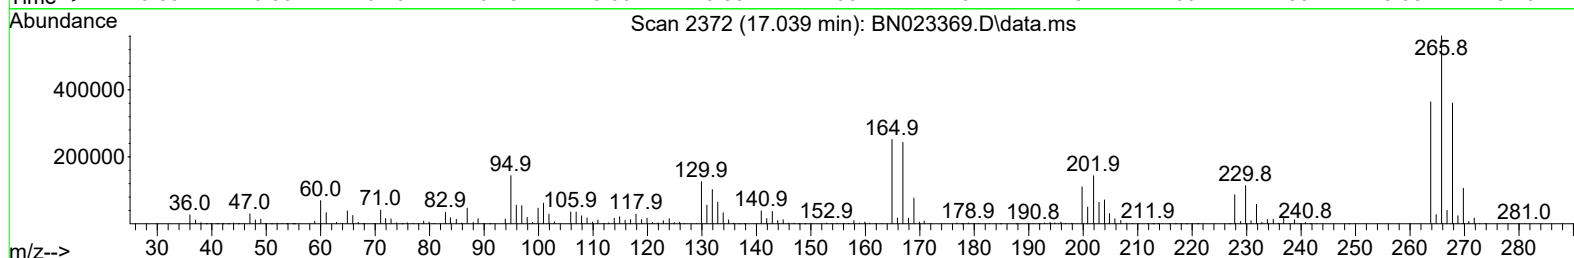


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122322\
Data File : BN023369.D
Acq On : 23 Dec 2022 12:12
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 24 06:14:44 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 24 06:14:40 2022
Response via : Initial Calibration

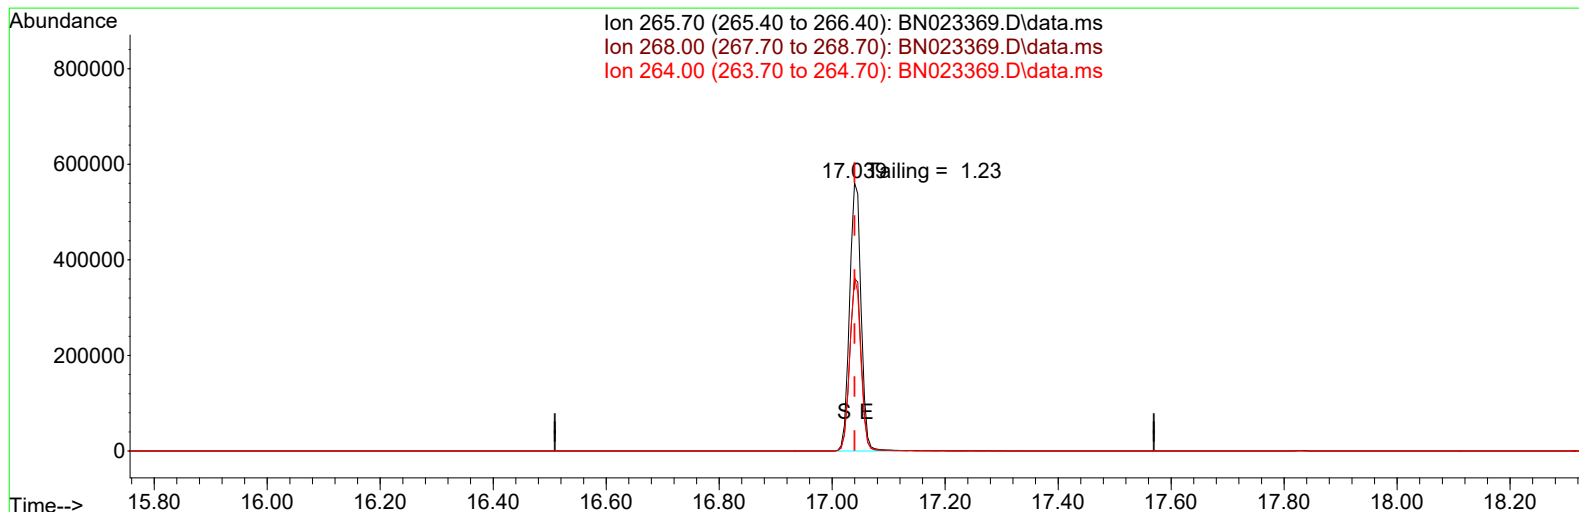

TIC: BN023369.D\data.ms

(70) Pentachlorophenol (C)




17.039min (0.000) 29295.54 ng

response 797537

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.21
264.00	61.60	64.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122322\
Data File : BN023369.D
Acq On : 23 Dec 2022 12:12
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 24 06:14:44 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 24 06:14:40 2022
Response via : Initial Calibration

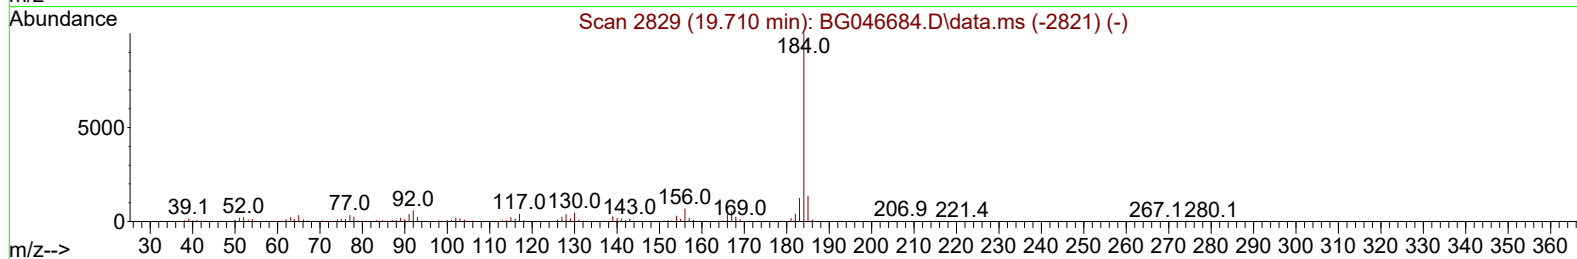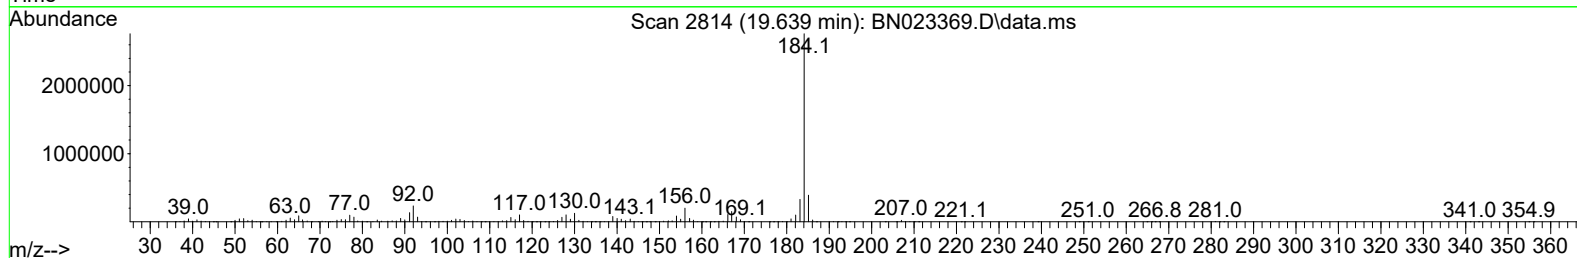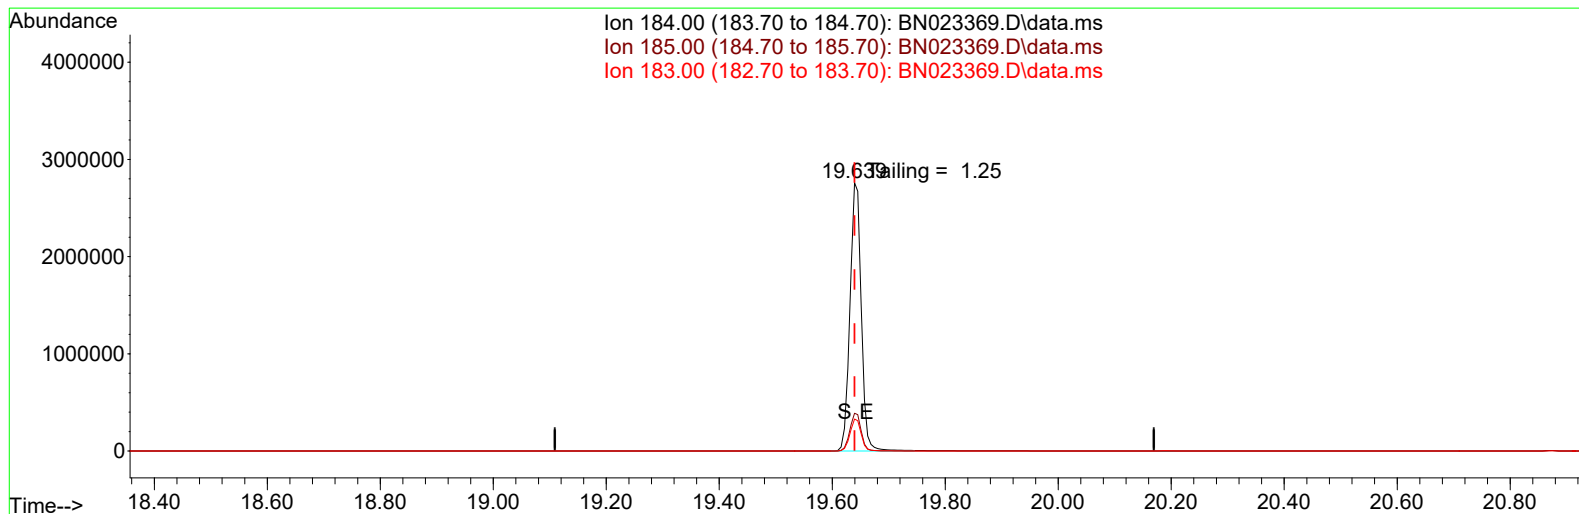

TIC: BN023369.D\data.ms

(77) Benzidine**19.639min (0.000) 2281554.44 ng****response 3868137**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.10
183.00	13.20	11.96
0.00	0.00	0.00