
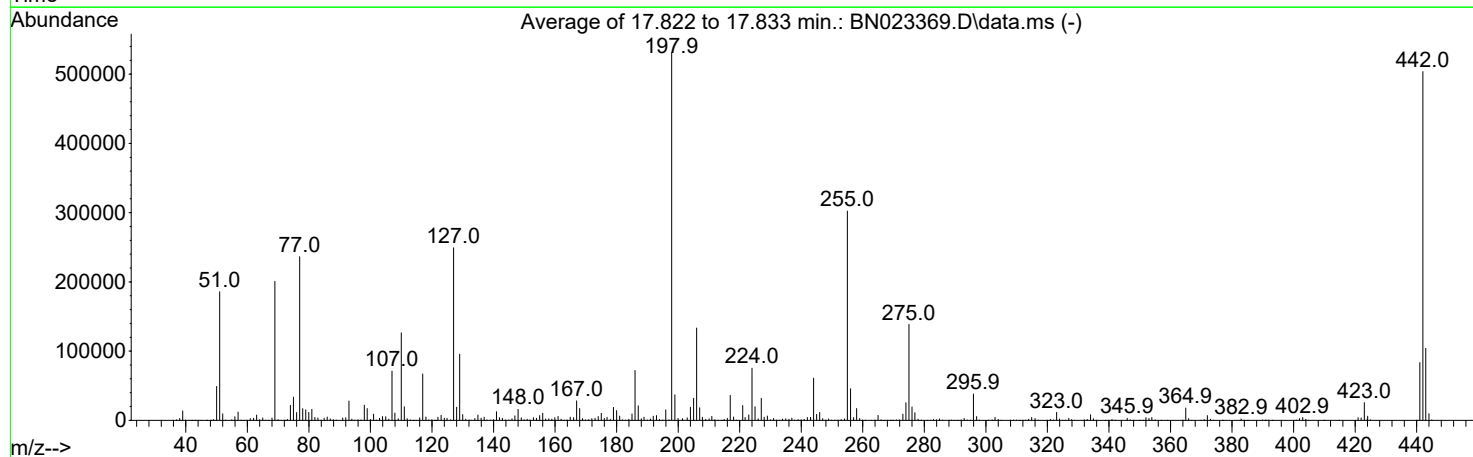


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122322\
 Data File : BN023369.D
 Acq On : 23 Dec 2022 12:12
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN120822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 23 16:36:53 2022

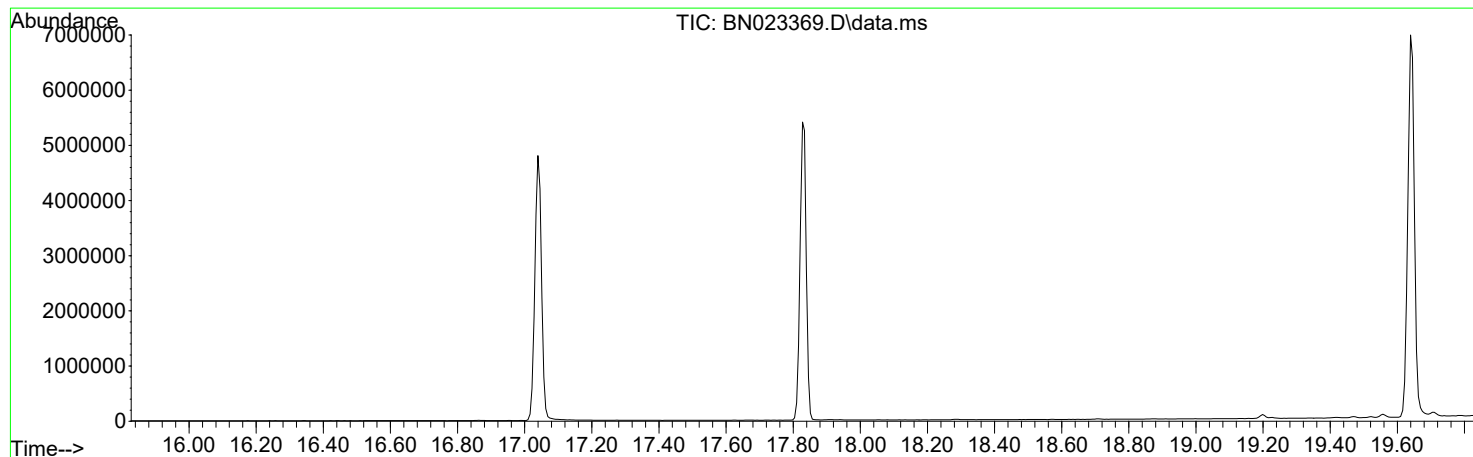




AutoFind: Scans 2505, 2506, 2507; Background Corrected with Scan 2498

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.0	185728	PASS
68	69	0.00	2	1.8	3579	PASS
69	198	0.00	100	37.8	200832	PASS
70	69	0.00	2	0.5	1071	PASS
127	198	10	80	46.9	249365	PASS
197	198	0.00	2	0.1	706	PASS
198	198	100	100	100.0	531264	PASS
199	198	5	9	6.9	36904	PASS
275	198	10	60	26.1	138605	PASS
365	198	1	100	3.3	17794	PASS
441	198	0.01	100	15.7	83496	PASS
442	442	50	100	100.0	503659	PASS
443	442	15	24	20.7	104125	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122322\
Data File : BN023369.D
Acq On : 23 Dec 2022 12:12
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 24 06:14:44 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 24 06:14:40 2022
Response via : Initial Calibration

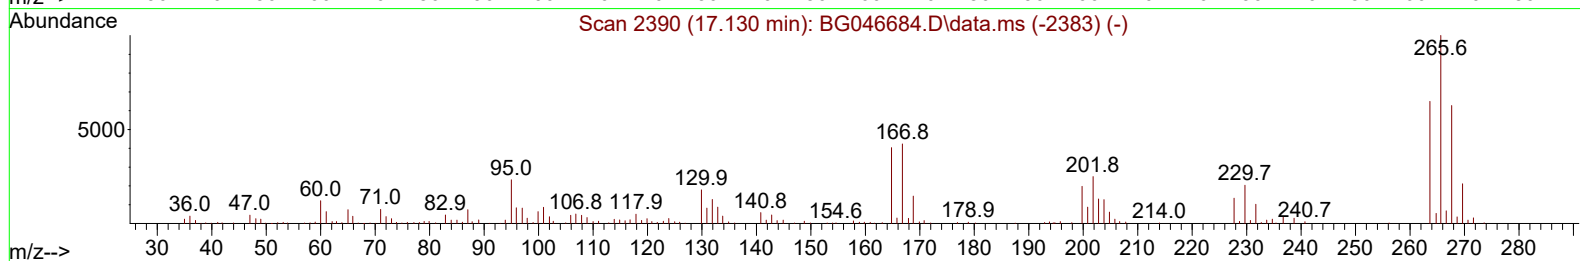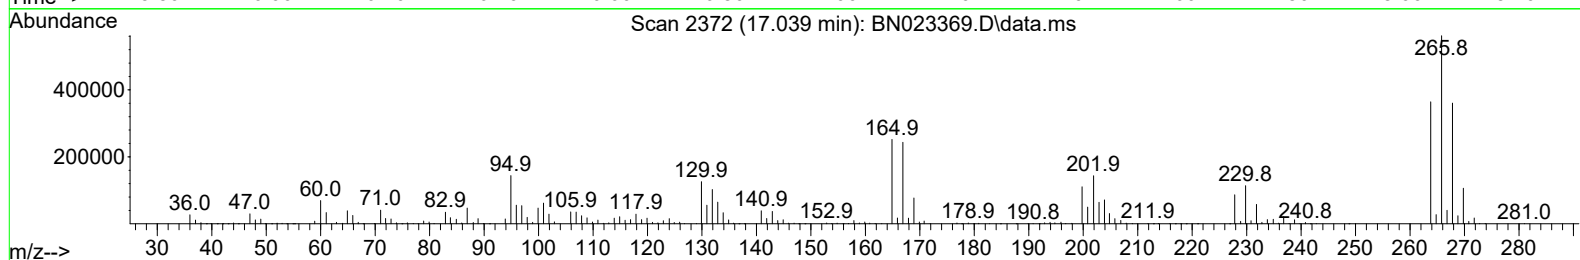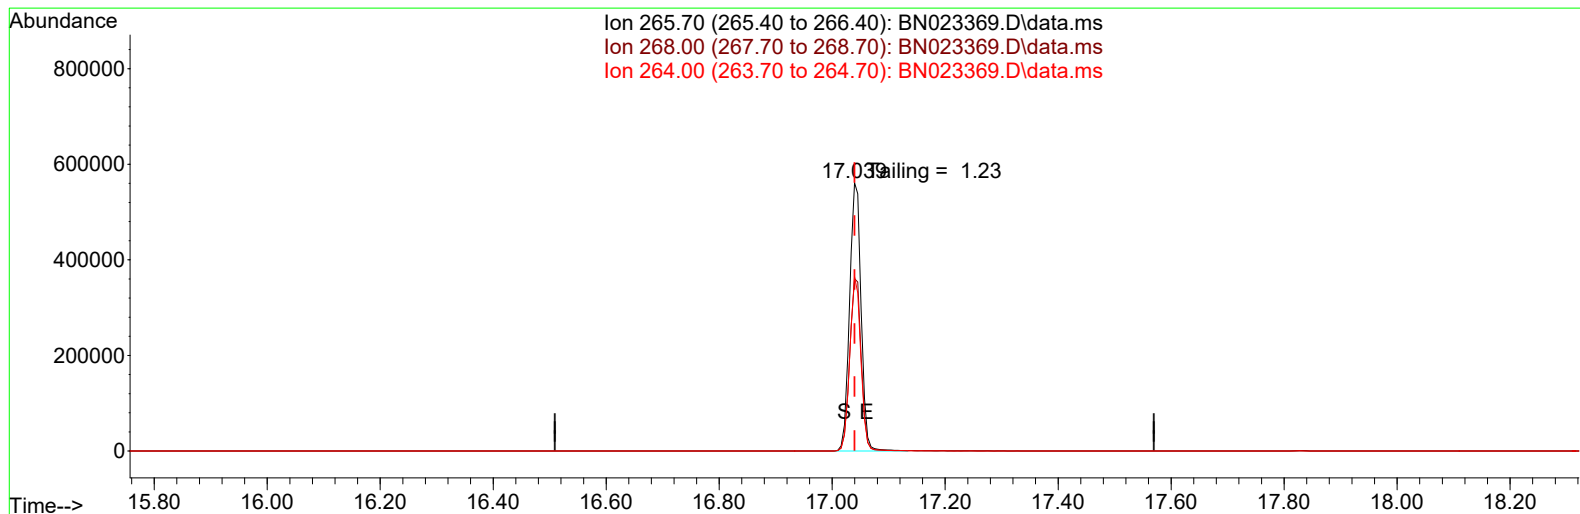

TIC: BN023369.D\data.ms

(70) Pentachlorophenol (C)

17.039min (0.000) 29295.54 ng




response 797537

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.21
264.00	61.60	64.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122322\
Data File : BN023369.D
Acq On : 23 Dec 2022 12:12
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 24 06:14:44 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 24 06:14:40 2022
Response via : Initial Calibration

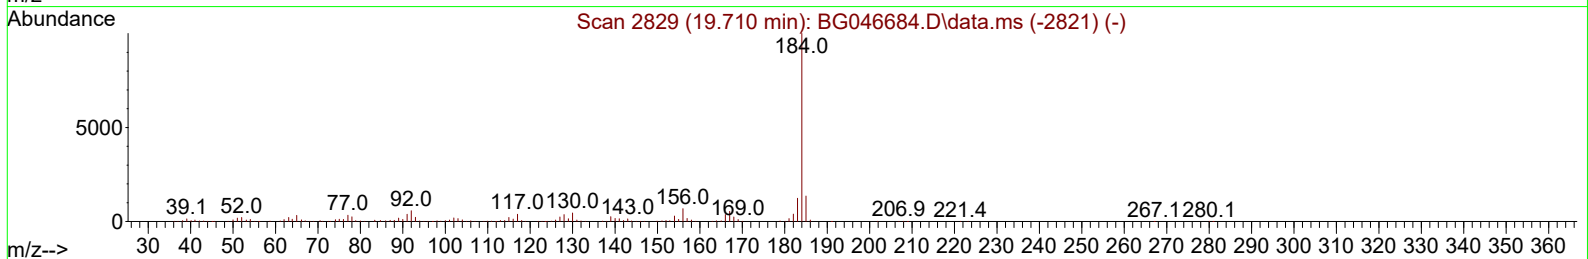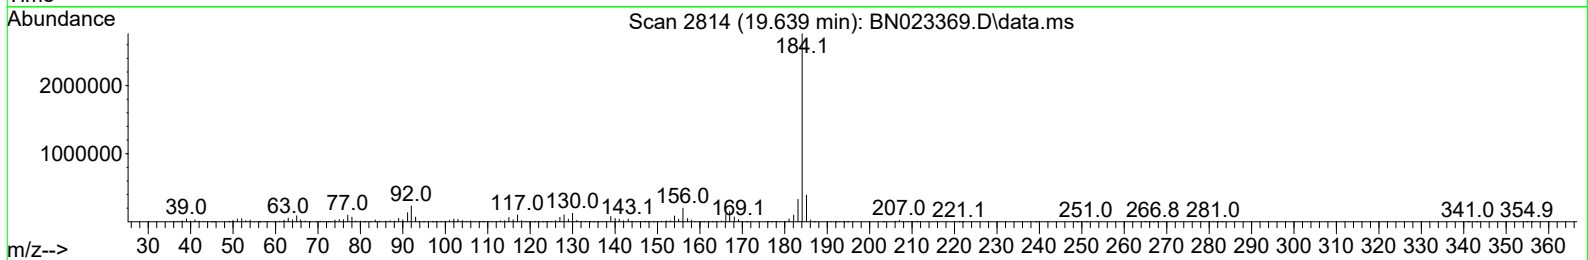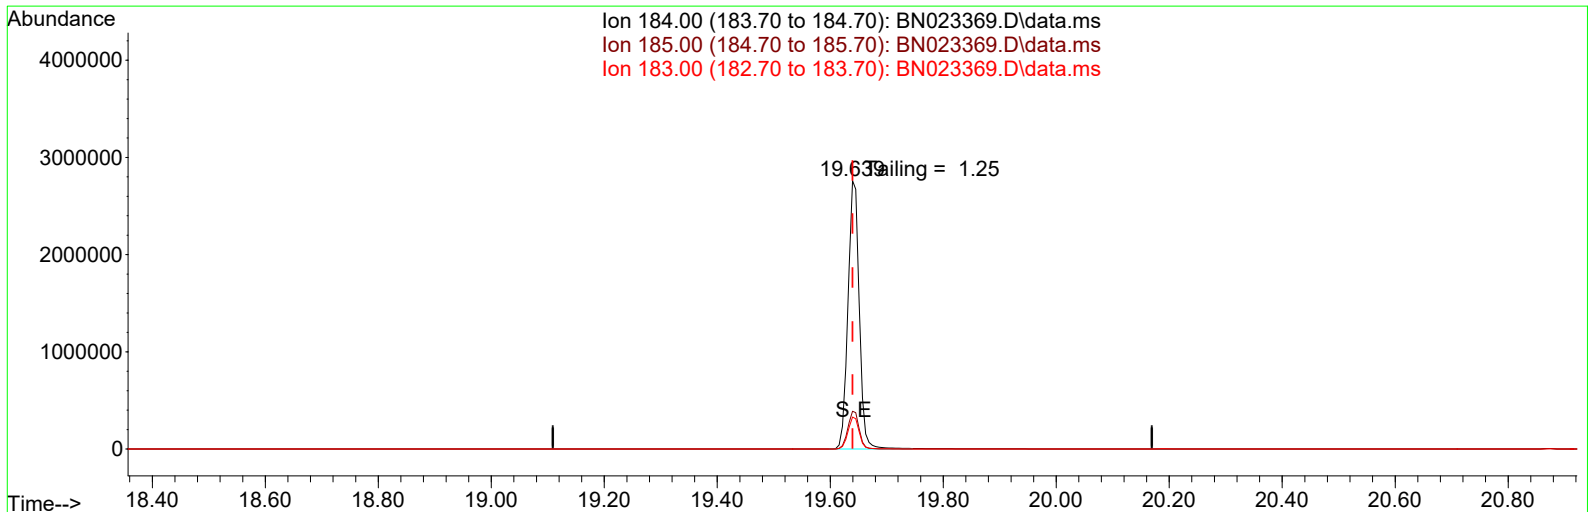

TIC: BN023369.D\data.ms

(77) Benzidine

19.639min (0.000) 2281554.44 ng

response 3868137

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.10
183.00	13.20	11.96
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/23/2022	BNA_N	<u>BN023369.D</u>
Compound Name	Response	Retention Time
DDT	1523513	20.874
DDD	348186	20.433
DDE	6731	19.922
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
354917	1878430	18.89

Instrument :
BNA_N
ClientSampleId :
DFTPP