
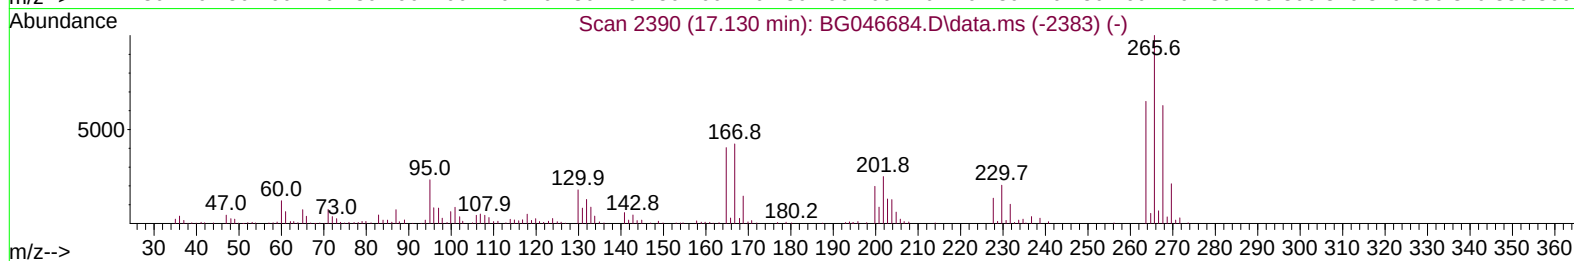
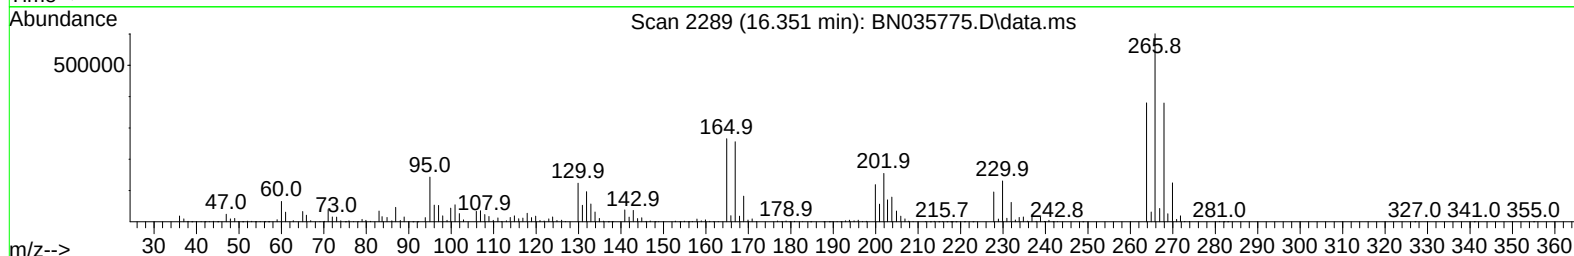


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN122324\  
Data File : BN035775.D  
Acq On : 23 Dec 2024 09:43  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 57 Sample Multiplier: 1

Quant Time: Dec 24 06:25:00 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Dec 24 06:24:48 2024  
Response via : Initial Calibration

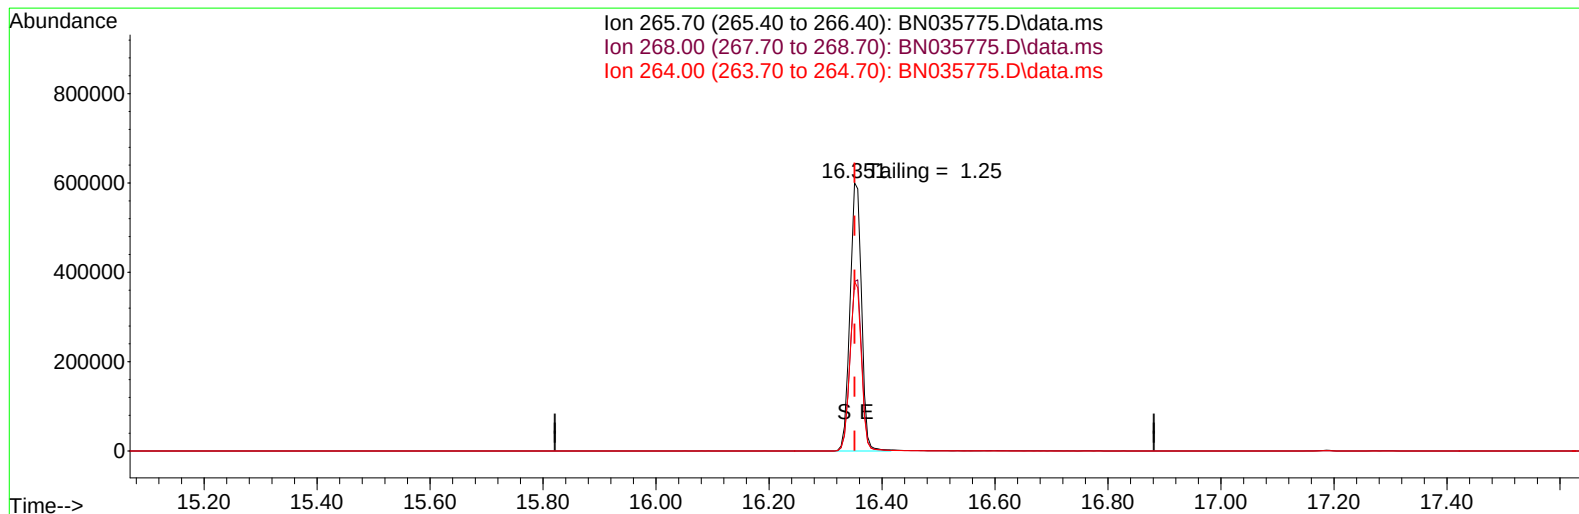

TIC: BN035775.D\data.ms

**(70) Pentachlorophenol (C)**




**16.351min ( 0.000) 26248.44 ng**

**response 857335**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 63.12  |
| 264.00 | 61.60  | 63.23  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN122324\  
Data File : BN035775.D  
Acq On : 23 Dec 2024 09:43  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 57 Sample Multiplier: 1

Quant Time: Dec 24 06:25:00 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Dec 24 06:24:48 2024  
Response via : Initial Calibration

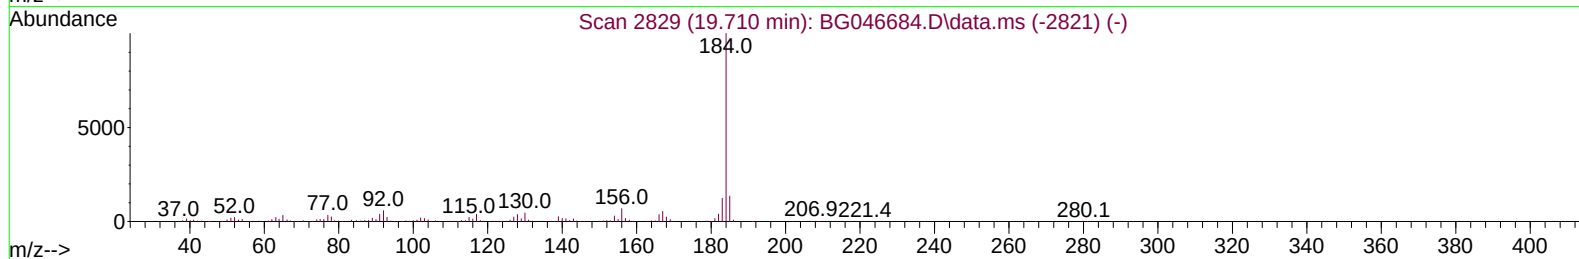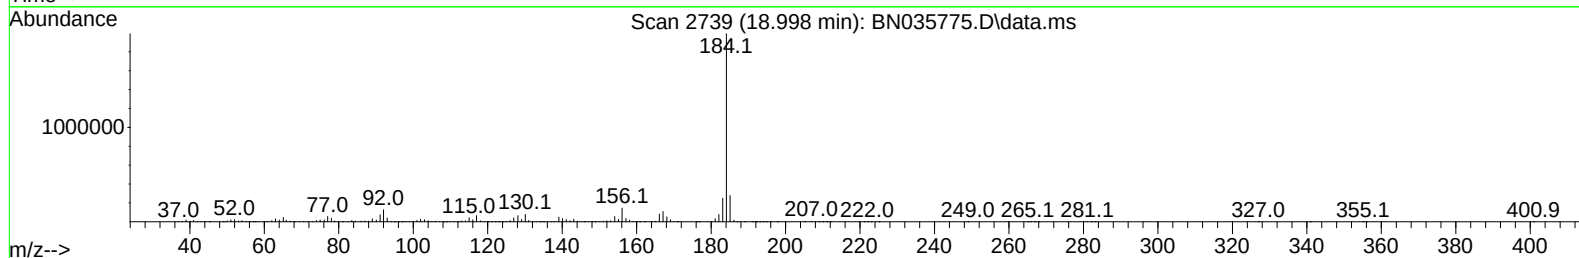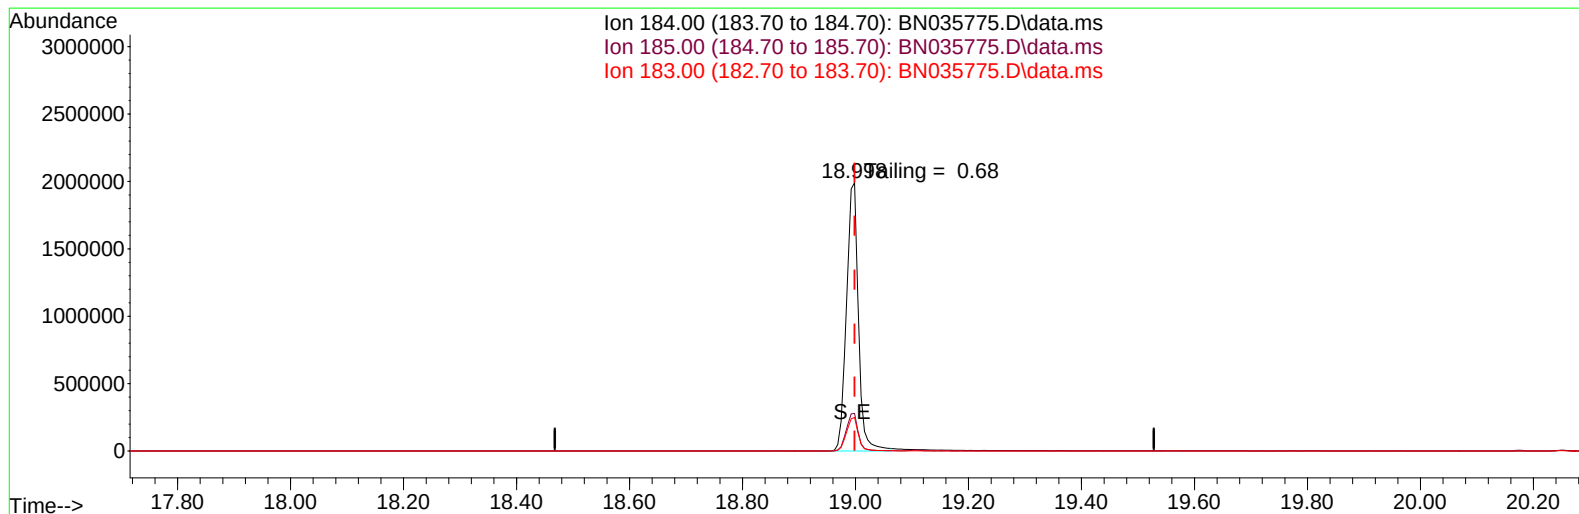

TIC: BN035775.D\data.ms

**(77) Benzidine**

18.998min ( 0.000) 0.00 ng

response 2997835

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 14.00  |
| 183.00 | 13.20  | 12.55  |
| 0.00   | 0.00   | 0.00   |