
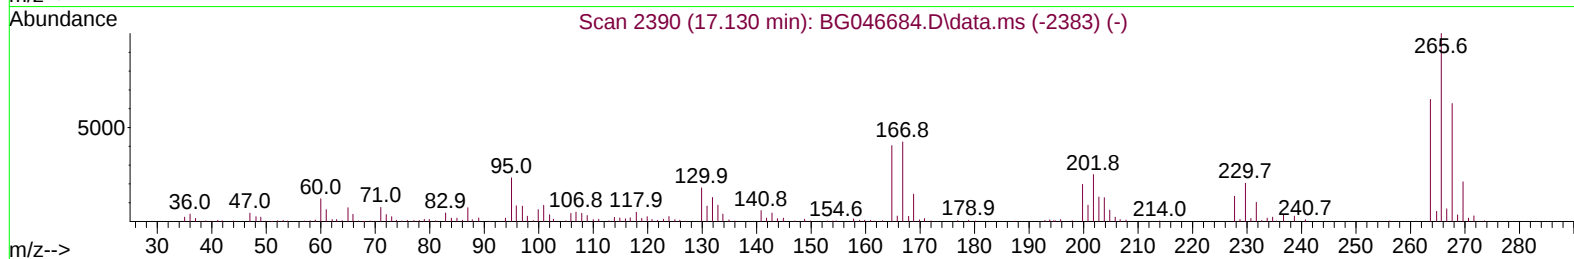
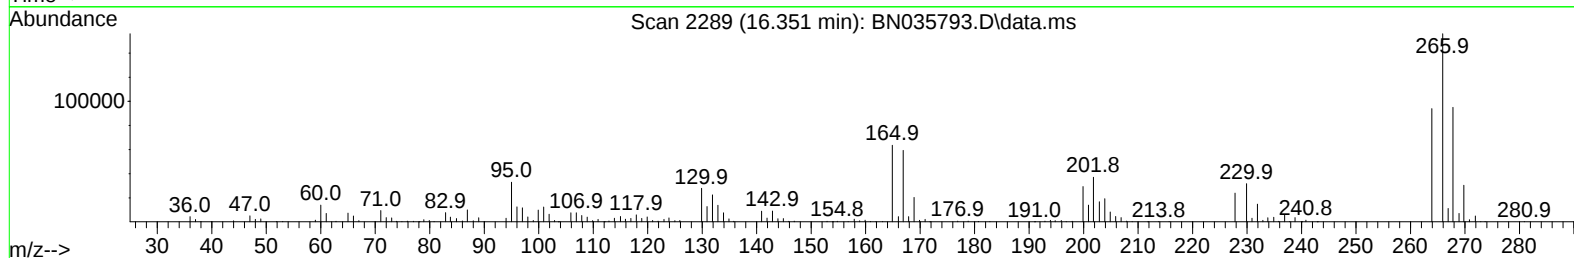


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122324\
Data File : BN035793.D
Acq On : 23 Dec 2024 20:26
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 75 Sample Multiplier: 1

Quant Time: Dec 24 06:28:14 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 24 06:28:04 2024
Response via : Initial Calibration

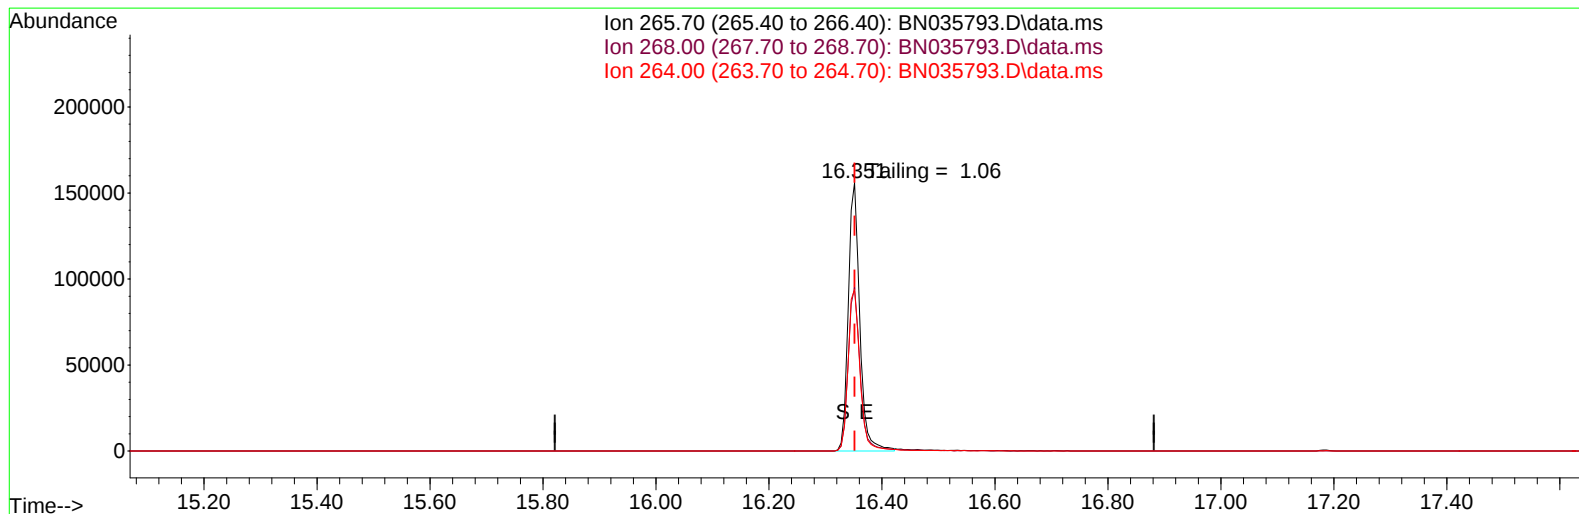

TIC: BN035793.D\data.ms

(70) Pentachlorophenol (C)




16.351min (0.000) 22129.06 ng

response 222810

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.87
264.00	61.60	60.23
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122324\
Data File : BN035793.D
Acq On : 23 Dec 2024 20:26
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 75 Sample Multiplier: 1

Quant Time: Dec 24 06:28:14 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 24 06:28:04 2024
Response via : Initial Calibration

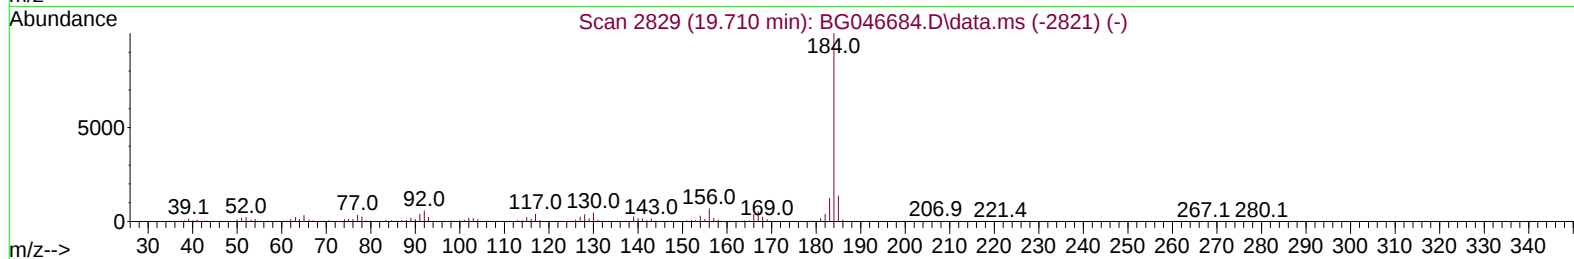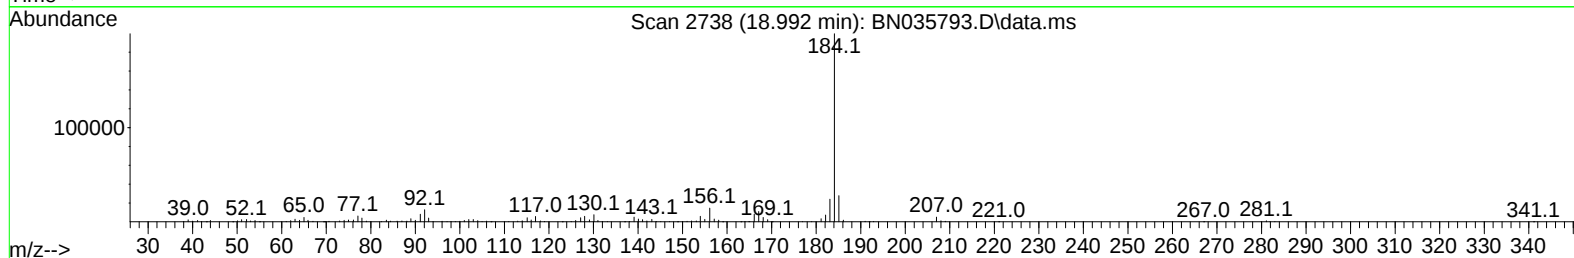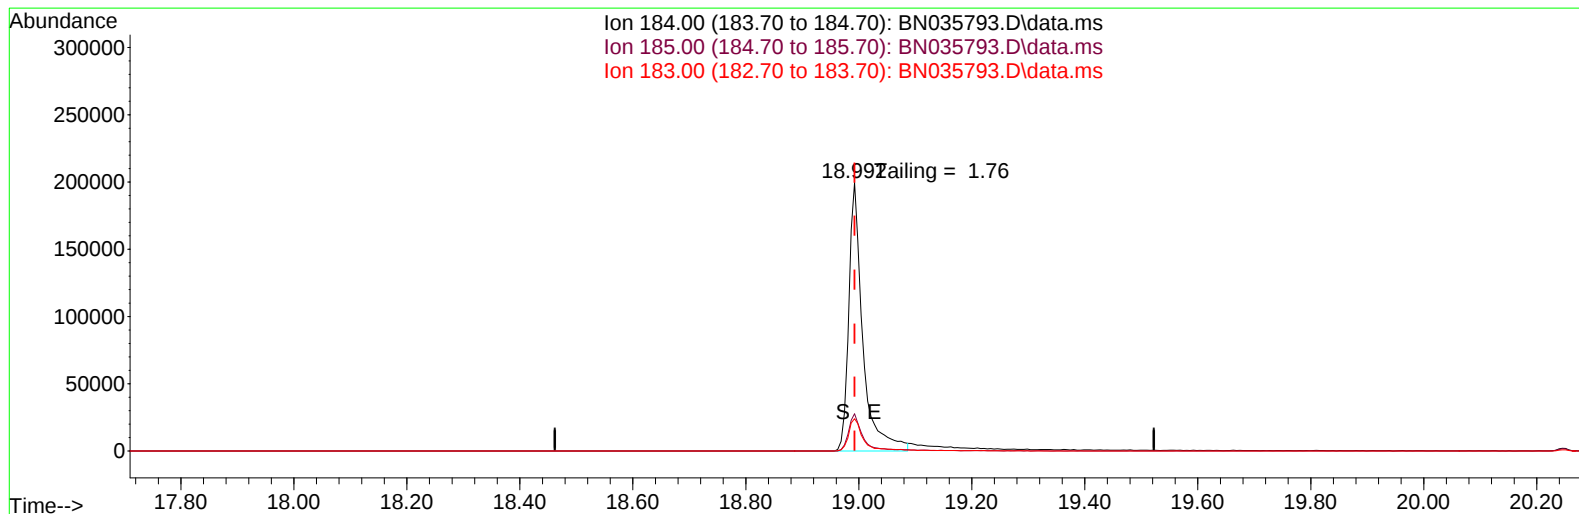

TIC: BN035793.D\data.ms

(77) Benzidine

18.992min (0.000) 0.00 ng

response 368634

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.92
183.00	13.20	12.06
0.00	0.00	0.00