
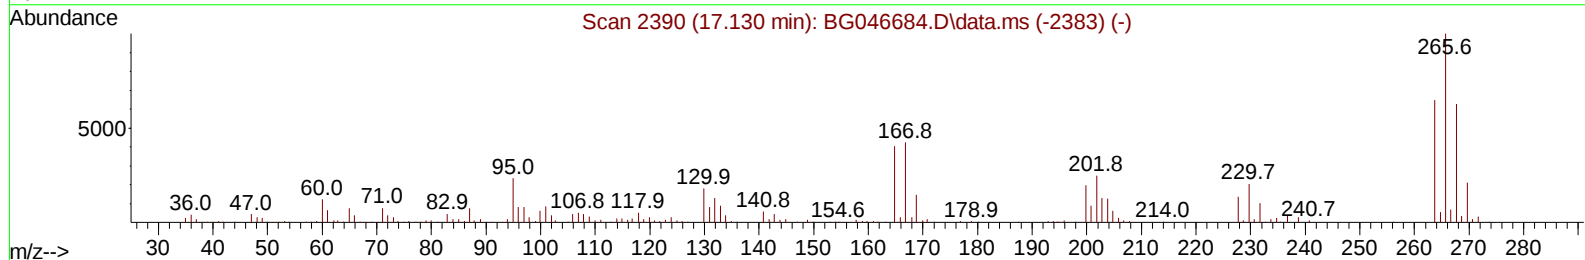
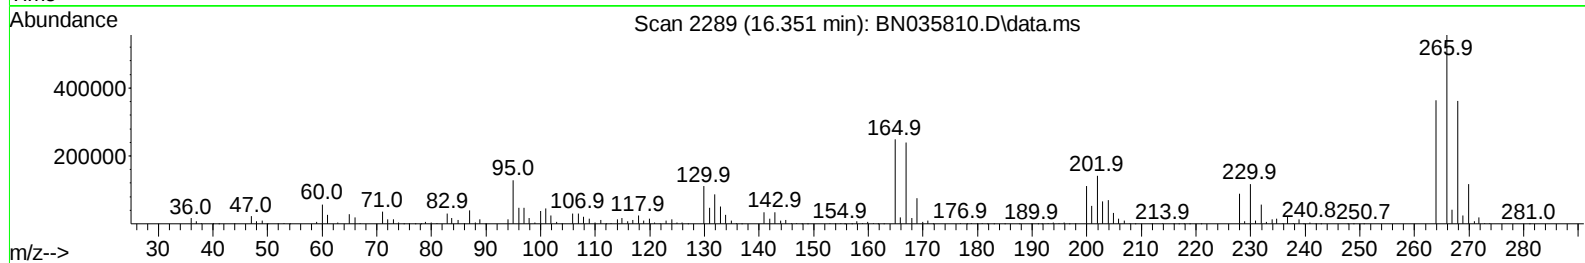


Quant Time: Dec 25 00:46:53 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 00:46:49 2024
Response via : Initial Calibration

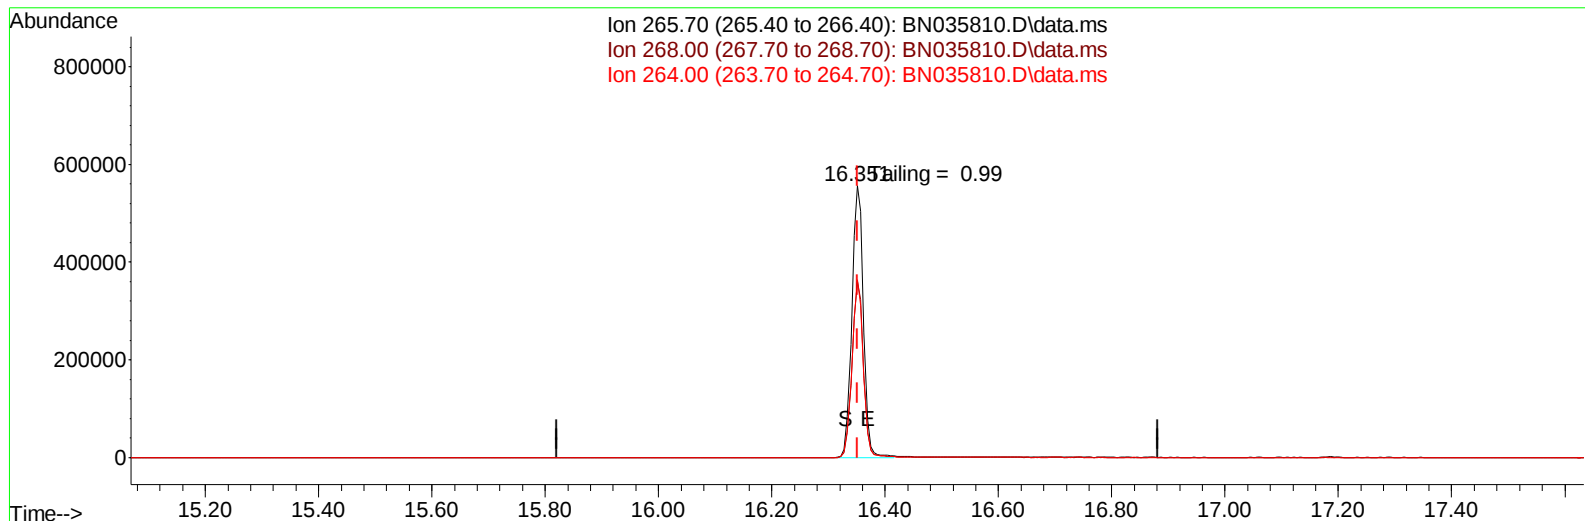

TIC: BN035810.D\data.ms




(70) Pentachlorophenol (C)

16.351min (0.000) 26136.96 ng

response **791954**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.05
264.00	61.60	65.35
0.00	0.00	0.00

Quant Time: Dec 25 00:46:53 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 00:46:49 2024
Response via : Initial Calibration

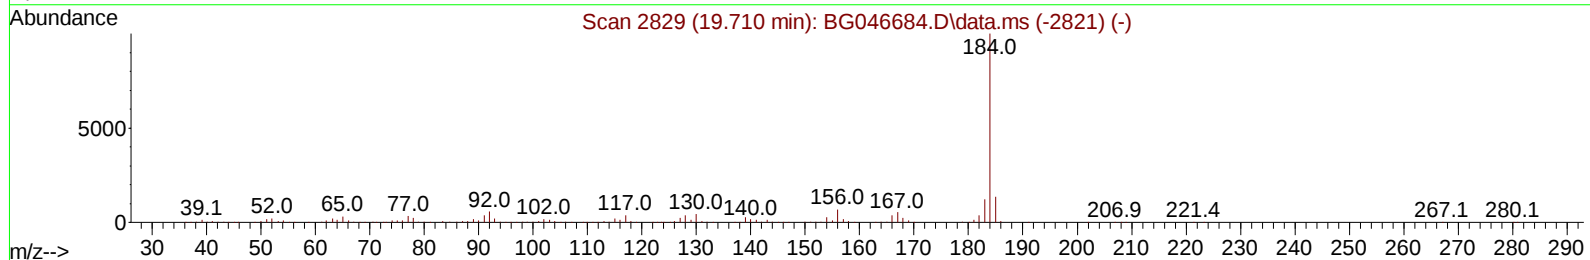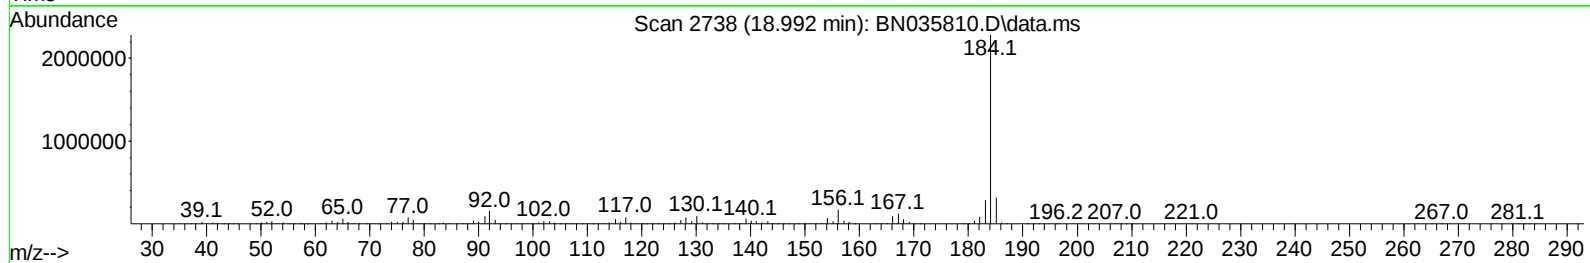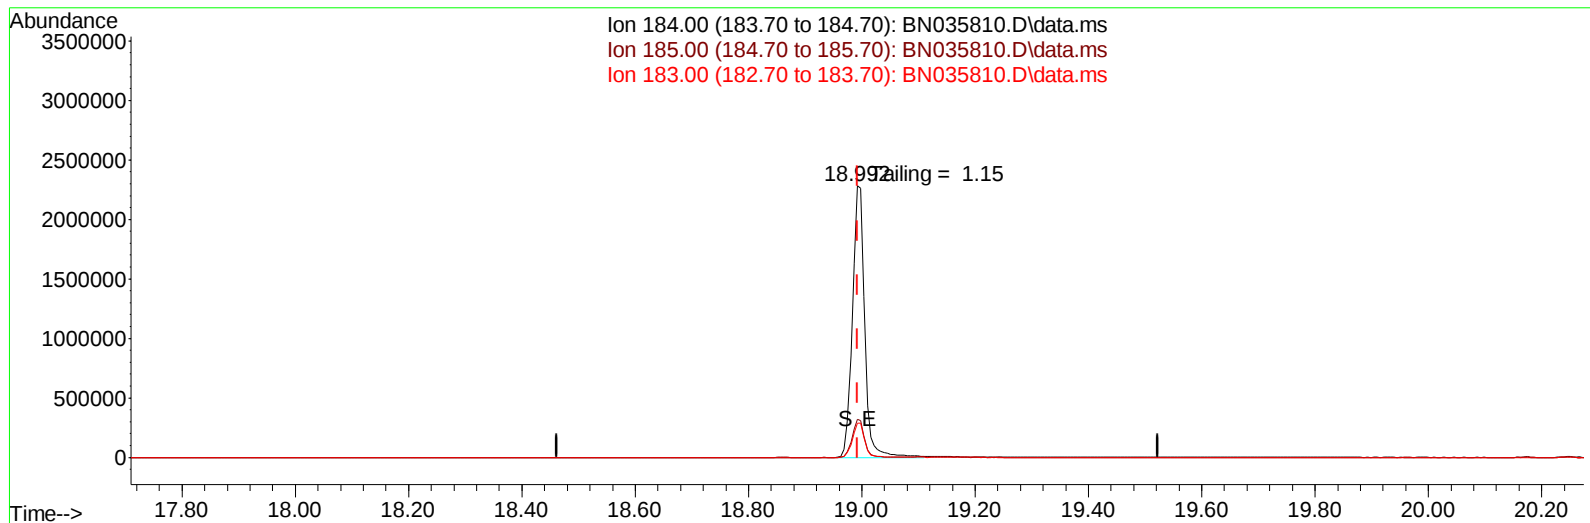

TIC: BN035810.D\data.ms

(77) Benzidine

18.992min (0.000) 0.00 ng

response 3507772

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.96
183.00	13.20	12.67
0.00	0.00	0.00