
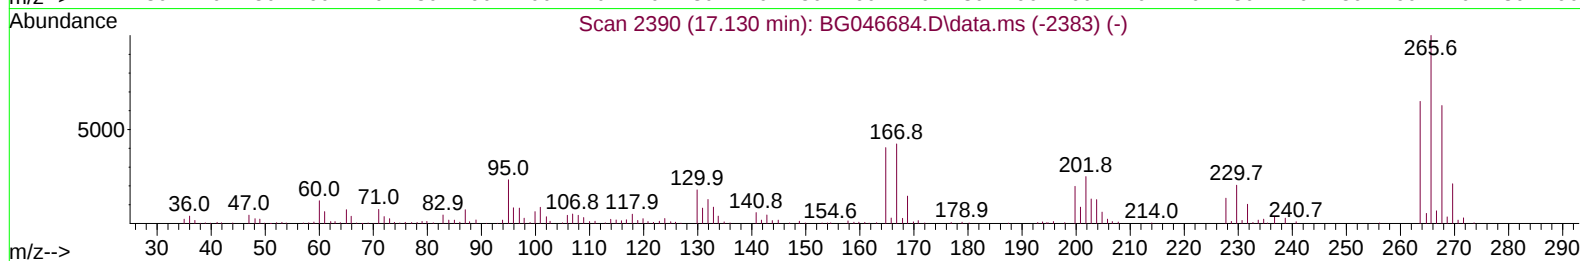
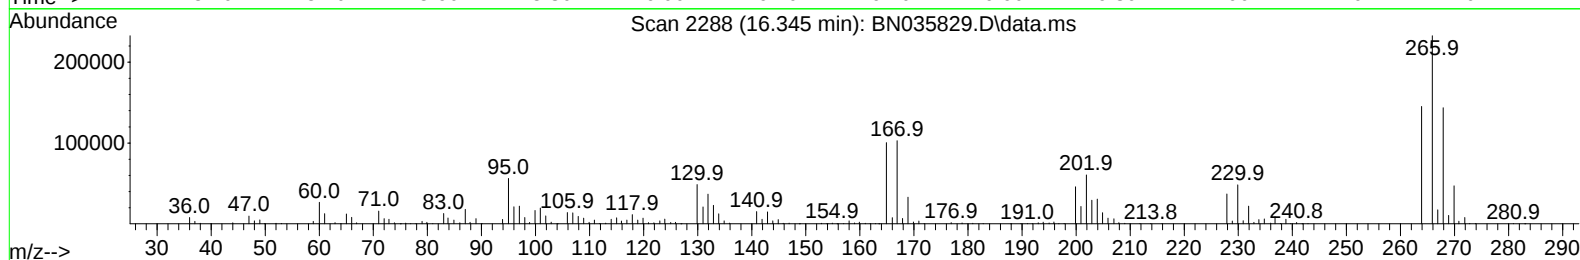


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122324\
Data File : BN035829.D
Acq On : 24 Dec 2024 19:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 21 Sample Multiplier: 1

Quant Time: Dec 25 04:24:00 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

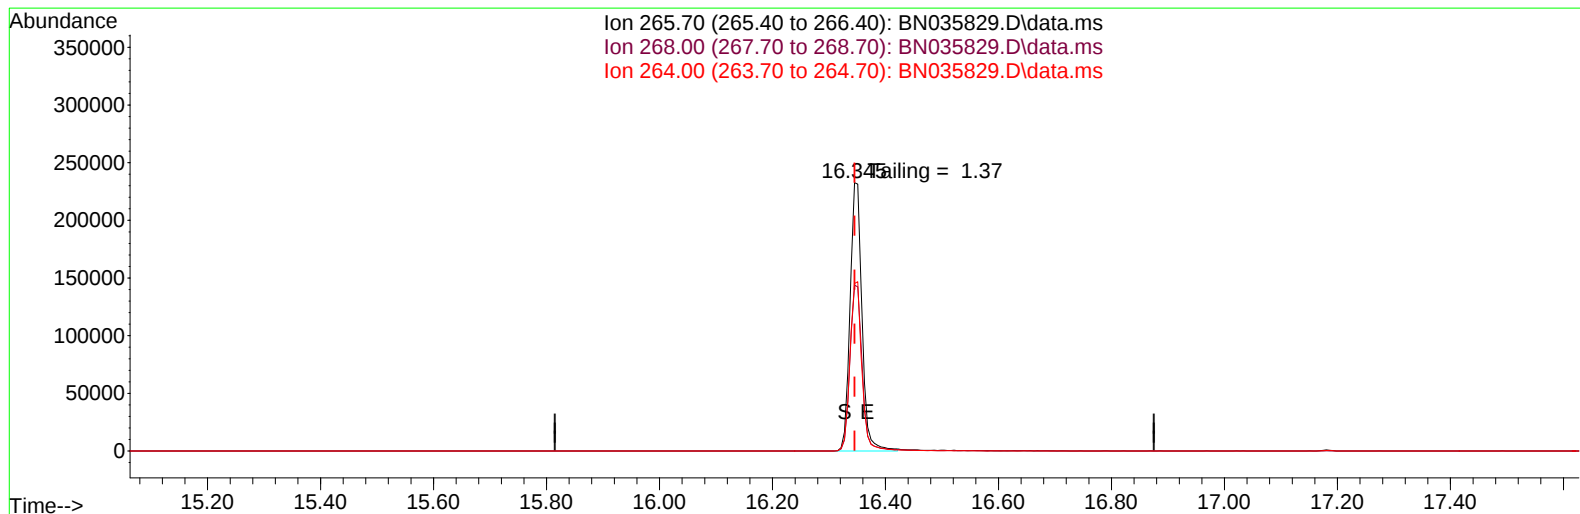

TIC: BN035829.D\data.ms

(70) Pentachlorophenol (C)




16.345min (0.000) 23024.60 ng

response 344759

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.74
264.00	61.60	62.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122324\
Data File : BN035829.D
Acq On : 24 Dec 2024 19:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 21 Sample Multiplier: 1

Quant Time: Dec 25 04:24:00 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

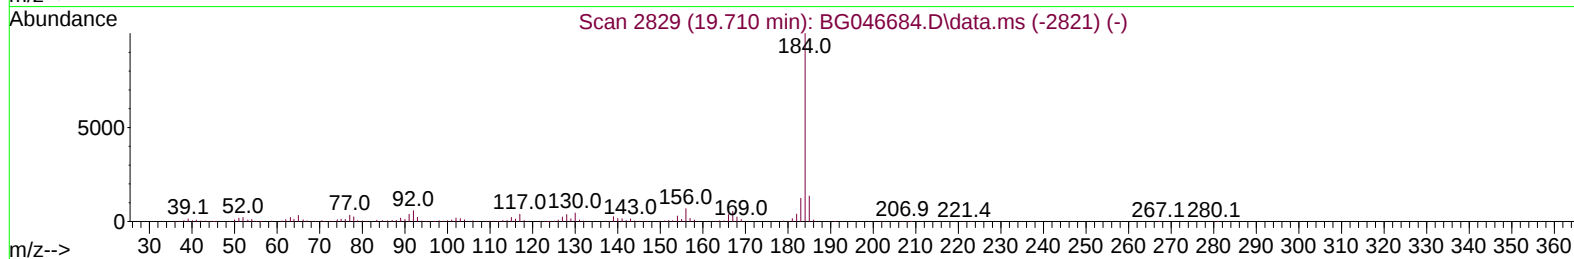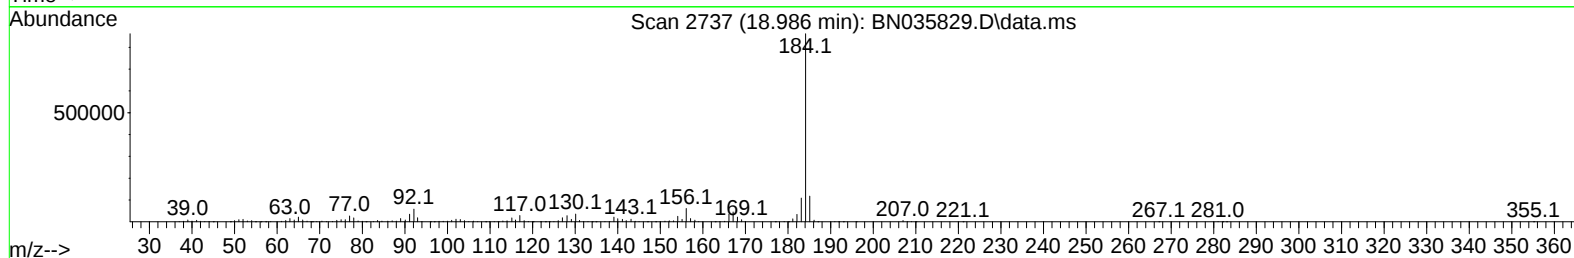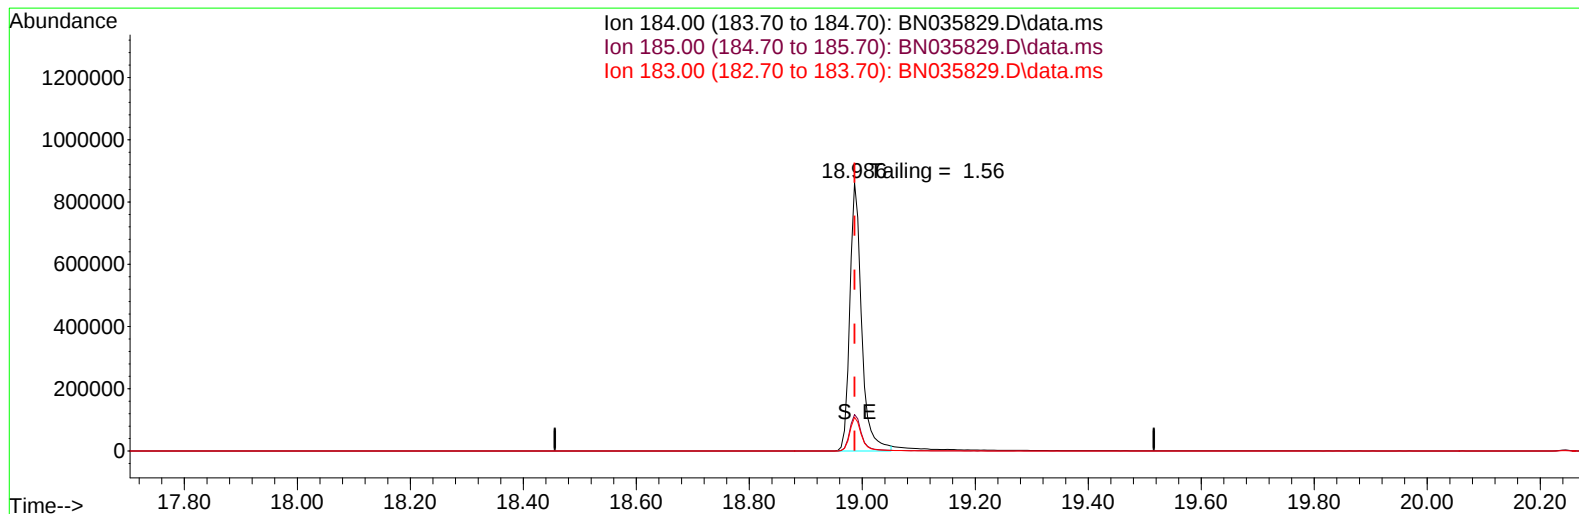

TIC: BN035829.D\data.ms

(77) Benzidine

18.986min (0.000) 0.00 ng

response 1299882

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.60
183.00	13.20	12.60
0.00	0.00	0.00