
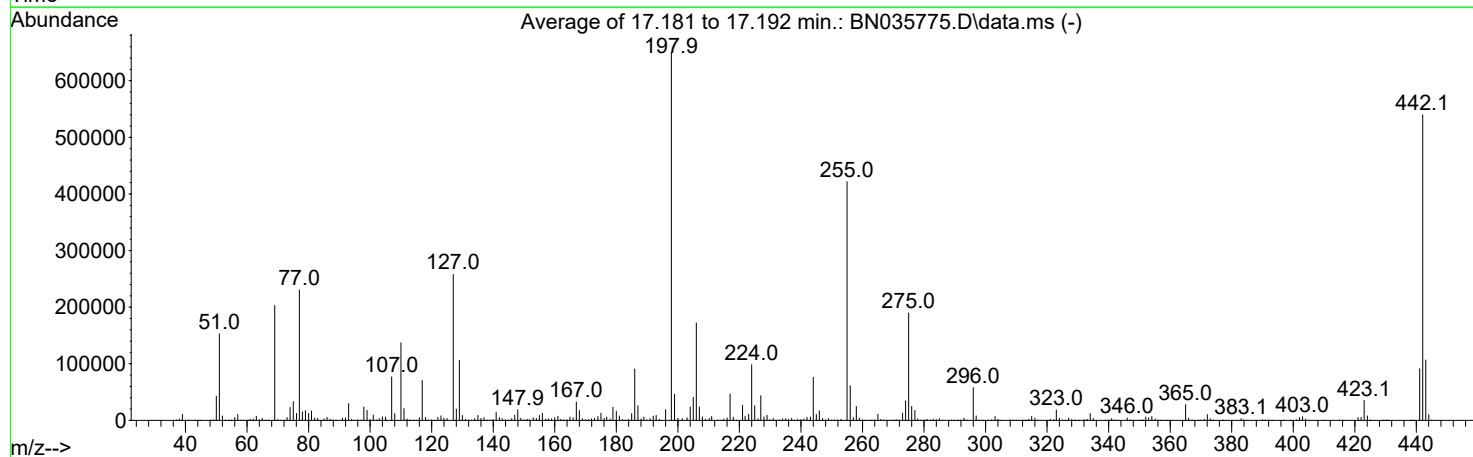


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122324\
Data File : BN035775.D
Acq On : 23 Dec 2024 09:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN112724.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Dec 19 23:06:19 2024

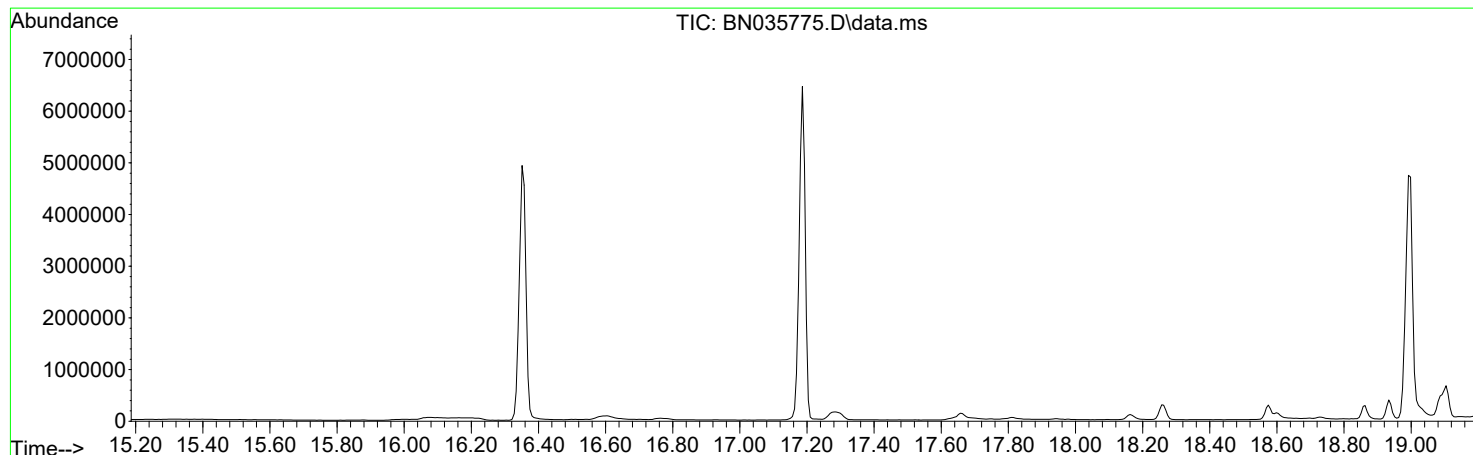

AutoFind: Scans 2430, 2431, 2432; Background Corrected with Scan 2422

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	23.6	153048	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	31.2	202884	PASS
70	69	0.00	2	0.6	1170	PASS
127	198	10	80	39.7	257941	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	649856	PASS
199	198	5	9	7.1	46155	PASS
275	198	10	60	29.2	189589	PASS
365	198	1	100	4.3	28056	PASS
441	198	0.01	100	14.0	91216	PASS
442	442	50	100	100.0	539989	PASS
443	442	15	24	19.7	106520	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
12/23/2024	BNA_N	<u>BN035775.D</u>
Compound Name	Response	Retention Time
DDT	1726374	20.251
DDD	285443	19.804
DDE	9189	19.286
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
294632	2021006	14.58

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122324\
Data File : BN035775.D
Acq On : 23 Dec 2024 09:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 24 06:25:00 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 24 06:24:48 2024
Response via : Initial Calibration

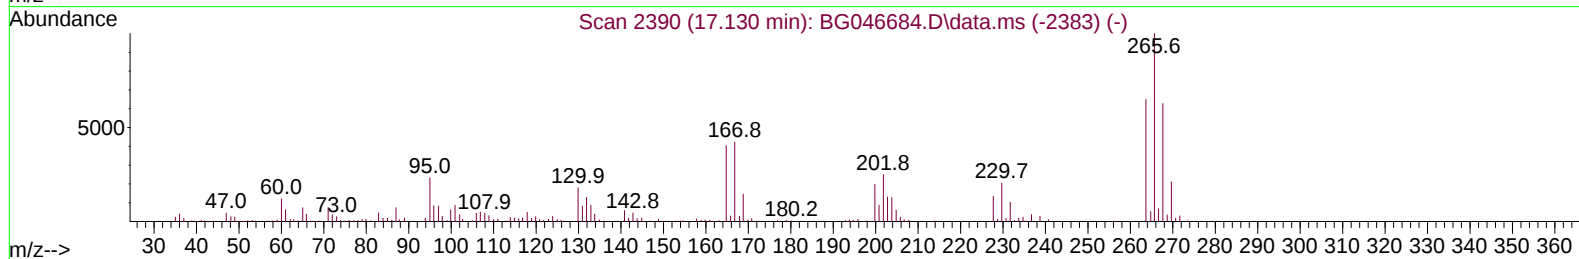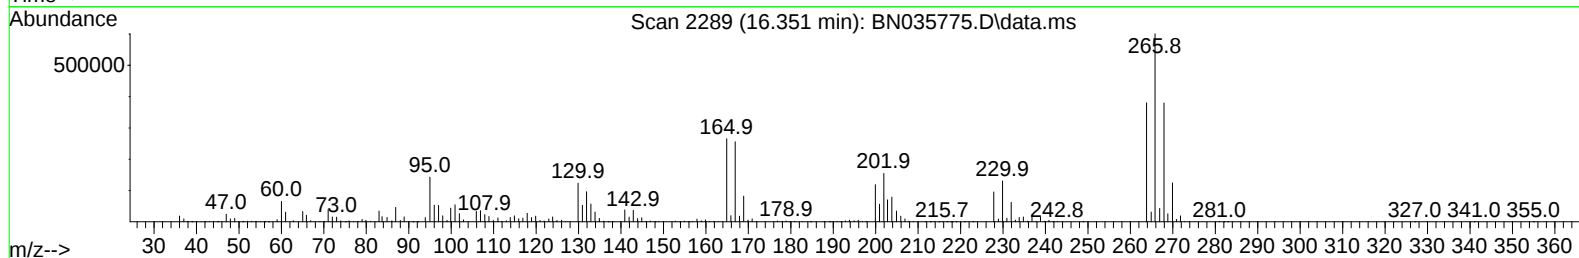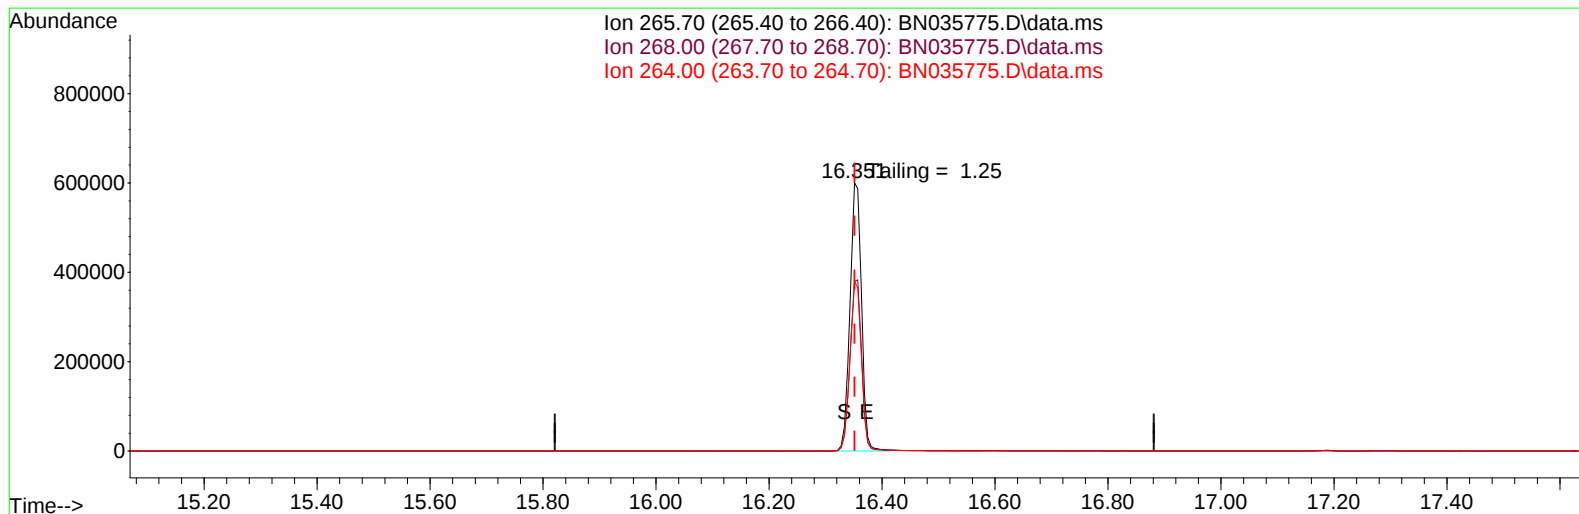

TIC: BN035775.D\data.ms

(70) Pentachlorophenol (C)

16.351min (0.000) 26248.44 ng




response 857335

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.12
264.00	61.60	63.23
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122324\
Data File : BN035775.D
Acq On : 23 Dec 2024 09:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 24 06:25:00 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 24 06:24:48 2024
Response via : Initial Calibration

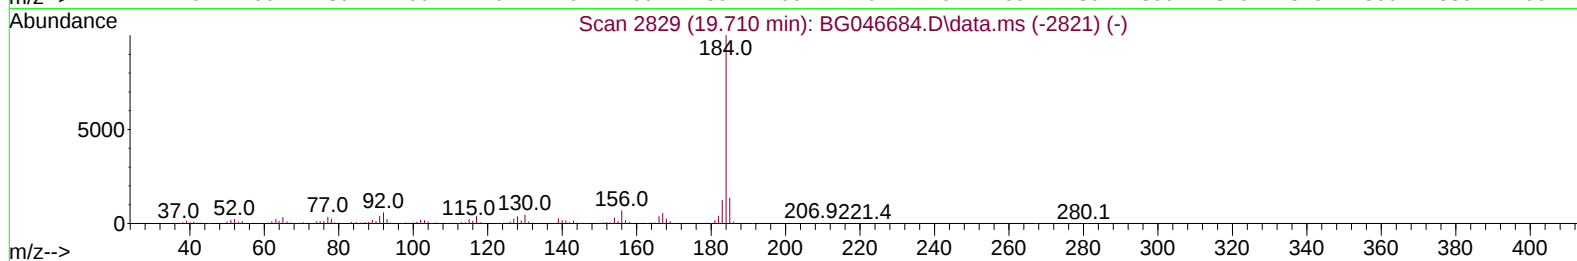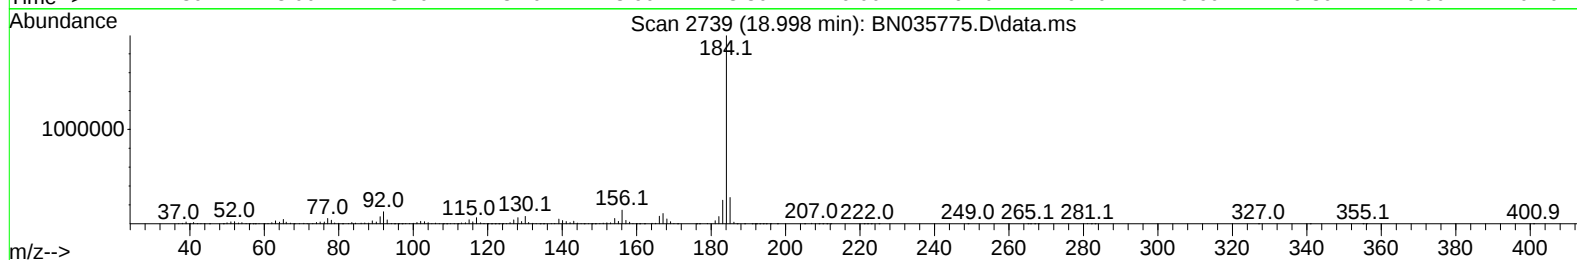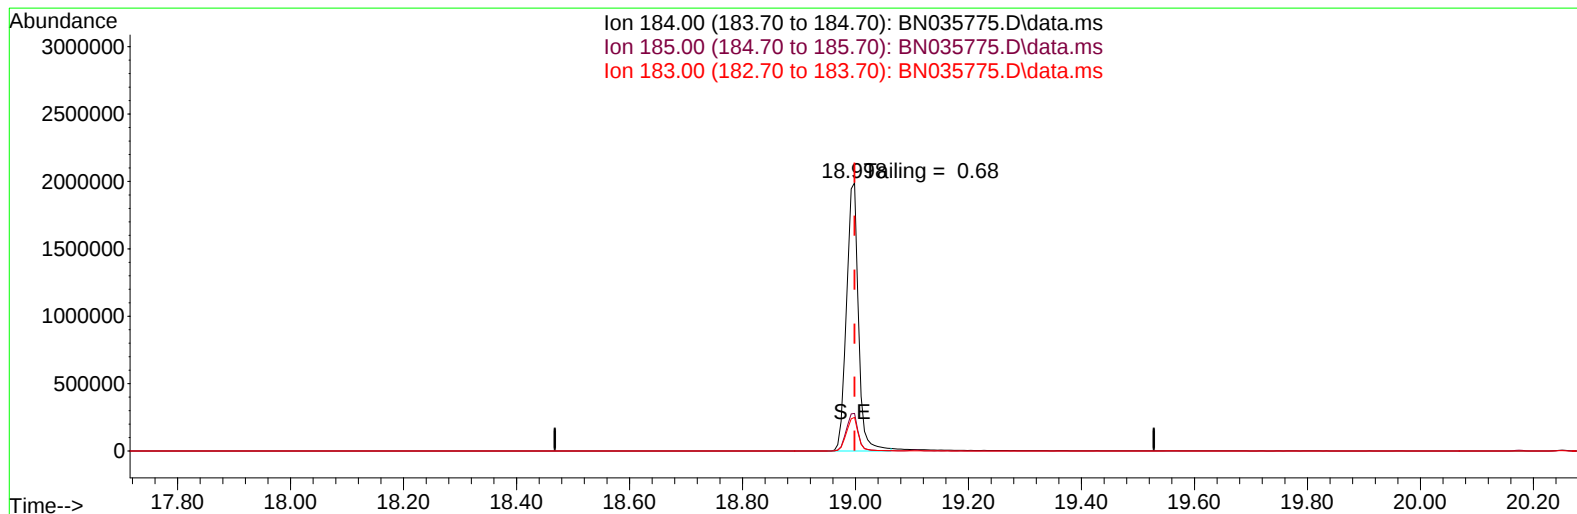

TIC: BN035775.D\data.ms

(77) Benzidine

18.998min (0.000) 0.00 ng

response 2997835

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.00
183.00	13.20	12.55
0.00	0.00	0.00