
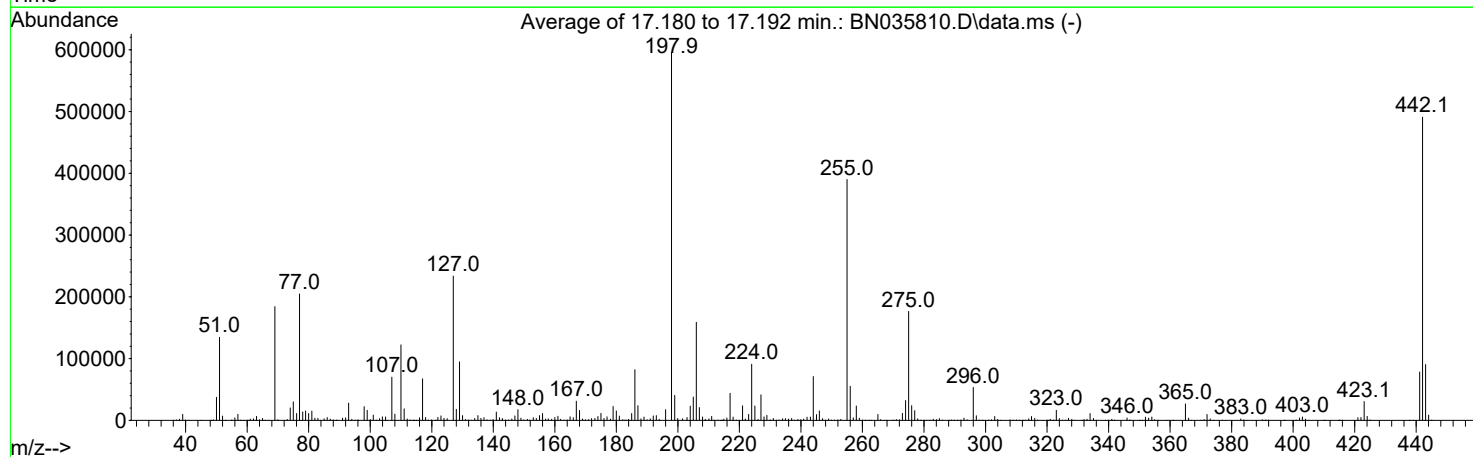


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122324\
Data File : BN035810.D
Acq On : 24 Dec 2024 07:45
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN112724.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Dec 19 23:06:19 2024

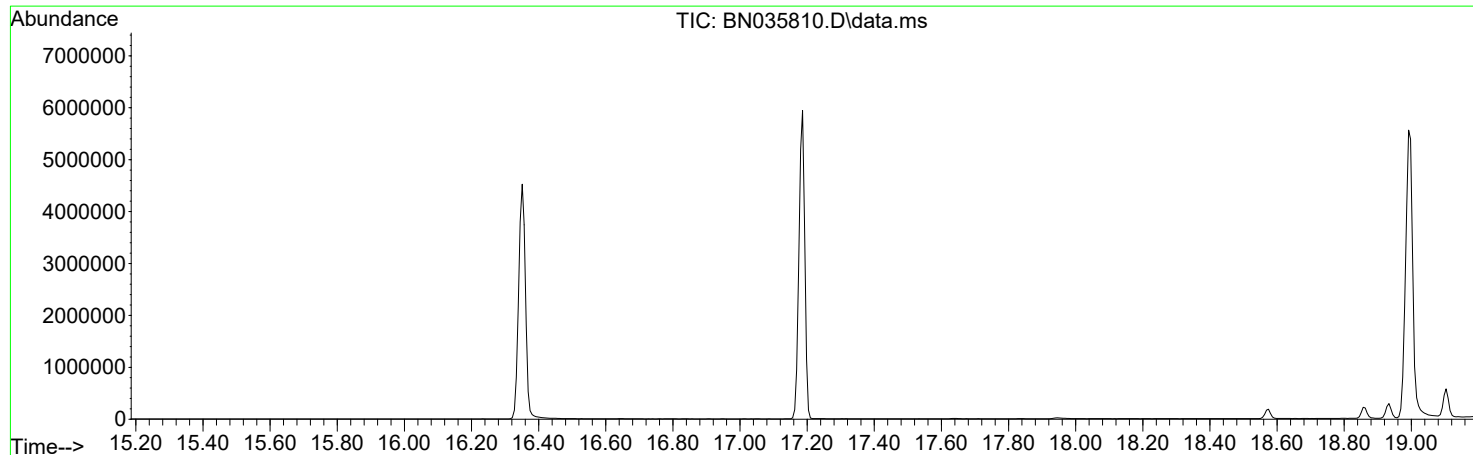

AutoFind: Scans 2430, 2431, 2432; Background Corrected with Scan 2422

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	22.6	134565	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	30.9	184267	PASS
70	69	0.00	2	0.5	1000	PASS
127	198	10	80	39.2	233707	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	595477	PASS
199	198	5	9	6.8	40509	PASS
275	198	10	60	29.6	176405	PASS
365	198	1	100	4.5	26707	PASS
441	198	0.01	100	13.2	78309	PASS
442	442	50	100	100.0	490880	PASS
443	442	15	24	18.4	90491	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
12/23/2024	BNA_N	<u>BN035810.D</u>
Compound Name	Response	Retention Time
DDT	1784590	20.251
DDD	187693	19.804
DDE	5273	19.286
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
192966	1977556	9.76

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122324\
Data File : BN035810.D
Acq On : 24 Dec 2024 07:45
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 25 00:46:53 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 00:46:49 2024
Response via : Initial Calibration

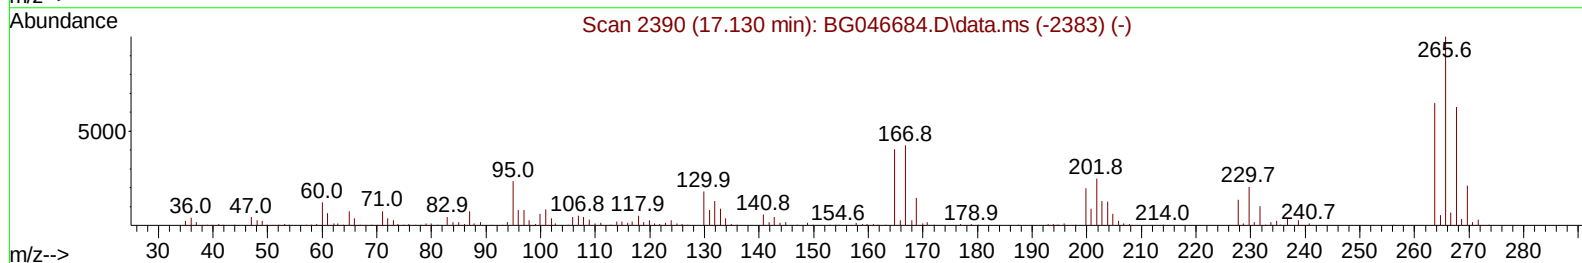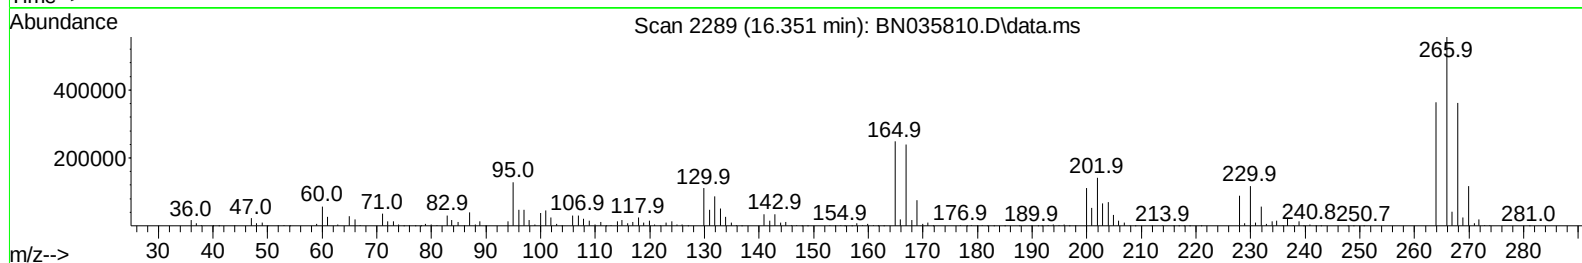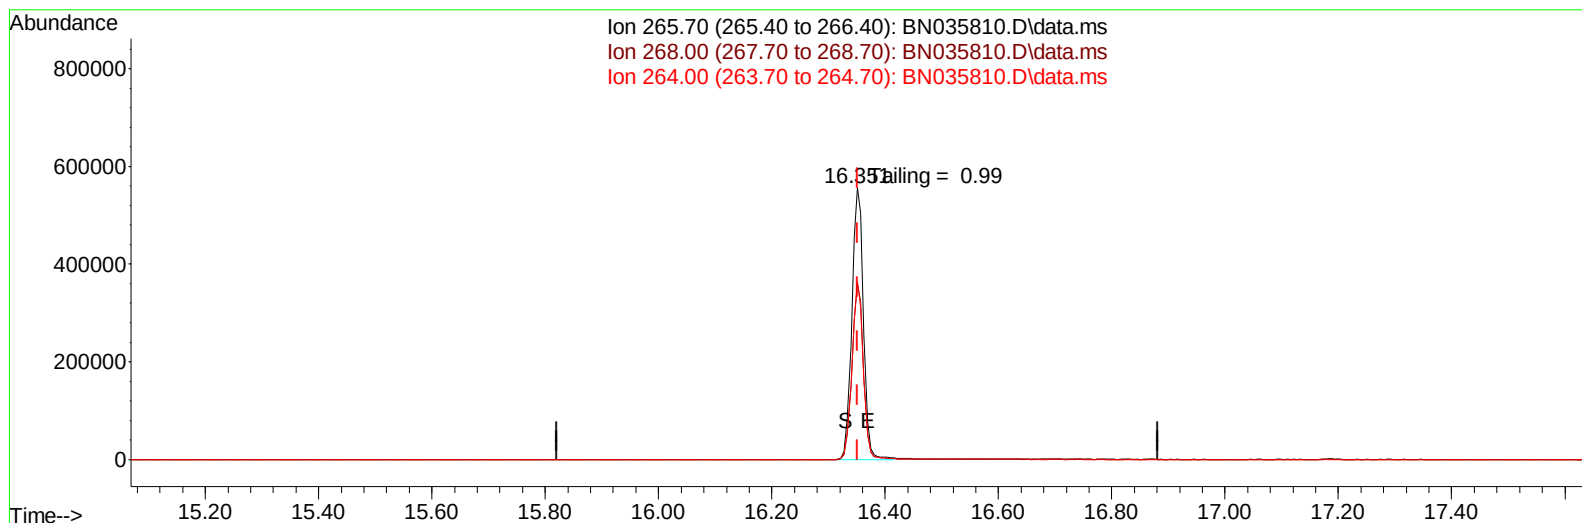

TIC: BN035810.D\data.ms

(70) Pentachlorophenol (C)

16.351min (0.000) 26136.96 ng




response 791954

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.05
264.00	61.60	65.35
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122324\
Data File : BN035810.D
Acq On : 24 Dec 2024 07:45
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 25 00:46:53 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 00:46:49 2024
Response via : Initial Calibration

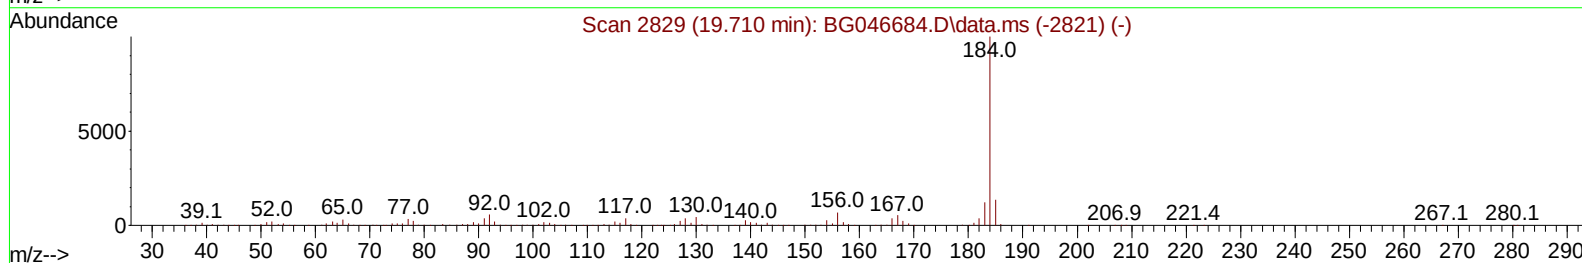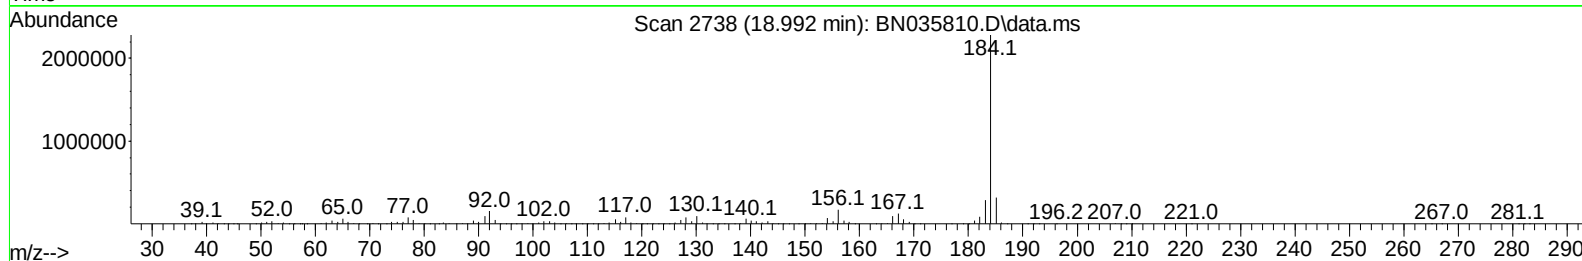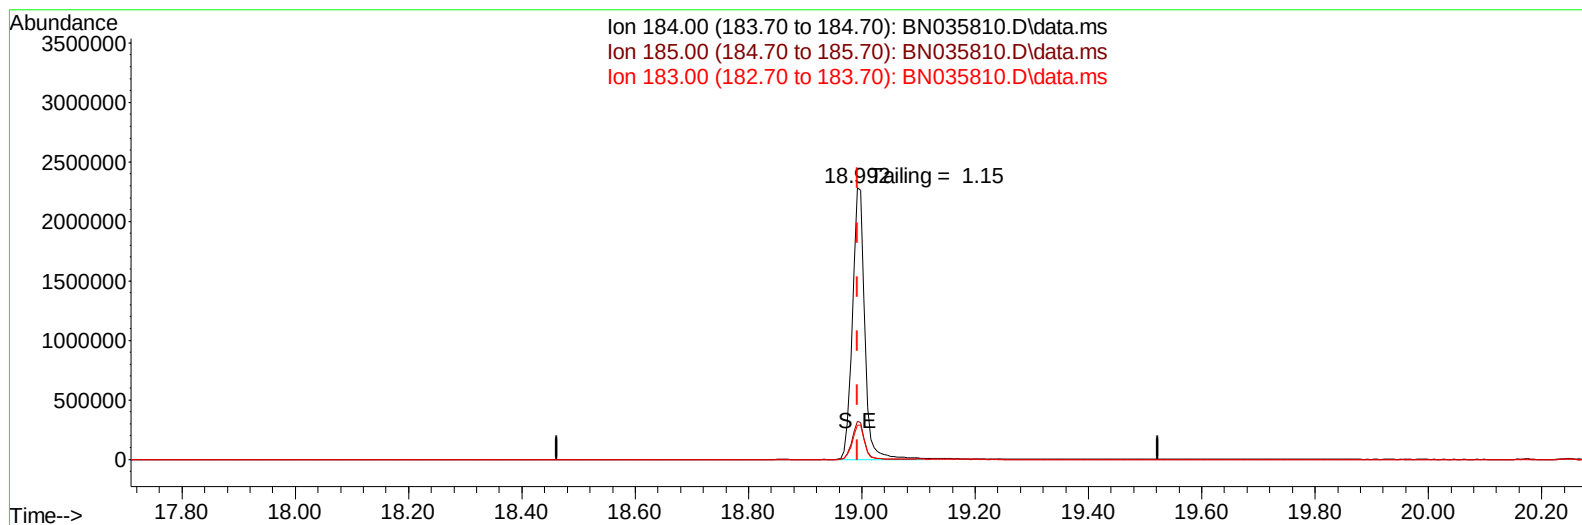

TIC: BN035810.D\data.ms

(77) Benzidine

18.992min (0.000) 0.00 ng

response 3507772

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.96
183.00	13.20	12.67
0.00	0.00	0.00