
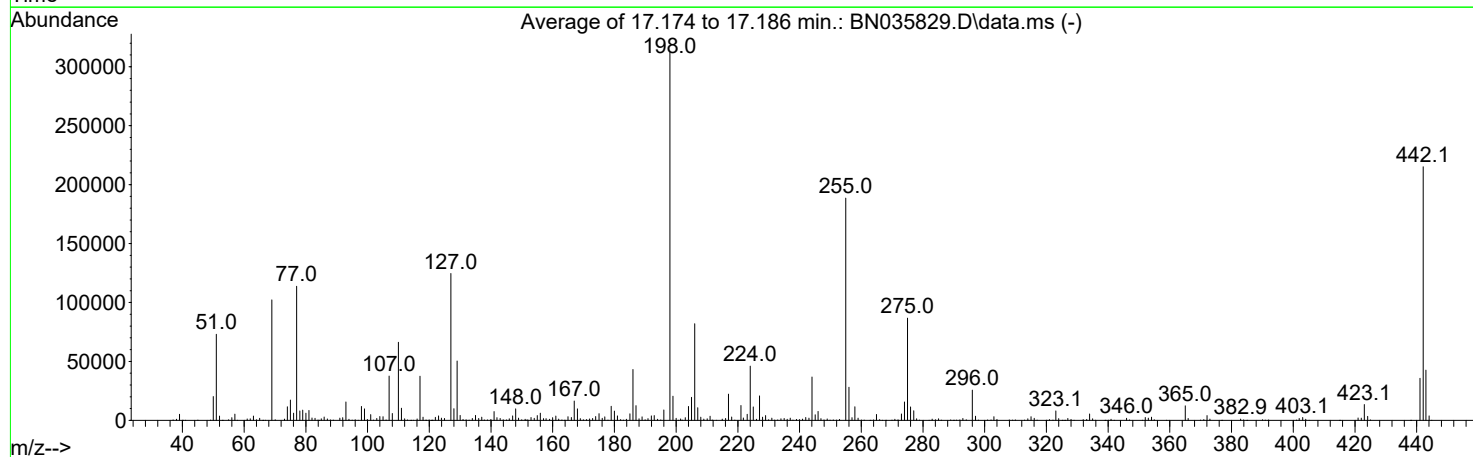


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122324\
Data File : BN035829.D
Acq On : 24 Dec 2024 19:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN112724.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Dec 19 23:06:19 2024

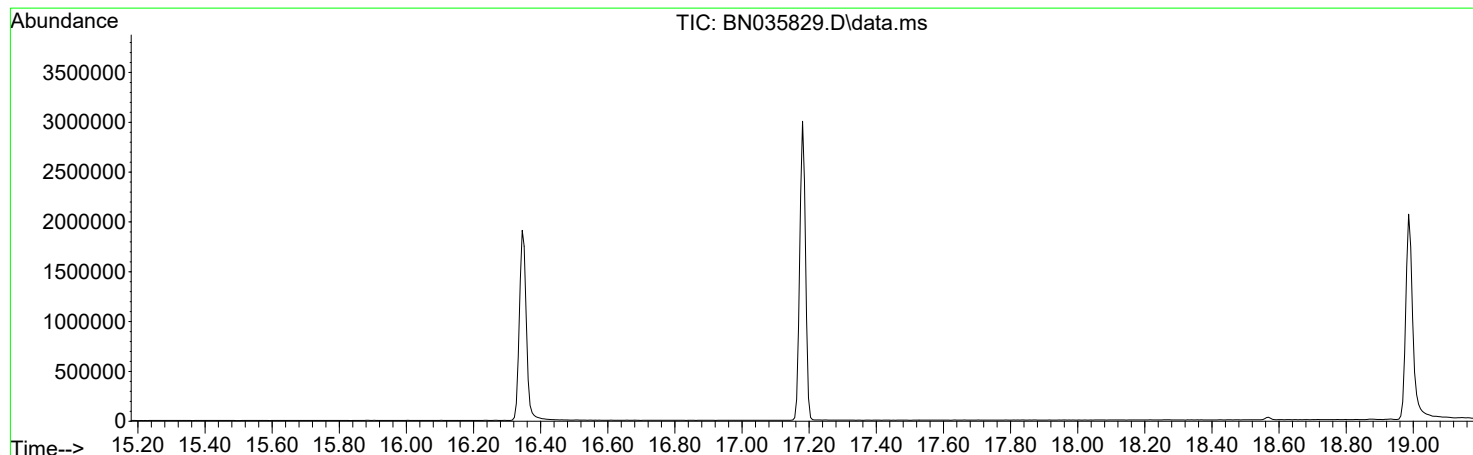

AutoFind: Scans 2429, 2430, 2431; Background Corrected with Scan 2422

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.4	72981	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	32.7	102160	PASS
70	69	0.00	2	0.5	531	PASS
127	198	10	80	39.9	124571	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	312085	PASS
199	198	5	9	6.6	20517	PASS
275	198	10	60	27.8	86749	PASS
365	198	1	100	3.9	12312	PASS
441	198	0.01	100	11.4	35683	PASS
442	442	50	100	100.0	215104	PASS
443	442	15	24	19.8	42619	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
12/23/2024	BNA_N	<u>BN035829.D</u>
Compound Name	Response	Retention Time
DDT	824107	20.245
DDD	86807	19.798
DDE	4191	19.28
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
90998	915105	9.94

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122324\
Data File : BN035829.D
Acq On : 24 Dec 2024 19:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 25 04:24:00 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

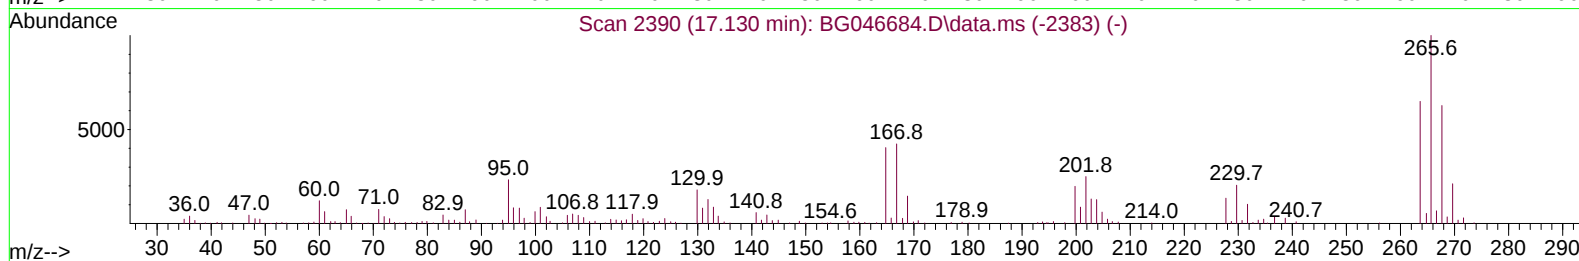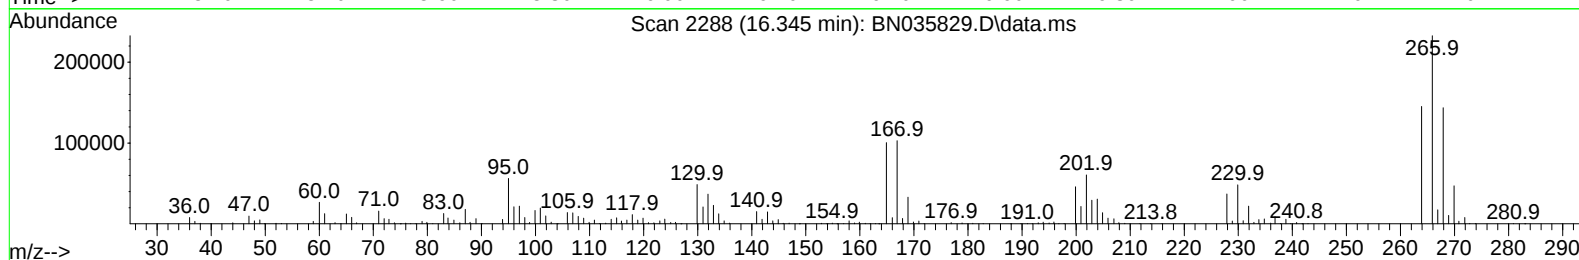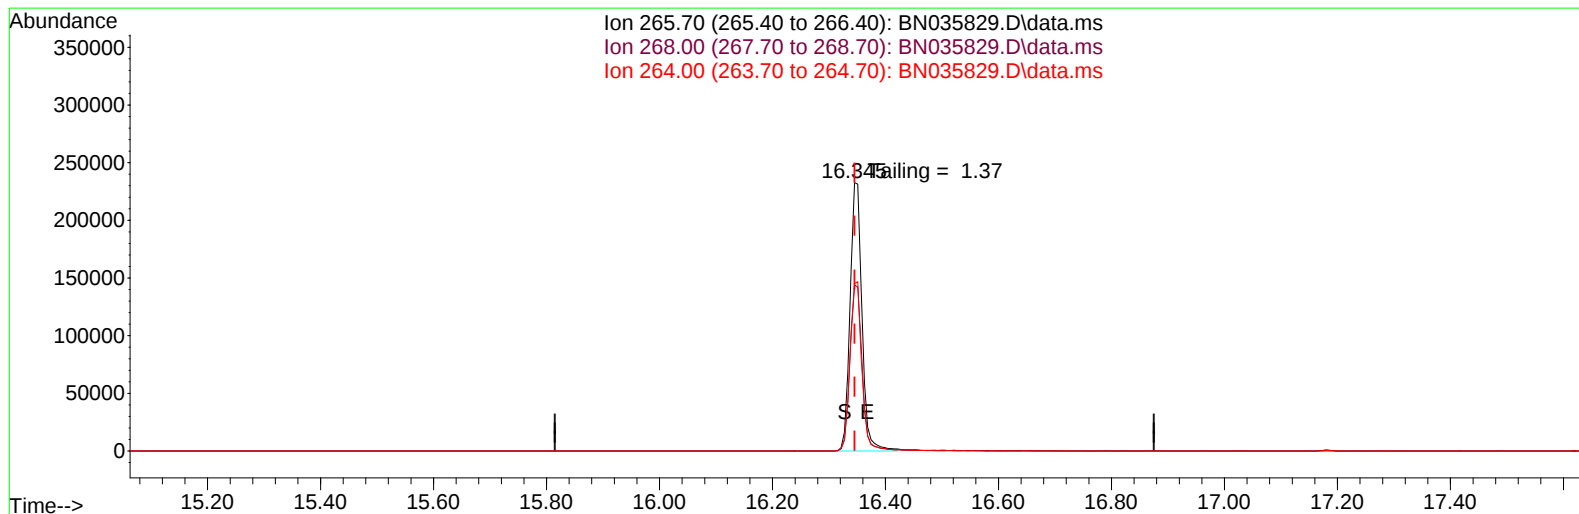

TIC: BN035829.D\data.ms

(70) Pentachlorophenol (C)

16.345min (0.000) 23024.60 ng




response 344759

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.74
264.00	61.60	62.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122324\
Data File : BN035829.D
Acq On : 24 Dec 2024 19:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 25 04:24:00 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

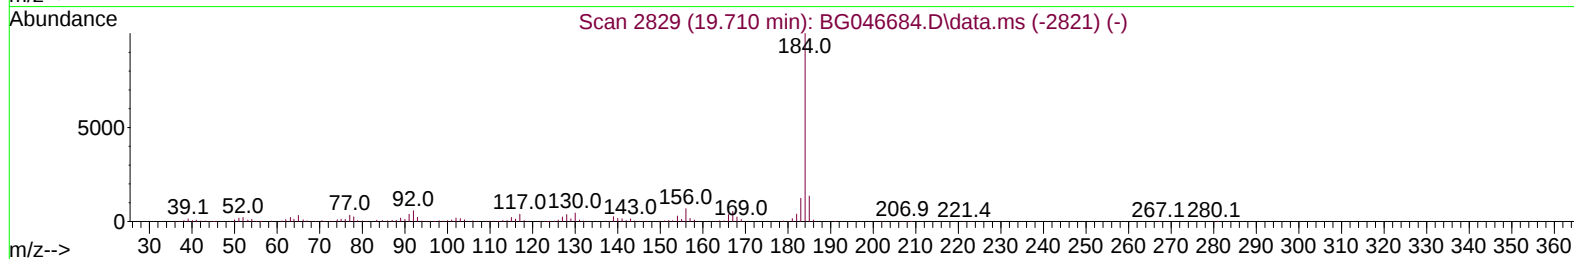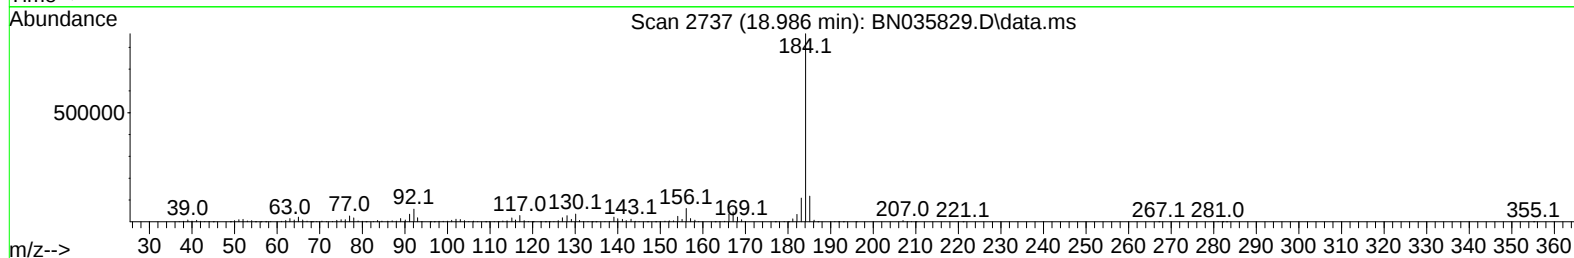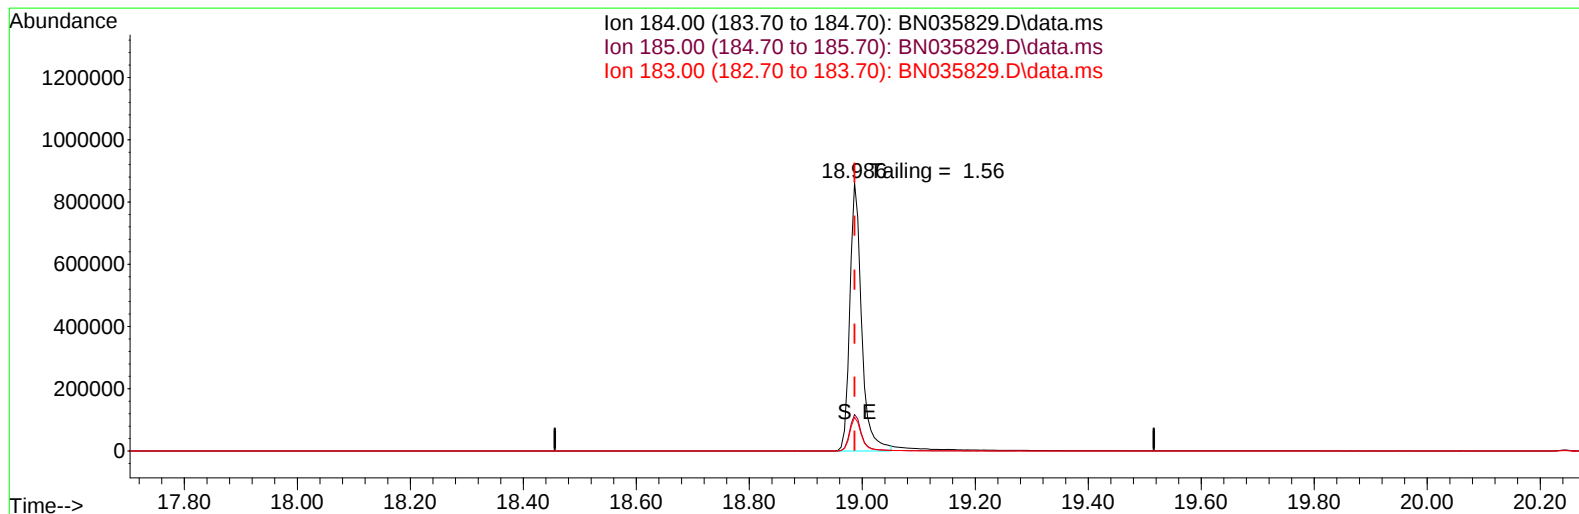

TIC: BN035829.D\data.ms

(77) Benzidine

18.986min (0.000) 0.00 ng

response 1299882

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.60
183.00	13.20	12.60
0.00	0.00	0.00