

Data File : BN004206.D
Acq On : 26 Dec 2018 17:11
Operator : JU/SJ
Sample : J6489-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9F54

Quant Time: Dec 27 04:49:08 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN121218MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 27 04:46:35 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	28210	20.00	ng/ul	0.00
18) Naphthalene-d8	10.62	136	139367	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.46	164	84242	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.21	188	197030	20.00	ng/ul	0.00
77) Chrysene-d12	21.40	240	240656	20.00	ng/ul	0.00
85) Perylene-d12	23.73	264	268165	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.28	96	2164	5.02	ng/uL	0.00
5) Phenol-d5	6.99	99	12915	4.66	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.16	67	37743	25.00	ng/ul	0.00
9) 2-Chlorophenol-d4	7.35	132	43681	20.10	ng/ul	0.00
13) 4-Methylphenol-d8	8.53	113	28310	12.18	ng/ul	0.00
19) Nitrobenzene-d5	8.99	128	28567	25.87	ng/ul	0.00
22) 2-Nitrophenol-d4	9.71	143	34054	27.23	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.25	165	57351	25.00	ng/ul	0.00
29) 4-Chloroaniline-d4	10.77	131	3245	1.51	ng/ul	0.00
43) Dimethylphthalate-d6	13.87	166	213765	28.43	ng/ul	0.00
46) Acenaphthylene-d8	14.16	160	257484	28.86	ng/ul	0.00
51) 4-Nitrophenol-d4	14.69	143	7351	4.73	ng/ul	0.01
57) Fluorene-d10	15.46	176	184740	28.41	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.59	200	36677	25.85	ng/ul	0.00
70) Anthracene-d10	17.31	188	298327	29.96	ng/ul	0.00
78) Pyrene-d10	19.61	212	339287	31.52	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.58	264	447416	30.75	ng/ul	0.00


Target Compounds					Qvalue	
17) Hexachloroethane	8.92	117	1316	1.668	ng/ul#	6


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN004206.D
Acq On : 26 Dec 2018 17:11
Operator : JU/SJ
Sample : J6489-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9F54

Quant Time: Dec 27 04:49:08 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN121218MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 27 04:46:35 2018
Response via : Initial Calibration

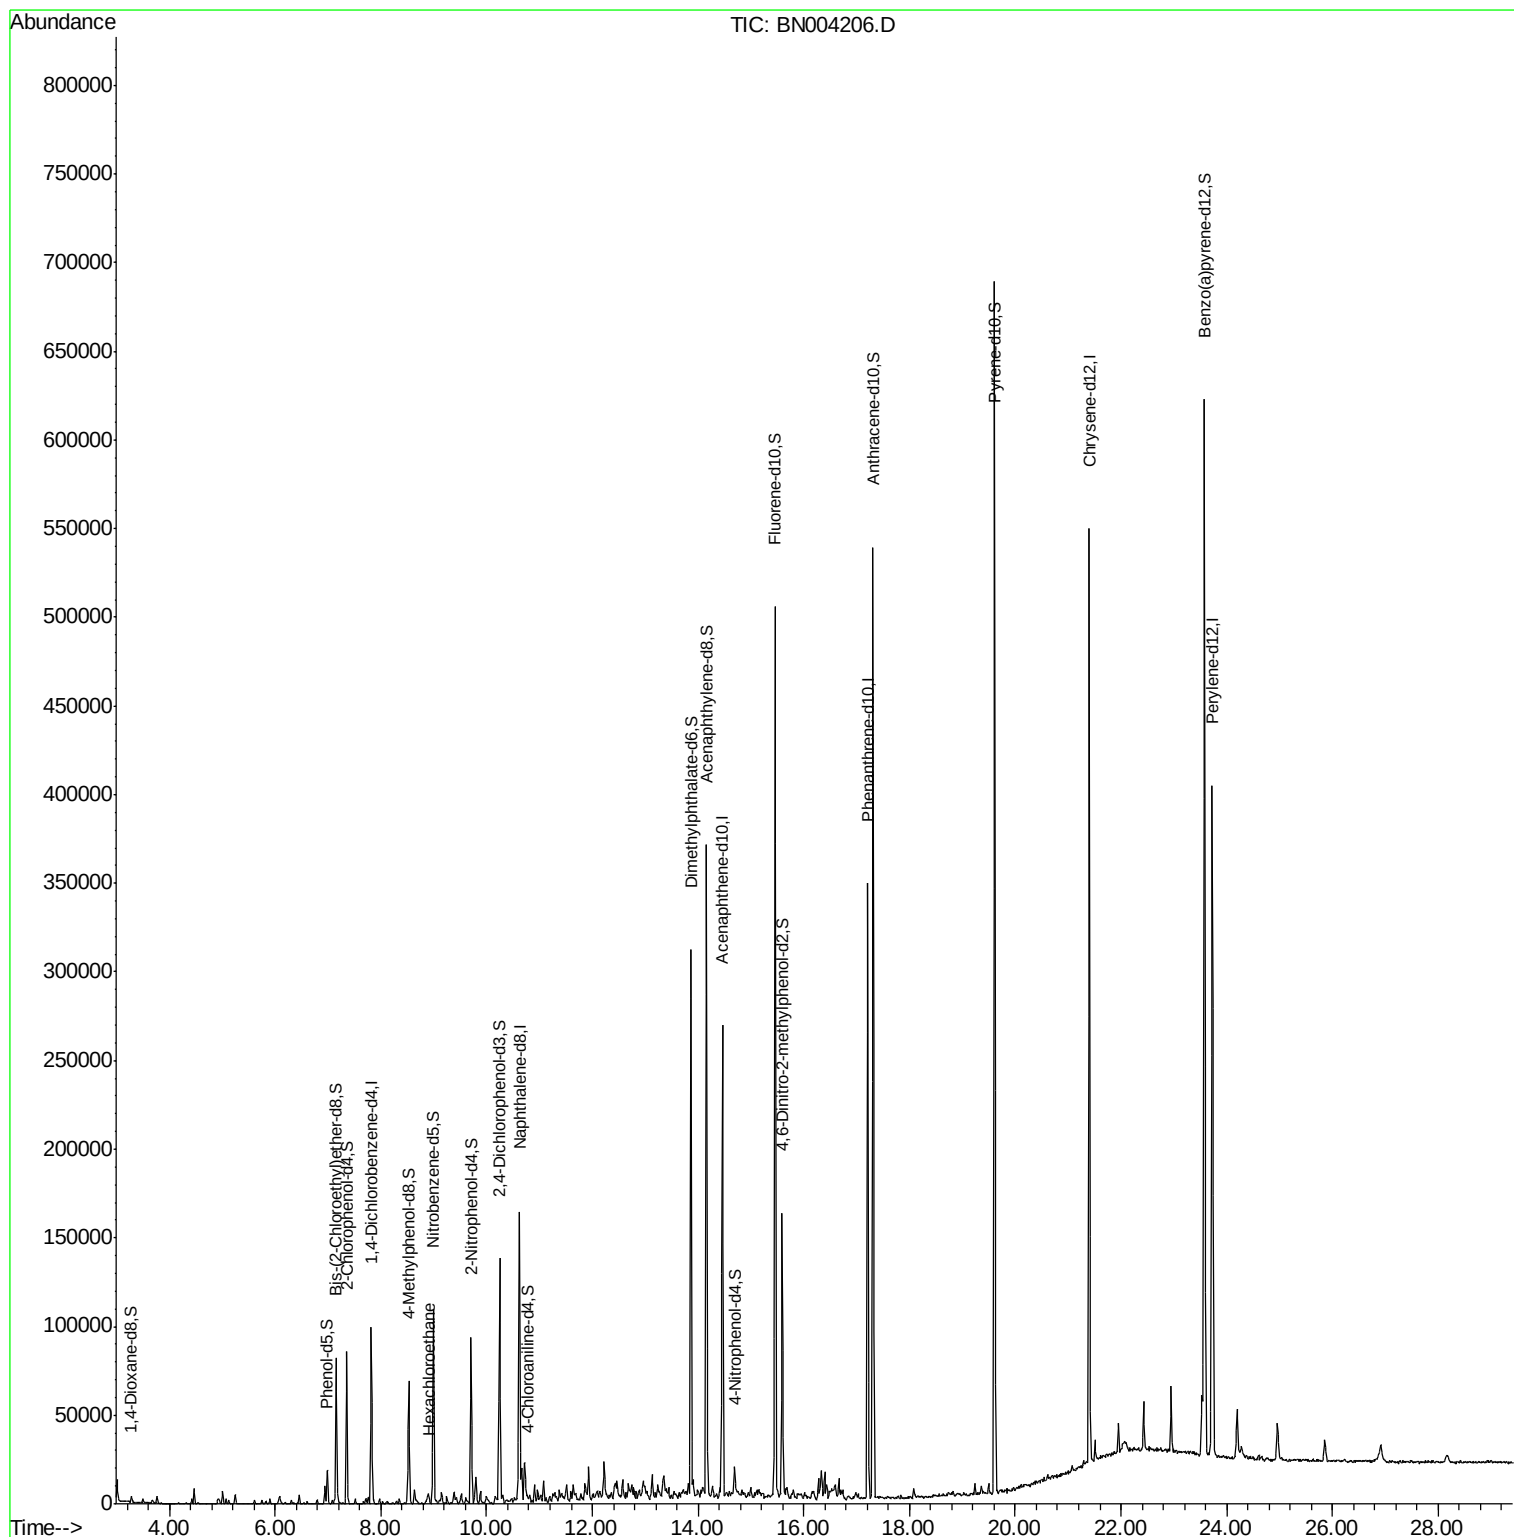

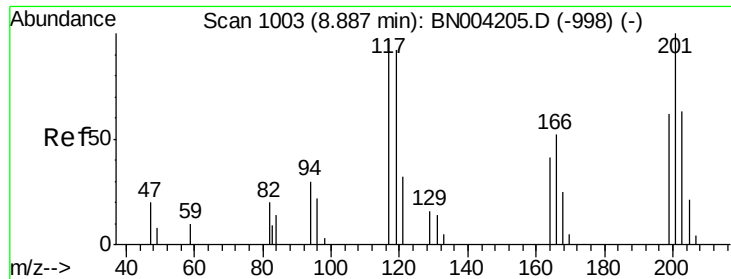

#17
 Hexachloroethane
 Concen: 1.668 ng/ul
 RT: 8.92 min Scan# 1009
 Delta R.T. 0.04 min
 Lab File: BN004206.D
 Acq: 26 Dec 2018 17:11

Instrument :
 BNA_N
 ClientSampleId :
 F9F54

Tgt Ion:117 Resp: 1316
 Ion Ratio Lower Upper
 117 100
 201 0.0 82.1 123.1#
 199 0.0 50.6 76.0#

