

Data File : BN004220.D
Acq On : 27 Dec 2018 01:19
Operator : JU/SJ
Sample : PB115982BL
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK82

Quant Time: Dec 27 05:45:45 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN121218MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 27 04:46:35 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	24963	20.00	ng/ul	0.00
18) Naphthalene-d8	10.62	136	126196	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.46	164	80927	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.21	188	190624	20.00	ng/ul	0.00
77) Chrysene-d12	21.39	240	237012	20.00	ng/ul	0.00
85) Perylene-d12	23.72	264	268541	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.28	96	3853	10.10	ng/uL	0.00
5) Phenol-d5	6.99	99	106987	43.60	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.16	67	64995	48.65	ng/ul	0.00
9) 2-Chlorophenol-d4	7.36	132	86422	44.94	ng/ul	0.00
13) 4-Methylphenol-d8	8.53	113	108410	52.71	ng/ul	0.00
19) Nitrobenzene-d5	8.99	128	56812	56.82	ng/ul	0.00
22) 2-Nitrophenol-d4	9.71	143	71966	63.55	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.24	165	115493	55.60	ng/ul	0.00
29) 4-Chloroaniline-d4	10.76	131	212617	109.40	ng/ul	0.00
43) Dimethylphthalate-d6	13.87	166	652868	90.38	ng/ul	0.00
46) Acenaphthylene-d8	14.16	160	672359	78.44	ng/ul	0.00
51) 4-Nitrophenol-d4	14.69	143	116478	77.99	ng/ul	0.00
57) Fluorene-d10	15.46	176	516495	82.69	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.60	200	127792	93.08	ng/ul	0.00
70) Anthracene-d10	17.31	188	887579	92.15	ng/ul	0.00
78) Pyrene-d10	19.61	212	1037193	97.82	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.58	264	1436343	98.59	ng/ul	0.00


Target Compounds					Qvalue	
15) N-Nitroso-di-n-propylamine	8.53	70	2189	1.441	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN004220.D
Acq On : 27 Dec 2018 01:19
Operator : JU/SJ
Sample : PB115982BL
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK82

Quant Time: Dec 27 05:45:45 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN121218MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 27 04:46:35 2018
Response via : Initial Calibration

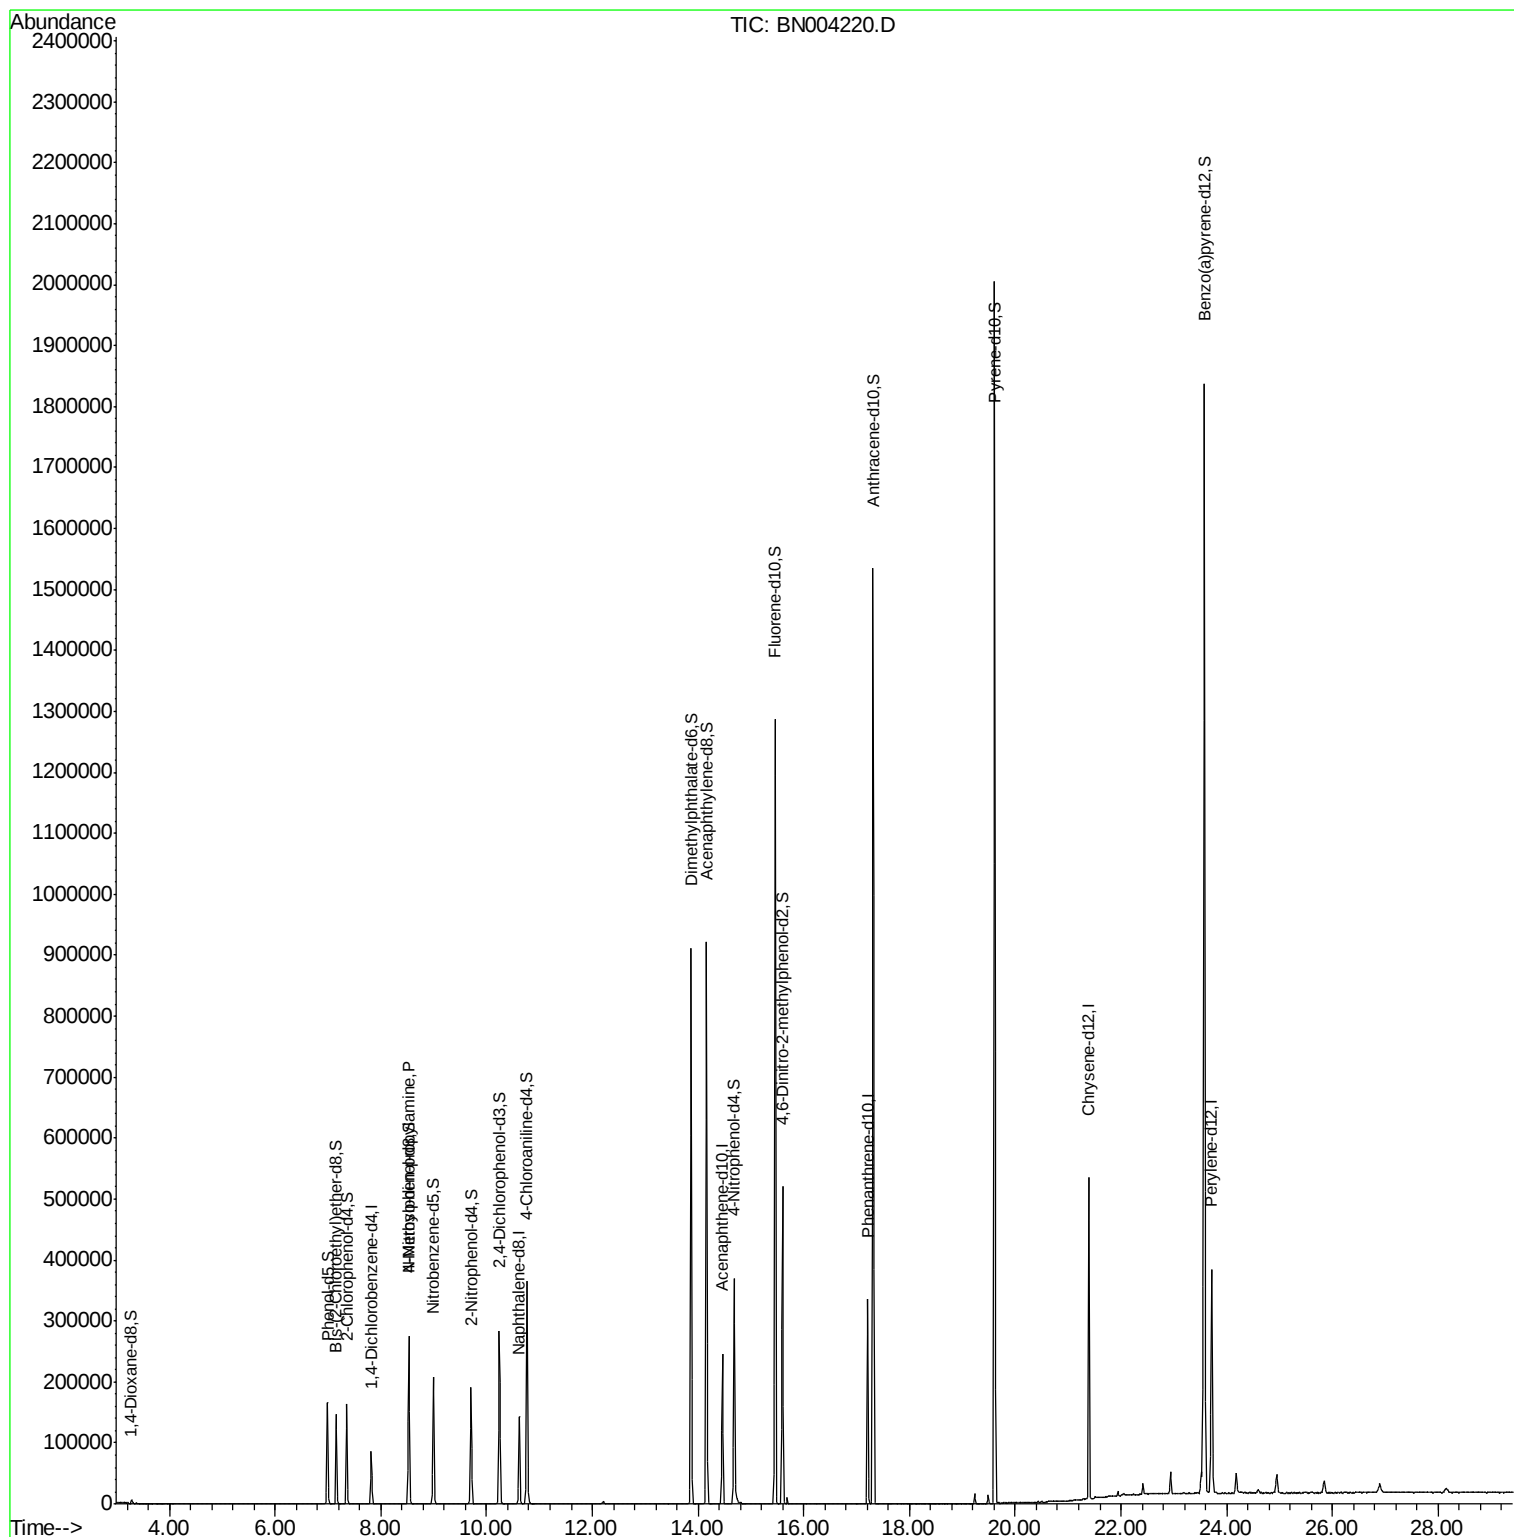

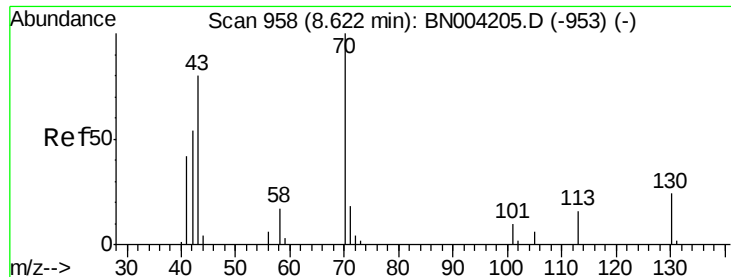

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.441 ng/ul
 RT: 8.53 min Scan# 942
 Delta R.T. -0.09 min
 Lab File: BN004220.D
 Acq: 27 Dec 2018 01:19

Instrument :
 BNA_N
 ClientSampleId :
 SBLK82

Tgt Ion:	70	Resp:	2189
Ion	Ratio	Lower	Upper
70	100		
42	366.1	42.3	63.5#
101	0.0	8.7	13.1#
130	0.0	20.2	30.2#

