

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN122618\
 Data File : BN004229.D
 Acq On : 27 Dec 2018 06:32
 Operator : JU/SJ
 Sample : J6541-02
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9F72

Quant Time: Dec 27 07:58:45 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN121218MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 27 05:47:30 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	25973	20.00	ng/ul	0.00
18) Naphthalene-d8	10.62	136	126085	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.46	164	82486	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.21	188	200862	20.00	ng/ul	0.00
77) Chrysene-d12	21.39	240	248083	20.00	ng/ul	0.00
85) Perylene-d12	23.72	264	288412	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.28	96	2008	5.06	ng/uL	0.00
5) Phenol-d5	6.99	99	10830	4.24	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.16	67	31398	22.59	ng/ul	0.00
9) 2-Chlorophenol-d4	7.35	132	36697	18.34	ng/ul	0.00
13) 4-Methylphenol-d8	8.53	113	22909	10.71	ng/ul	0.00
19) Nitrobenzene-d5	8.99	128	24094	24.12	ng/ul	0.00
22) 2-Nitrophenol-d4	9.71	143	28093	24.83	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.25	165	46913	22.61	ng/ul	0.00
29) 4-Chloroaniline-d4	10.77	131	3496	1.80	ng/ul	0.00
43) Dimethylphthalate-d6	13.86	166	189033	25.67	ng/ul	0.00
46) Acenaphthylene-d8	14.16	160	225399	25.80	ng/ul	0.00
51) 4-Nitrophenol-d4	14.69	143	4987	3.28	ng/ul	0.01
57) Fluorene-d10	15.46	176	166315	26.12	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.59	200	31509	21.78	ng/ul	0.00
70) Anthracene-d10	17.30	188	281433	27.73	ng/ul	0.00
78) Pyrene-d10	19.60	212	329283	29.67	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.57	264	446287	28.52	ng/ul	0.00


Target Compounds					Qvalue	
44) Dimethylphthalate	13.91	163	13571	1.888	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN122618\
Data File : BN004229.D
Acq On : 27 Dec 2018 06:32
Operator : JU/SJ
Sample : J6541-02
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9F72

Quant Time: Dec 27 07:58:45 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN121218MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 27 05:47:30 2018
Response via : Initial Calibration

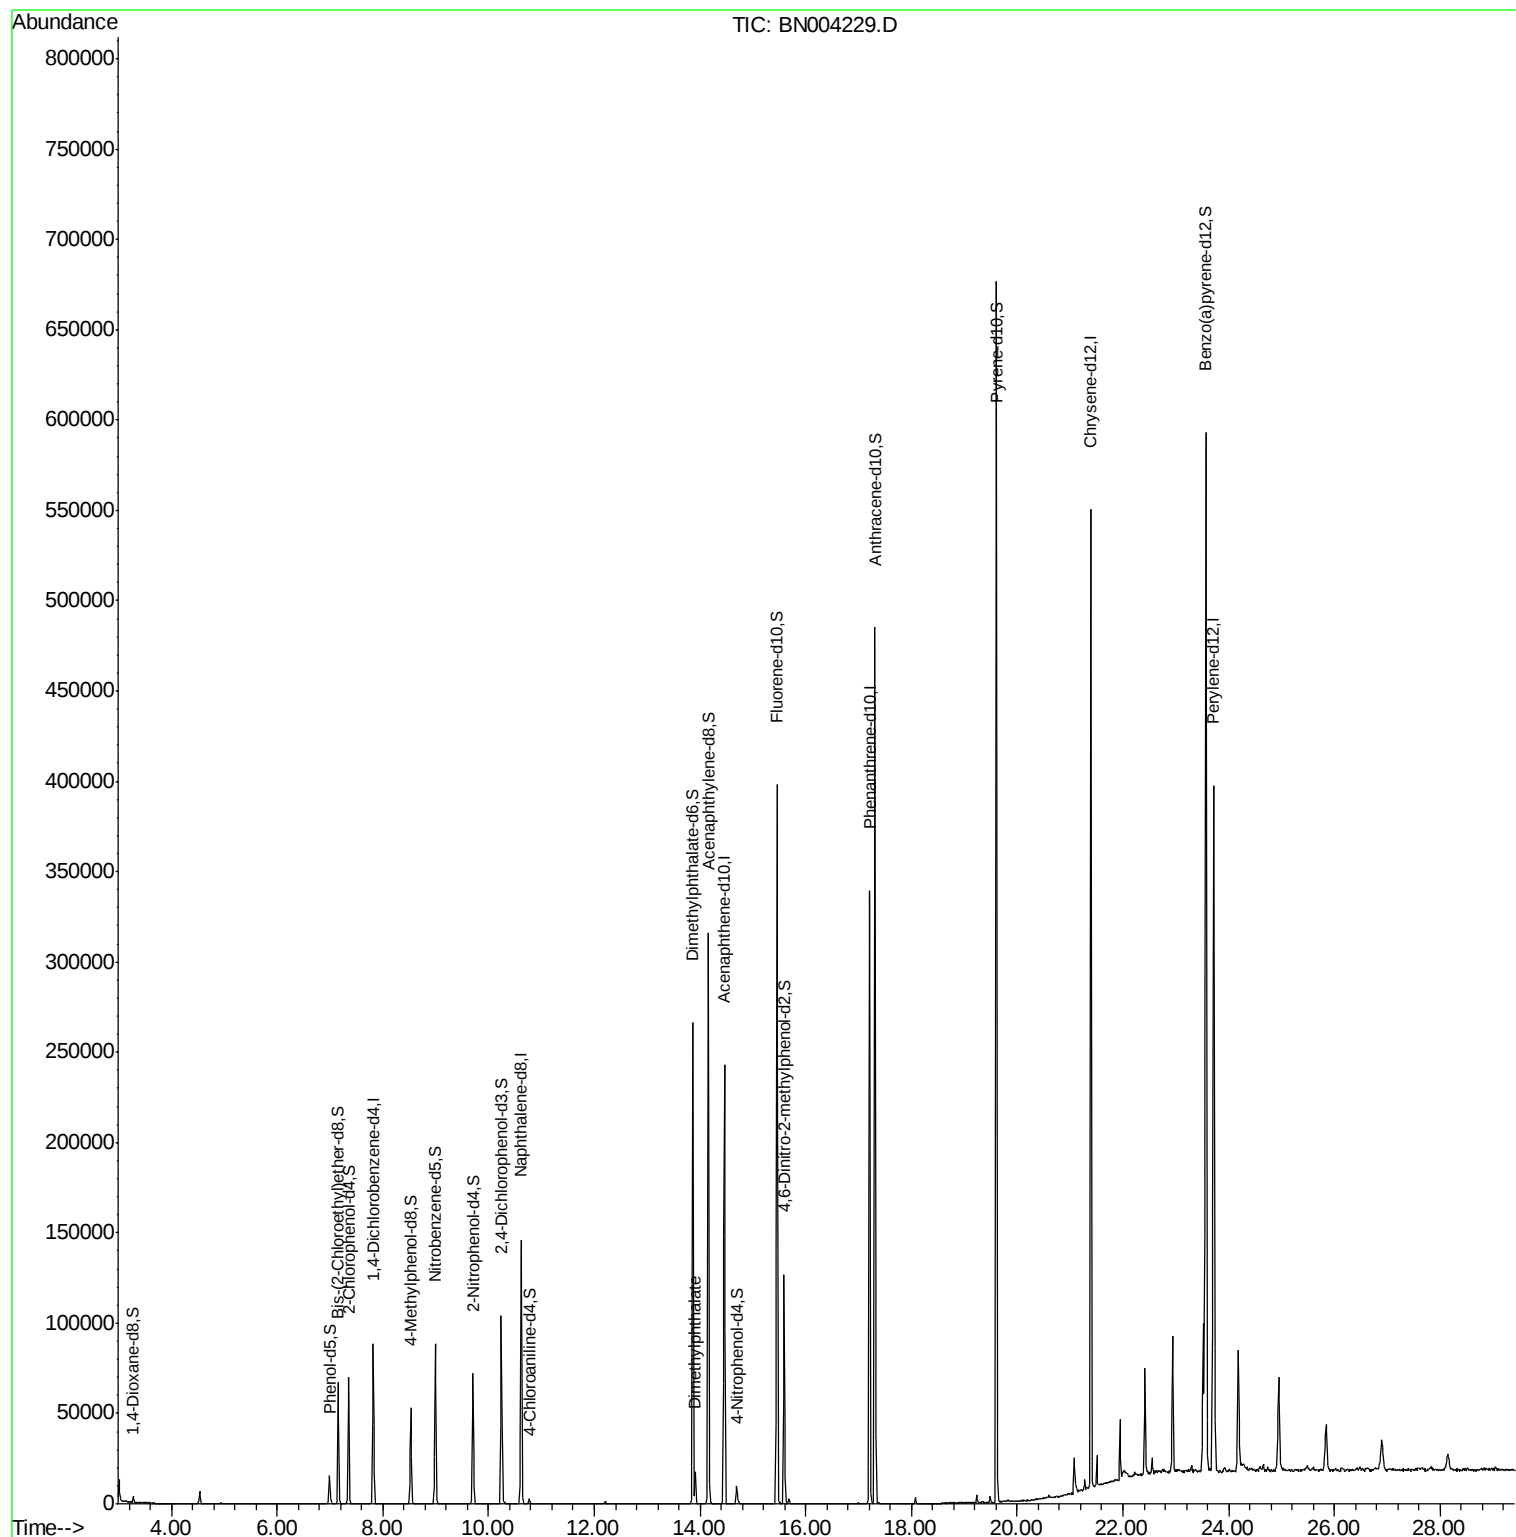

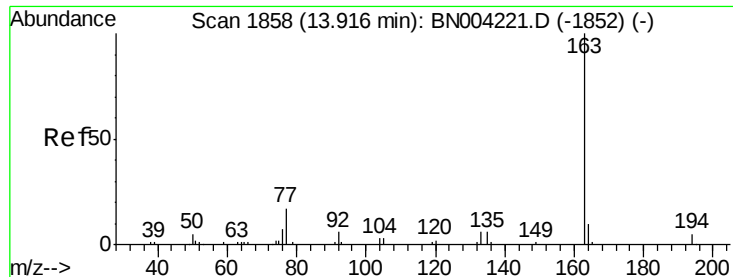

#44

Dimethylphthalate

Concen: 1.888 ng/ul

RT: 13.91 min Scan# 1857

Delta R.T. -0.01 min

Lab File: BN004229.D

Acq: 27 Dec 2018 06:32

Instrument :

BNA_N

ClientSampleId :

F9F72


Tgt Ion:163 Resp: 13571

Ion Ratio Lower Upper

163 100

194 4.4 3.4 5.0

164 10.4 7.9 11.9

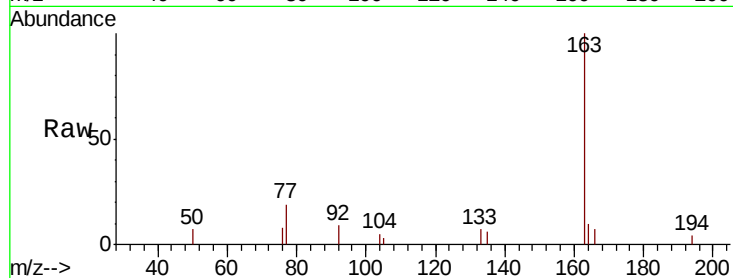

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

