

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN122618\
 Data File : BN004201.D
 Acq On : 26 Dec 2018 14:17
 Operator : JU/SJ
 Sample : J6485-09
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 ETO89

Quant Time: Dec 27 04:14:47 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN121218MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 27 04:11:48 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	23414	20.00	ng/ul	0.00
18) Naphthalene-d8	10.62	136	111784	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.46	164	71289	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.21	188	170000	20.00	ng/ul	0.00
77) Chrysene-d12	21.40	240	208475	20.00	ng/ul	0.00
85) Perylene-d12	23.72	264	234914	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.28	96	2663	7.44	ng/uL	0.00
5) Phenol-d5	6.99	99	17103	7.43	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.16	67	38782	30.95	ng/ul	0.00
9) 2-Chlorophenol-d4	7.35	132	46911	26.01	ng/ul	0.00
13) 4-Methylphenol-d8	8.52	113	31946	16.56	ng/ul	0.00
19) Nitrobenzene-d5	8.99	128	29177	32.94	ng/ul	0.00
22) 2-Nitrophenol-d4	9.71	143	34543	34.44	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.24	165	54663	29.71	ng/ul	0.00
29) 4-Chloroaniline-d4	10.77	131	6547	3.80	ng/ul	0.00
43) Dimethylphthalate-d6	13.87	166	214007	33.63	ng/ul	0.00
46) Acenaphthylene-d8	14.16	160	256813	34.01	ng/ul	0.00
51) 4-Nitrophenol-d4	14.69	143	8086	6.15	ng/ul	0.00
57) Fluorene-d10	15.46	176	185252	33.67	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.59	200	34574	28.24	ng/ul	0.00
70) Anthracene-d10	17.31	188	298602	34.76	ng/ul	0.00
78) Pyrene-d10	19.60	212	336639	36.10	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.57	264	442309	34.71	ng/ul	0.00


Target Compounds					Ovalue	
6) Phenol	7.02	94	2714	1.168	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN122618\
Data File : BN004201.D
Acq On : 26 Dec 2018 14:17
Operator : JU/SJ
Sample : J6485-09
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
ETO89

Quant Time: Dec 27 04:14:47 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN121218MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 27 04:11:48 2018
Response via : Initial Calibration

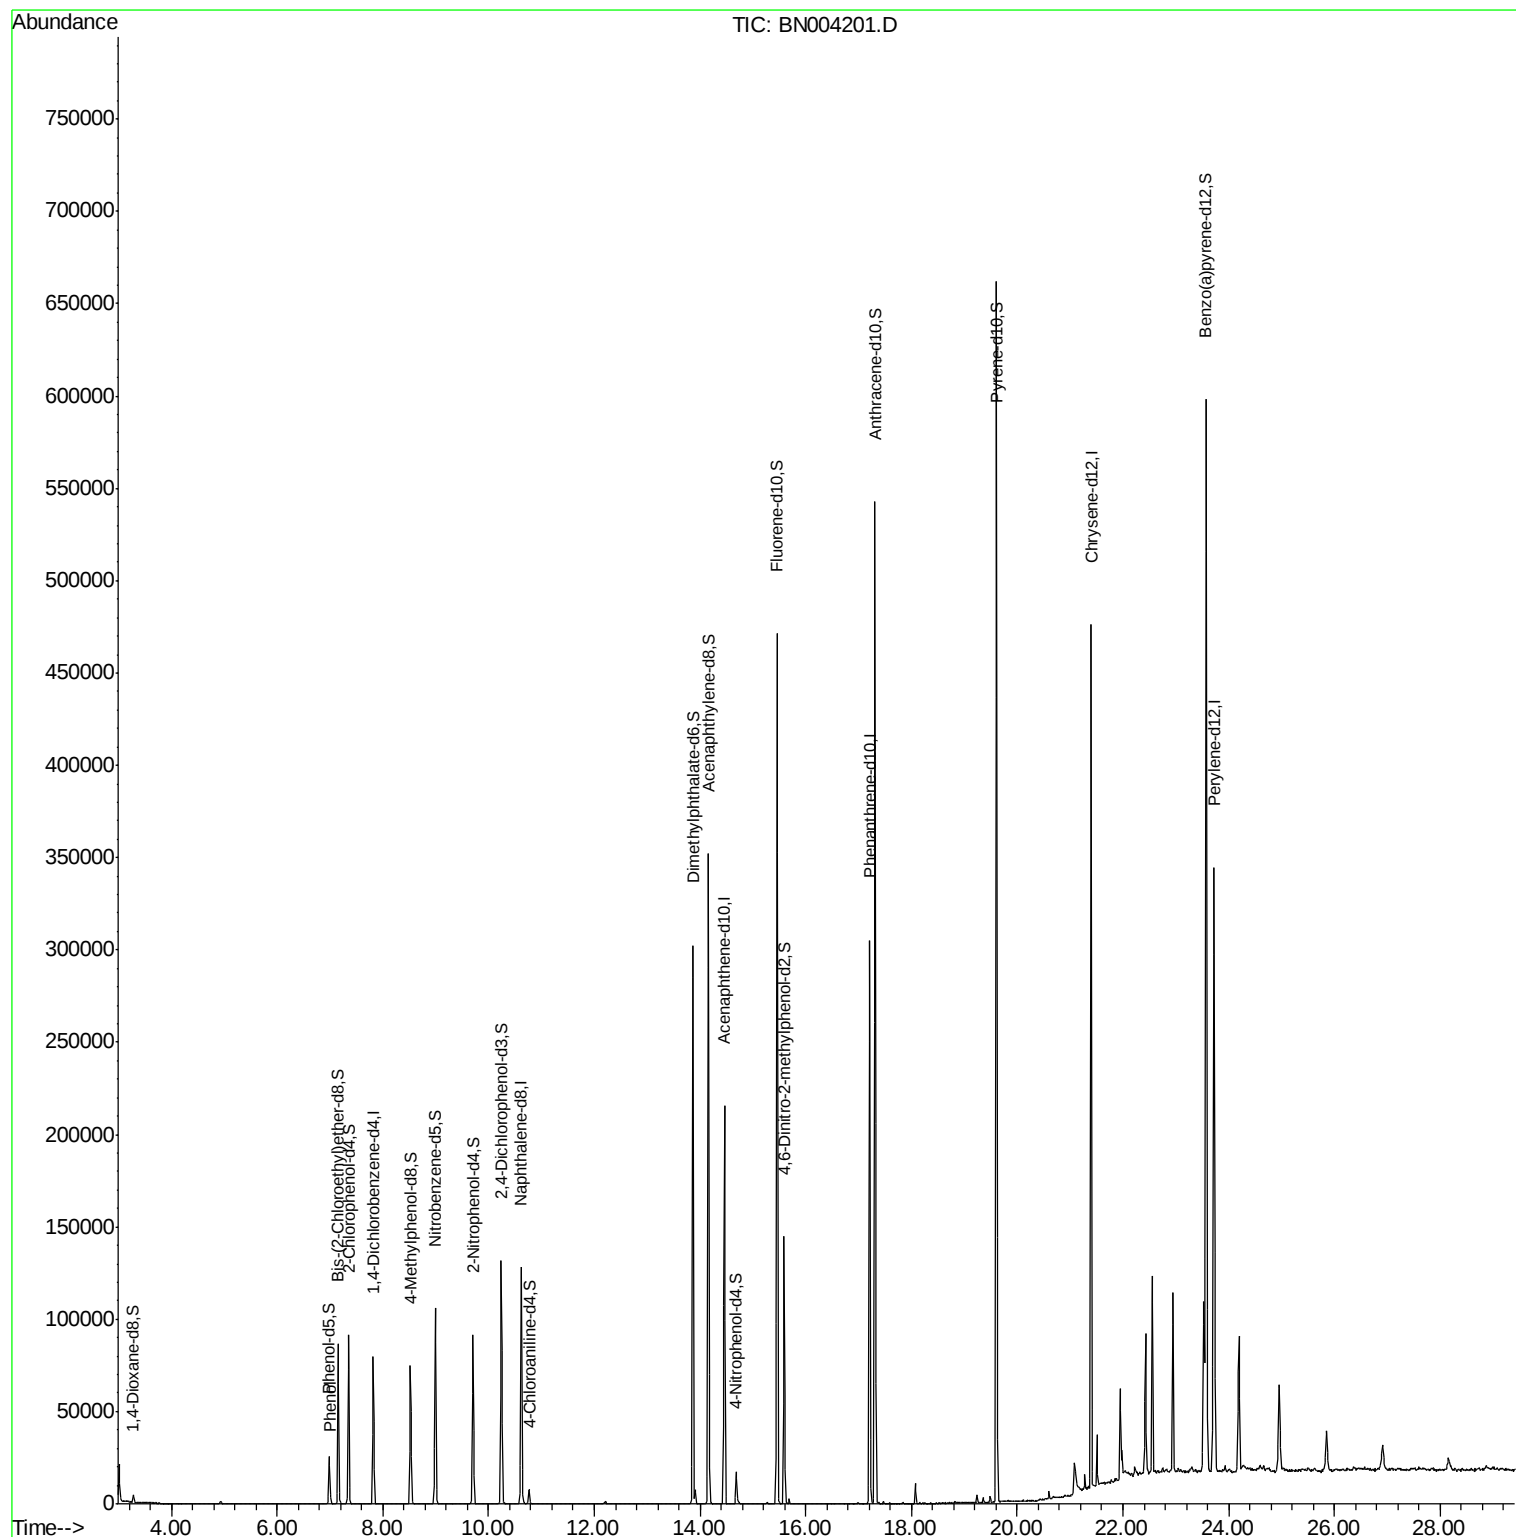

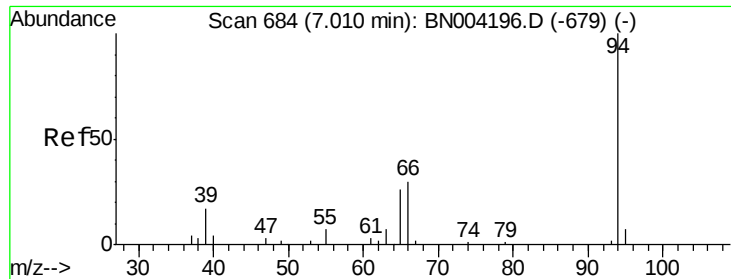

#6

Phenol

Concen: 1.168 ng/ul

RT: 7.02 min Scan# 685

Delta R.T. 0.01 min

Lab File: BN004201.D

Acq: 26 Dec 2018 14:17

Instrument :

BNA_N

ClientSampleId :

ETO89

Tot Ion: 94 Resp: 2714

Ion Ratio Lower Upper

94 100

65 25.8 21.2 31.8

66 36.0 26.9 40.3

