

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN122618\
 Data File : BN004231.D
 Acq On : 27 Dec 2018 08:18
 Operator : JU/SJ
 Sample : J6541-05
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9F79

Quant Time: Dec 27 10:32:35 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN121218MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 27 05:47:30 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	26737	20.00	ng/ul	0.00
18) Naphthalene-d8	10.62	136	131845	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.46	164	84836	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.21	188	201214	20.00	ng/ul	0.00
77) Chrysene-d12	21.40	240	255224	20.00	ng/ul	0.00
85) Perylene-d12	23.72	264	293227	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.28	96	2091	5.12	ng/uL	0.00
5) Phenol-d5	6.99	99	12341	4.70	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.15	67	32712	22.86	ng/ul	0.00
9) 2-Chlorophenol-d4	7.35	132	38447	18.67	ng/ul	0.00
13) 4-Methylphenol-d8	8.53	113	25629	11.63	ng/ul	0.00
19) Nitrobenzene-d5	8.99	128	25924	24.82	ng/ul	0.00
22) 2-Nitrophenol-d4	9.70	143	30654	25.91	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.24	165	50479	23.26	ng/ul	0.00
29) 4-Chloroaniline-d4	0.00	131	0	0.00	ng/ul	
43) Dimethylphthalate-d6	13.86	166	203934	26.93	ng/ul	0.00
46) Acenaphthylene-d8	14.16	160	237861	26.47	ng/ul	0.00
51) 4-Nitrophenol-d4	14.70	143	6290	4.02	ng/ul	0.02
57) Fluorene-d10	15.45	176	174793	26.69	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.59	200	33289	22.97	ng/ul	0.00
70) Anthracene-d10	17.31	188	294384	28.95	ng/ul	0.00
78) Pyrene-d10	19.60	212	343196	30.06	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.57	264	467865	29.41	ng/ul	0.00


Target Compounds				Ovalue	
33) 4-Chloro-3-methylphenol	11.91	107	6660	2.741	ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN122618\
Data File : BN004231.D
Acq On : 27 Dec 2018 08:18
Operator : JU/SJ
Sample : J6541-05
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9F79

Quant Time: Dec 27 10:32:35 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN121218MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 27 05:47:30 2018
Response via : Initial Calibration

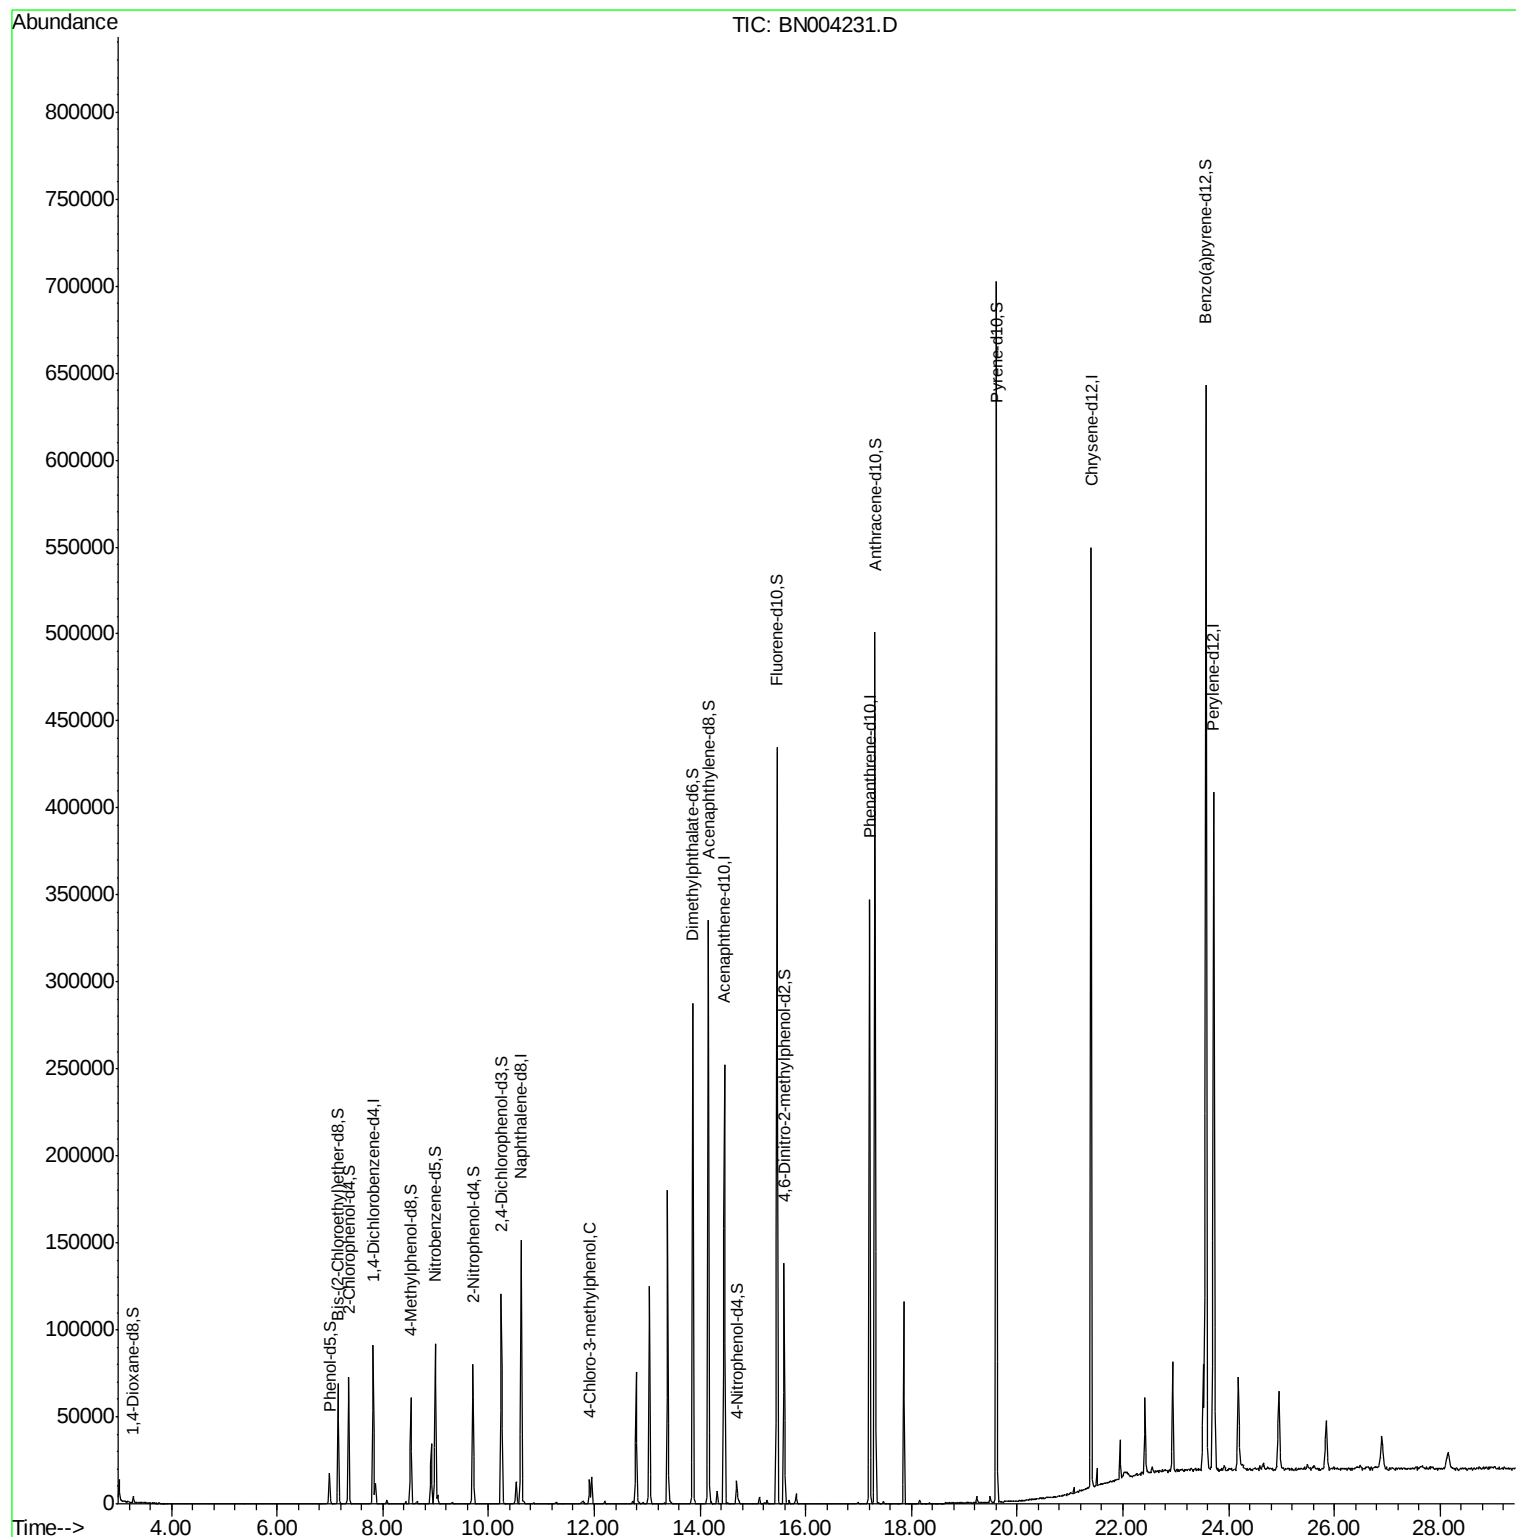

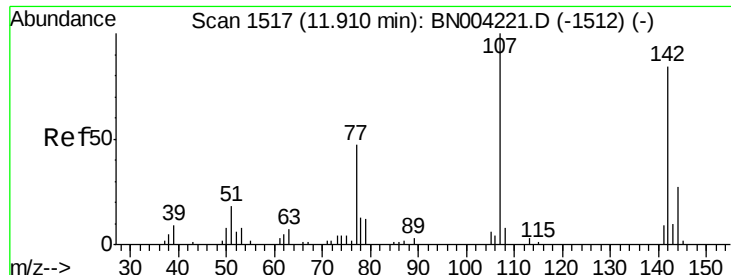

#33

4-Chloro-3-methylphenol

Concen: 2.741 ng/ul

RT: 11.91 min Scan# 1517

Delta R.T. 0.00 min

Lab File: BN004231.D

Acq: 27 Dec 2018 08:18

Instrument :

BNA_N

ClientSampleId :

F9F79



Tot Ion:107 Resp: 6660

Ion Ratio Lower Upper

107 100

144 28.1 21.1 31.7

142 80.4 65.0 97.4

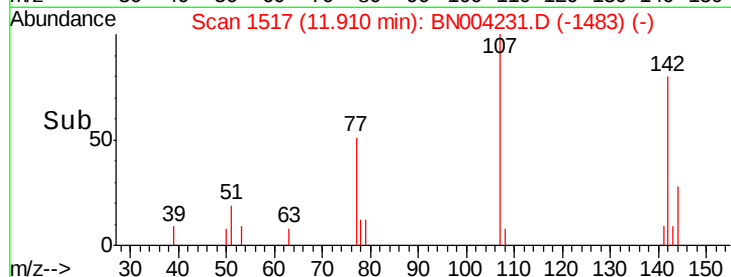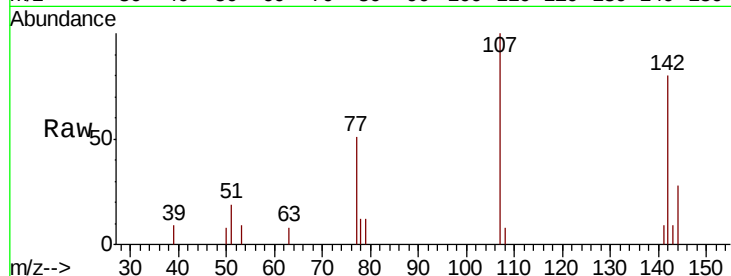

Abundance Ion 107.00 (106.70 to 107.70): E

Ion 144.00 (143.70 to 144.70): E

Ion 142.00 (141.70 to 142.70): E

